

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041422\
 Data File : PS018992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2022 20:58
 Operator : AJ\MA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 02:04:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041422.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 15 02:03:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.803	2564.8E6	551.0E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.029	2.533	3103.0E6	648.6E6	682.500	682.500
2) T	3,5-DICHL...	6.435	5.978	3344.0E6	802.6E6	697.500	697.500
3) T	4-Nitroph...	7.065	6.419	631.3E6	290.2E6	682.500	682.500
5) T	DICAMBA	7.415	6.968	9813.3E6	2386.0E6	705.000	705.000
6) T	MCP	7.587	7.067	790.3E6	190.9E6	70.500	70.500
7) T	MCPA	7.736	7.280	1056.4E6	263.0E6	69.750	69.750
8) T	DICHLORPROP	8.110	7.591	2424.3E6	611.4E6	705.000	705.000
9) T	2,4-D	8.342	7.884	2716.3E6	683.2E6	705.000	705.000
10) T	Pentachlo...	8.648	8.311	31904.7E6	7898.2E6	712.500	712.500
11) T	2,4,5-TP ...	9.201	8.672	13273.9E6	3489.6E6	712.500	712.500
12) T	2,4,5-T	9.487	9.051	12802.7E6	3163.4E6	712.500	712.500
13) T	2,4-DB	10.042	9.558	2205.8E6	433.8E6	712.500	712.500
14) T	DINOSEB	11.198	9.883	10875.9E6	2394.2E6	705.000	705.000
15) T	Picloram	11.024	10.867	17270.2E6	4293.8E6	712.500	712.500
16) T	DCPA	11.466	10.814	16175.1E6	4256.5E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041422\
Data File : PS018992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2022 20:58
Operator : AJ\MA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 02:04:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041422.M
Quant Title : 8080.M
QLast Update : Fri Apr 15 02:03:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

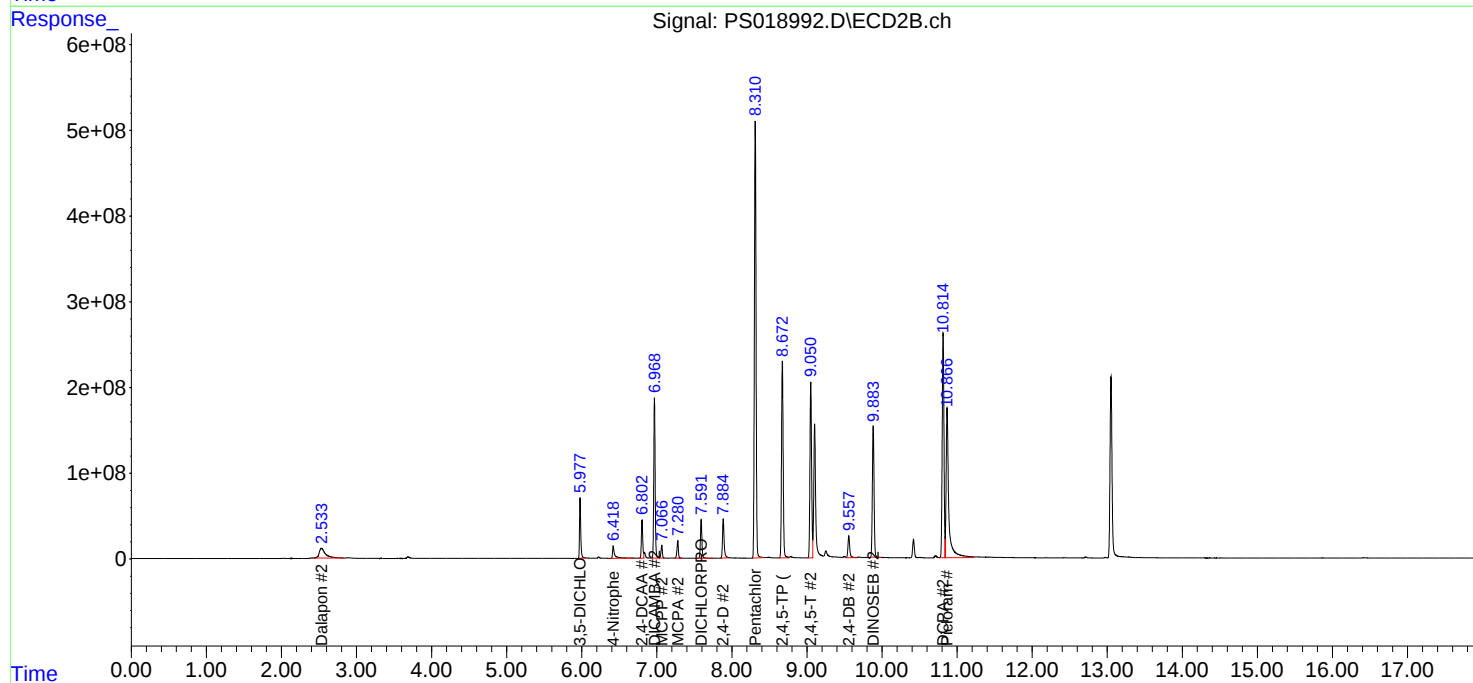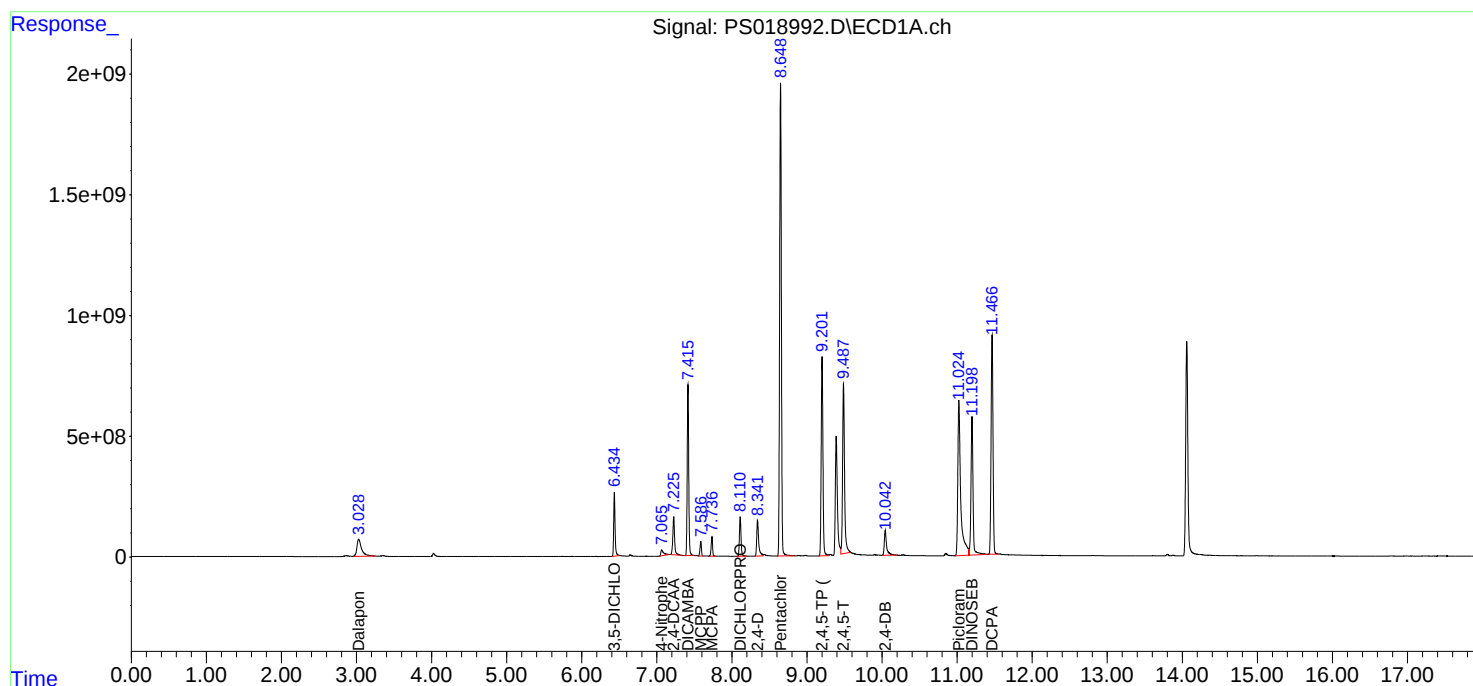


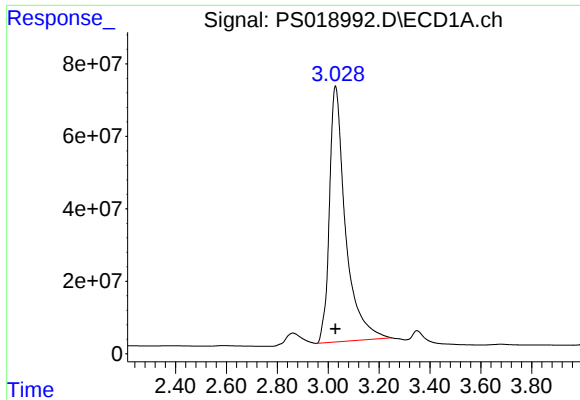

#1 Dalapon


R.T.: 3.029 min
Delta R.T.: 0.000 min
Response: 3102971100
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

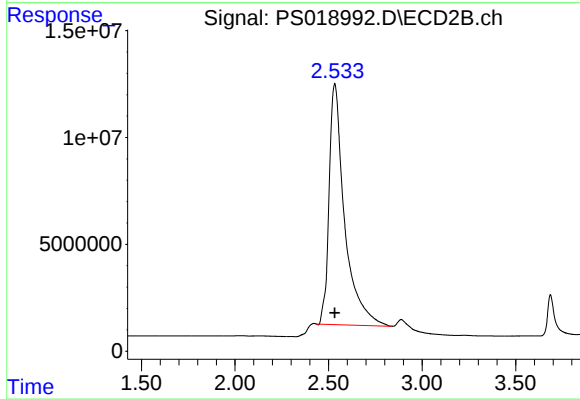


#1 Dalapon

R.T.: 2.533 min
Delta R.T.: 0.000 min
Response: 648619310
Conc: 682.50 ng/ml

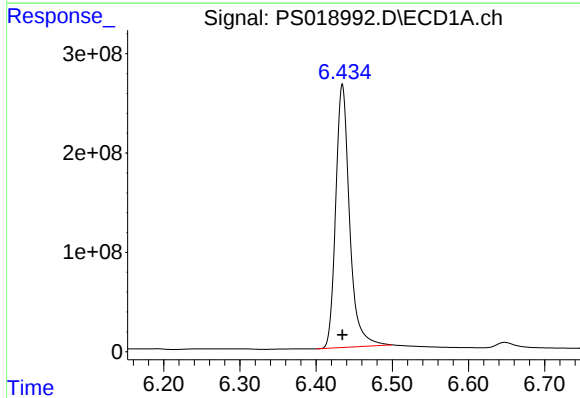


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 3344035511
Conc: 697.50 ng/ml

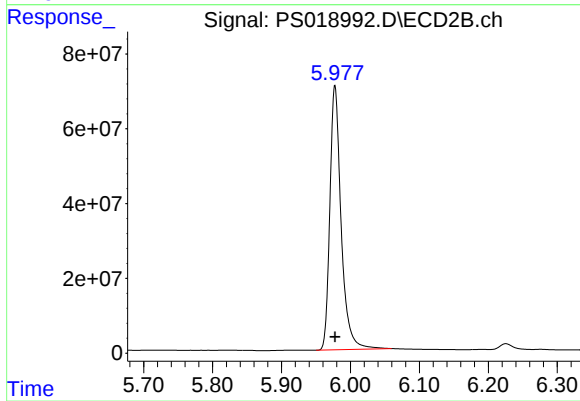

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 802579798
Conc: 697.50 ng/ml

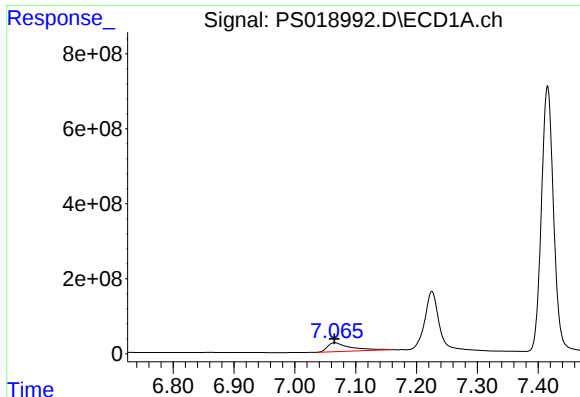

#3 4-Nitrophenol


R.T.: 7.065 min
Delta R.T.: 0.000 min
Response: 631347981
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

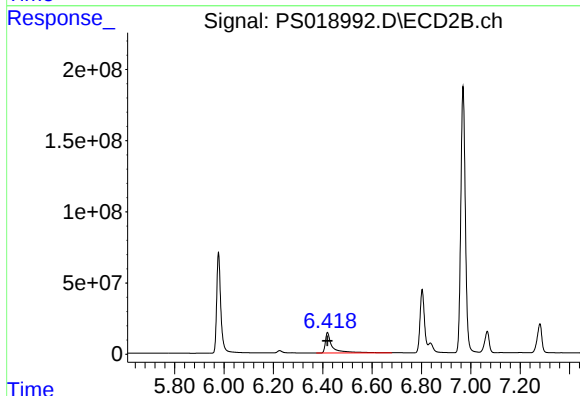


#3 4-Nitrophenol

R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 290173034
Conc: 682.50 ng/ml

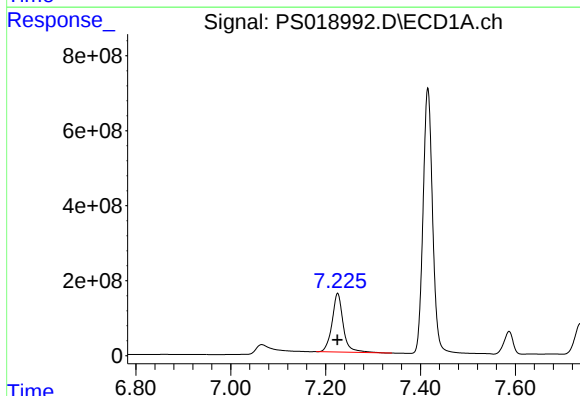


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 2564788939
Conc: 750.00 ng/ml

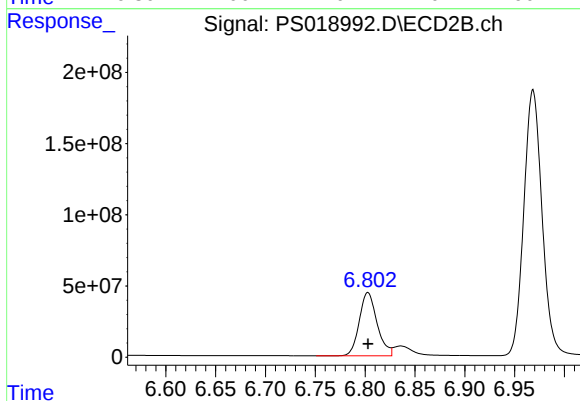

#4 2,4-DCAA


R.T.: 6.803 min
Delta R.T.: 0.000 min
Response: 551005041
Conc: 750.00 ng/ml

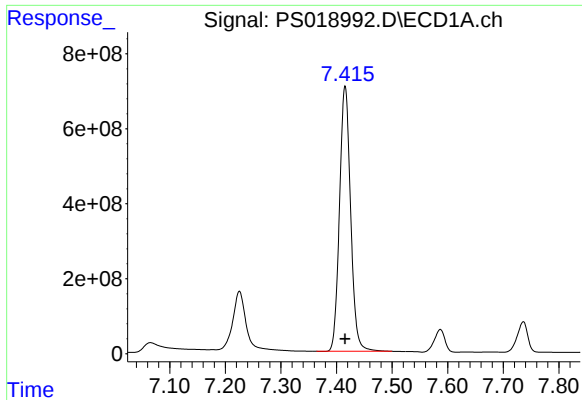

#5 DICAMBA


R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 9813261745
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

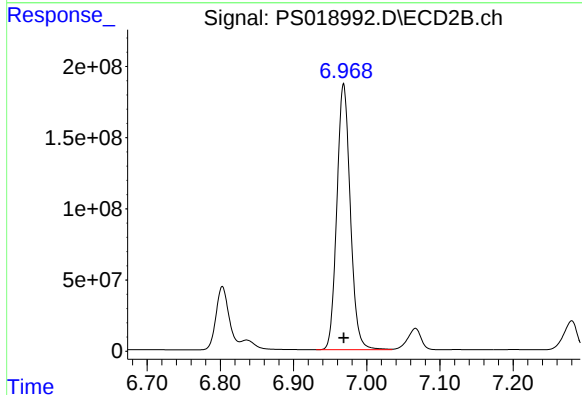


#5 DICAMBA

R.T.: 6.968 min
Delta R.T.: 0.000 min
Response: 2386031749
Conc: 705.00 ng/ml

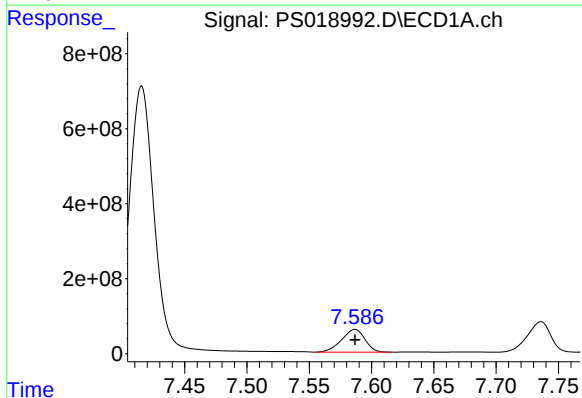


#6 MCP

R.T.: 7.587 min
Delta R.T.: 0.000 min
Response: 790273180
Conc: 70.50 ug/ml

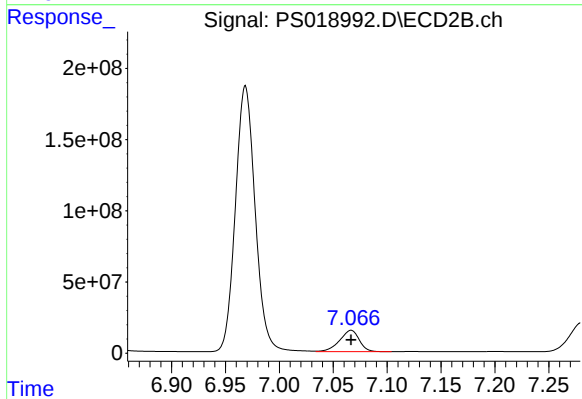

#6 MCP


R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 190918925
Conc: 70.50 ug/ml

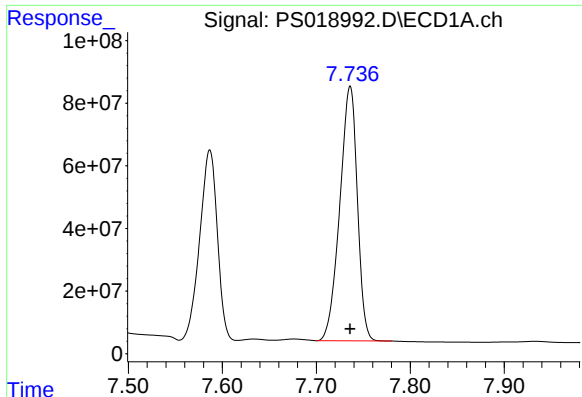

#7 MCPA


R.T.: 7.736 min
Delta R.T.: 0.000 min
Response: 1056376612
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

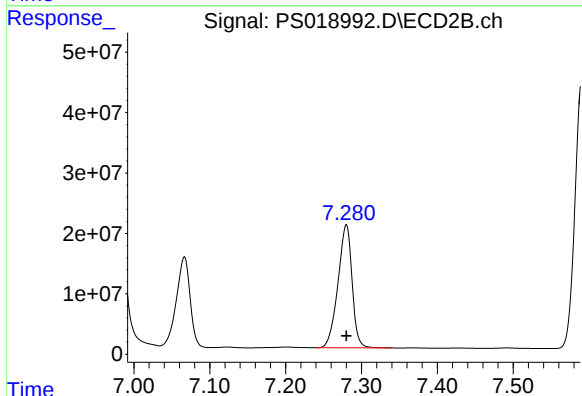


#7 MCPA

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 263023301
Conc: 69.75 ug/ml

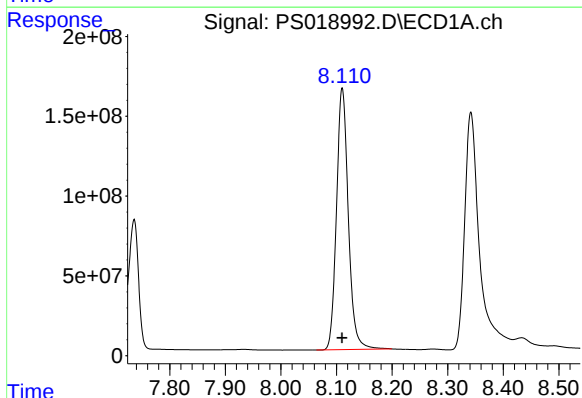


#8 DICHLORPROP

R.T.: 8.110 min
Delta R.T.: 0.000 min
Response: 2424311119
Conc: 705.00 ng/ml

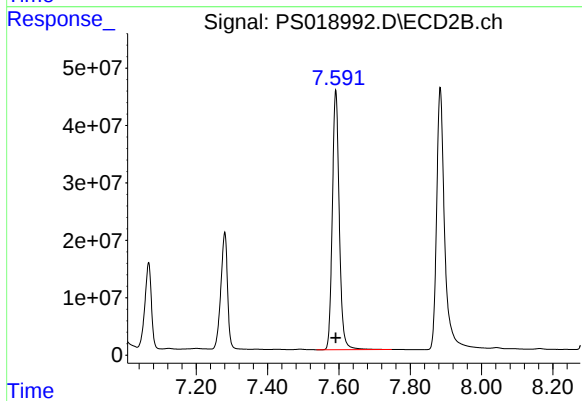

#8 DICHLORPROP


R.T.: 7.591 min
Delta R.T.: 0.000 min
Response: 611400470
Conc: 705.00 ng/ml

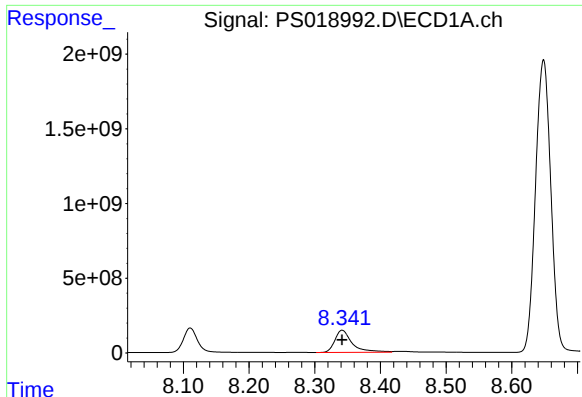

#9 2,4-D


R.T.: 8.342 min
Delta R.T.: 0.000 min
Response: 2716302937
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

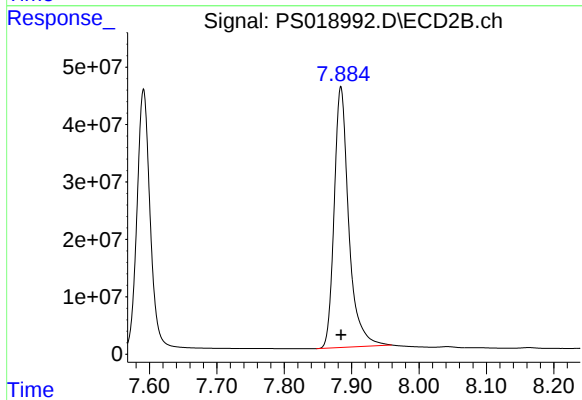


#9 2,4-D

R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 683189238
Conc: 705.00 ng/ml

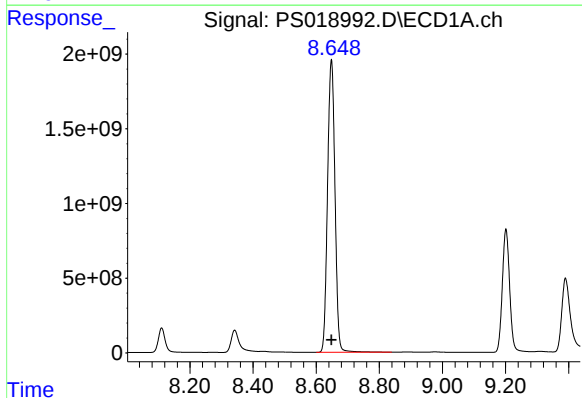


#10 Pentachlorophenol

R.T.: 8.648 min
Delta R.T.: 0.000 min
Response: 31904729199
Conc: 712.50 ng/ml

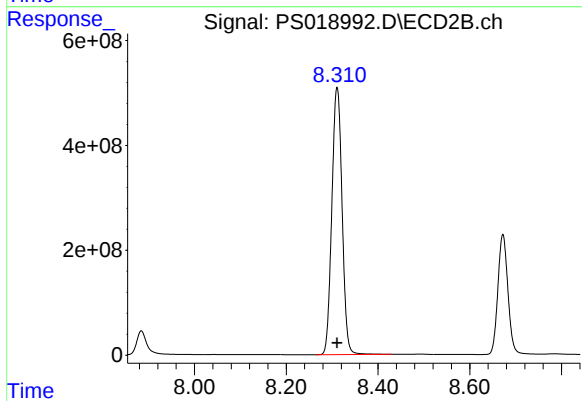

#10 Pentachlorophenol


R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 7898239013
Conc: 712.50 ng/ml

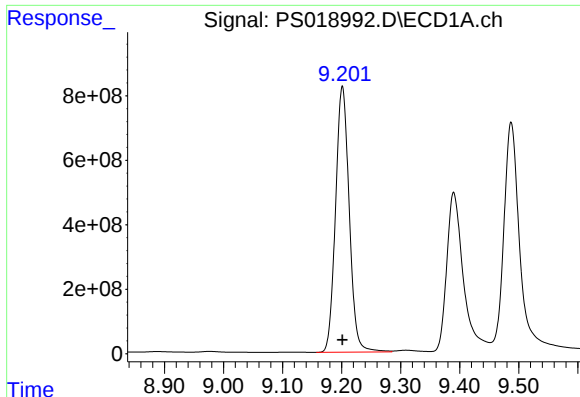

#11 2,4,5-TP (SILVEX)


R.T.: 9.201 min
Delta R.T.: 0.000 min
Response: 13273914460
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

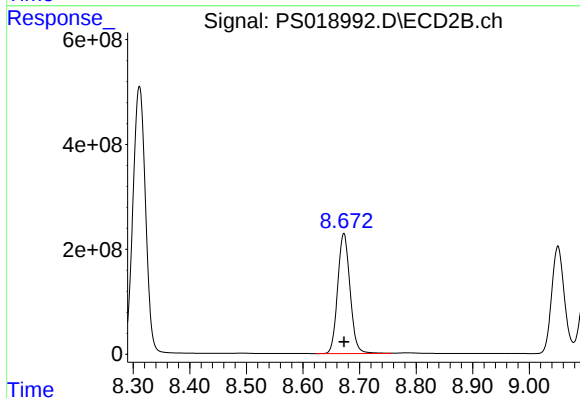


#11 2,4,5-TP (SILVEX)

R.T.: 8.672 min
Delta R.T.: 0.000 min
Response: 3489621903
Conc: 712.50 ng/ml

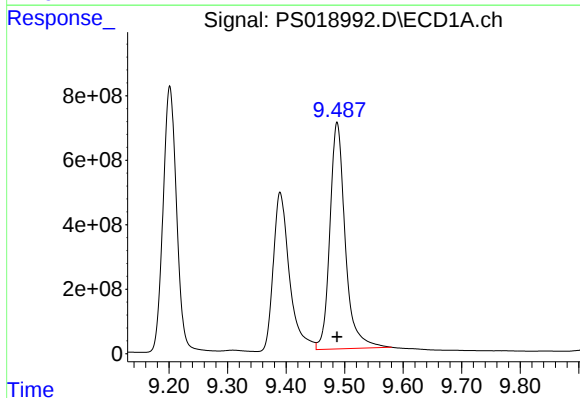


#12 2,4,5-T

R.T.: 9.487 min
Delta R.T.: 0.000 min
Response: 12802728836
Conc: 712.50 ng/ml

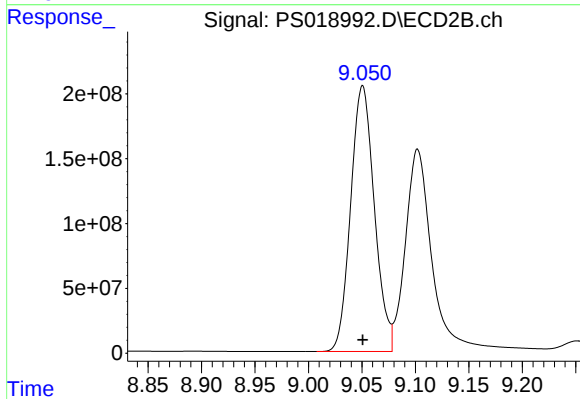

#12 2,4,5-T


R.T.: 9.051 min
Delta R.T.: 0.000 min
Response: 3163382162
Conc: 712.50 ng/ml

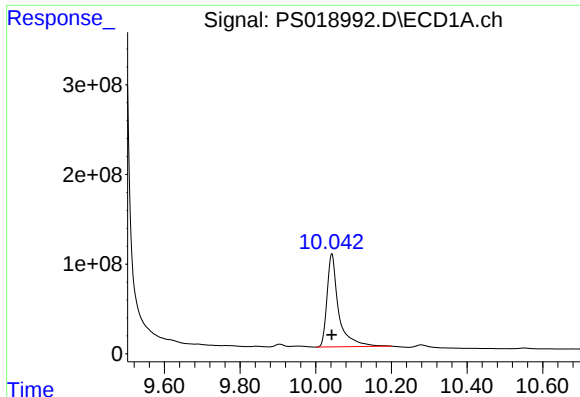

#13 2,4-DB


R.T.: 10.042 min
Delta R.T.: 0.000 min
Response: 2205765871
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

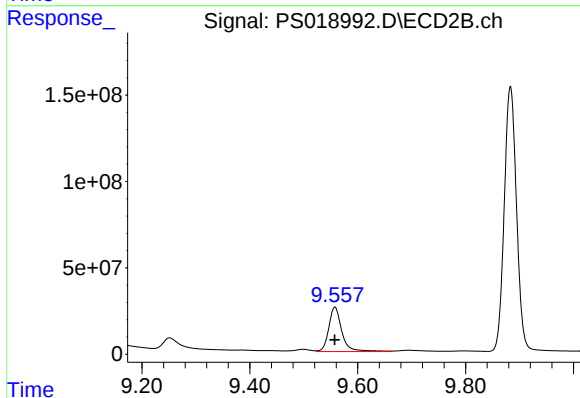


#13 2,4-DB

R.T.: 9.558 min
Delta R.T.: 0.000 min
Response: 433829753
Conc: 712.50 ng/ml

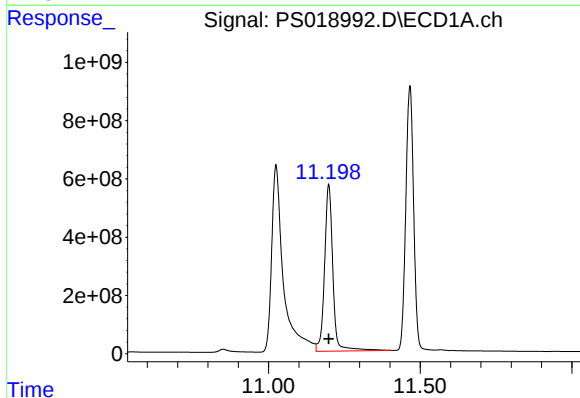


#14 DINOSEB

R.T.: 11.198 min
Delta R.T.: 0.000 min
Response: 10875853721
Conc: 705.00 ng/ml

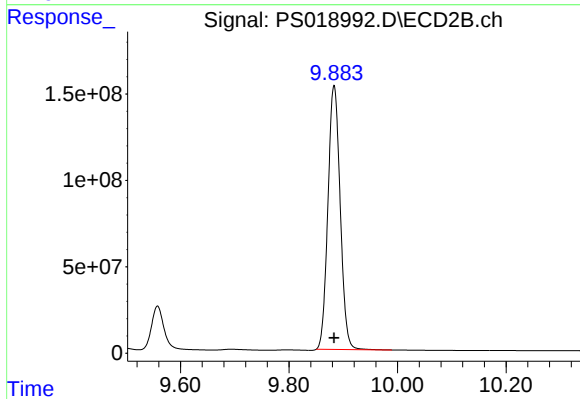

#14 DINOSEB


R.T.: 9.883 min
Delta R.T.: 0.000 min
Response: 2394172408
Conc: 705.00 ng/ml

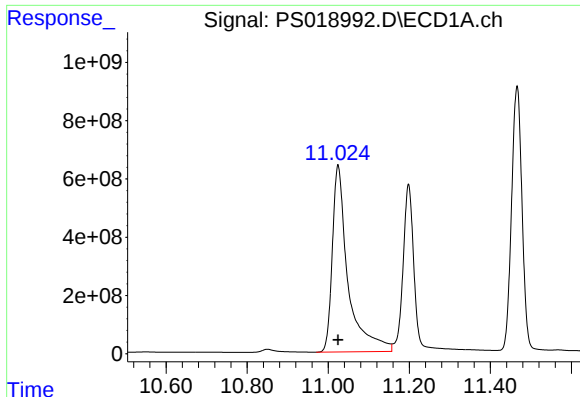

#15 Picloram


R.T.: 11.024 min
Delta R.T.: 0.000 min
Response: 17270222923
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

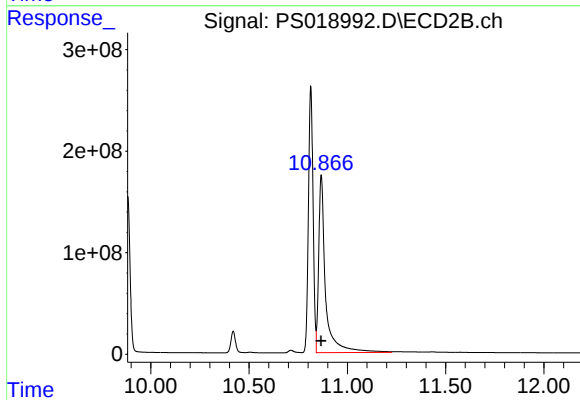


#15 Picloram

R.T.: 10.867 min
Delta R.T.: 0.000 min
Response: 4293781263
Conc: 712.50 ng/ml

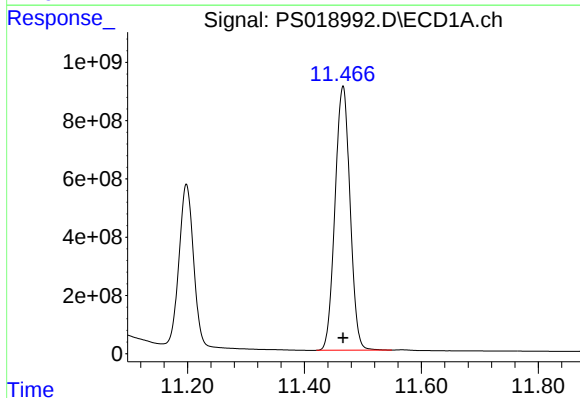

#16 DCPA

R.T.: 11.466 min
Delta R.T.: 0.000 min
Response: 16175075946
Conc: 720.00 ng/ml

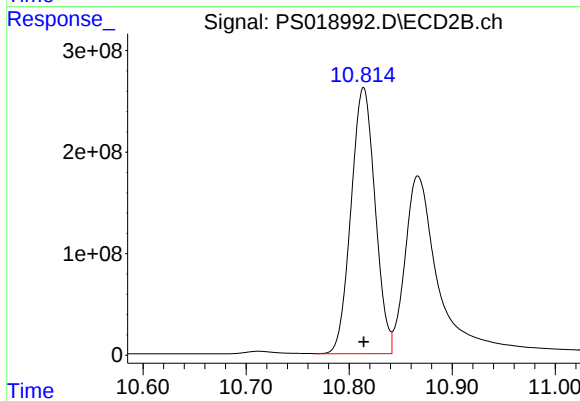

#16 DCPA

R.T.: 10.814 min
Delta R.T.: 0.000 min
Response: 4256516918
Conc: 720.00 ng/ml