

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS041423\  
Data File : PS022720.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Apr 2023 08:11  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 14 22:08:37 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS041223.M  
Quant Title : 8080.M  
QLast Update : Wed Apr 12 14:05:56 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----  
System Monitoring Compounds

Target Compounds  
-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS041423\  
Data File : PS022720.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Apr 2023 08:11  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 14 22:08:37 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS041223.M  
Quant Title : 8080.M  
QLast Update : Wed Apr 12 14:05:56 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

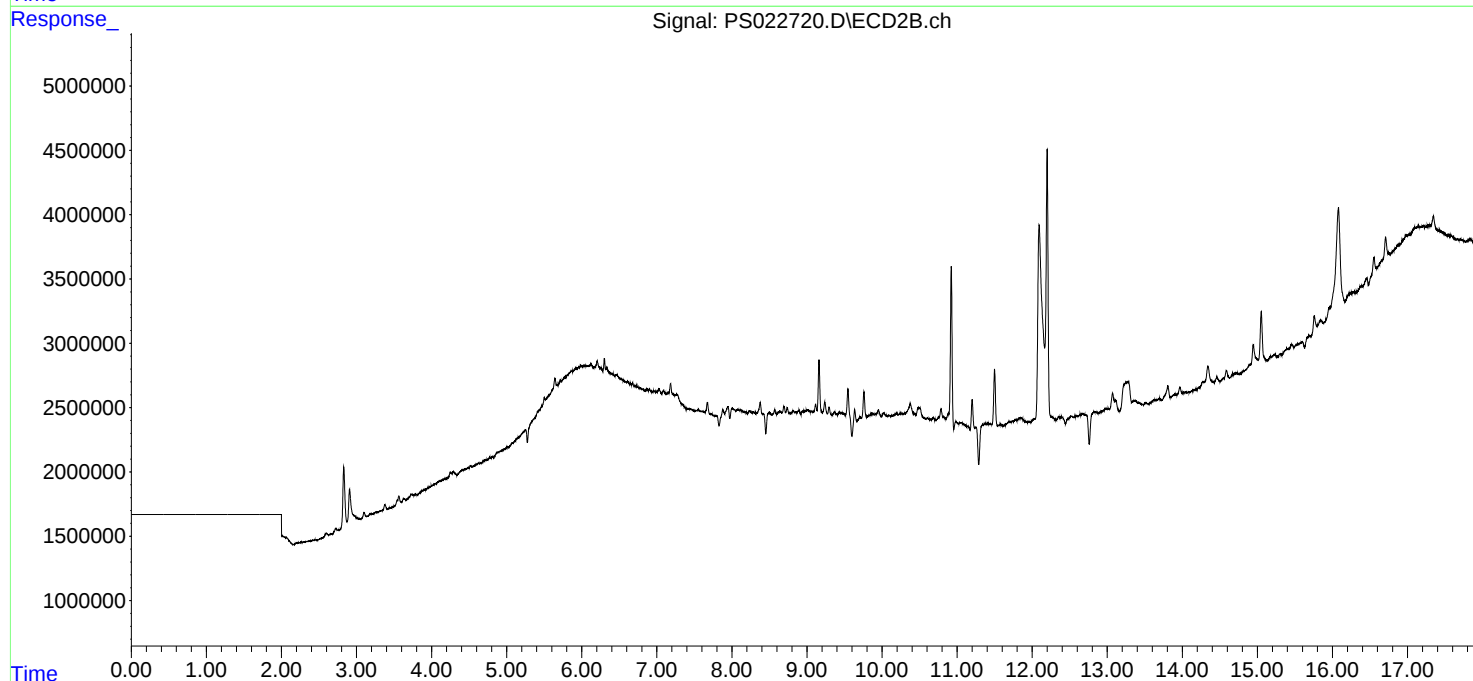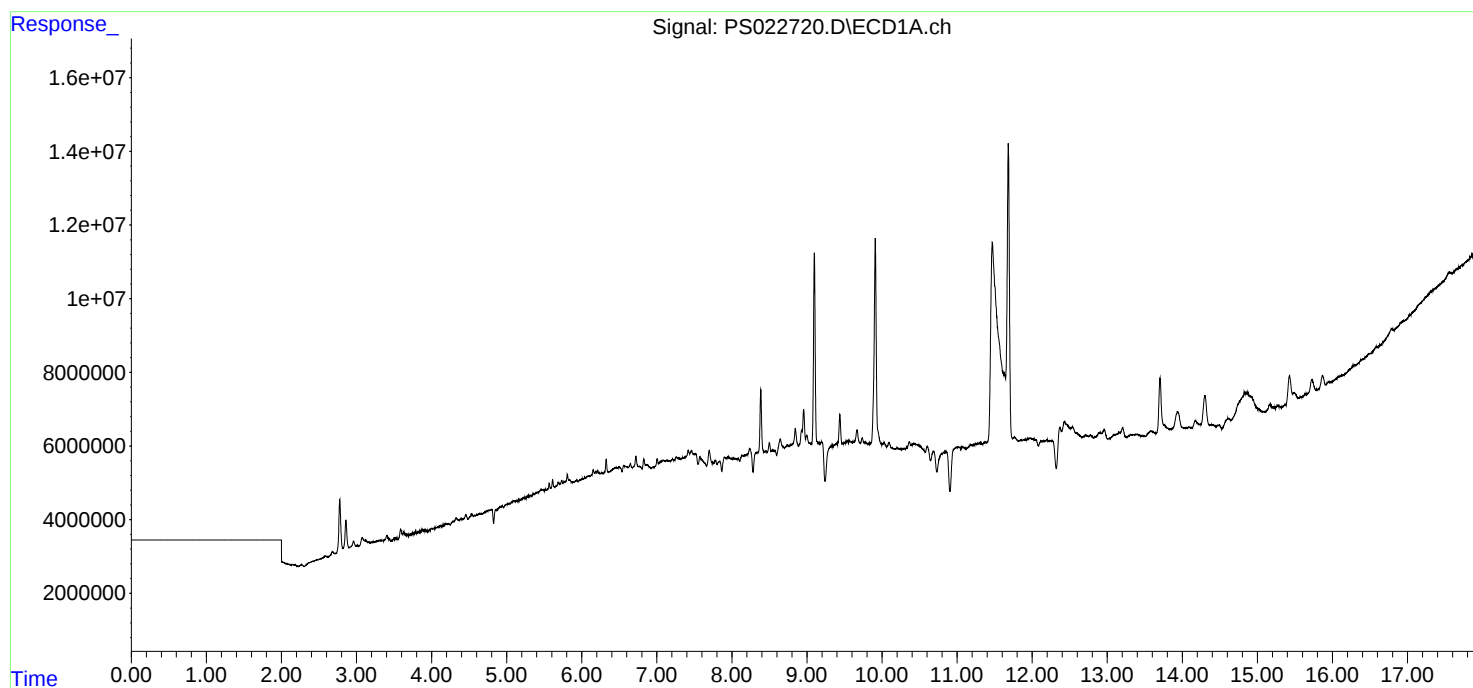


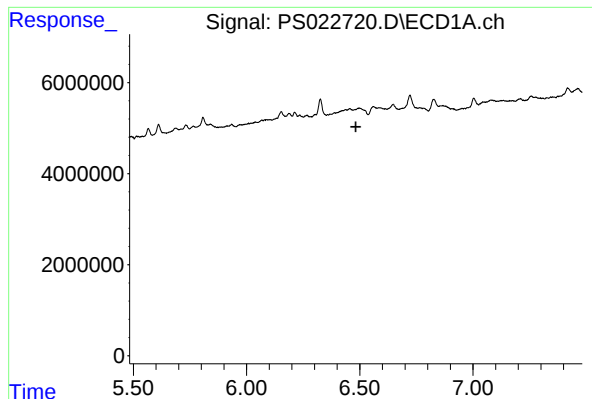

#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 6.483 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

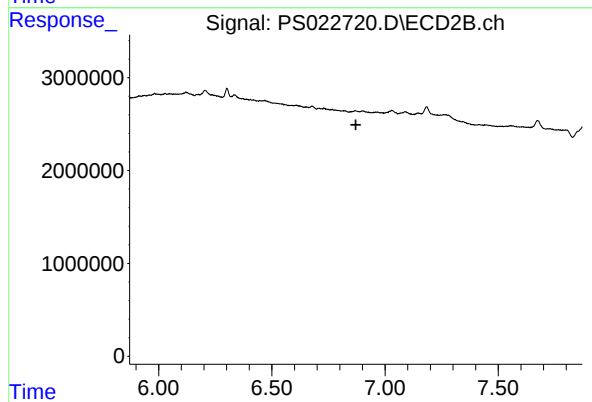

#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 6.871 min  
Response: 0  
Conc: N.D.