

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041520\
 Data File : PS009759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 10:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 11:45:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.927	271.1E6	261.8E6	490.101	476.659
Target Compounds							
5) T	DICAMBA	0.000	7.096	0	3060889	N.D.	1.333
10) T	Pentachlo...	0.000	8.449	0	3018625	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.811	0	4827065	N.D.	1.619
12) T	2,4,5-T	0.000	9.191	0	6762286	N.D.	2.291
15) T	Picloram	11.034	11.012	33889208	45672482	11.166	11.216
16) T	DCPA	0.000	10.961	0	6965418	N.D.	1.798



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041520\
Data File : PS009759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 10:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 11:45:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

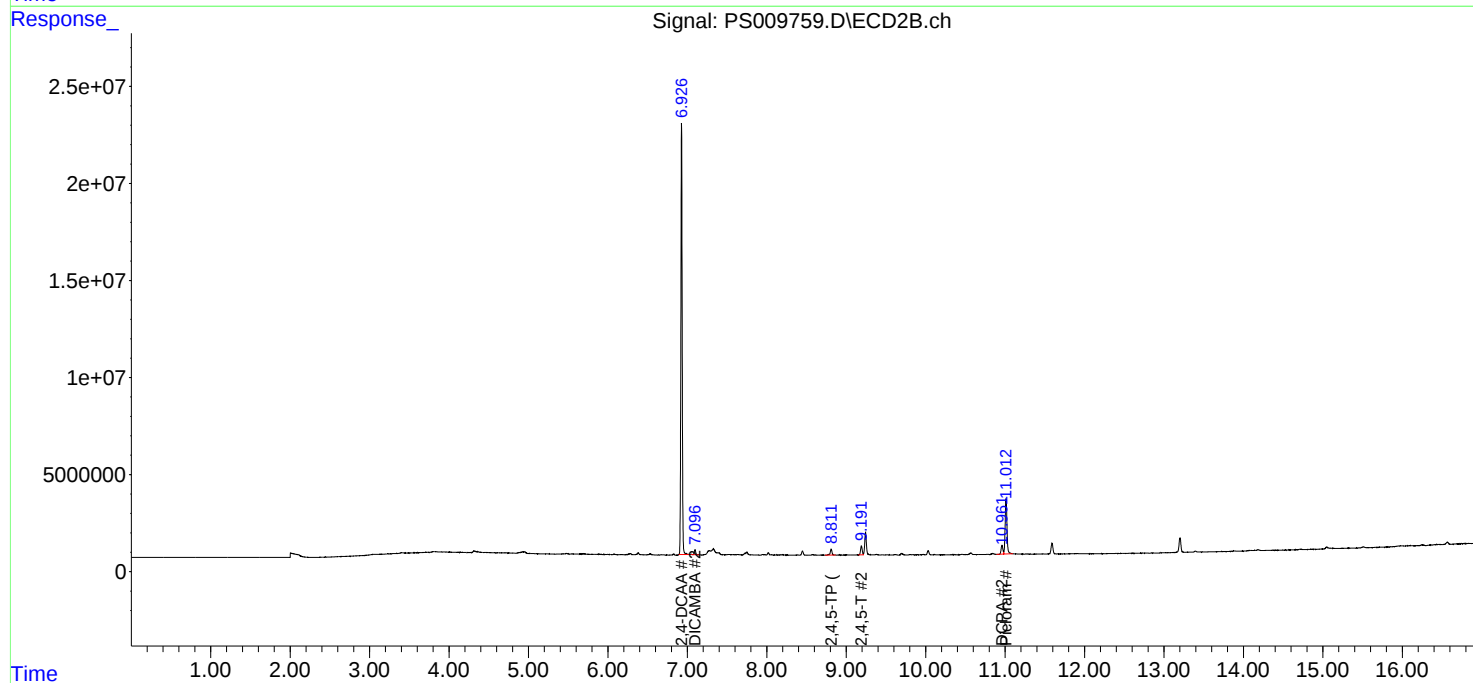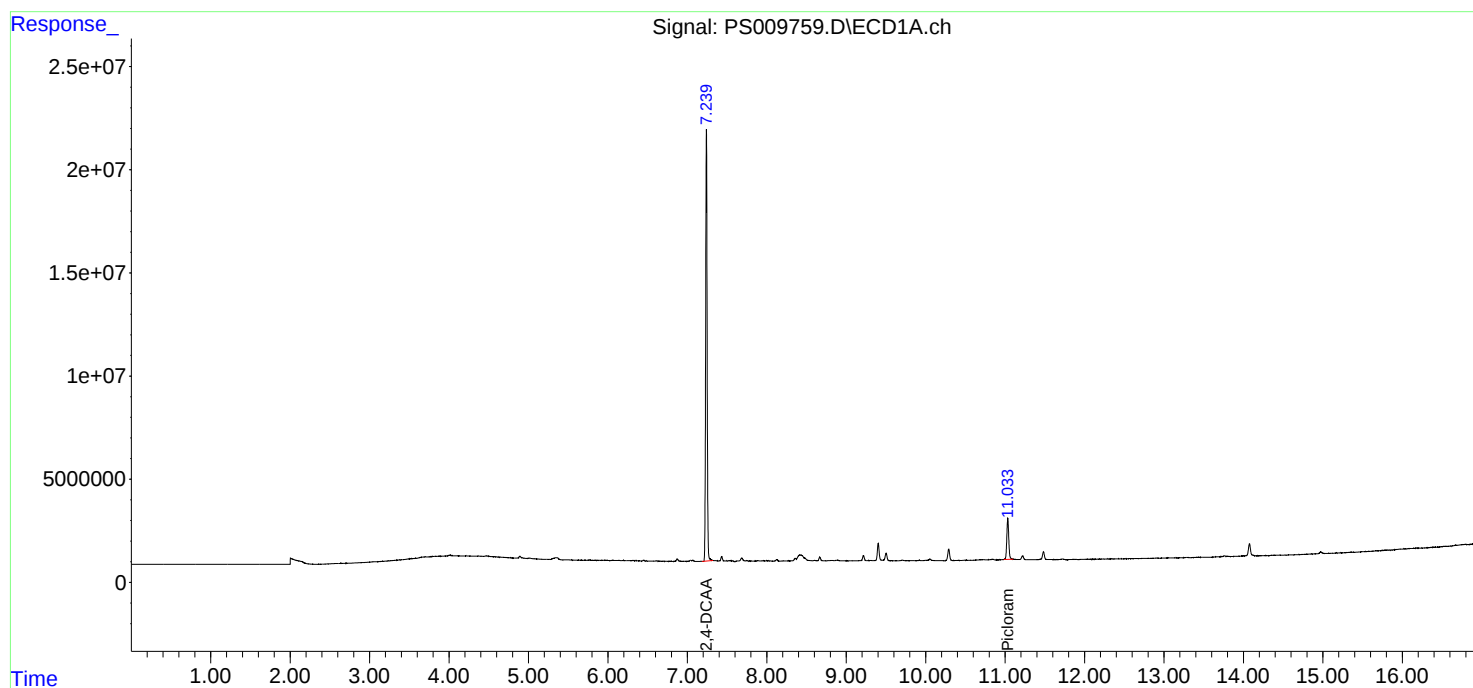


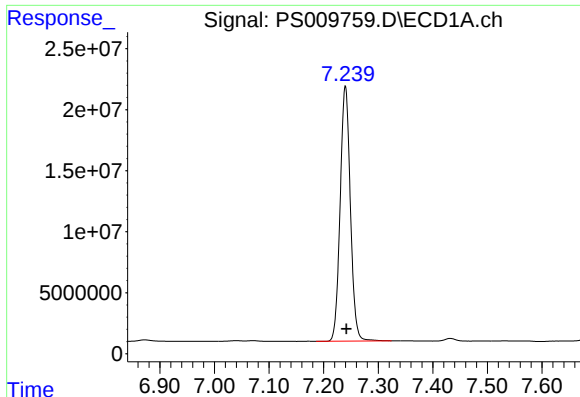

#4 2,4-DCAA


R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 271109302
Conc: 490.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

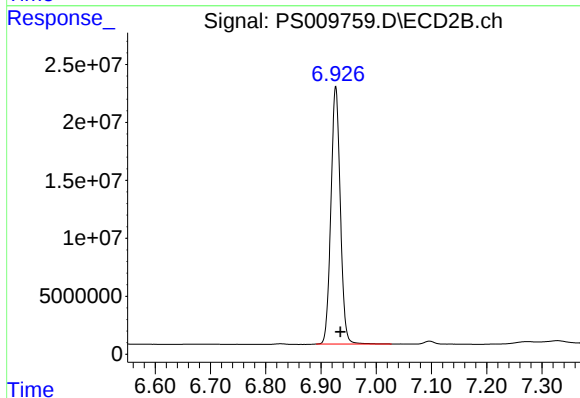


#4 2,4-DCAA

R.T.: 6.927 min
Delta R.T.: -0.008 min
Response: 261780041
Conc: 476.66 ng/ml

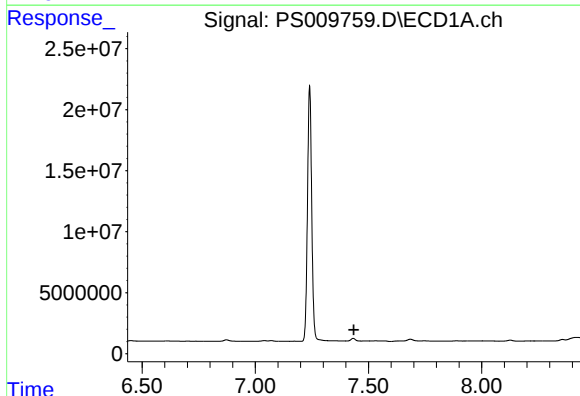


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.435 min
Response: 0
Conc: N.D.

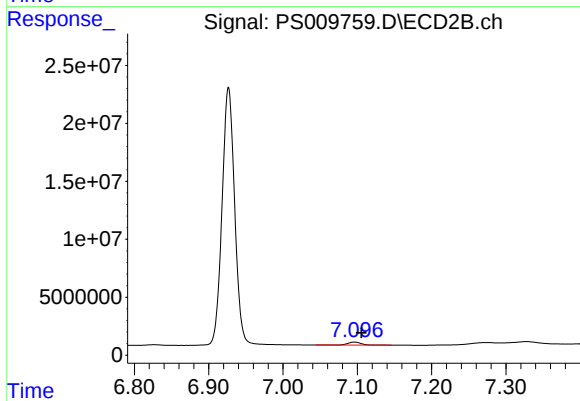

#5 DICAMBA


R.T.: 7.096 min
Delta R.T.: -0.009 min
Response: 3060889
Conc: 1.33 ng/ml

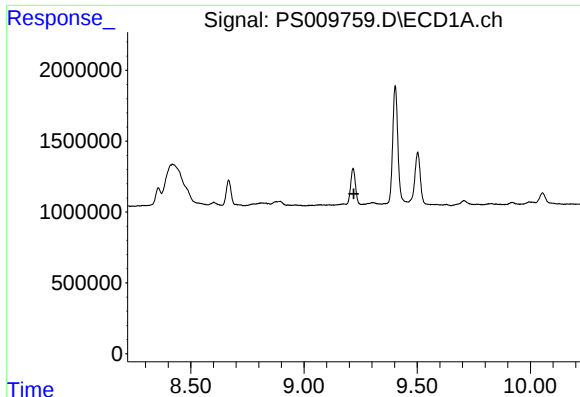

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

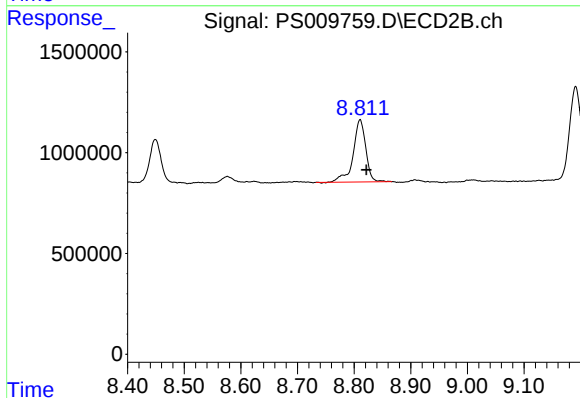


#11 2,4,5-TP (SILVEX)

R.T.: 8.811 min
Delta R.T.: -0.011 min
Response: 4827065
Conc: 1.62 ng/ml

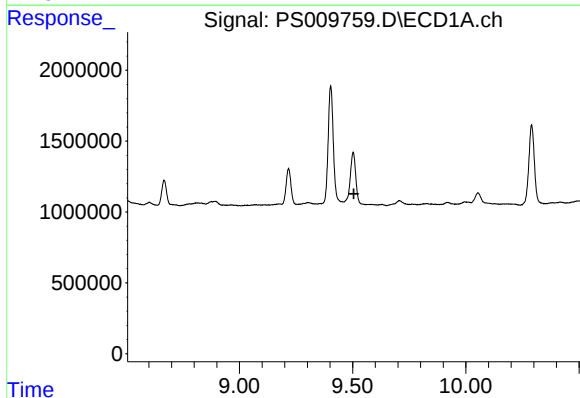


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.505 min
Response: 0
Conc: N.D.

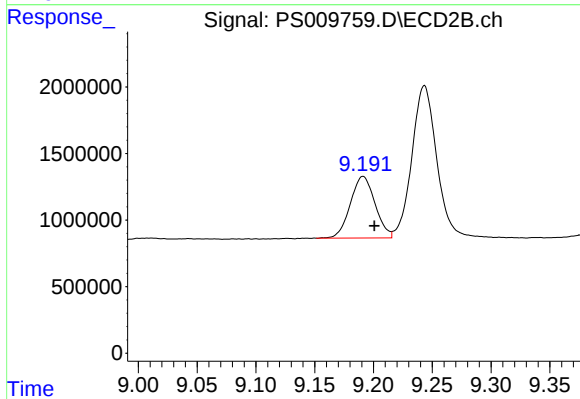

#12 2,4,5-T


R.T.: 9.191 min
Delta R.T.: -0.010 min
Response: 6762286
Conc: 2.29 ng/ml

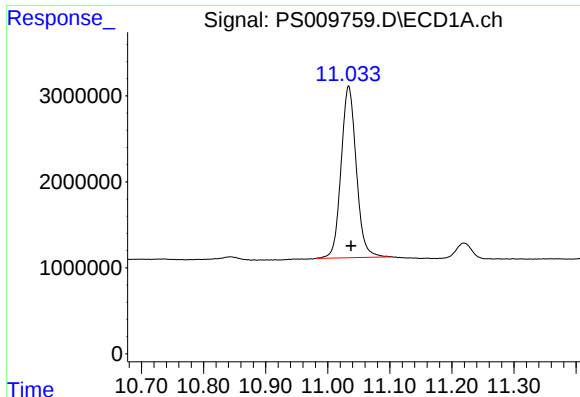

#15 Picloram


R.T.: 11.034 min
Delta R.T.: -0.004 min
Response: 33889208
Conc: 11.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

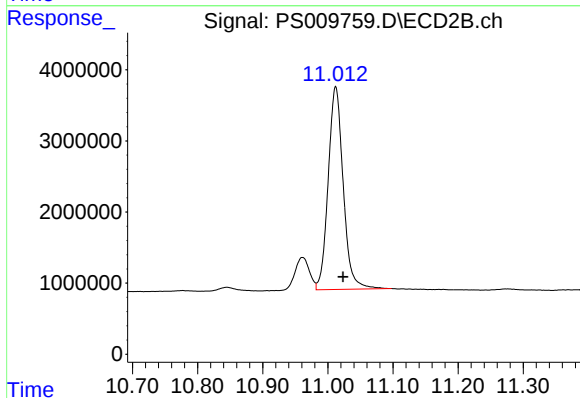


#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.011 min
Response: 45672482
Conc: 11.22 ng/ml

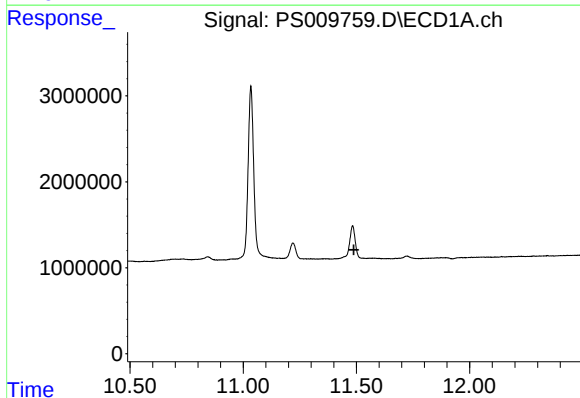

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

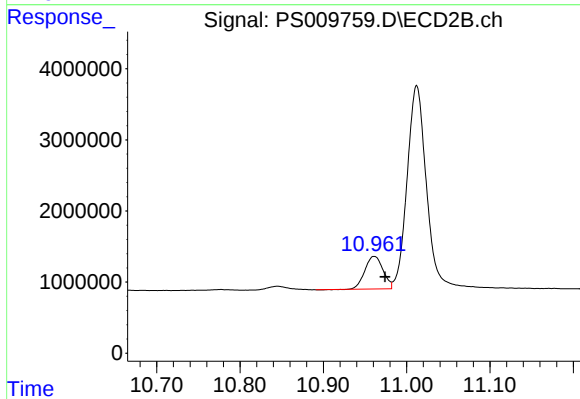

#16 DCPA

R.T.: 10.961 min
Delta R.T.: -0.013 min
Response: 6965418
Conc: 1.80 ng/ml