

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041520\
 Data File : PS009763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 11:43
 Operator : DD\AJ
 Sample : PB128184TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 12:03:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.238	6.927	412.2E6	397.9E6	745.221	724.502
Target Compounds							
8) T	DICHLORPROP	0.000	7.749	0	5000754	N.D.	9.013
9) T	2,4-D	8.424	0.000	12440575	0	23.596	N.D. #
12) T	2,4,5-T	0.000	9.244	0	10307440	N.D.	3.491
15) T	Picloram	11.032	11.013	20178091	33165472	6.649	8.144
16) T	DCPA	0.000	11.013	0	33165472	N.D.	8.563



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041520\
Data File : PS009763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 11:43
Operator : DD\AJ
Sample : PB128184TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 12:03:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

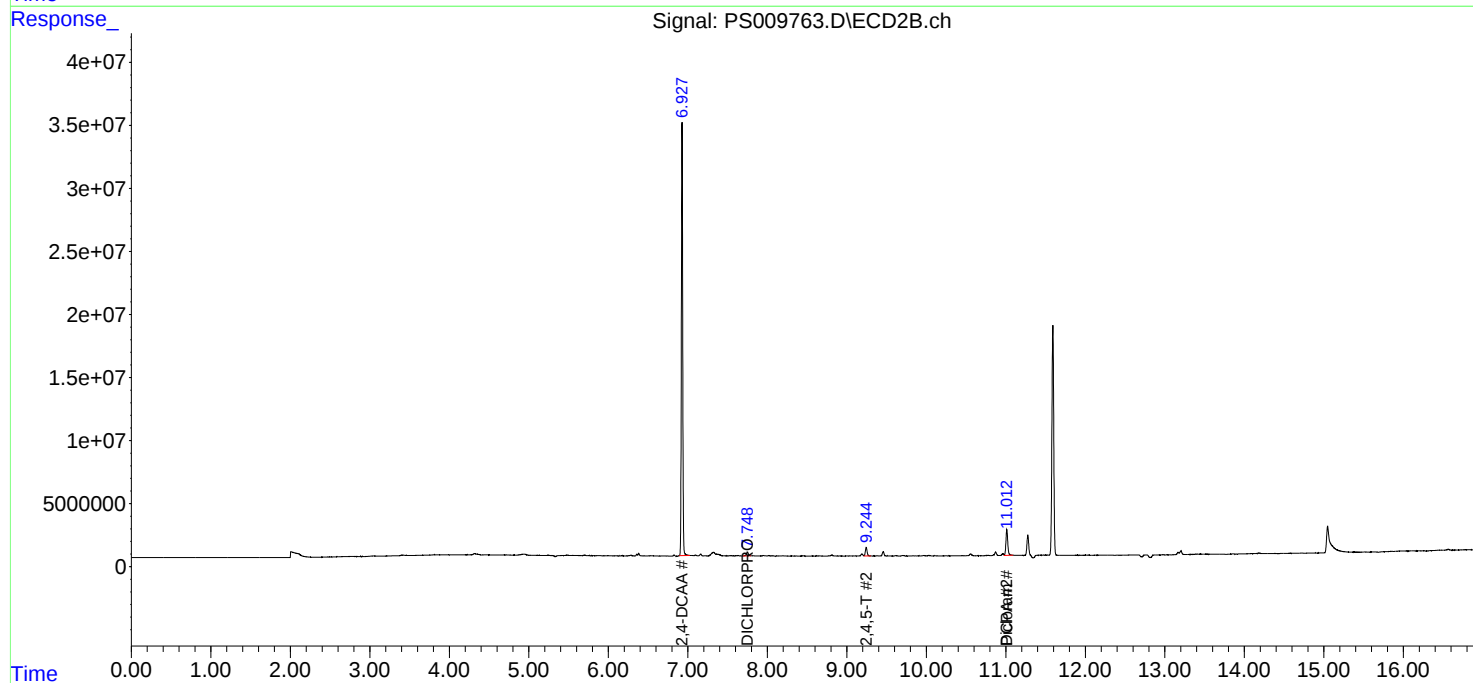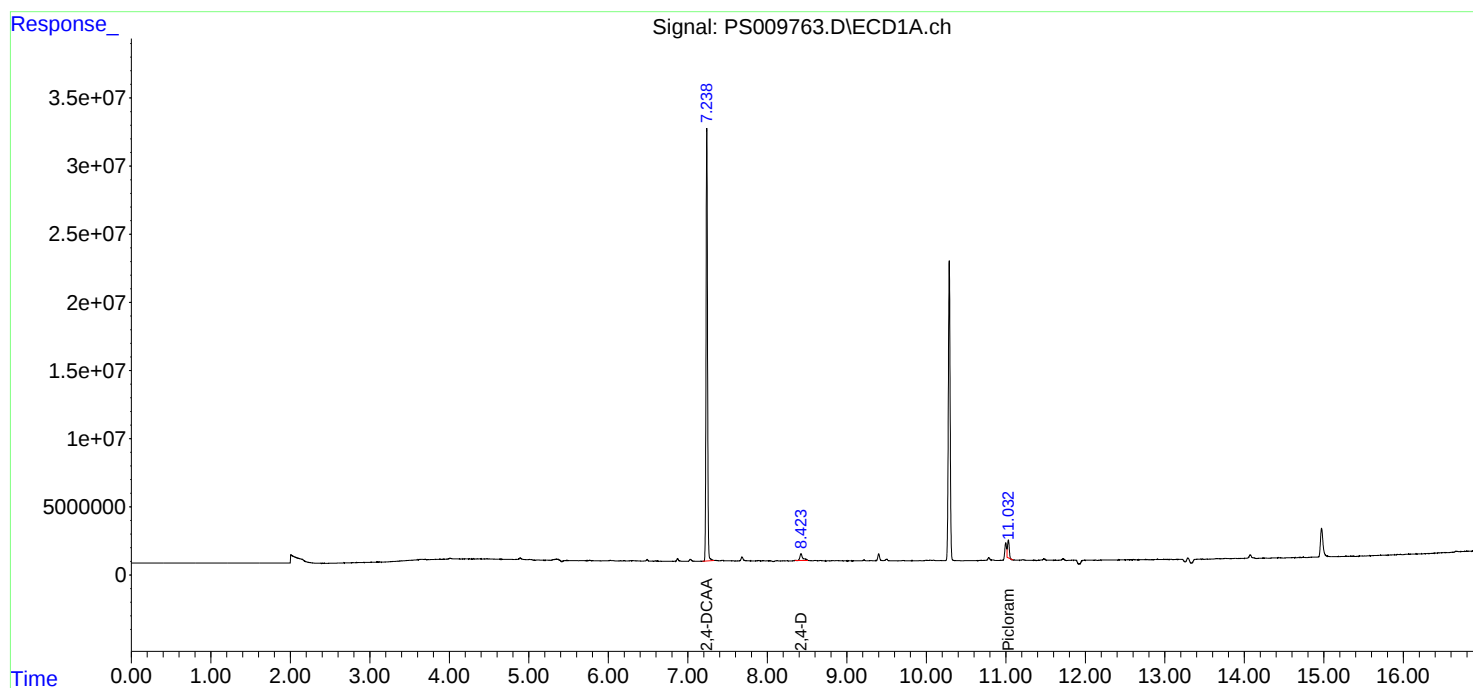


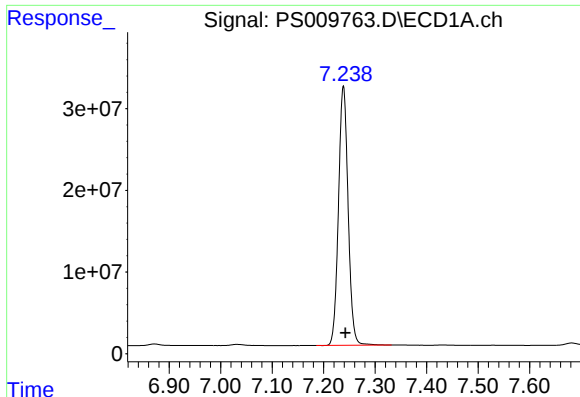

#4 2,4-DCAA


R.T.: 7.238 min
Delta R.T.: -0.004 min
Response: 412233940
Conc: 745.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

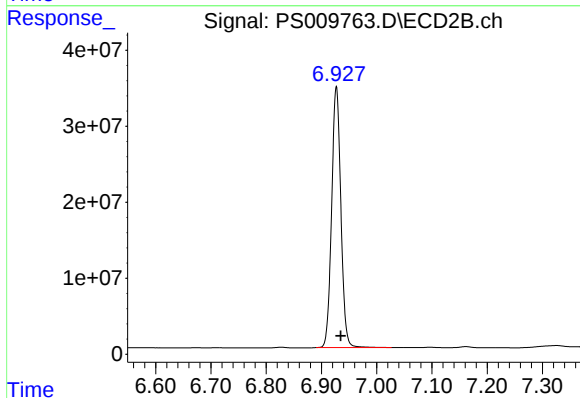


#4 2,4-DCAA

R.T.: 6.927 min
Delta R.T.: -0.008 min
Response: 397895071
Conc: 724.50 ng/ml

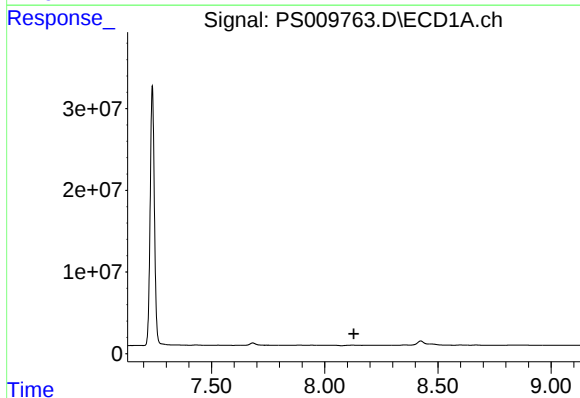


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

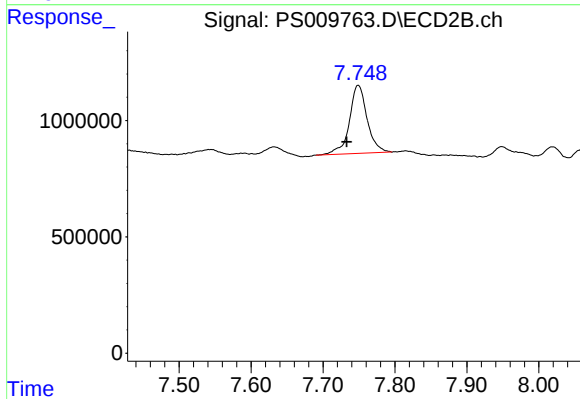

#8 DICHLORPROP


R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 5000754
Conc: 9.01 ng/ml

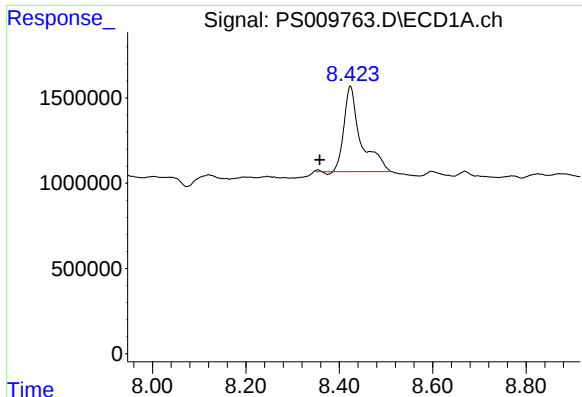

#9 2,4-D


R.T.: 8.424 min
Delta R.T.: 0.066 min
Response: 12440575
Conc: 23.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

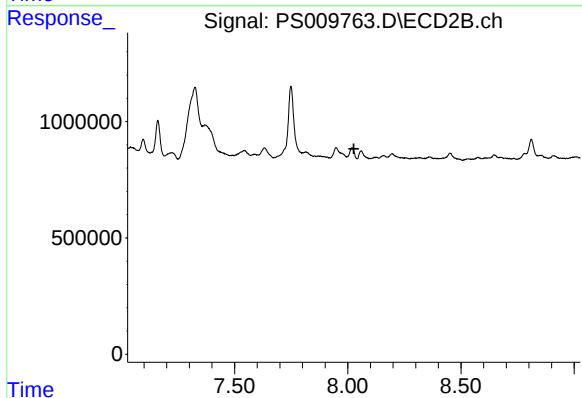


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

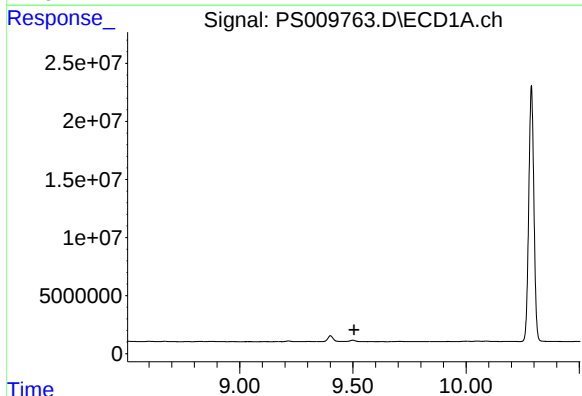


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.505 min
Response: 0
Conc: N.D.

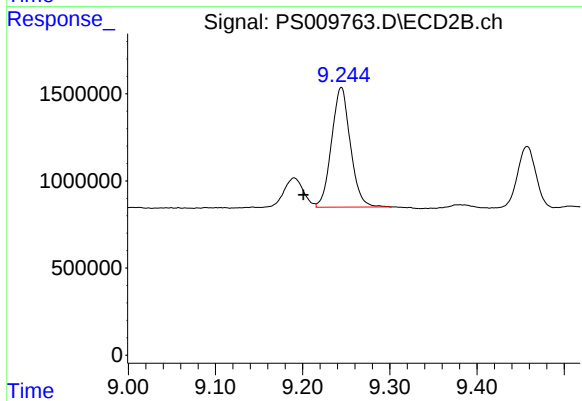

#12 2,4,5-T


R.T.: 9.244 min
Delta R.T.: 0.043 min
Response: 10307440
Conc: 3.49 ng/ml

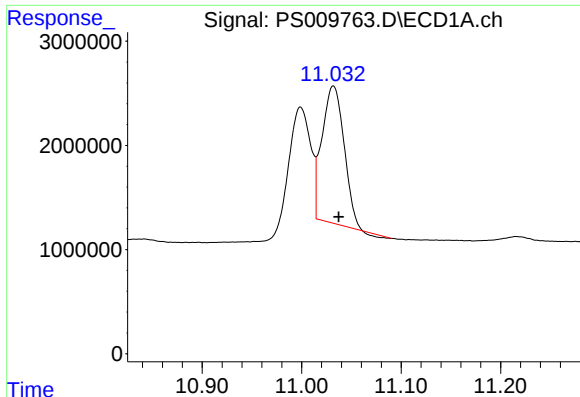

#15 Picloram


R.T.: 11.032 min
Delta R.T.: -0.006 min
Response: 20178091
Conc: 6.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

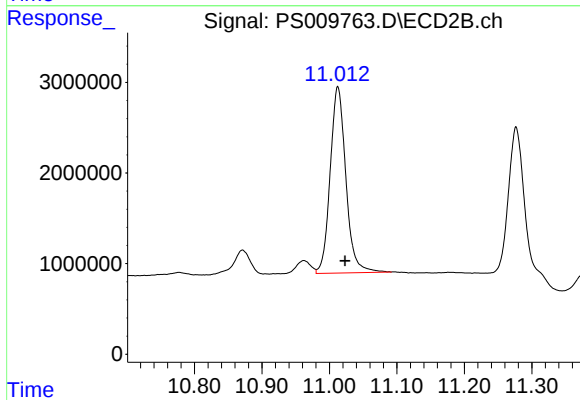


#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.011 min
Response: 33165472
Conc: 8.14 ng/ml

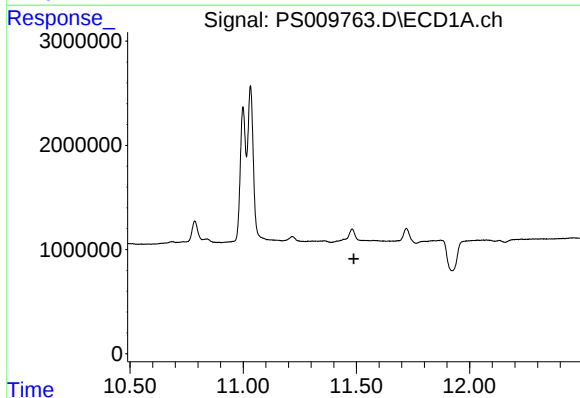

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

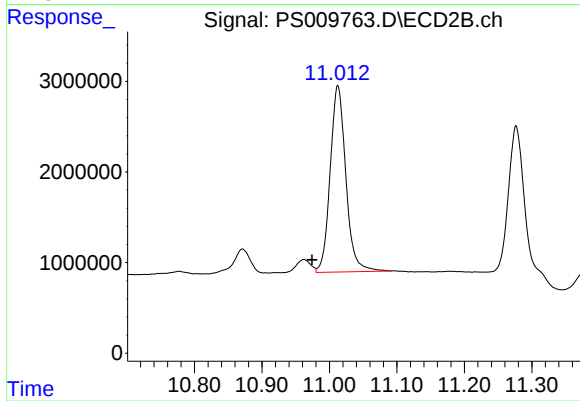

#16 DCPA

R.T.: 11.013 min
Delta R.T.: 0.039 min
Response: 33165472
Conc: 8.56 ng/ml