

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041621\
 Data File : PS014654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 09:45
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 10:53:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) T	3,5-DICHL...	6.429f	0.000	12832817	0	6.193 N.D. #
5) T	DICAMBA	0.000	7.119f	0	6206028	N.D. 3.068
6) T	MCP	0.000	7.119	0	6206028	N.D. 3.685
12) T	2,4,5-T	9.327f	0.000	8289019	0	1.008 N.D. #
15) T	Picloram	10.896	10.977	8076332	17901738	<MDL 4.774 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041621\
Data File : PS014654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 09:45
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 10:53:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

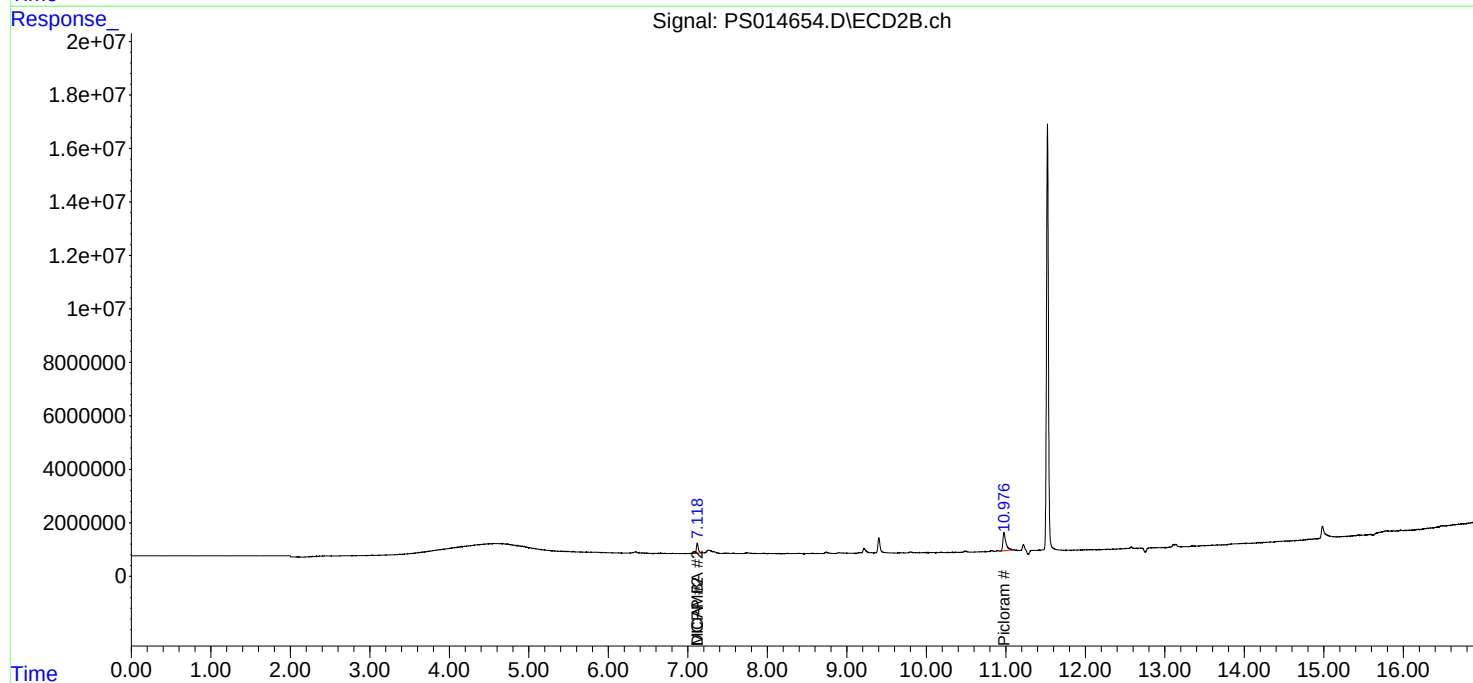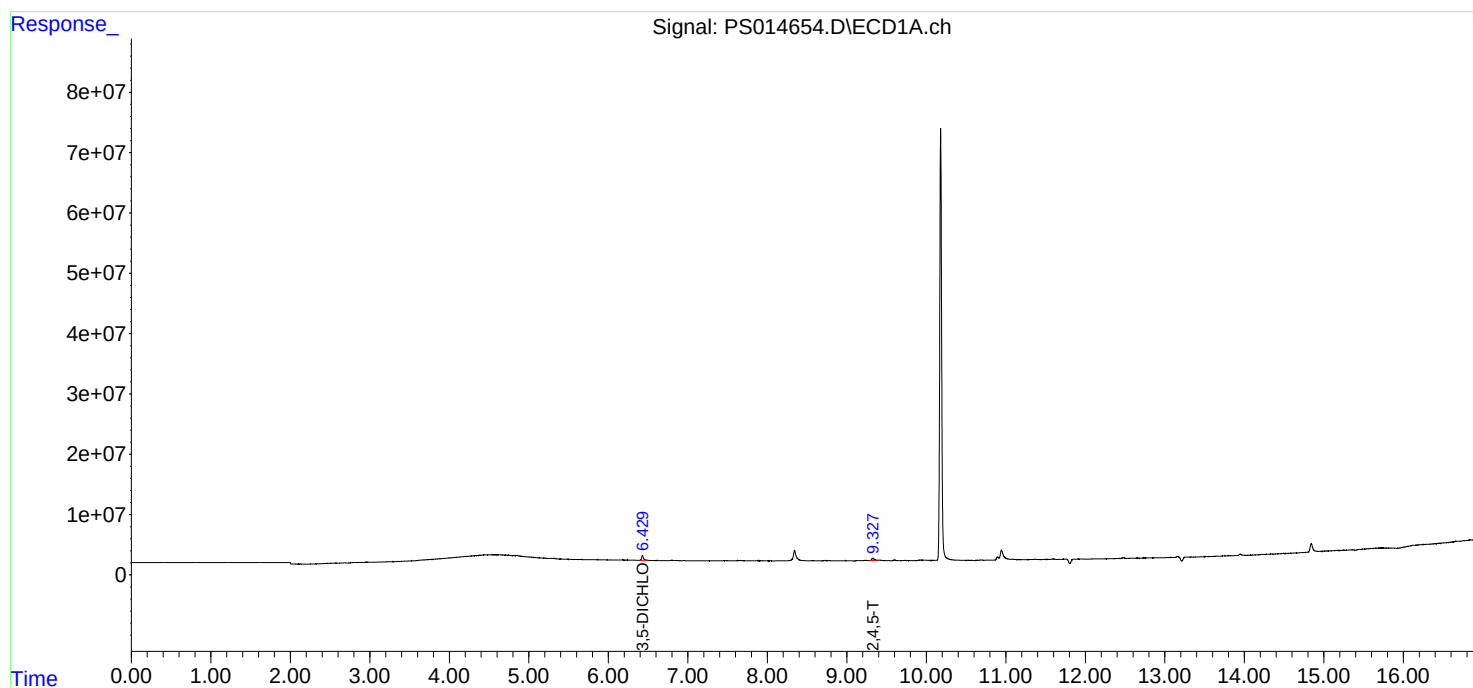


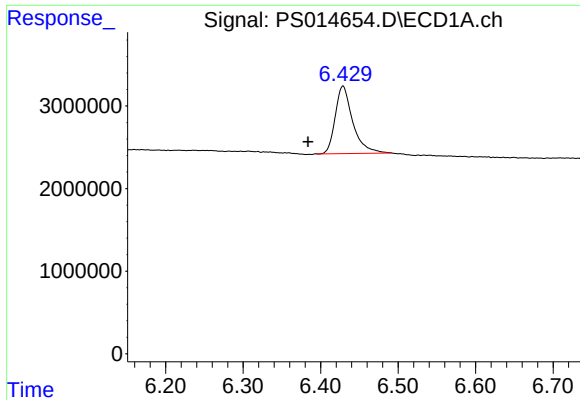

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.429 min
Delta R.T.: 0.045 min
Response: 12832817
Conc: 6.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

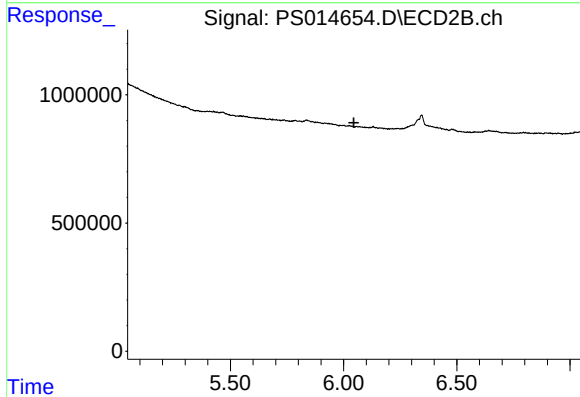


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

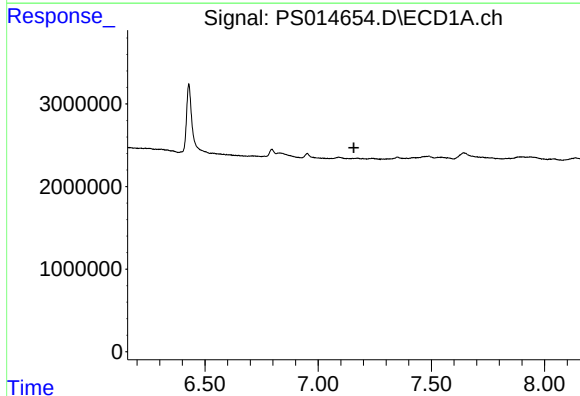


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

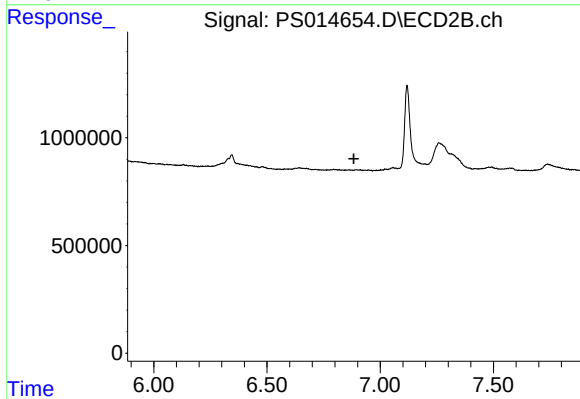

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

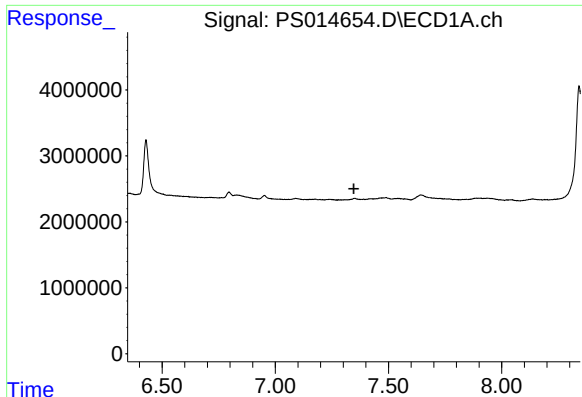

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

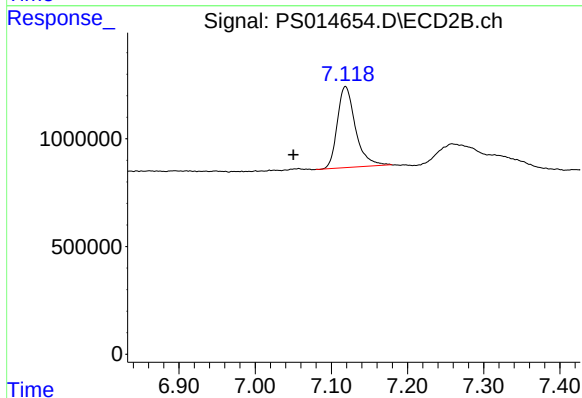


#5 DICAMBA

R.T.: 7.119 min
Delta R.T.: 0.068 min
Response: 6206028
Conc: 3.07 ng/ml

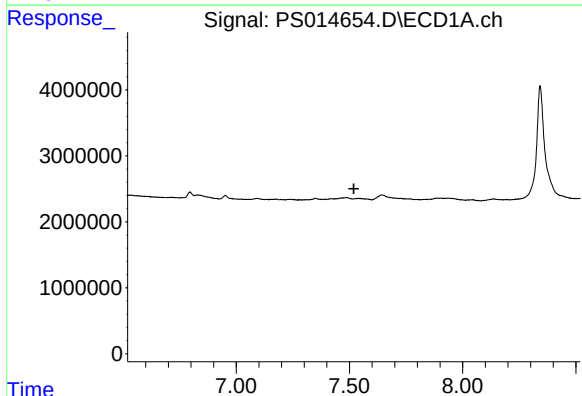


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

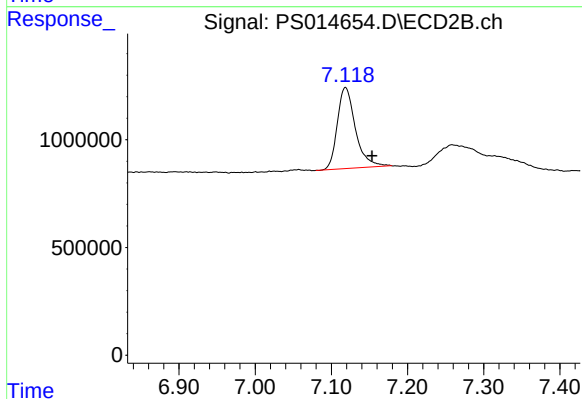

#6 MCP


R.T.: 7.119 min
Delta R.T.: -0.035 min
Response: 6206028
Conc: 3.69 ug/ml

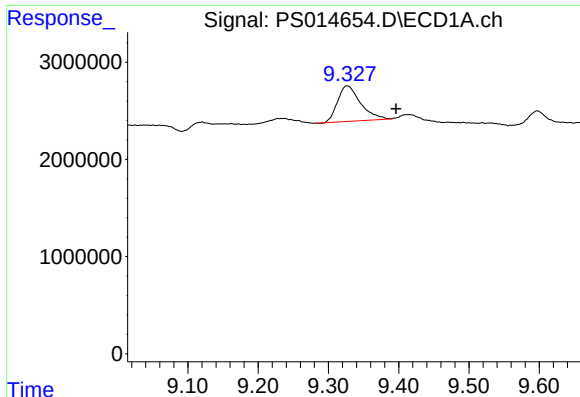

#12 2,4,5-T


R.T.: 9.327 min
Delta R.T.: -0.069 min
Response: 8289019
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

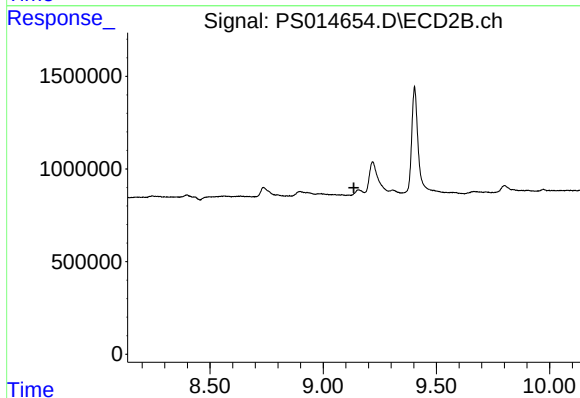


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.135 min
Response: 0
Conc: N.D.

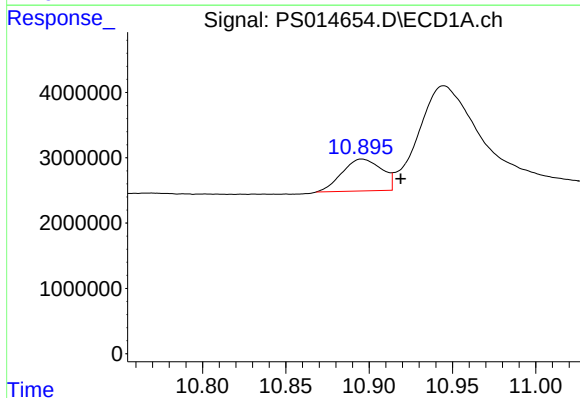

#15 Picloram

R.T.: 10.896 min
Delta R.T.: -0.023 min
Response: 8076332
Conc: N.D.

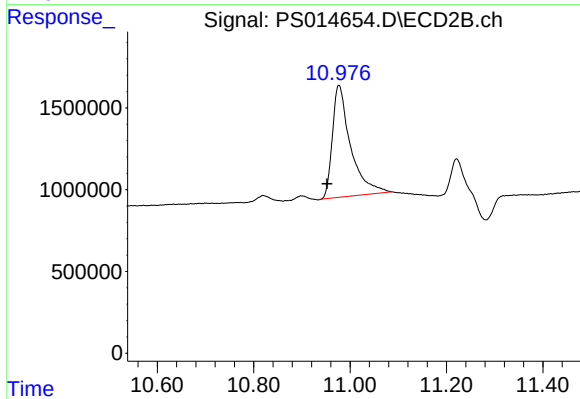

#15 Picloram

R.T.: 10.977 min
Delta R.T.: 0.024 min
Response: 17901738
Conc: 4.77 ng/ml