

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041621\
 Data File : PS014655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 10:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 10:53:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	6.885	750.7E6	281.2E6	493.510	604.138
Target Compounds							
2) T	3,5-DICHL...	6.429f	0.000	13562596	0	6.546	N.D. #
5) T	DICAMBA	0.000	7.119f	0	6208394	N.D.	3.070
6) T	MCP	0.000	7.119	0	6208394	N.D.	3.687
12) T	2,4,5-T	9.330f	0.000	7659965	0	<MDL	N.D. #
15) T	Picloram	10.899	10.980	5611579	16520735	<MDL	4.406 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041621\
Data File : PS014655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 10:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 10:53:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

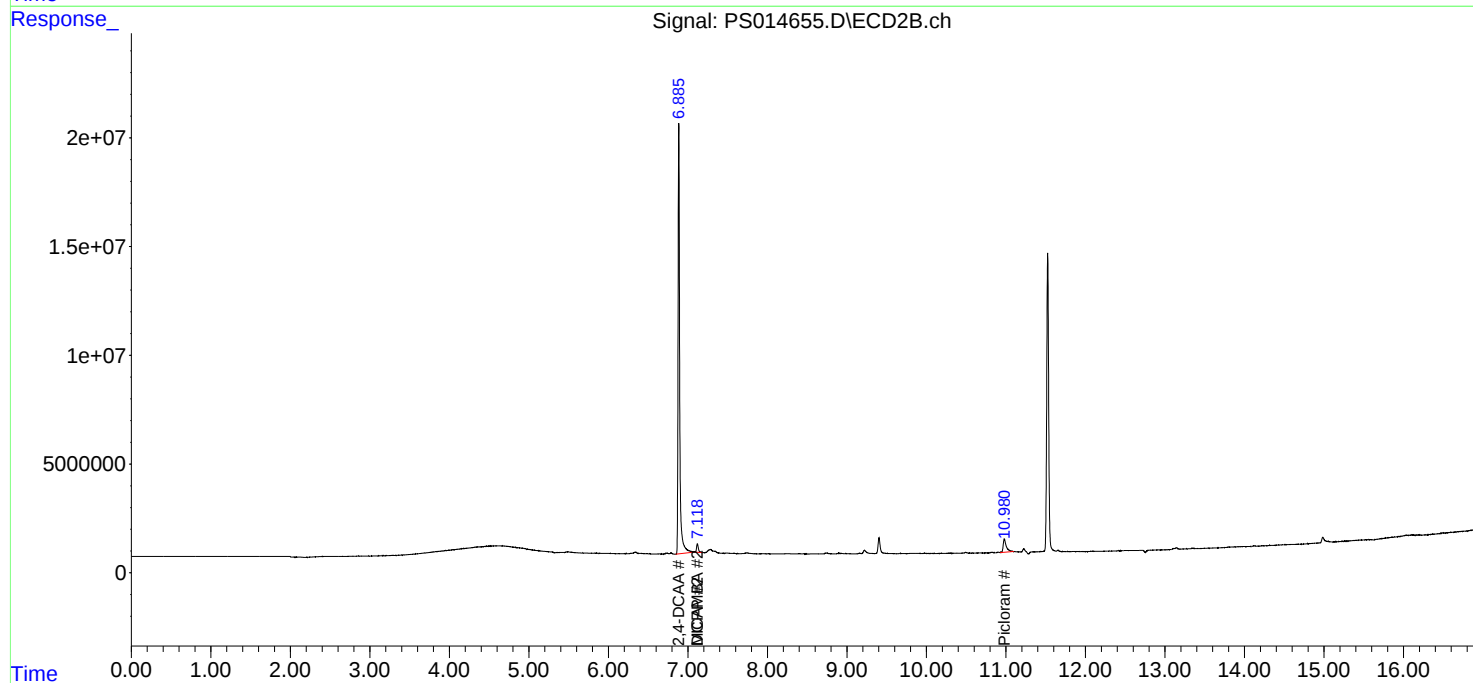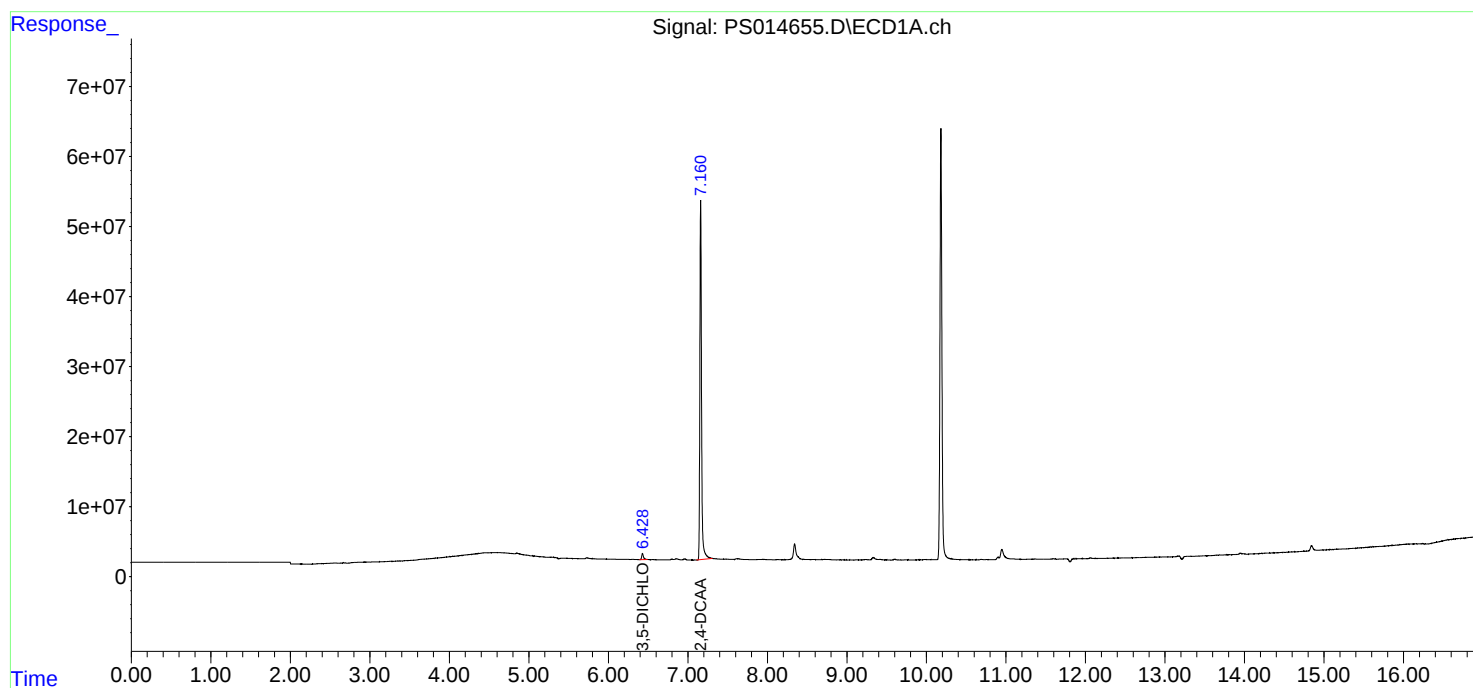


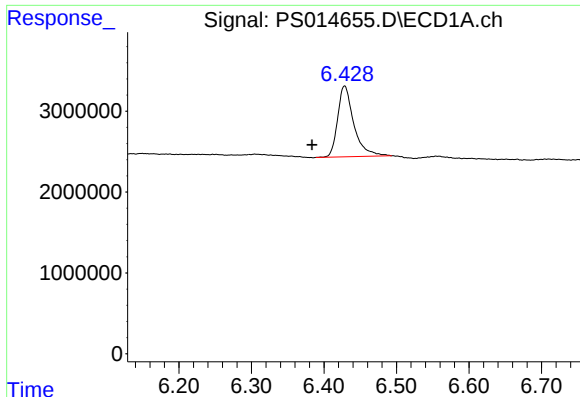

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.429 min
Delta R.T.: 0.045 min
Response: 13562596
Conc: 6.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

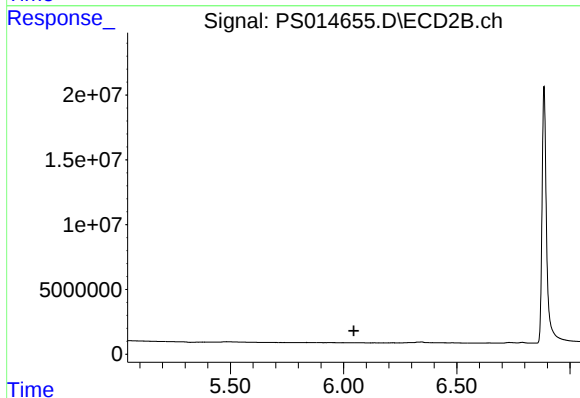


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

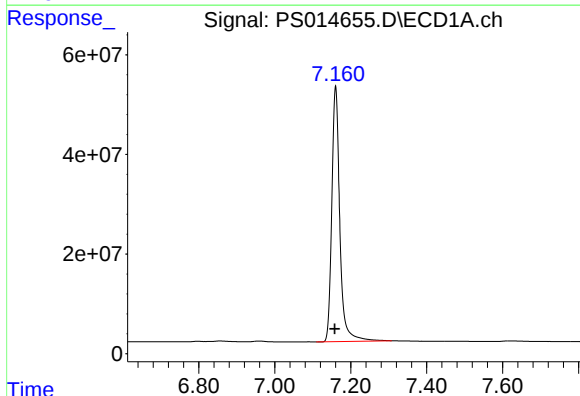


#4 2,4-DCAA

R.T.: 7.160 min
Delta R.T.: 0.002 min
Response: 750725716
Conc: 493.51 ng/ml

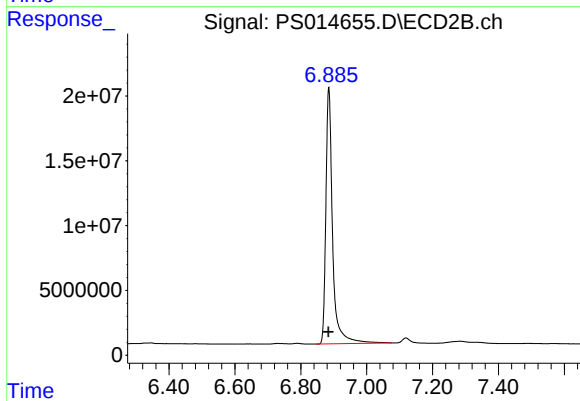

#4 2,4-DCAA


R.T.: 6.885 min
Delta R.T.: 0.001 min
Response: 281198784
Conc: 604.14 ng/ml

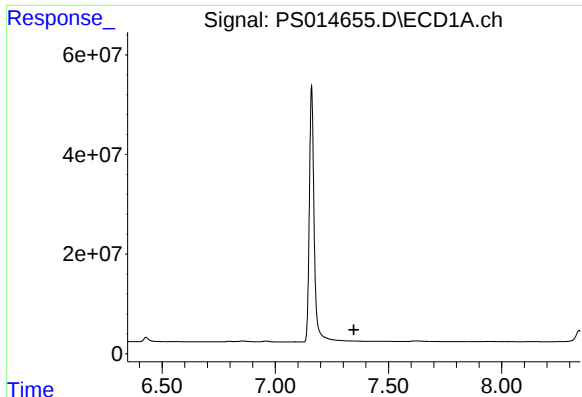

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

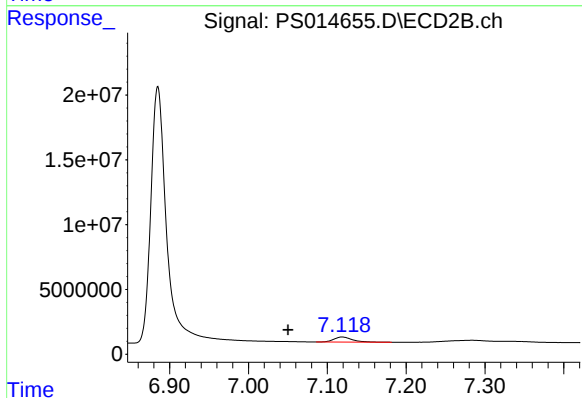


#5 DICAMBA

R.T.: 7.119 min
Delta R.T.: 0.068 min
Response: 6208394
Conc: 3.07 ng/ml

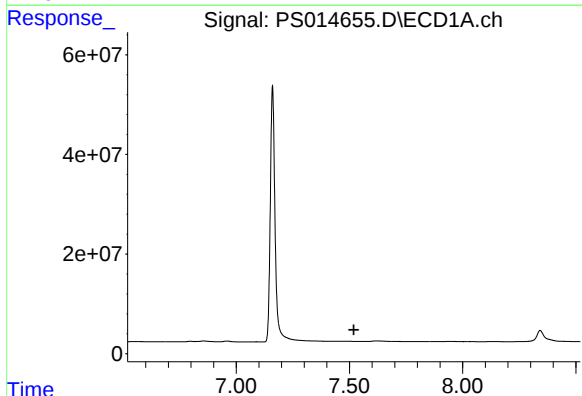


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

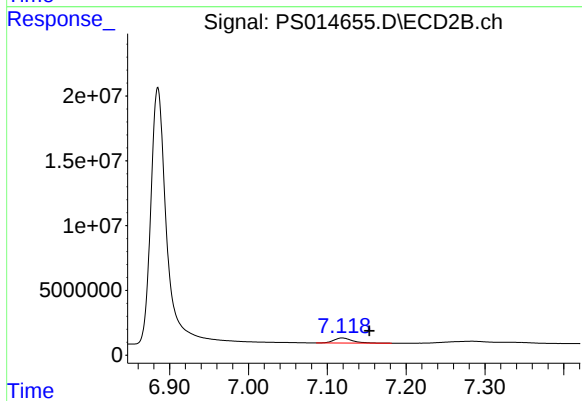

#6 MCP


R.T.: 7.119 min
Delta R.T.: -0.035 min
Response: 6208394
Conc: 3.69 ug/ml

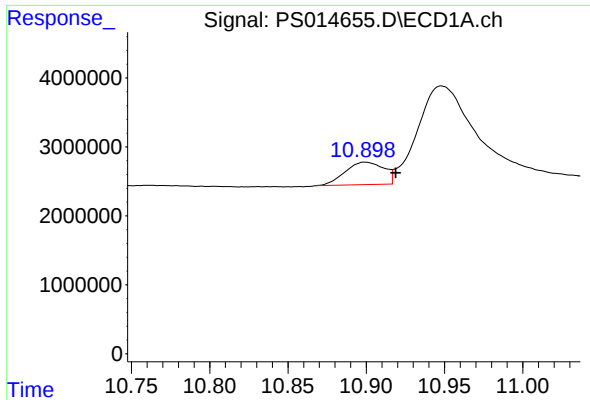

#15 Picloram

R.T.: 10.899 min
Delta R.T.: -0.020 min
Response: 5611579
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

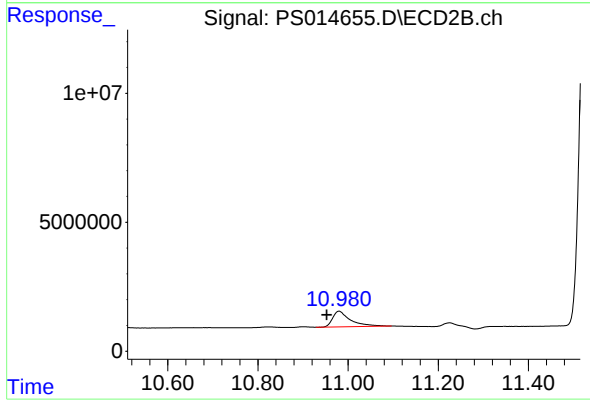

#15 Picloram

R.T.: 10.980 min
Delta R.T.: 0.028 min
Response: 16520735
Conc: 4.41 ng/ml