

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
 Data File : PS009817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 06:49
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:47:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.925	0	1927925	N.D.	3.893
Target Compounds							
2) T	3,5-DICHL...	6.491	0.000	165.9E6	0	201.779	N.D. #
3) T	4-Nitroph...	0.000	6.529	0	1953538	N.D.	6.433
5) T	DICAMBA	0.000	7.094	0	4742120	N.D.	2.384
6) T	MCP	0.000	7.207	0	859740	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.722	0	1754537	N.D.	3.486
9) T	2,4-D	0.000	8.016	0	3503774	N.D.	5.847
10) T	Pentachlo...	8.669	8.448	9518563	6280075	1.281	1.006
11) T	2,4,5-TP ...	9.219	8.809	6216631	6651300	2.101	2.543
12) T	2,4,5-T	9.503	9.188	13223349	13016186	4.769	4.988
13) T	2,4-DB	0.000	9.713	0	7430120	N.D.	20.955
14) T	DINOSEB	0.000	10.030	0	4631201	N.D.	2.352
15) T	Picloram	11.035	11.009	105.8E6	120.3E6	34.137	35.377
16) T	DCPA	0.000	10.959	0	9471387	N.D.	2.825


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
Data File : PS009817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 06:49
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:47:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

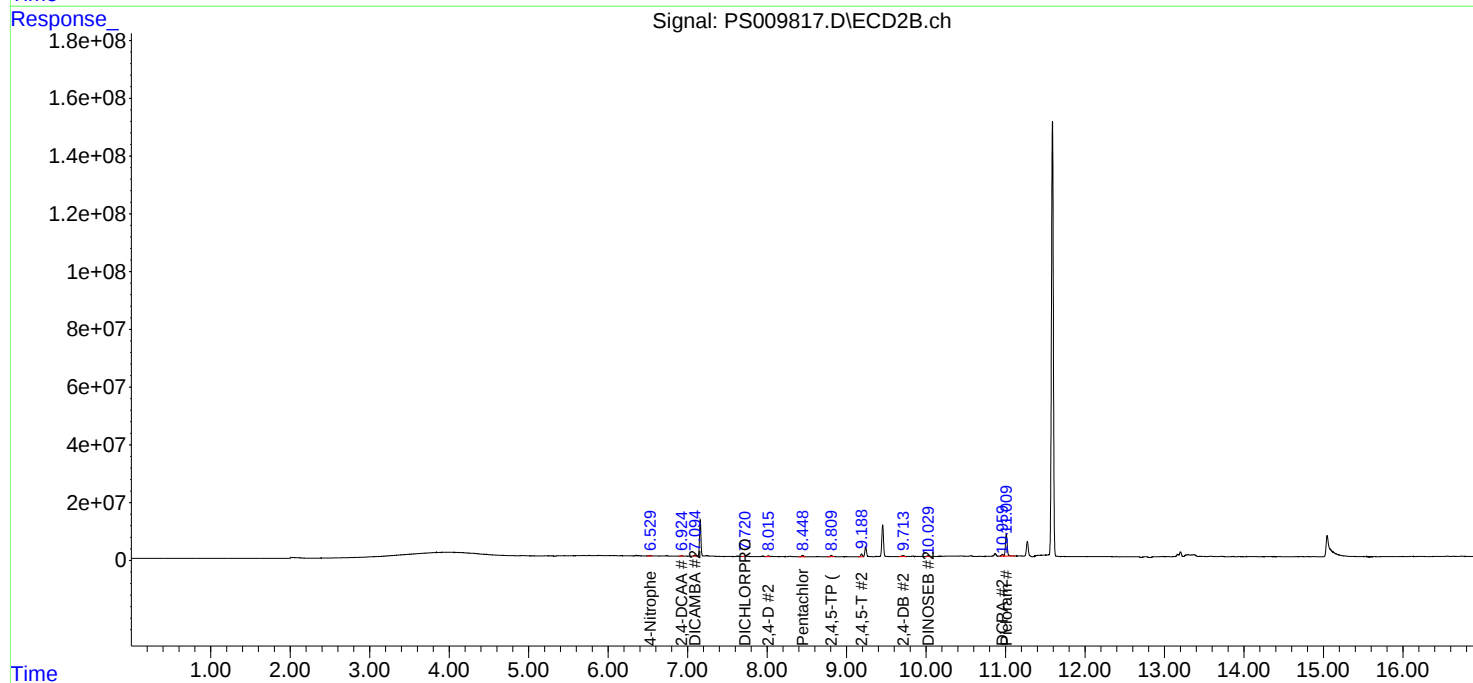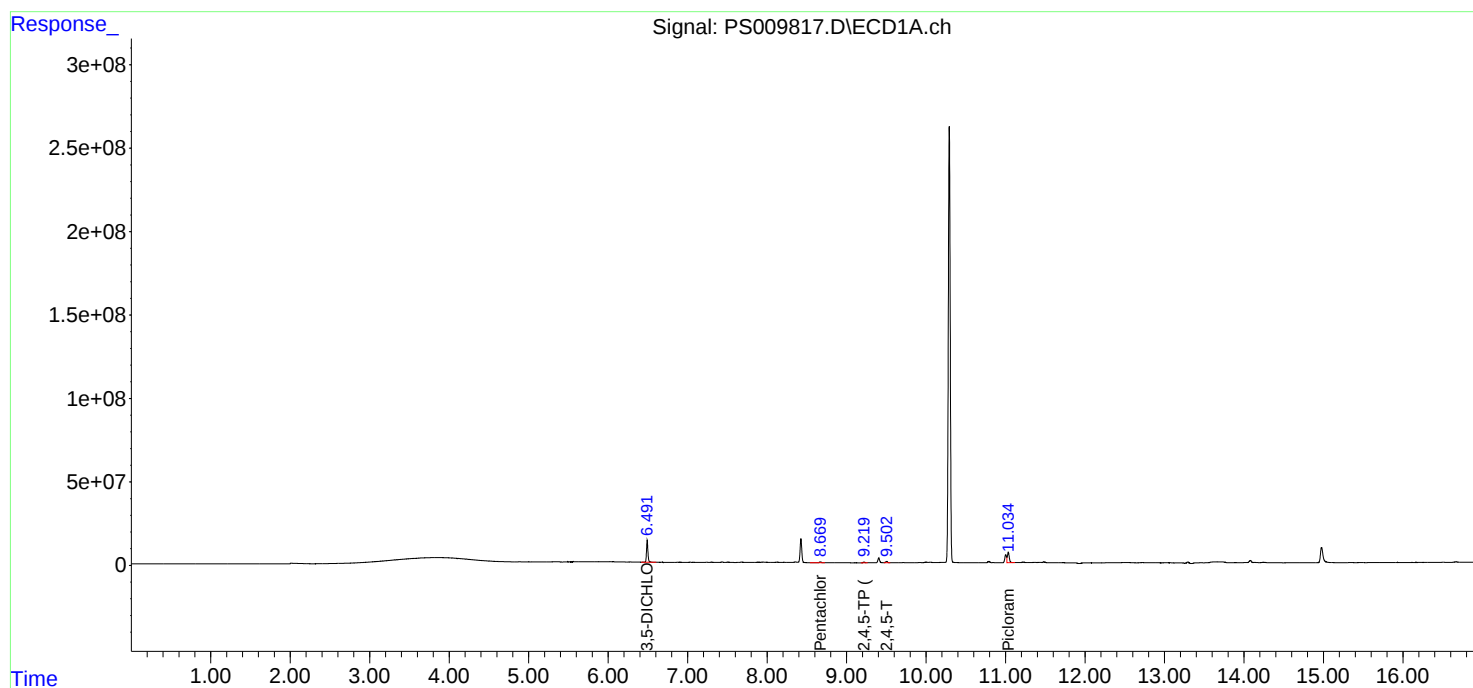

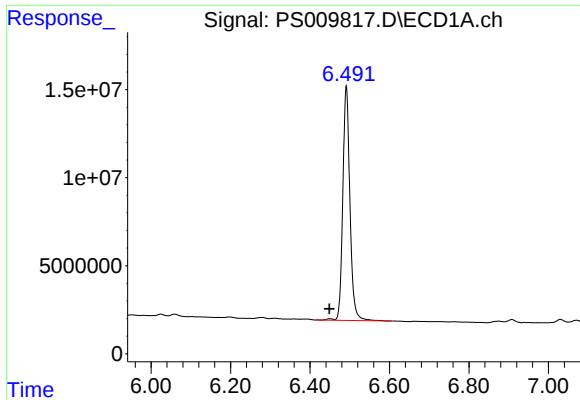


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.491 min
Delta R.T.: 0.043 min
Response: 165928324
Conc: 201.78 ng/ml

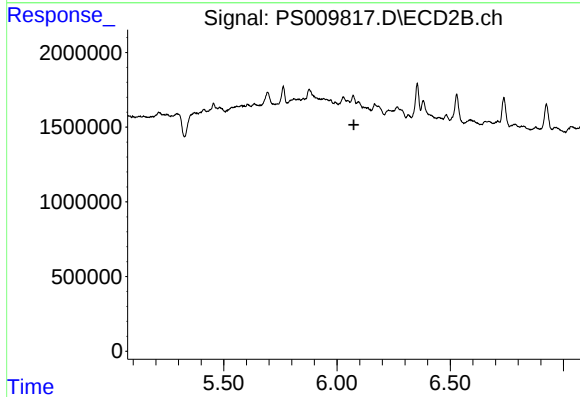


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.075 min
Response: 0
Conc: N.D.

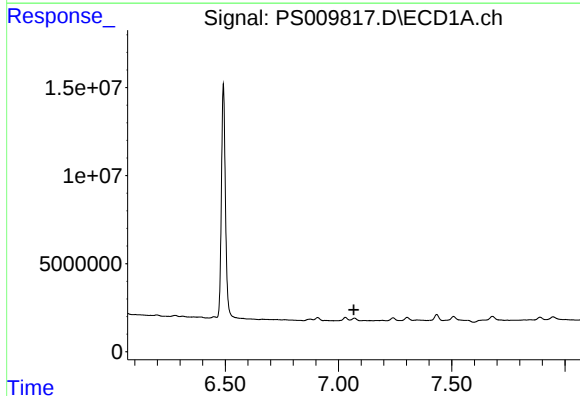


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.068 min
Response: 0
Conc: N.D.

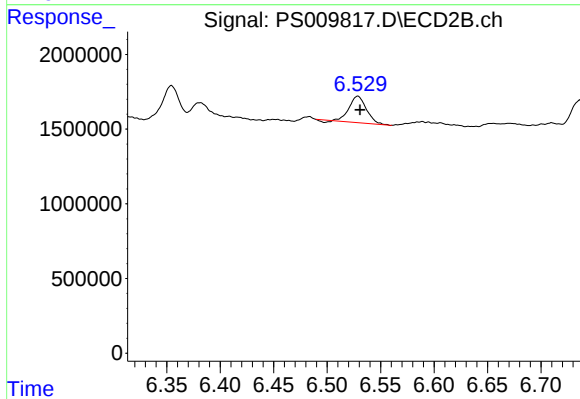


#3 4-Nitrophenol

R.T.: 6.529 min
Delta R.T.: -0.002 min
Response: 1953538
Conc: 6.43 ng/ml

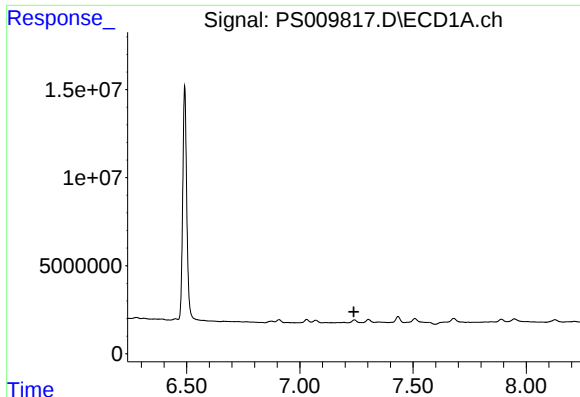


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.239 min
Response: 0
Conc: N.D.

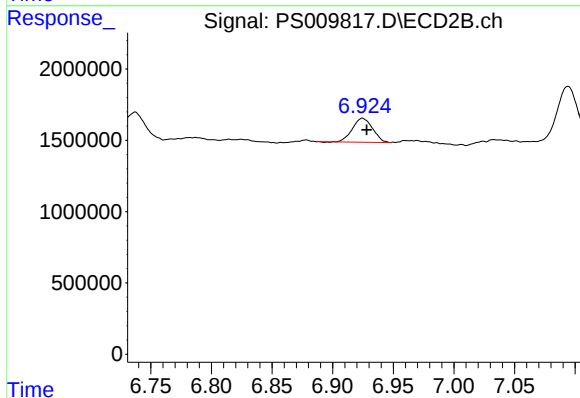


#4 2,4-DCAA

R.T.: 6.925 min
Delta R.T.: -0.004 min
Response: 1927925
Conc: 3.89 ng/ml

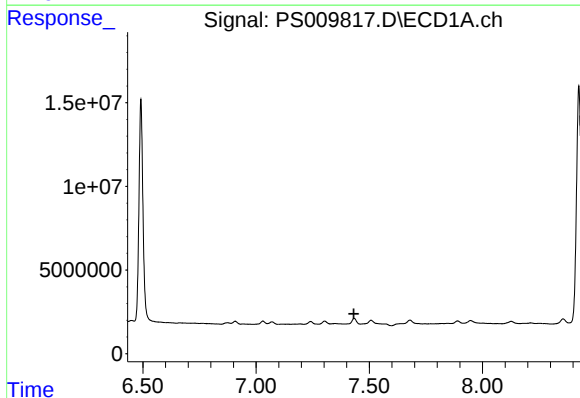


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

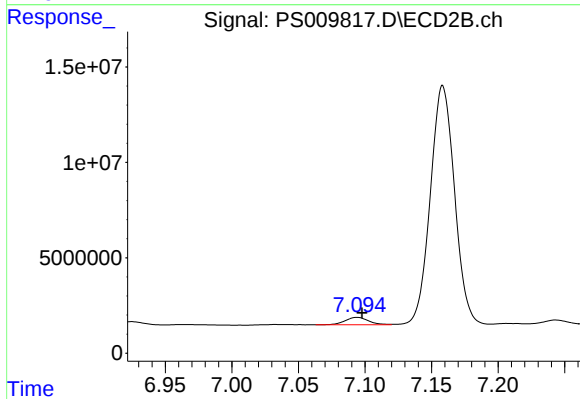


#5 DICAMBA

R.T.: 7.094 min
Delta R.T.: -0.004 min
Response: 4742120
Conc: 2.38 ng/ml

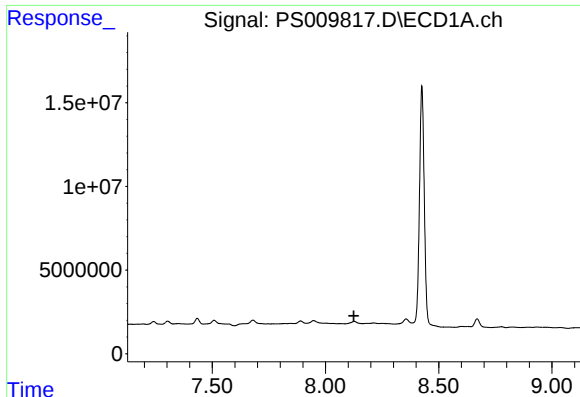


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

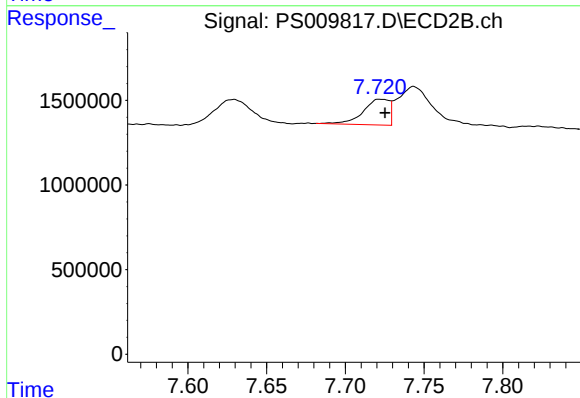


#8 DICHLORPROP

R.T.: 7.722 min
Delta R.T.: -0.003 min
Response: 1754537
Conc: 3.49 ng/ml

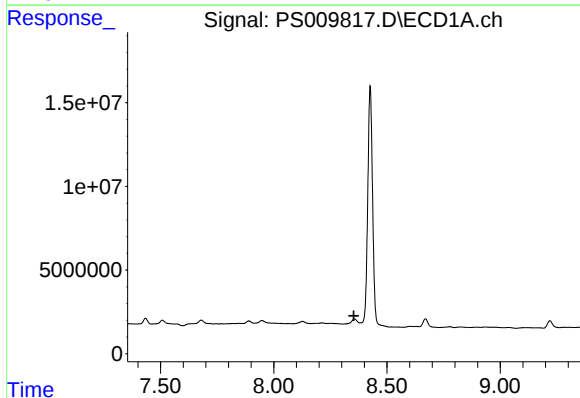


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

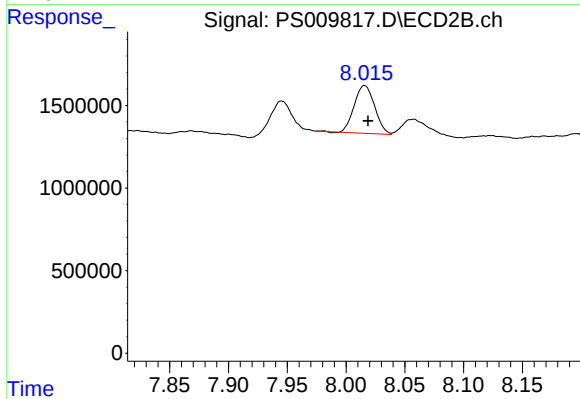


#9 2,4-D

R.T.: 8.016 min
Delta R.T.: -0.003 min
Response: 3503774
Conc: 5.85 ng/ml

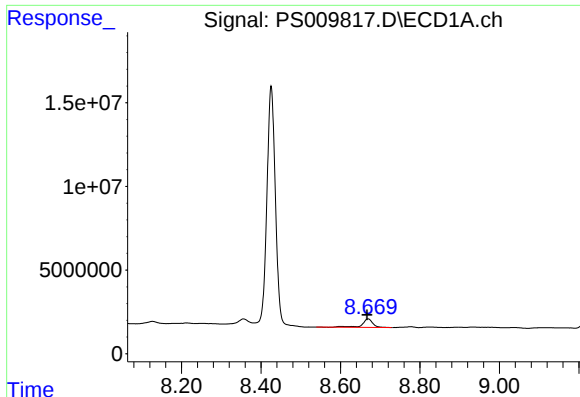


#10 Pentachlorophenol

R.T.: 8.669 min
Delta R.T.: 0.002 min
Response: 9518563
Conc: 1.28 ng/ml

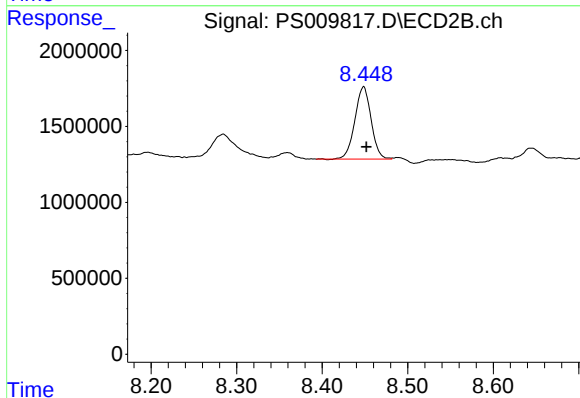


#10 Pentachlorophenol

R.T.: 8.448 min
Delta R.T.: -0.003 min
Response: 6280075
Conc: 1.01 ng/ml

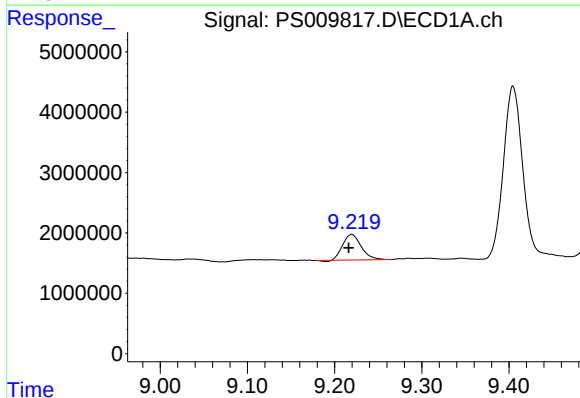


#11 2,4,5-TP (SILVEX)

R.T.: 9.219 min
Delta R.T.: 0.003 min
Response: 6216631
Conc: 2.10 ng/ml

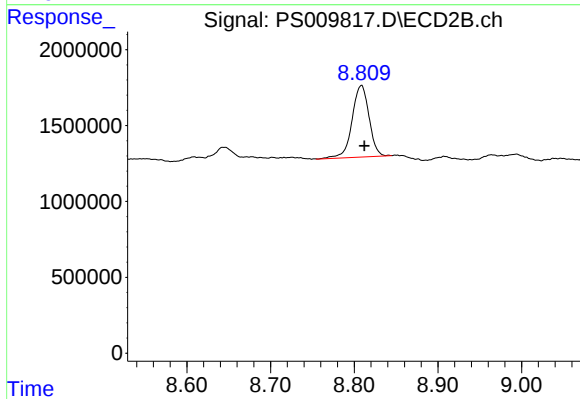


#11 2,4,5-TP (SILVEX)

R.T.: 8.809 min
Delta R.T.: -0.003 min
Response: 6651300
Conc: 2.54 ng/ml

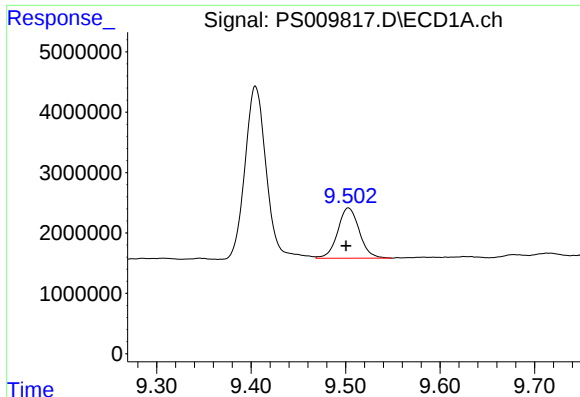


#12 2,4,5-T

R.T.: 9.503 min
Delta R.T.: 0.002 min
Response: 13223349
Conc: 4.77 ng/ml

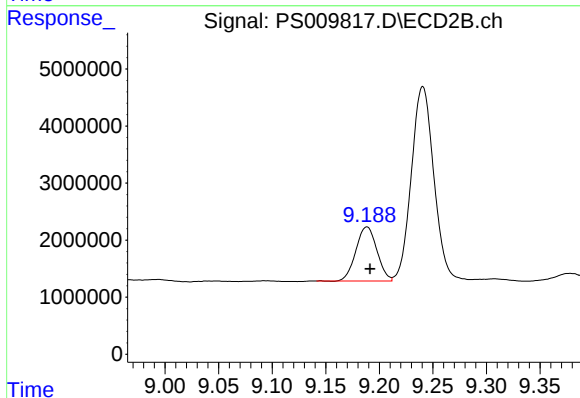


#12 2,4,5-T

R.T.: 9.188 min
Delta R.T.: -0.003 min
Response: 13016186
Conc: 4.99 ng/ml

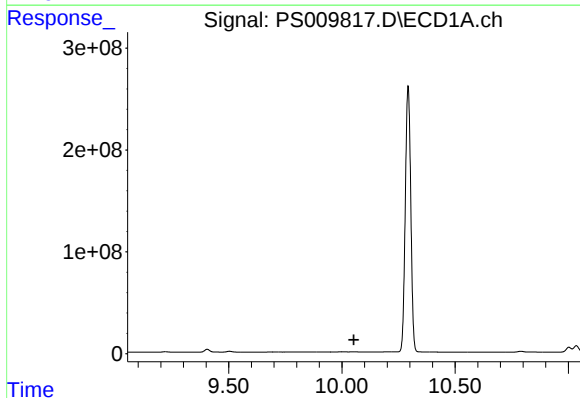


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.053 min
Response: 0
Conc: N.D.

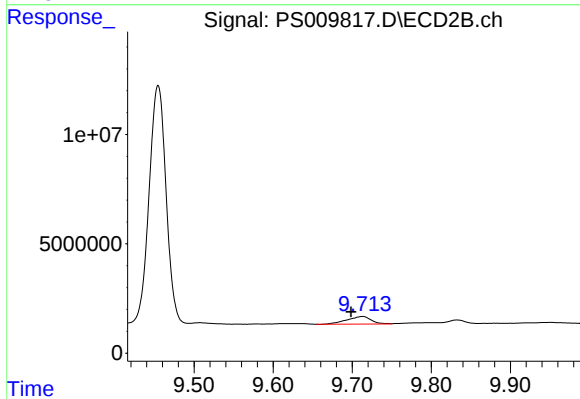


#13 2,4-DB

R.T.: 9.713 min
Delta R.T.: 0.014 min
Response: 7430120
Conc: 20.96 ng/ml

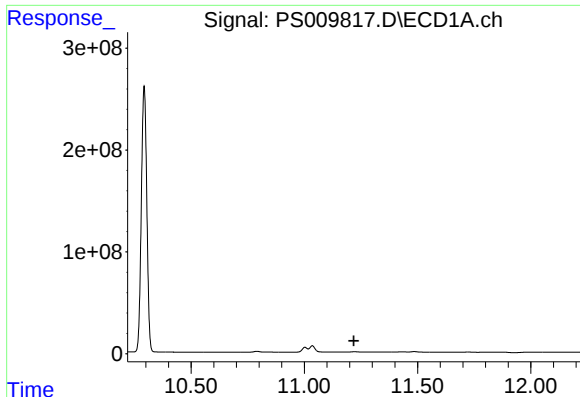


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.219 min
Response: 0
Conc: N.D.

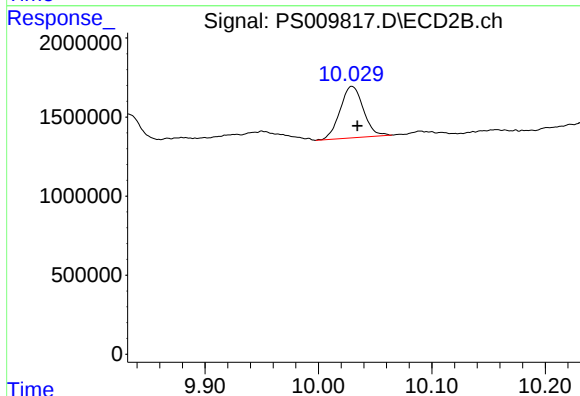


#14 DINOSEB

R.T.: 10.030 min
Delta R.T.: -0.005 min
Response: 4631201
Conc: 2.35 ng/ml

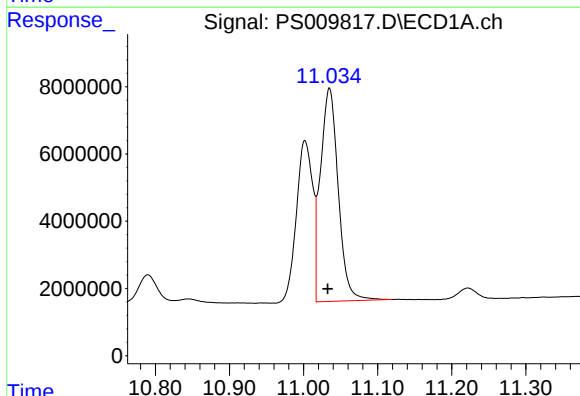


#15 Picloram

R.T.: 11.035 min
Delta R.T.: 0.002 min
Response: 105759283
Conc: 34.14 ng/ml

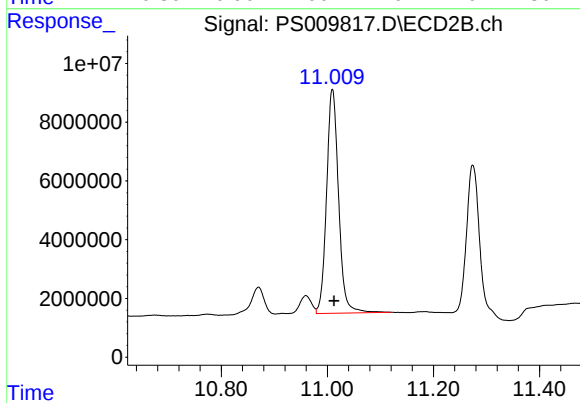


#15 Picloram

R.T.: 11.009 min
Delta R.T.: -0.003 min
Response: 120325913
Conc: 35.38 ng/ml

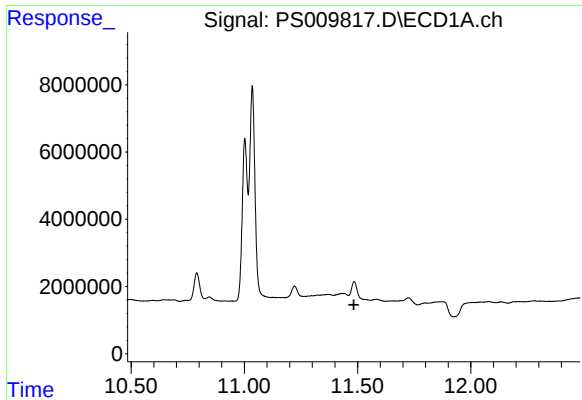

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.484 min
Response: 0
Conc: N.D.

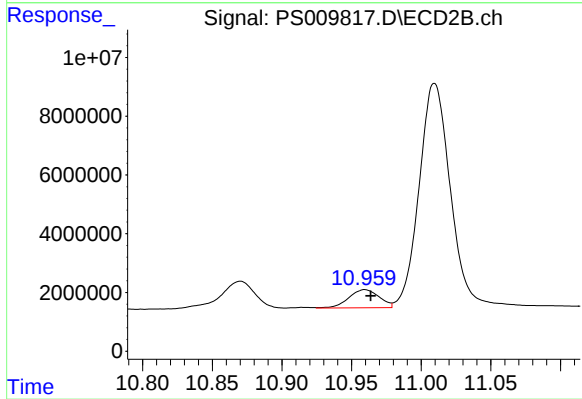

#16 DCPA

R.T.: 10.959 min
Delta R.T.: -0.004 min
Response: 9471387
Conc: 2.82 ng/ml