

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
 Data File : PS009817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 06:49
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 14:31:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds							
2) T	3,5-DICHL...	6.491	0.000	165.9E6	0	219.831	N.D. #
5) T	DICAMBA	0.000	7.094	0	6988150	N.D.	3.044
6) T	MCP	0.000	7.244	0	9953301	N.D.	5.472
8) T	DICHLORPROP	0.000	7.743	0	5354042	N.D.	9.650
9) T	2,4-D	8.426	8.016	212.7E6	3278805	403.378	4.988 #
10) T	Pentachlo...	8.669	8.448	9518563	7079457	1.354	<MDL #
11) T	2,4,5-TP ...	9.219	8.808	6216631	7828683	2.268	2.626
12) T	2,4,5-T	9.503	9.188	13223349	13057100	5.198	4.423
13) T	2,4-DB	0.000	9.711	0	6957144	N.D.	18.327
14) T	DINOSEB	0.000	10.030	0	4604034	N.D.	2.096
15) T	Picloram	11.035	11.010	86666256	121.5E6	28.556	29.837
16) T	DCPA	0.000	10.960	0	10007034	N.D.	2.584


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
Data File : PS009817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 06:49
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 14:31:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

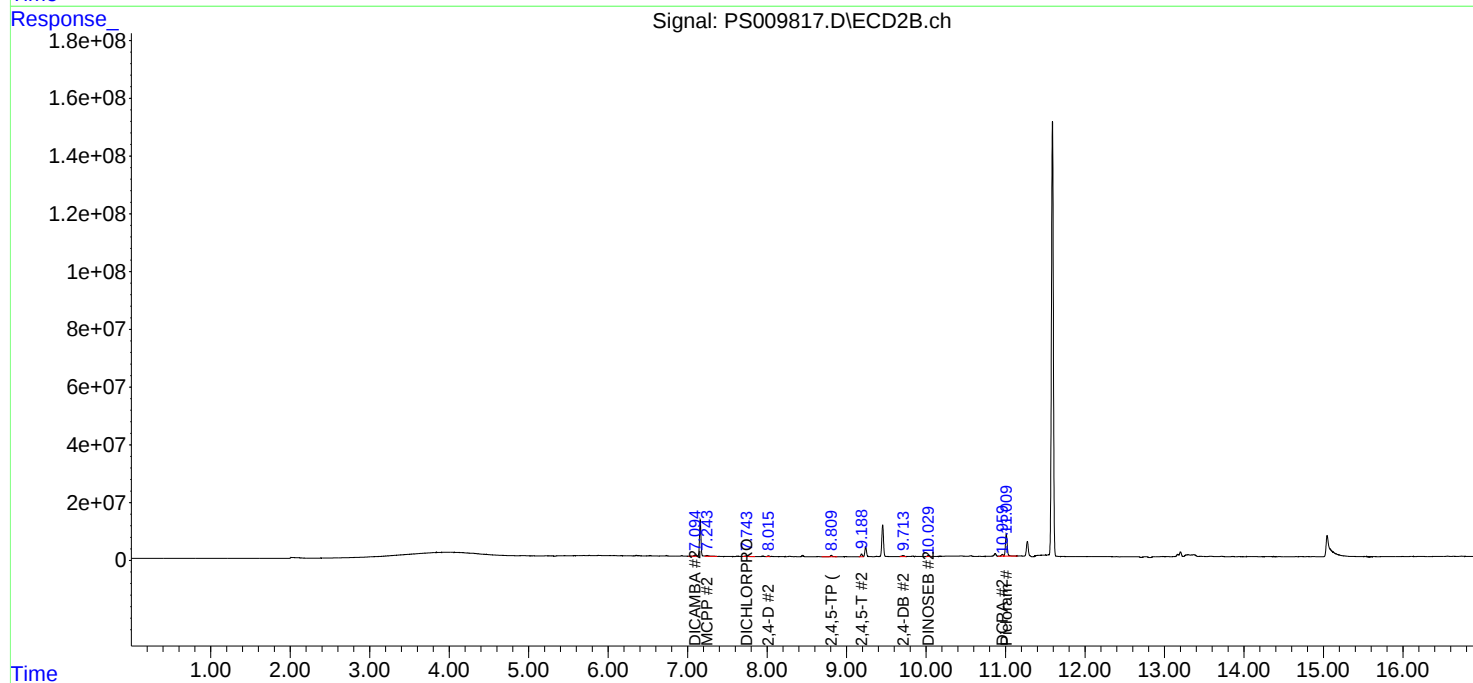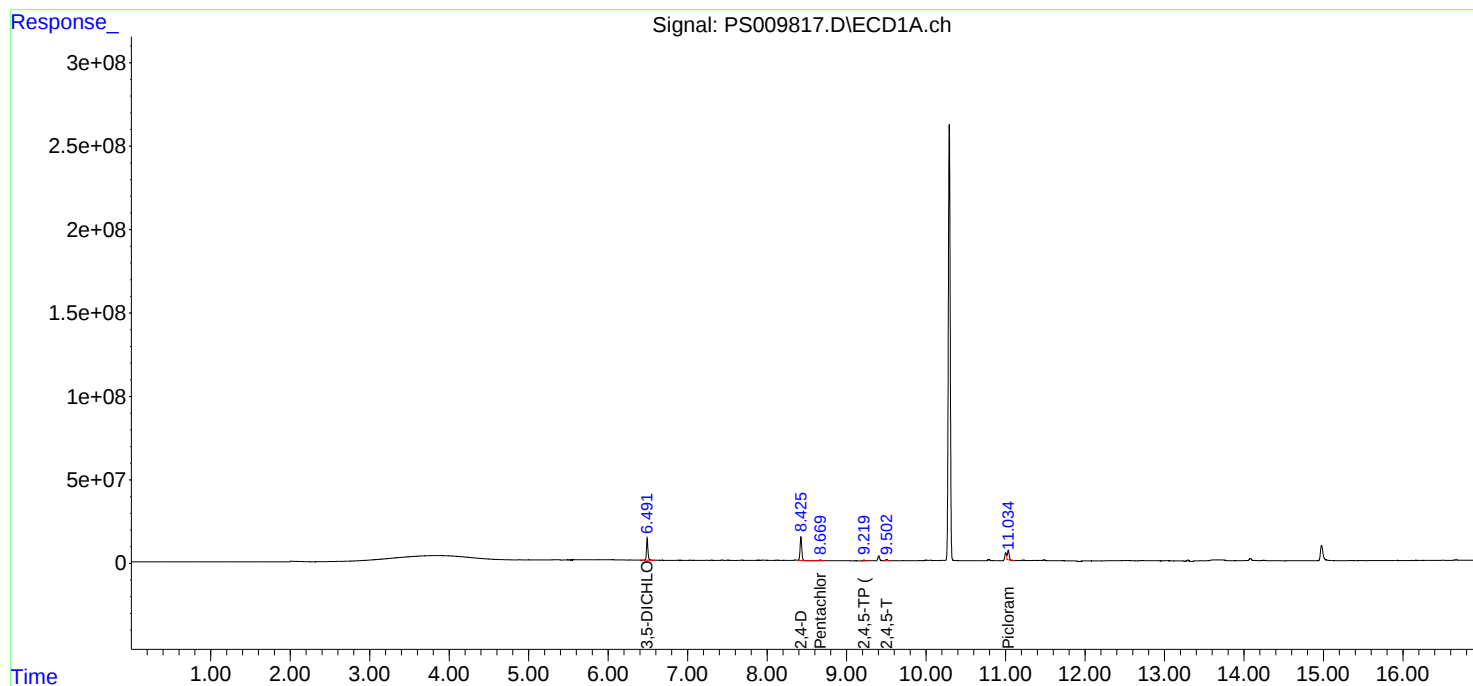

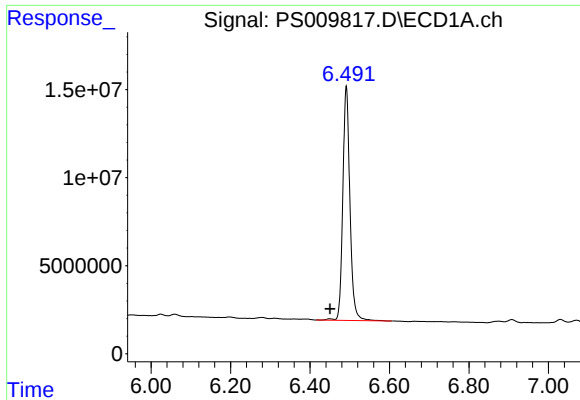


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.491 min
Delta R.T.: 0.041 min
Response: 165928324
Conc: 219.83 ng/ml

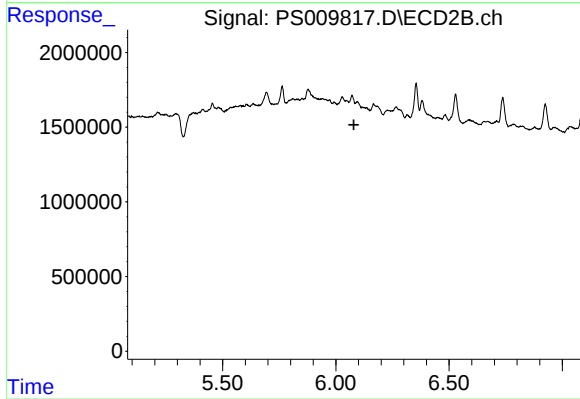


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.080 min
Response: 0
Conc: N.D.

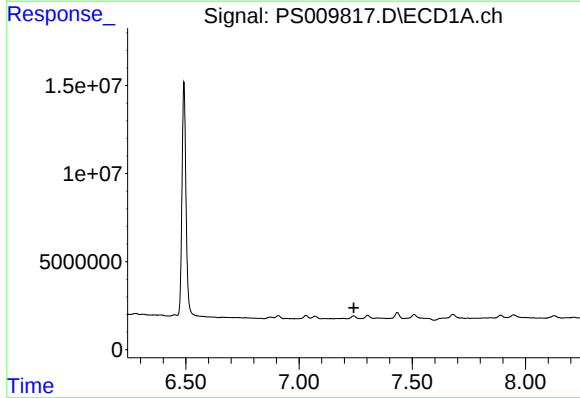


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.242 min
Response: 0
Conc: N.D.

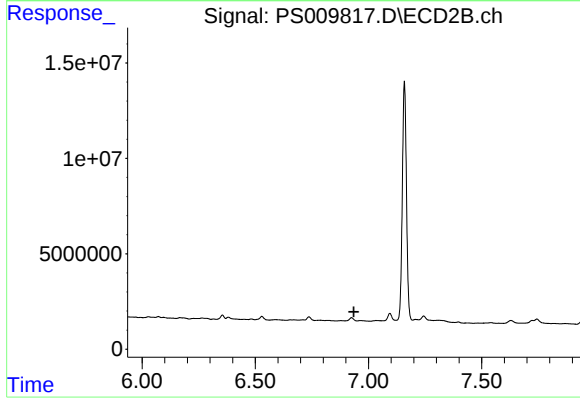


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

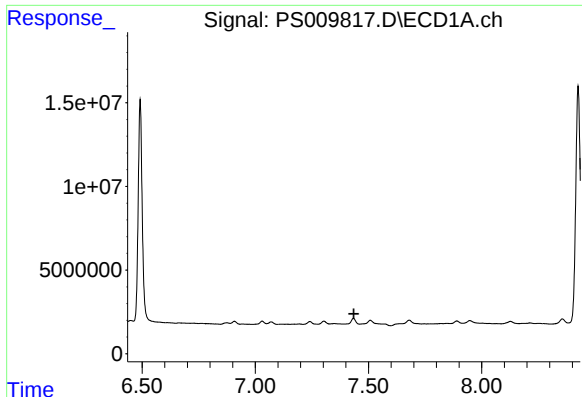


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 7.435 min
Response: 0
Conc: N.D.

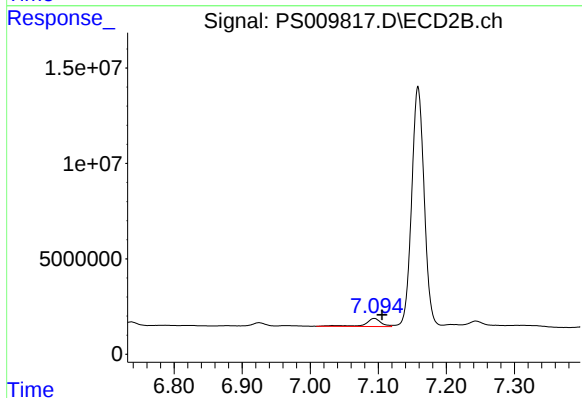


#5 DICAMBA

R.T.: 7.094 min
Delta R.T.: -0.012 min
Response: 6988150
Conc: 3.04 ng/ml

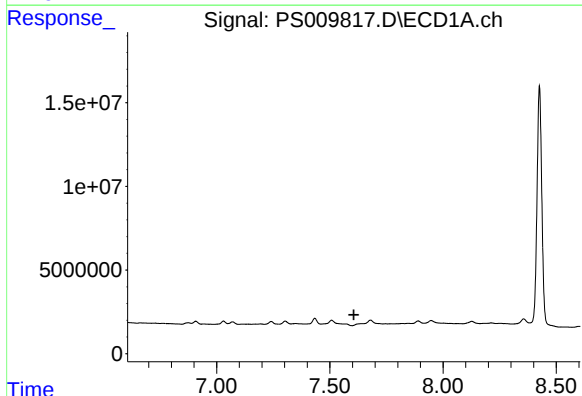


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.606 min
Response: 0
Conc: N.D.

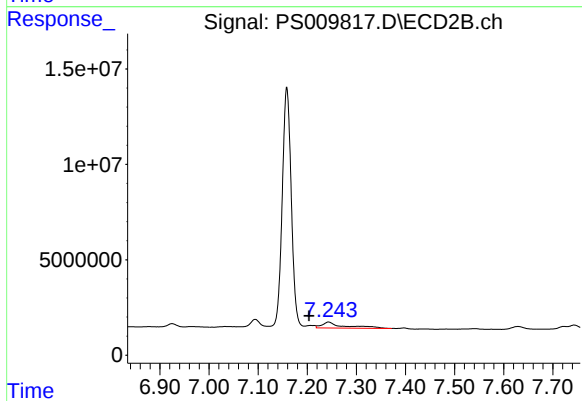


#6 MCP

R.T.: 7.244 min
Delta R.T.: 0.040 min
Response: 9953301
Conc: 5.47 ug/ml

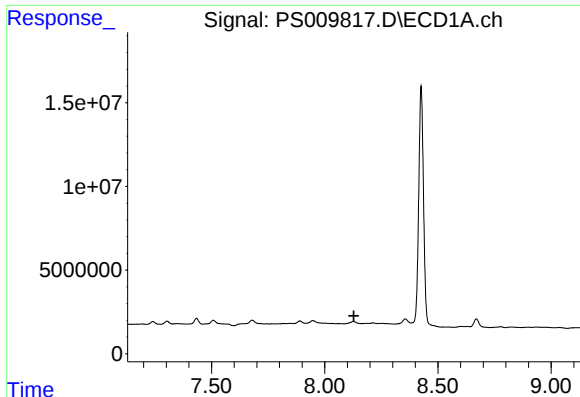


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

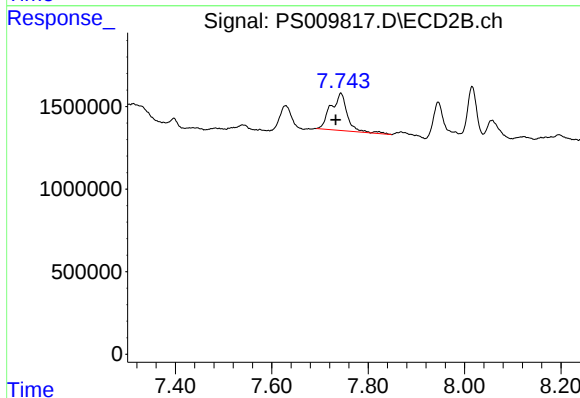


#8 DICHLORPROP

R.T.: 7.743 min
Delta R.T.: 0.010 min
Response: 5354042
Conc: 9.65 ng/ml

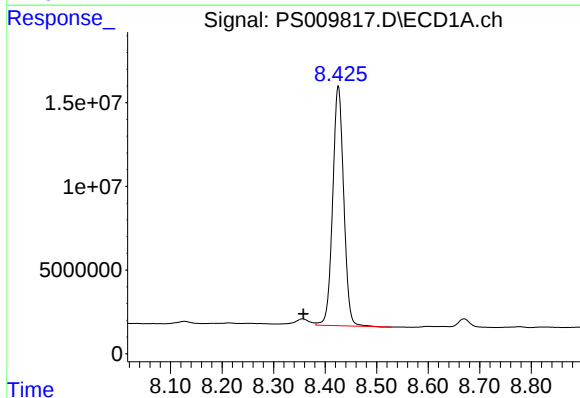


#9 2,4-D

R.T.: 8.426 min
Delta R.T.: 0.068 min
Response: 212670981
Conc: 403.38 ng/ml

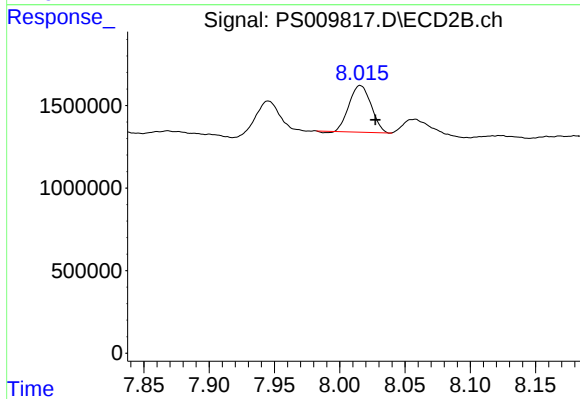


#9 2,4-D

R.T.: 8.016 min
Delta R.T.: -0.011 min
Response: 3278805
Conc: 4.99 ng/ml

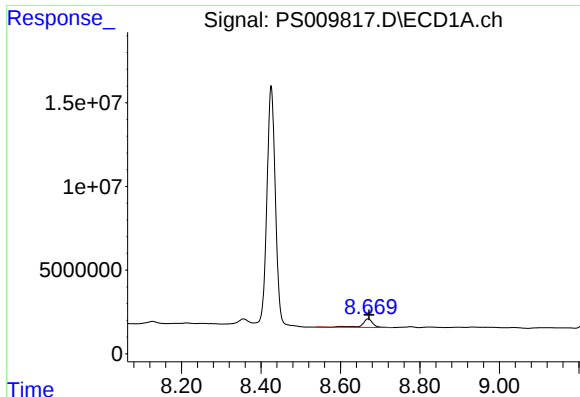


#10 Pentachlorophenol

R.T.: 8.669 min
Delta R.T.: -0.002 min
Response: 9518563
Conc: 1.35 ng/ml

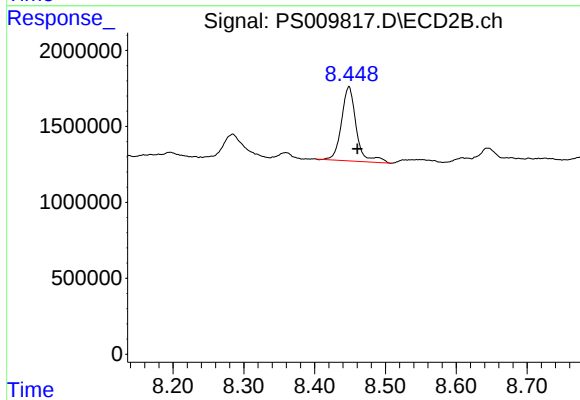


#10 Pentachlorophenol

R.T.: 8.448 min
Delta R.T.: -0.012 min
Response: 7079457
Conc: N.D.

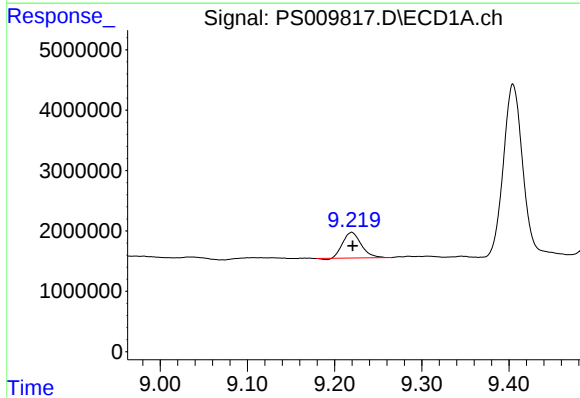


#11 2,4,5-TP (SILVEX)

R.T.: 9.219 min
Delta R.T.: -0.001 min
Response: 6216631
Conc: 2.27 ng/ml

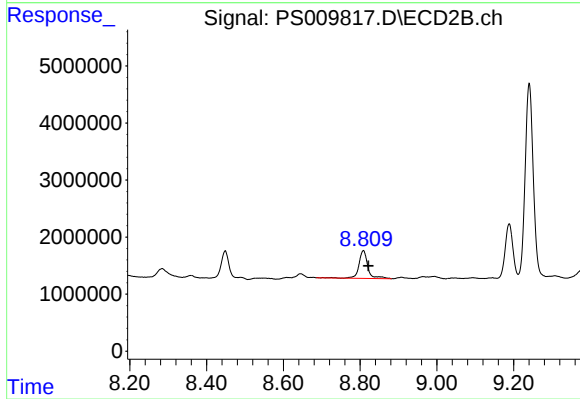


#11 2,4,5-TP (SILVEX)

R.T.: 8.808 min
Delta R.T.: -0.013 min
Response: 7828683
Conc: 2.63 ng/ml

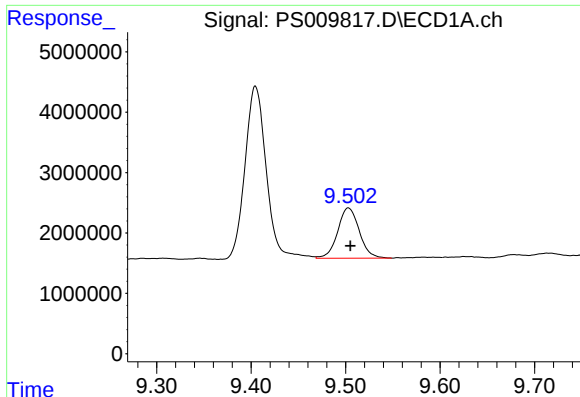


#12 2,4,5-T

R.T.: 9.503 min
Delta R.T.: -0.002 min
Response: 13223349
Conc: 5.20 ng/ml

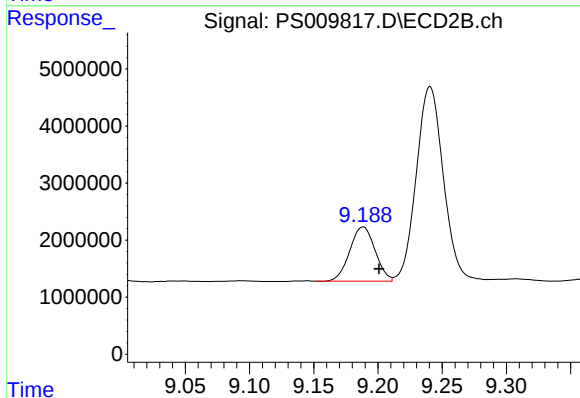


#12 2,4,5-T

R.T.: 9.188 min
Delta R.T.: -0.013 min
Response: 13057100
Conc: 4.42 ng/ml

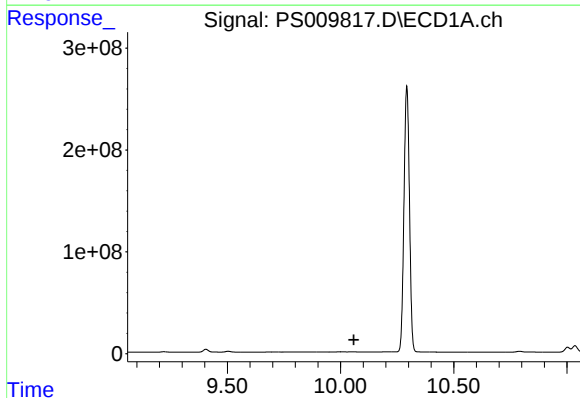


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

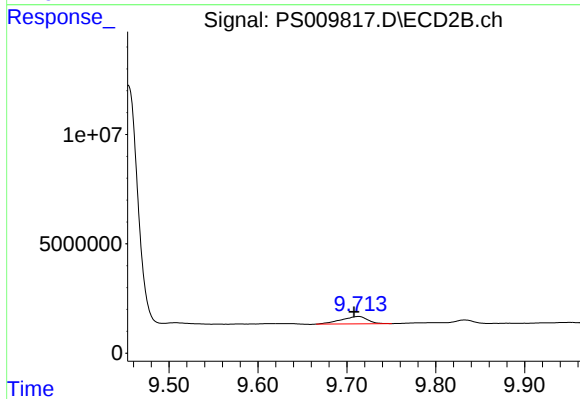


#13 2,4-DB

R.T.: 9.711 min
Delta R.T.: 0.003 min
Response: 6957144
Conc: 18.33 ng/ml

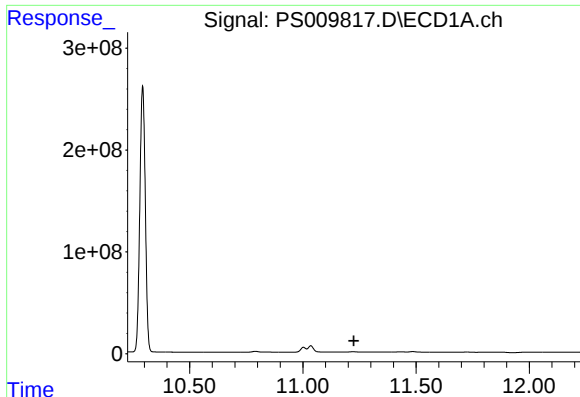


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.225 min
Response: 0
Conc: N.D.

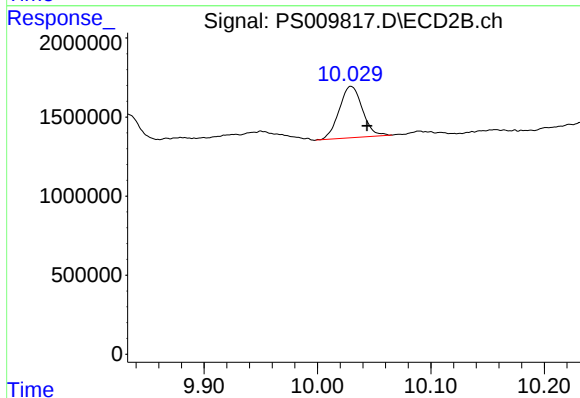


#14 DINOSEB

R.T.: 10.030 min
Delta R.T.: -0.014 min
Response: 4604034
Conc: 2.10 ng/ml

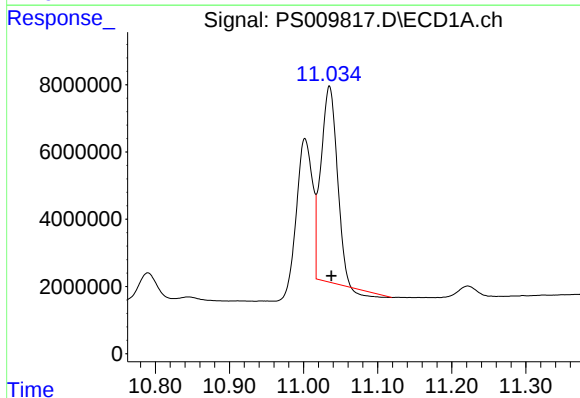


#15 Picloram

R.T.: 11.035 min
Delta R.T.: -0.003 min
Response: 86666256
Conc: 28.56 ng/ml

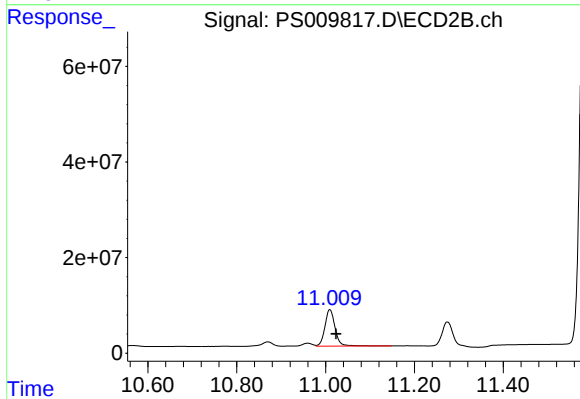


#15 Picloram

R.T.: 11.010 min
Delta R.T.: -0.014 min
Response: 121501078
Conc: 29.84 ng/ml

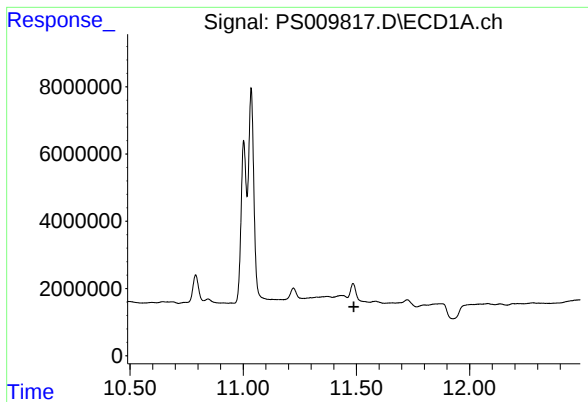

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

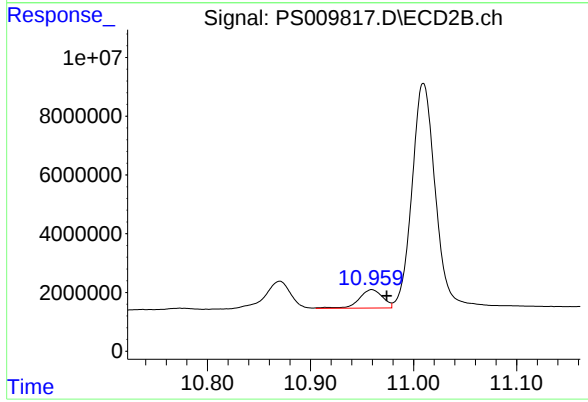

#16 DCPA

R.T.: 10.960 min
Delta R.T.: -0.015 min
Response: 10007034
Conc: 2.58 ng/ml