

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
 Data File : PS009822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 11:26
 Operator : DD\AJ
 Sample : PB128247TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 14:36:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.238	6.927	170.1E6	162.9E6	307.587	296.616
Target Compounds							
2) T	3,5-DICHL...	0.000	6.105	0	73304532	N.D.	90.131
3) T	4-Nitroph...	7.126	6.583	19765348	13533034	82.800	42.530 #
5) T	DICAMBA	7.422	7.061	6694238	13134765	3.146	5.722 #
7) T	MCPA	7.750	7.470	31276121	36633637	10.269	13.575 #
8) T	DICHLORPROP	0.000	7.745	0	15431156	N.D.	27.813
10) T	Pentachlo...	8.665	8.448	6431720	6636308	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.852	0	13168412	N.D.	4.417
12) T	2,4,5-T	9.444	9.190	30264707	3002110	11.897	1.017 #
14) T	DINOSEB	0.000	10.035	0	3024212	N.D.	1.377
15) T	Picloram	11.030	11.011	57718090	45856182	19.018	11.261 #
16) T	DCPA	0.000	10.961	0	6336628	N.D.	1.636


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
Data File : PS009822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 11:26
Operator : DD\AJ
Sample : PB128247TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 14:36:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

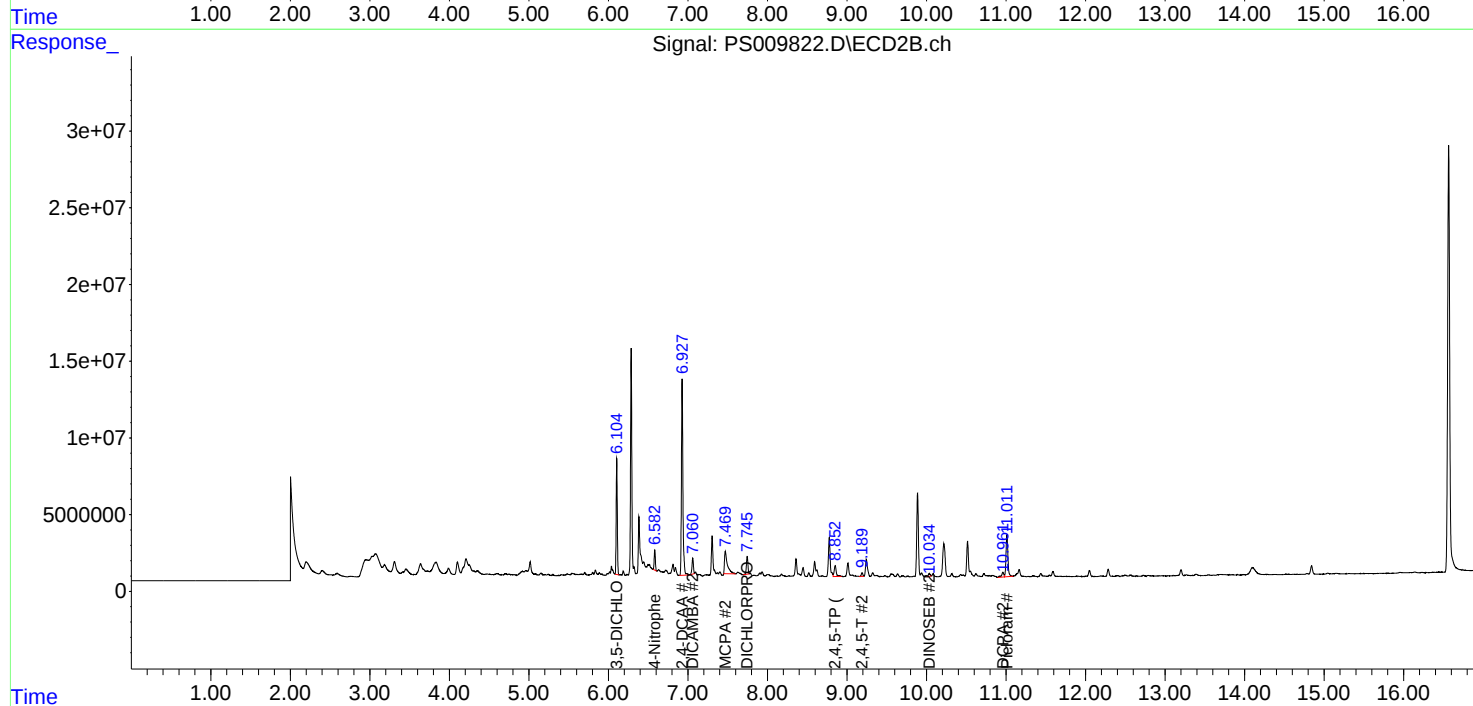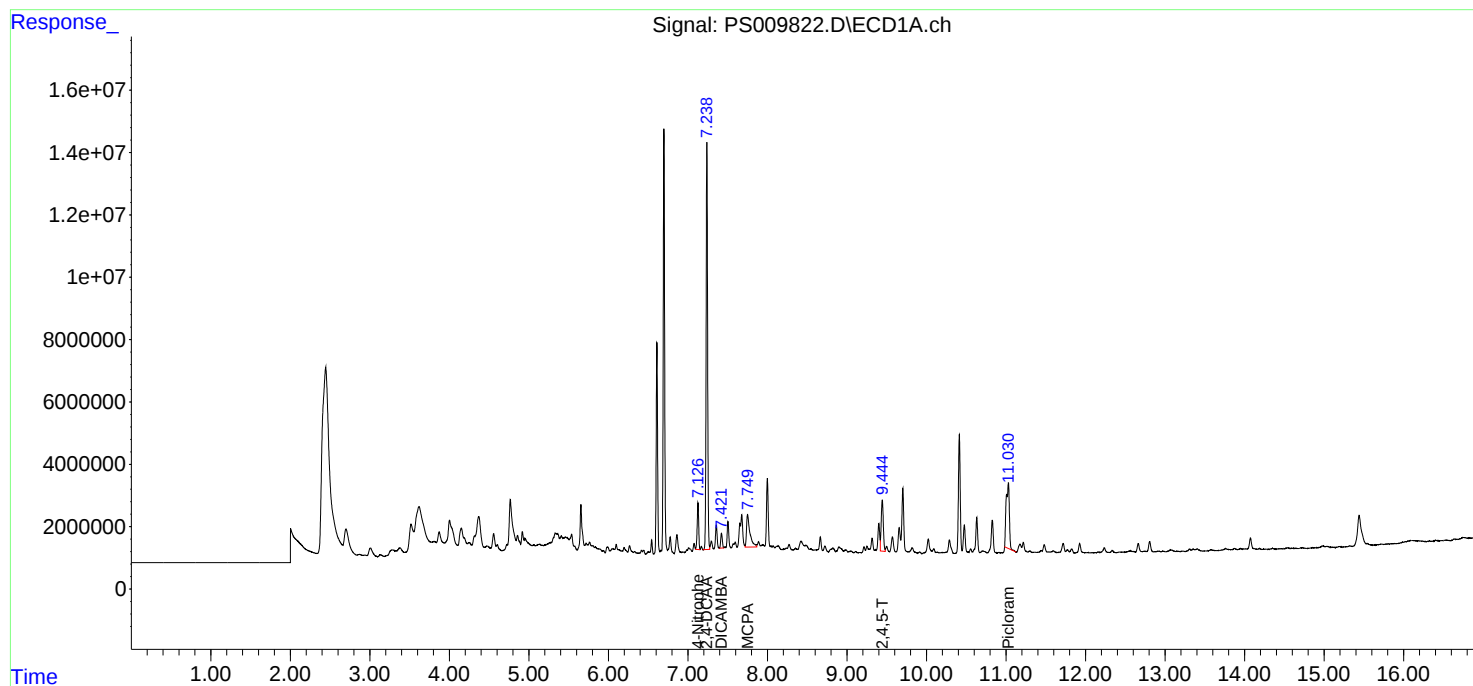

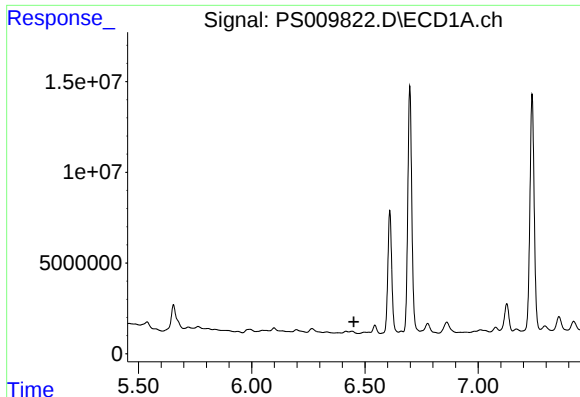


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

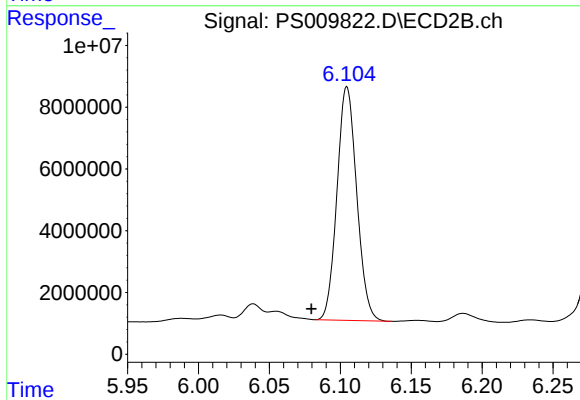


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.105 min
Delta R.T.: 0.025 min
Response: 73304532
Conc: 90.13 ng/ml

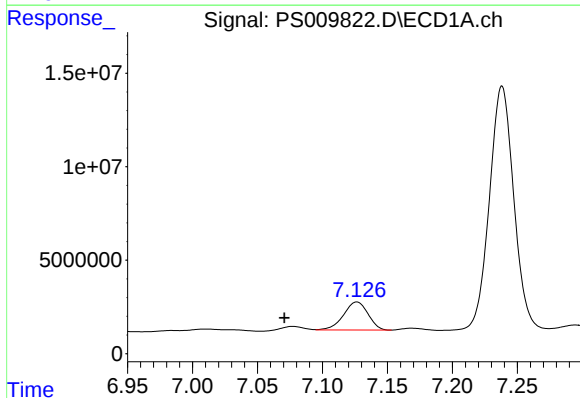


#3 4-Nitrophenol

R.T.: 7.126 min
Delta R.T.: 0.056 min
Response: 19765348
Conc: 82.80 ng/ml

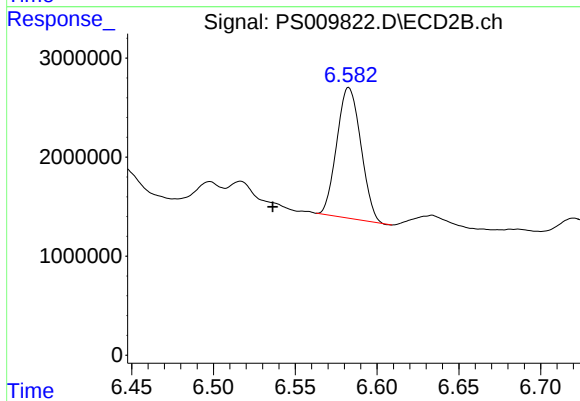


#3 4-Nitrophenol

R.T.: 6.583 min
Delta R.T.: 0.047 min
Response: 13533034
Conc: 42.53 ng/ml

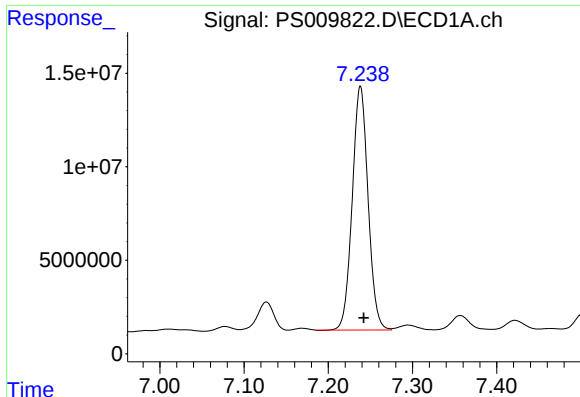


#4 2,4-DCAA

R.T.: 7.238 min
Delta R.T.: -0.004 min
Response: 170147992
Conc: 307.59 ng/ml

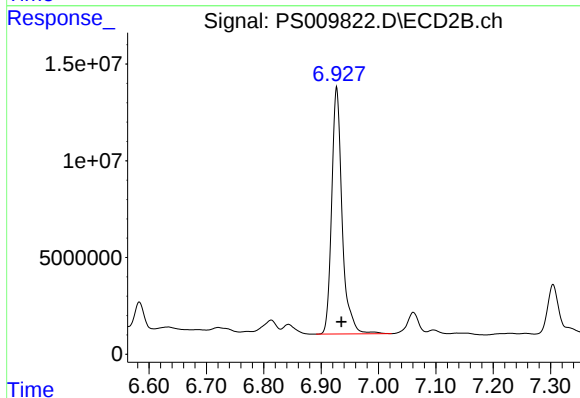


#4 2,4-DCAA

R.T.: 6.927 min
Delta R.T.: -0.008 min
Response: 162900741
Conc: 296.62 ng/ml

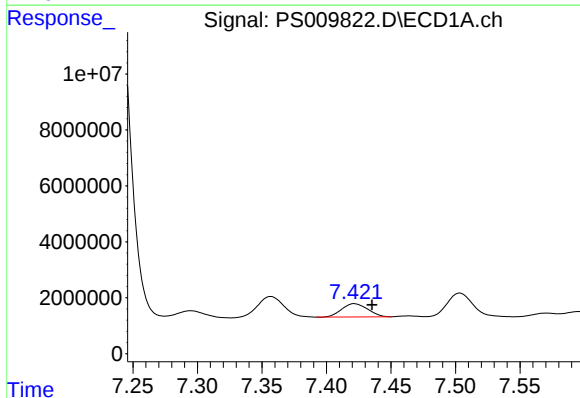


#5 DICAMBA

R.T.: 7.422 min
Delta R.T.: -0.014 min
Response: 6694238
Conc: 3.15 ng/ml

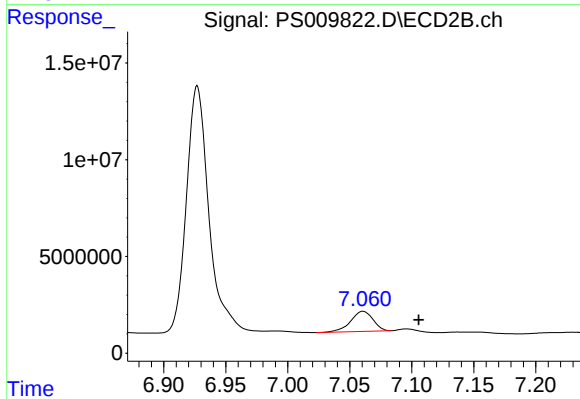


#5 DICAMBA

R.T.: 7.061 min
Delta R.T.: -0.045 min
Response: 13134765
Conc: 5.72 ng/ml

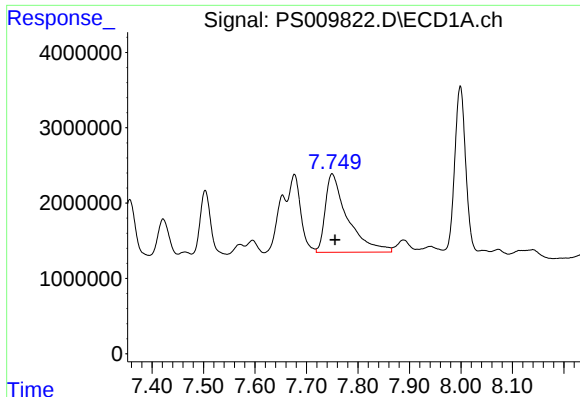


#7 MCPA

R.T.: 7.750 min
Delta R.T.: -0.006 min
Response: 31276121
Conc: 10.27 ug/ml

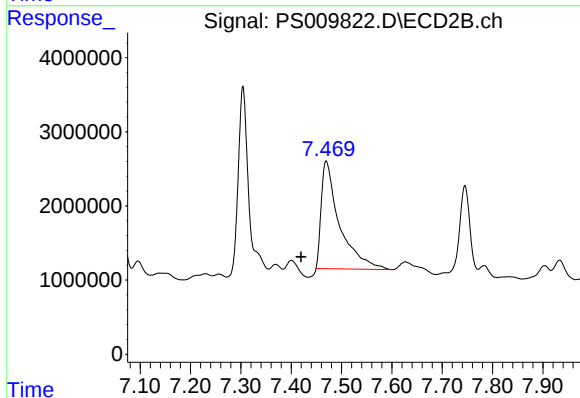


#7 MCPA

R.T.: 7.470 min
Delta R.T.: 0.050 min
Response: 36633637
Conc: 13.57 ug/ml

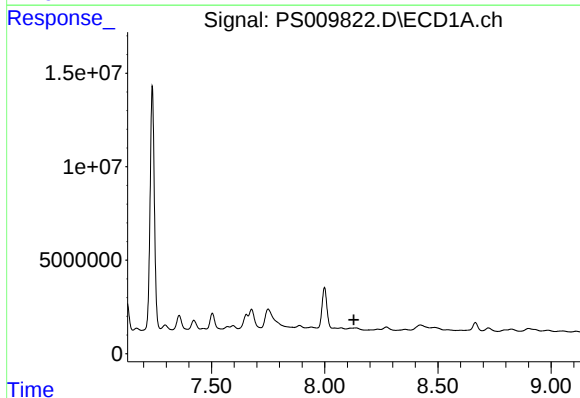


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

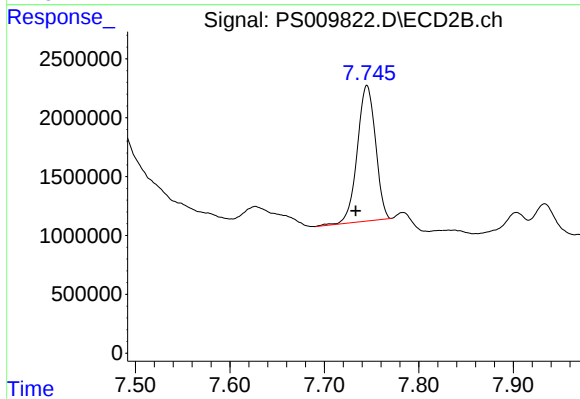


#8 DICHLORPROP

R.T.: 7.745 min
Delta R.T.: 0.012 min
Response: 15431156
Conc: 27.81 ng/ml

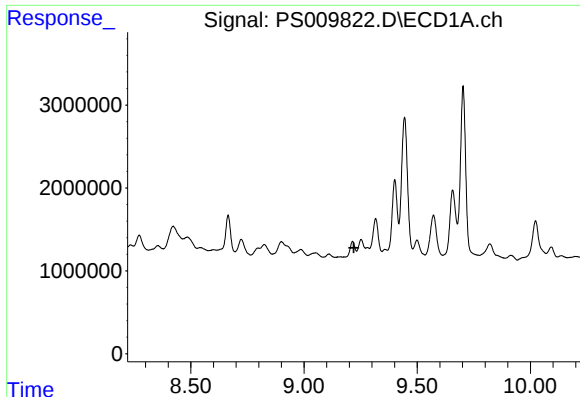


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

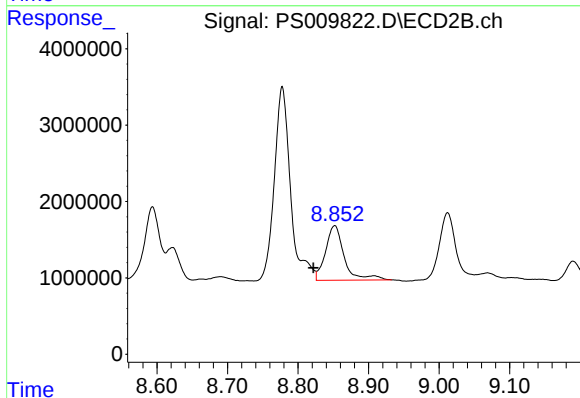


#11 2,4,5-TP (SILVEX)

R.T.: 8.852 min
Delta R.T.: 0.030 min
Response: 13168412
Conc: 4.42 ng/ml

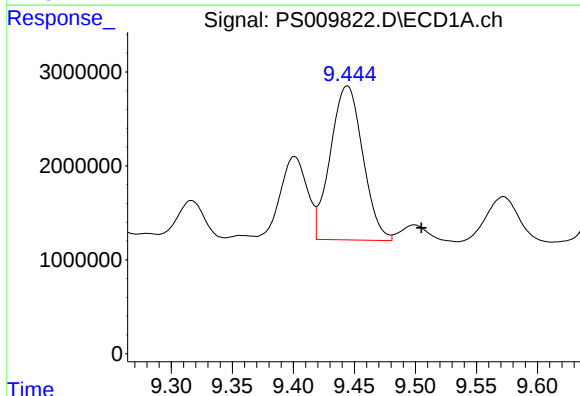


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 30264707
Conc: 11.90 ng/ml

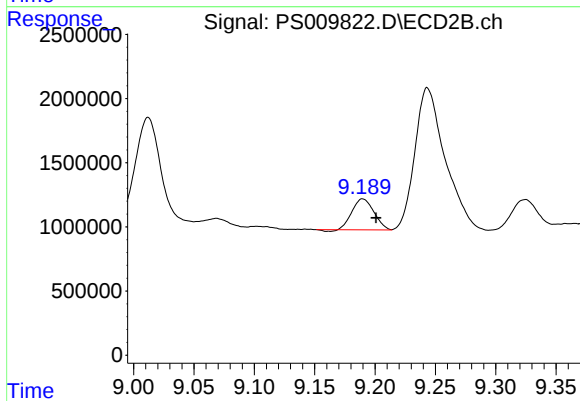


#12 2,4,5-T

R.T.: 9.190 min
Delta R.T.: -0.011 min
Response: 3002110
Conc: 1.02 ng/ml

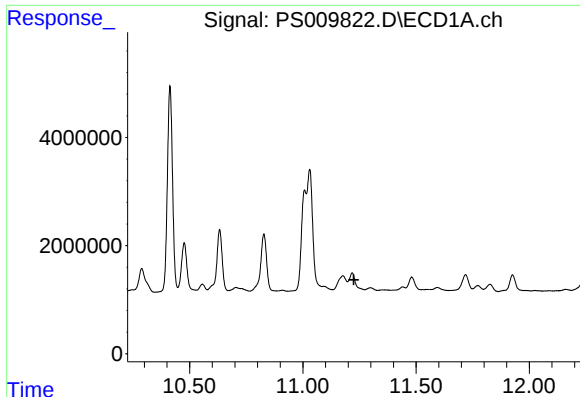


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.225 min
Response: 0
Conc: N.D.

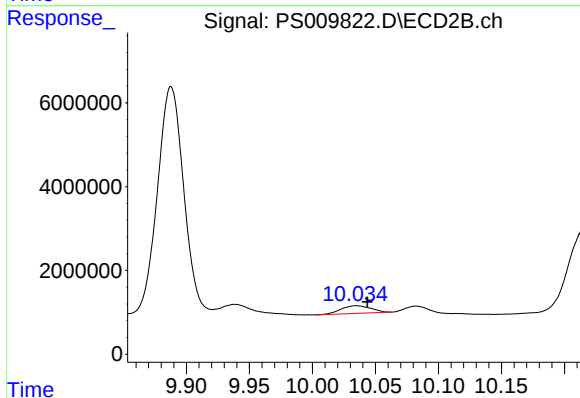


#14 DINOSEB

R.T.: 10.035 min
Delta R.T.: -0.009 min
Response: 3024212
Conc: 1.38 ng/ml

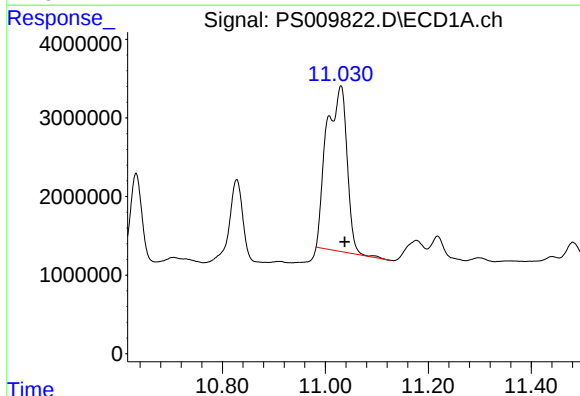


#15 Picloram

R.T.: 11.030 min
Delta R.T.: -0.007 min
Response: 57718090
Conc: 19.02 ng/ml

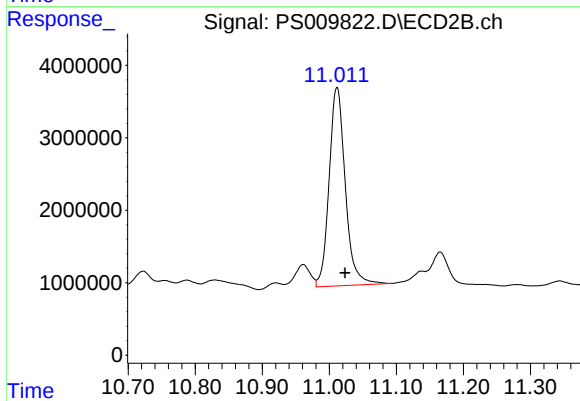


#15 Picloram

R.T.: 11.011 min
Delta R.T.: -0.012 min
Response: 45856182
Conc: 11.26 ng/ml

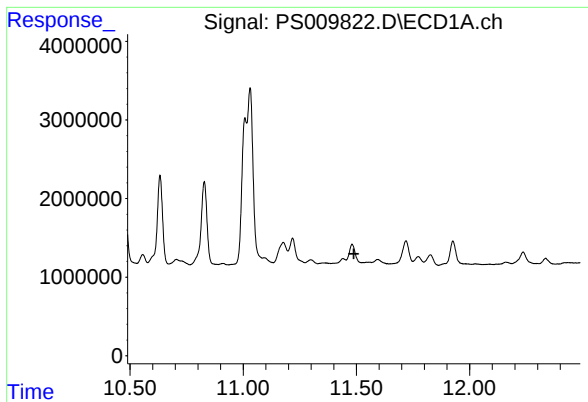

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

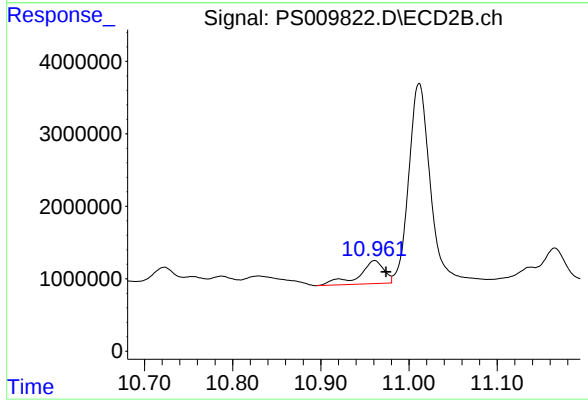

#16 DCPA

R.T.: 10.961 min
Delta R.T.: -0.013 min
Response: 6336628
Conc: 1.64 ng/ml