

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
 Data File : PS009823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 11:49
 Operator : DD\AJ
 Sample : L2123-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 14:36:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.238	6.927	173.2E6	164.6E6	313.191	299.633
Target Compounds							
2) T	3,5-DICHL...	0.000	6.105	0	65644760	N.D.	80.713
3) T	4-Nitroph...	7.126	6.583	21358879	14218242	89.475	44.684 #
5) T	DICAMBA	0.000	7.061	0	14969865	N.D.	6.521
7) T	MCPA	7.744	7.467	49863270	51329439	16.372	19.021
8) T	DICHLORPROP	0.000	7.745	0	15697165	N.D.	28.292
9) T	2,4-D	8.422	0.000	8258684	0	15.664	N.D. #
10) T	Pentachlo...	0.000	8.521	0	3611112	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.851	0	15562006	N.D.	5.220
12) T	2,4,5-T	9.444	9.246	30775473	11095644	12.098	3.758 #
14) T	DINOSEB	0.000	10.039	0	10562181	N.D.	4.809
15) T	Picloram	11.007	11.012	45303478	19821650	14.927	4.868 #
16) T	DCPA	0.000	11.012	0	19821650	N.D.	5.118


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
Data File : PS009823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 11:49
Operator : DD\AJ
Sample : L2123-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 14:36:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

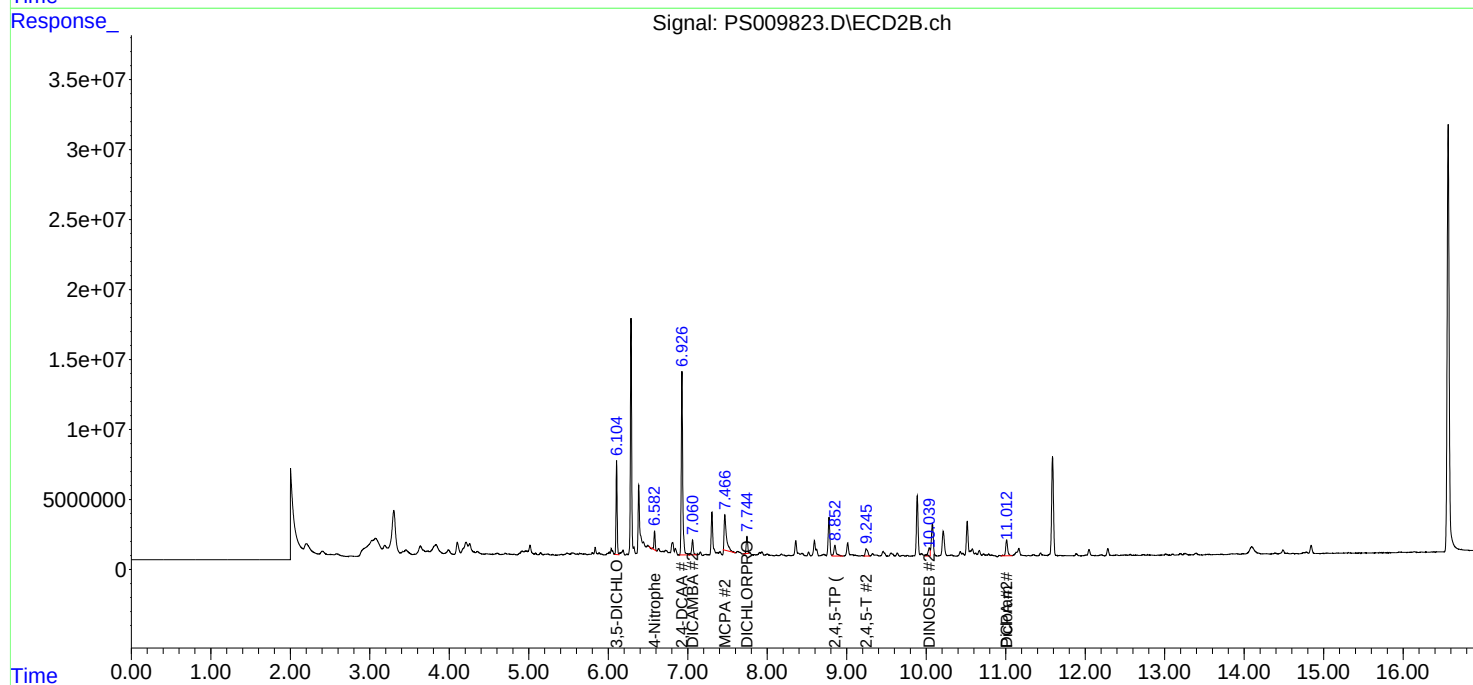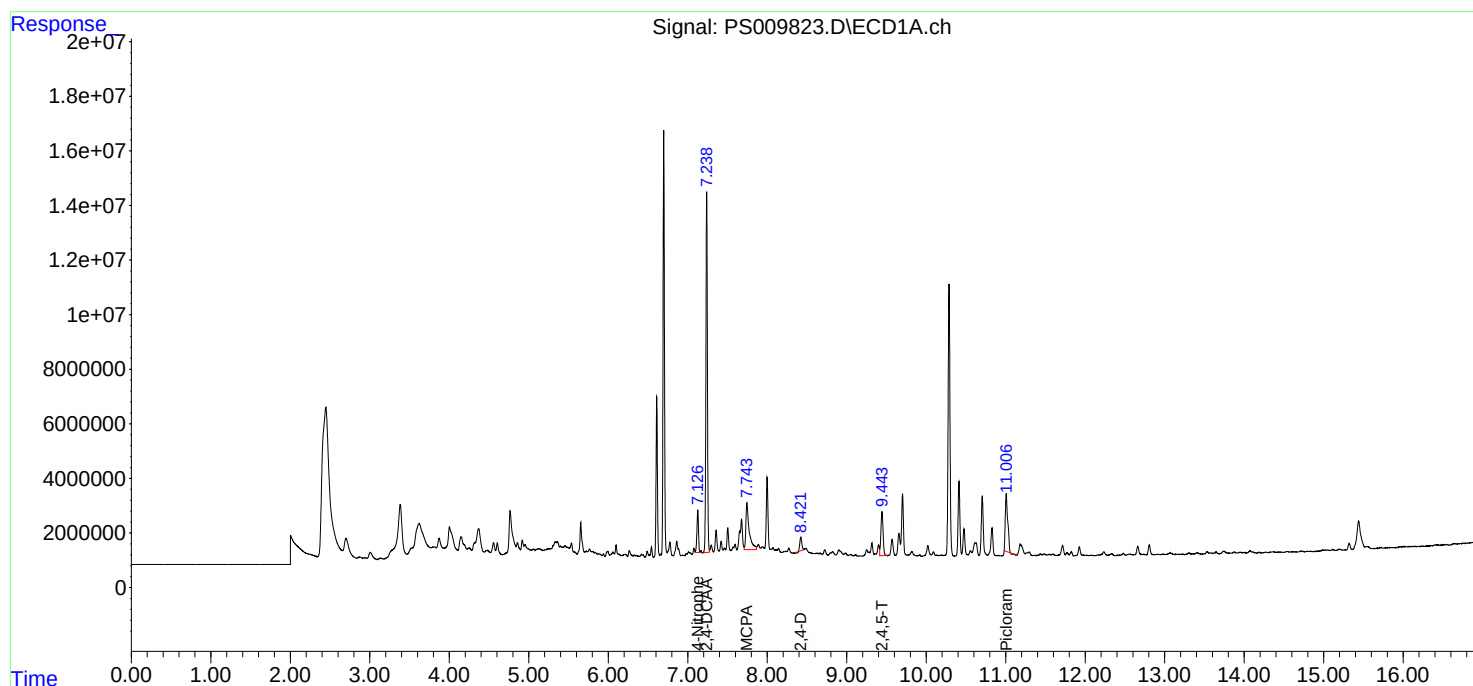

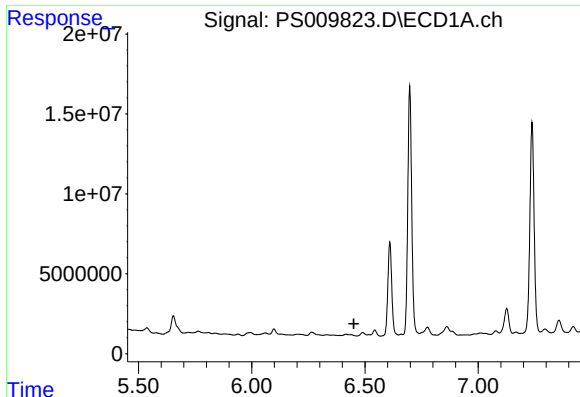


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

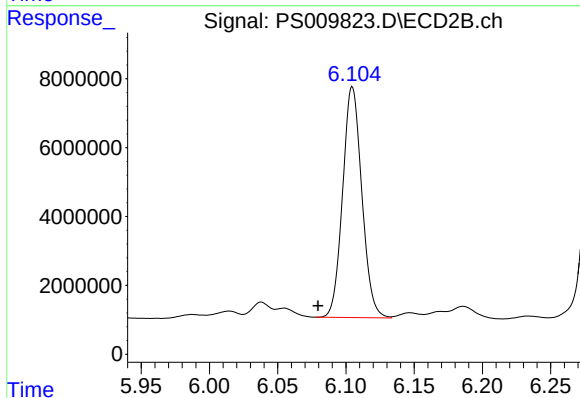


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.105 min
Delta R.T.: 0.025 min
Response: 65644760
Conc: 80.71 ng/ml

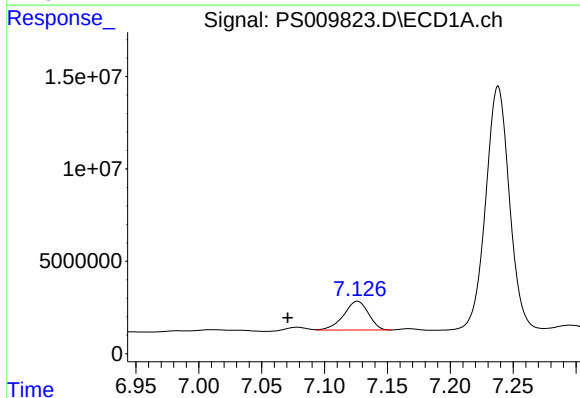


#3 4-Nitrophenol

R.T.: 7.126 min
Delta R.T.: 0.055 min
Response: 21358879
Conc: 89.48 ng/ml

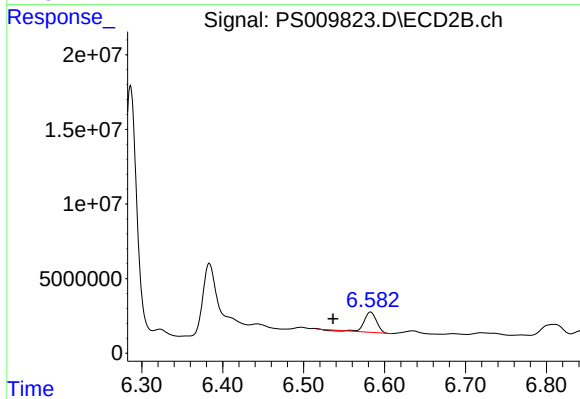


#3 4-Nitrophenol

R.T.: 6.583 min
Delta R.T.: 0.046 min
Response: 14218242
Conc: 44.68 ng/ml

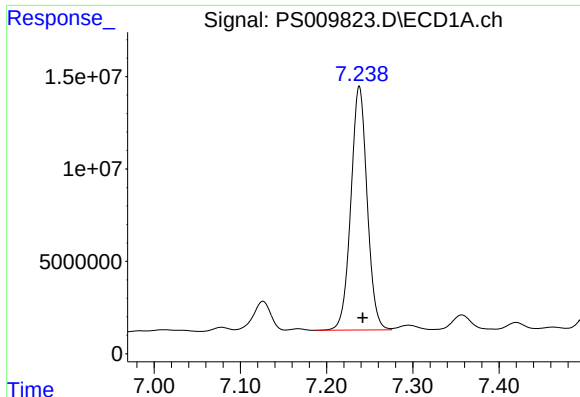


#4 2,4-DCAA

R.T.: 7.238 min
Delta R.T.: -0.004 min
Response: 173247831
Conc: 313.19 ng/ml

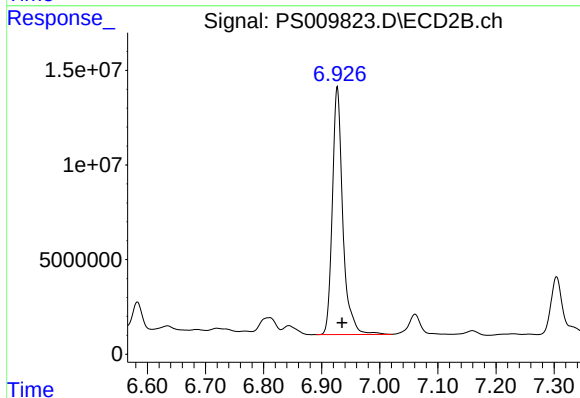


#4 2,4-DCAA

R.T.: 6.927 min
Delta R.T.: -0.008 min
Response: 164557646
Conc: 299.63 ng/ml

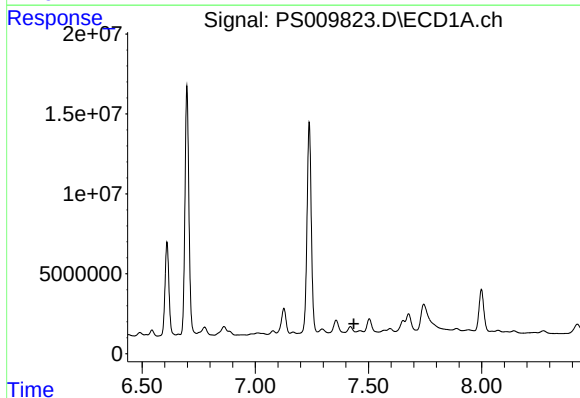


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 7.435 min
Response: 0
Conc: N.D.

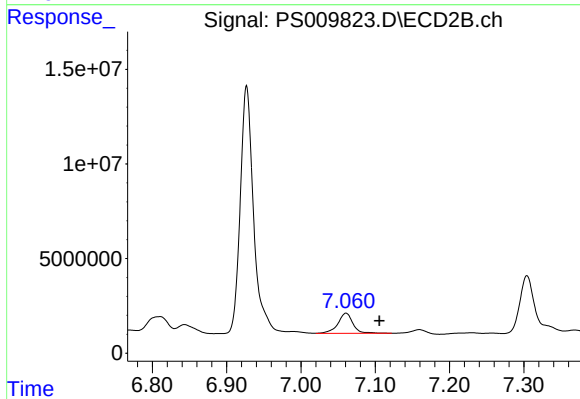


#5 DICAMBA

R.T.: 7.061 min
Delta R.T.: -0.045 min
Response: 14969865
Conc: 6.52 ng/ml

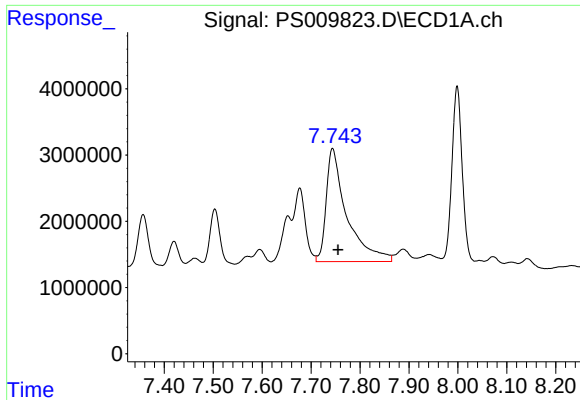


#7 MCPA

R.T.: 7.744 min
Delta R.T.: -0.011 min
Response: 49863270
Conc: 16.37 ug/ml

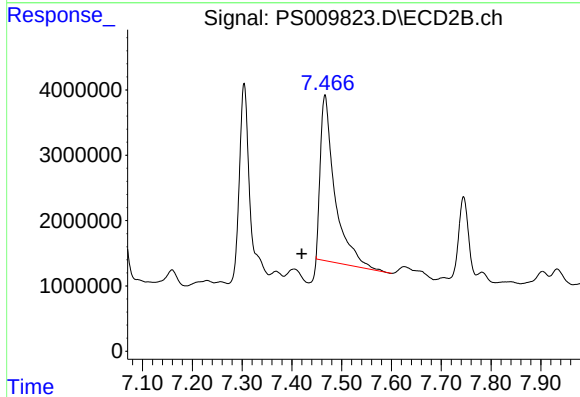


#7 MCPA

R.T.: 7.467 min
Delta R.T.: 0.047 min
Response: 51329439
Conc: 19.02 ug/ml

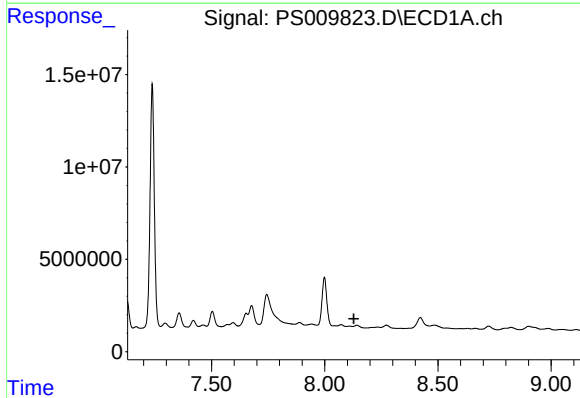


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

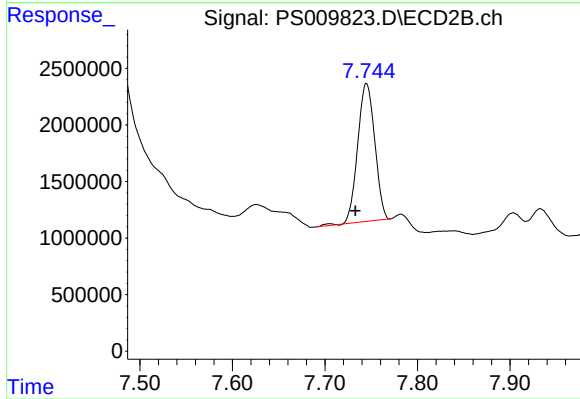


#8 DICHLORPROP

R.T.: 7.745 min
Delta R.T.: 0.012 min
Response: 15697165
Conc: 28.29 ng/ml

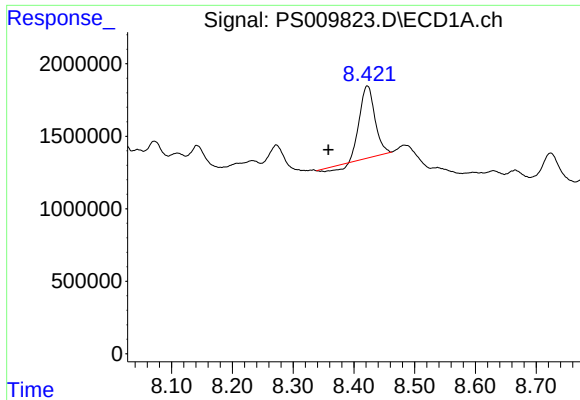


#9 2,4-D

R.T.: 8.422 min
Delta R.T.: 0.064 min
Response: 8258684
Conc: 15.66 ng/ml

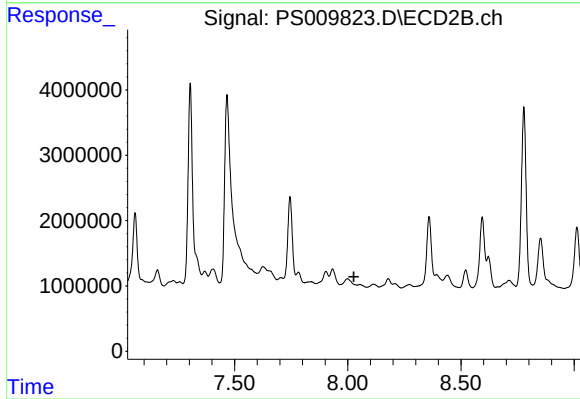


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

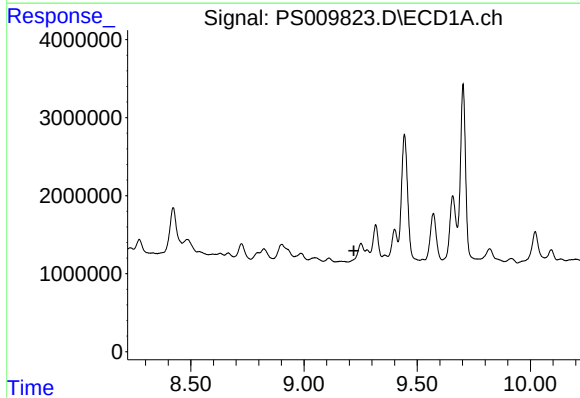


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.221 min
Response: 0
Conc: N.D.

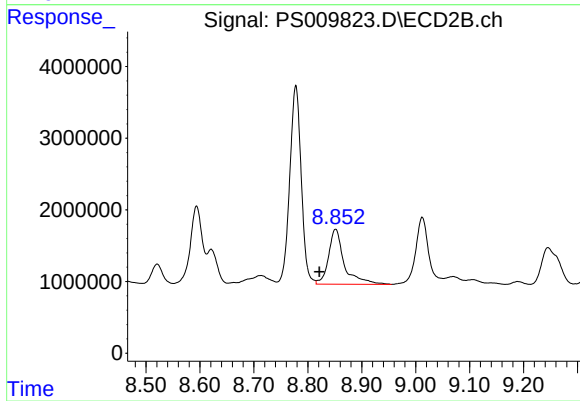


#11 2,4,5-TP (SILVEX)

R.T.: 8.851 min
Delta R.T.: 0.030 min
Response: 15562006
Conc: 5.22 ng/ml

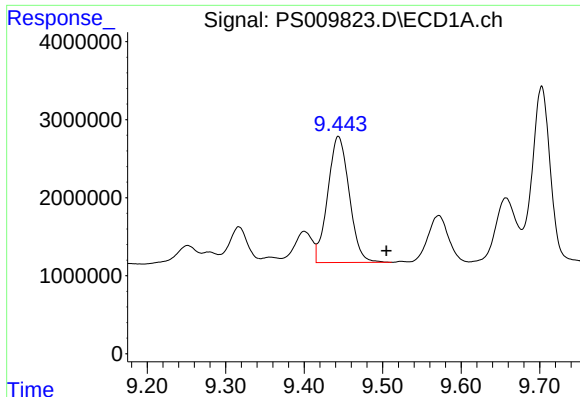


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 30775473
Conc: 12.10 ng/ml

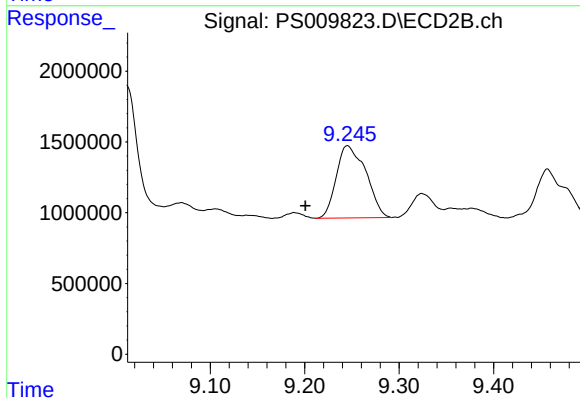


#12 2,4,5-T

R.T.: 9.246 min
Delta R.T.: 0.045 min
Response: 11095644
Conc: 3.76 ng/ml

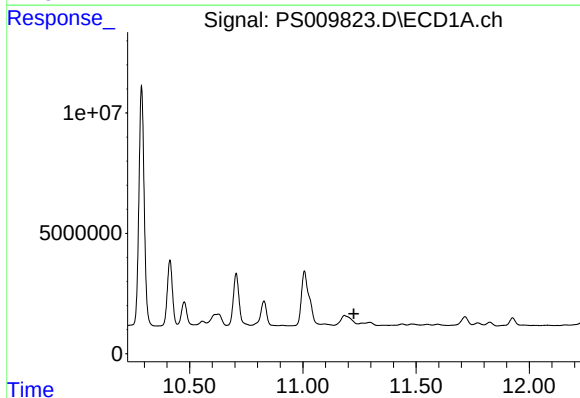


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.225 min
Response: 0
Conc: N.D.

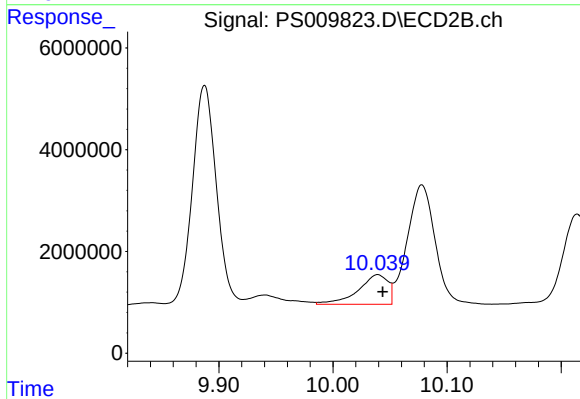


#14 DINOSEB

R.T.: 10.039 min
Delta R.T.: -0.004 min
Response: 10562181
Conc: 4.81 ng/ml

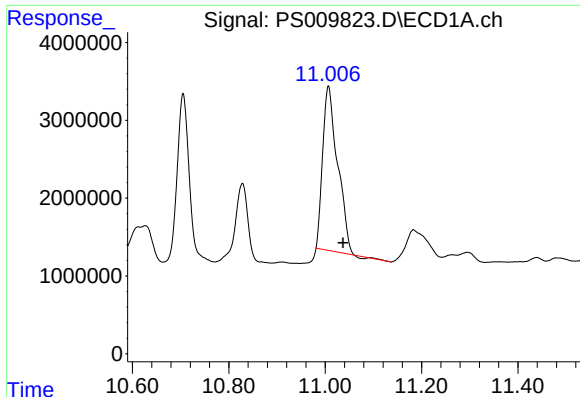


#15 Picloram

R.T.: 11.007 min
Delta R.T.: -0.031 min
Response: 45303478
Conc: 14.93 ng/ml

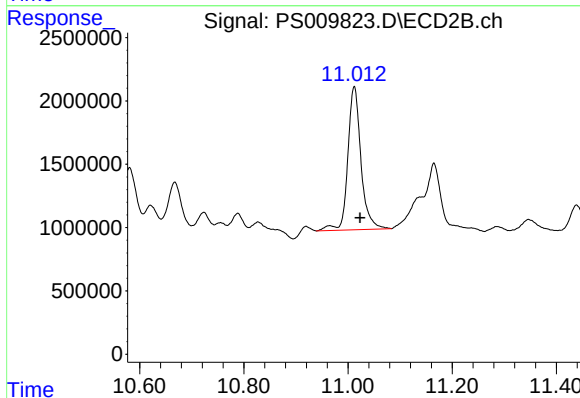


#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.011 min
Response: 19821650
Conc: 4.87 ng/ml

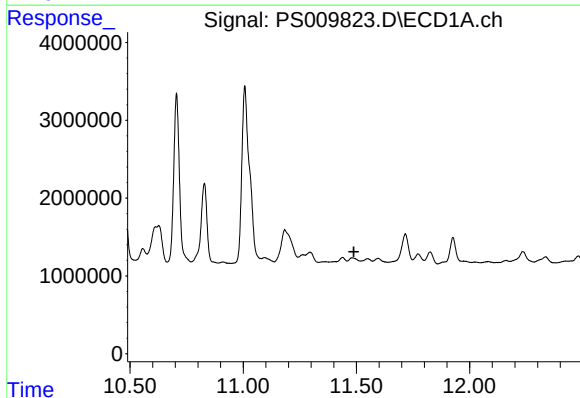

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

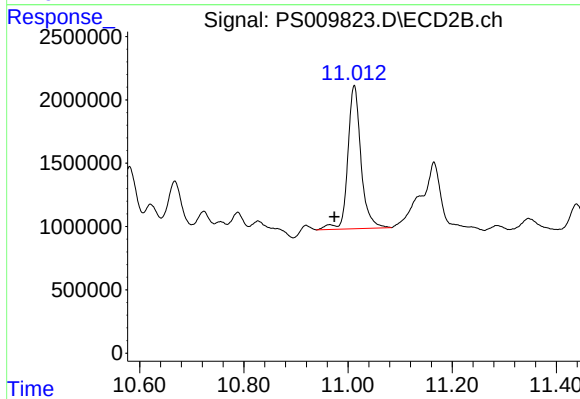

#16 DCPA

R.T.: 11.012 min
Delta R.T.: 0.038 min
Response: 19821650
Conc: 5.12 ng/ml