

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
 Data File : PS009827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 13:21
 Operator : DD\AJ
 Sample : L2252-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 14:37:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.949	7372051	13782694	13.327	25.096 #
Target Compounds							
1) T	Dalapon	0.000	2.586	0	19167614	N.D.	24.344
2) T	3,5-DICHL...	0.000	6.105	0	65699350	N.D.	80.781
5) T	DICAMBA	7.503	7.061	4979707	30677676	2.340	13.364 #
6) T	MCP	7.676	7.153	32255358	4784801	13.108	2.631 #
8) T	DICHLORPROP	0.000	7.745	0	20611871	N.D.	37.150
9) T	2,4-D	8.413	0.000	13986786	0	26.529	N.D. #
10) T	Pentachlo...	0.000	8.519	0	6015177	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.852	0	20274562	N.D.	6.801
12) T	2,4,5-T	9.444	9.261	46659772	8893089	18.342	3.012 #
14) T	DINOSEB	11.185	10.040	11609094	14746973	5.679	6.714
15) T	Picloram	11.007	11.013	51323948	5806332	16.911	1.426 #
16) T	DCPA	0.000	11.013	0	5806332	N.D.	1.499


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
Data File : PS009827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 13:21
Operator : DD\AJ
Sample : L2252-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 14:37:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

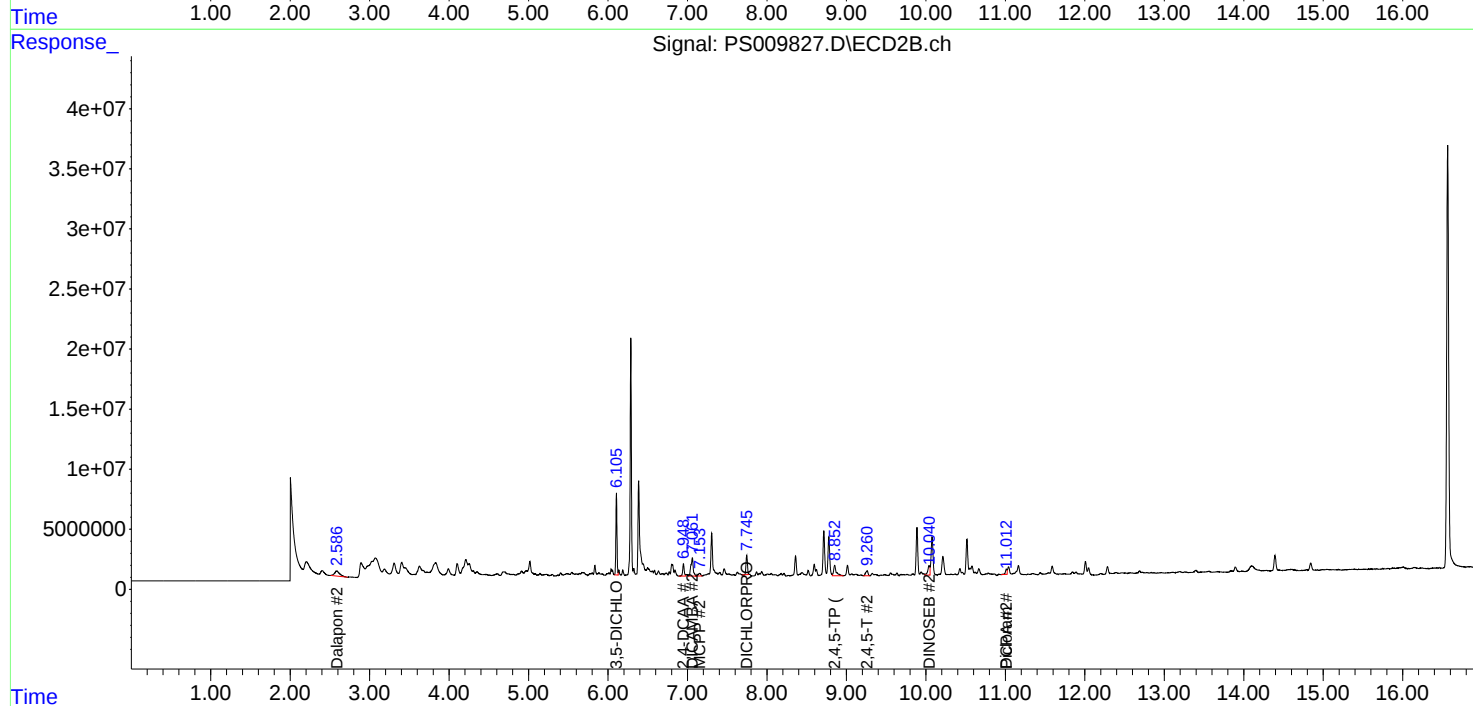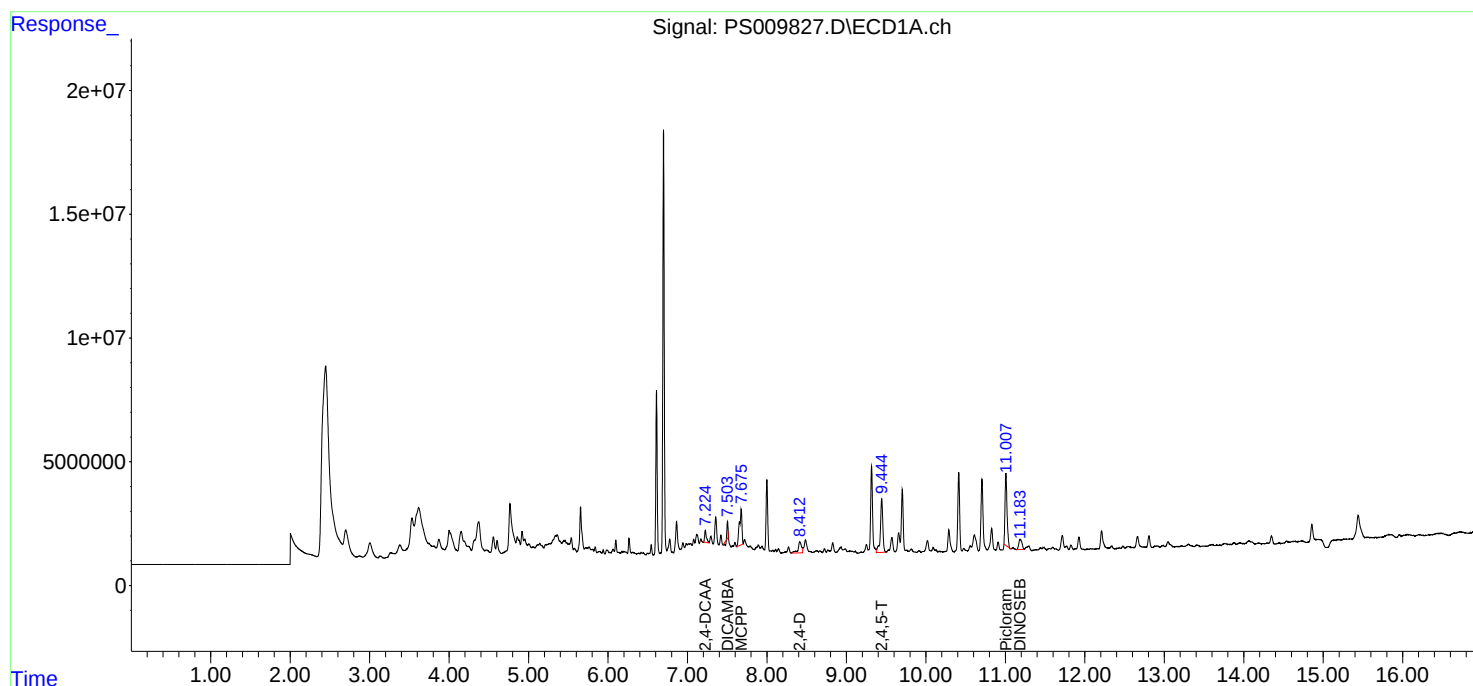

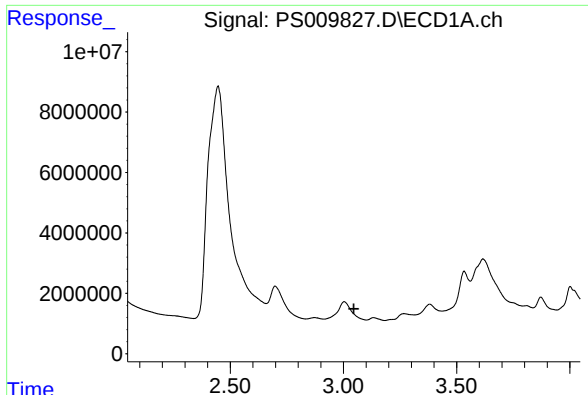


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

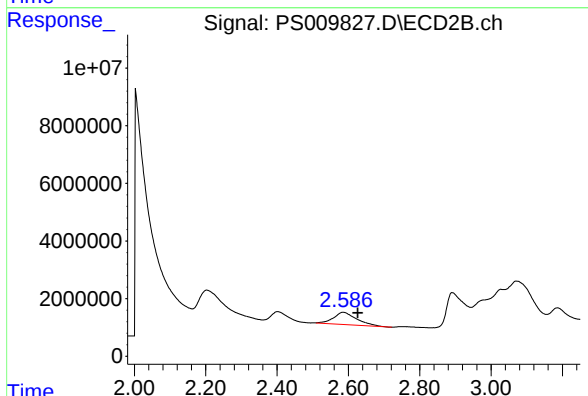


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.041 min
Response: 19167614
Conc: 24.34 ng/ml

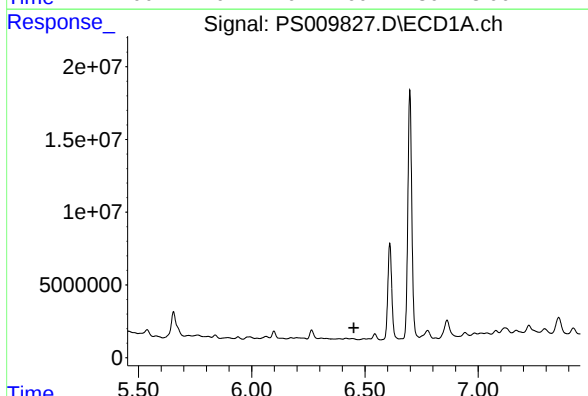


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

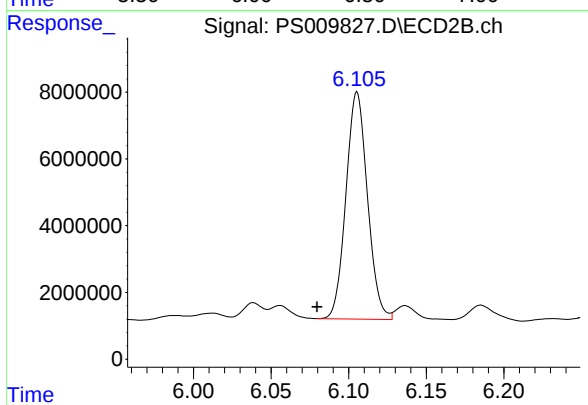


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.105 min
Delta R.T.: 0.026 min
Response: 65699350
Conc: 80.78 ng/ml

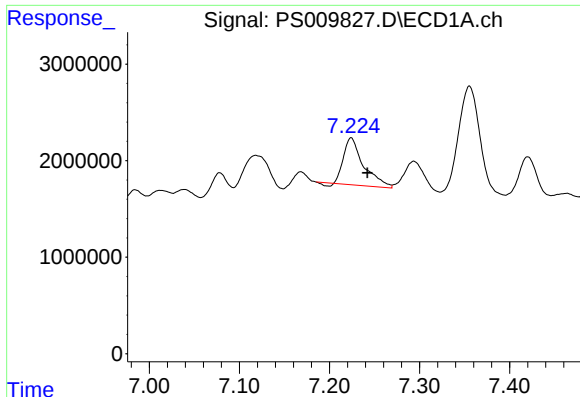


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: -0.018 min
Response: 7372051
Conc: 13.33 ng/ml

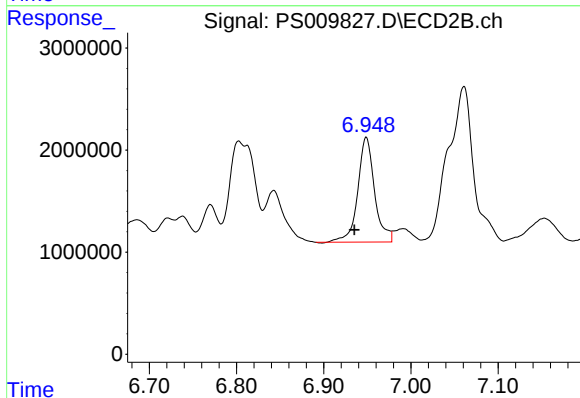


#4 2,4-DCAA

R.T.: 6.949 min
Delta R.T.: 0.014 min
Response: 13782694
Conc: 25.10 ng/ml

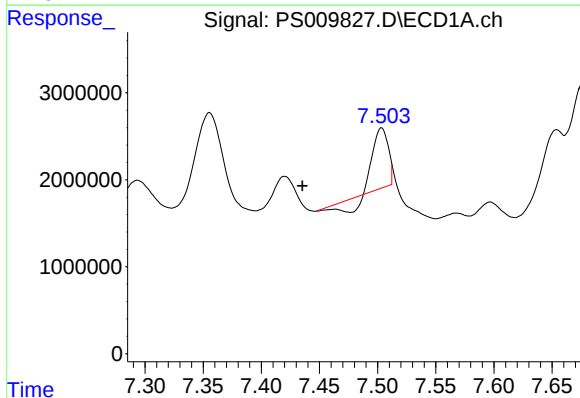


#5 DICAMBA

R.T.: 7.503 min
Delta R.T.: 0.068 min
Response: 4979707
Conc: 2.34 ng/ml

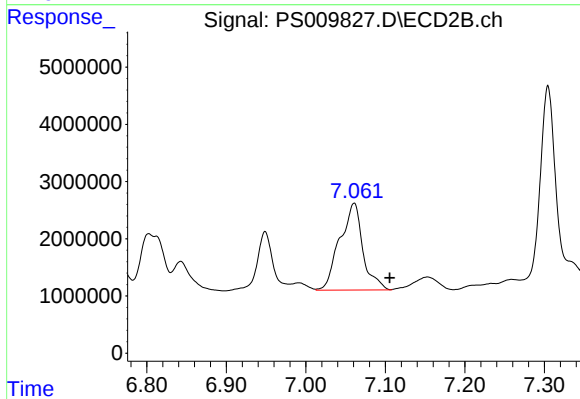


#5 DICAMBA

R.T.: 7.061 min
Delta R.T.: -0.045 min
Response: 30677676
Conc: 13.36 ng/ml

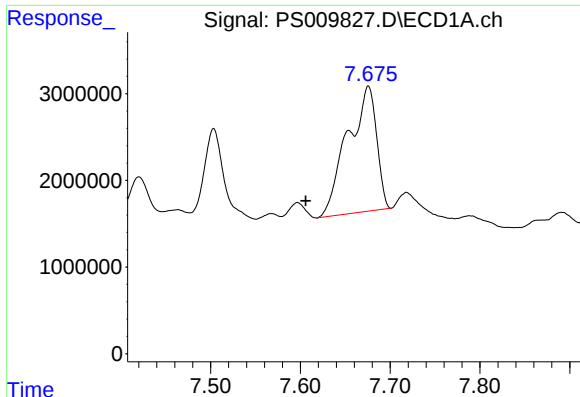


#6 MCP

R.T.: 7.676 min
Delta R.T.: 0.070 min
Response: 32255358
Conc: 13.11 ug/ml

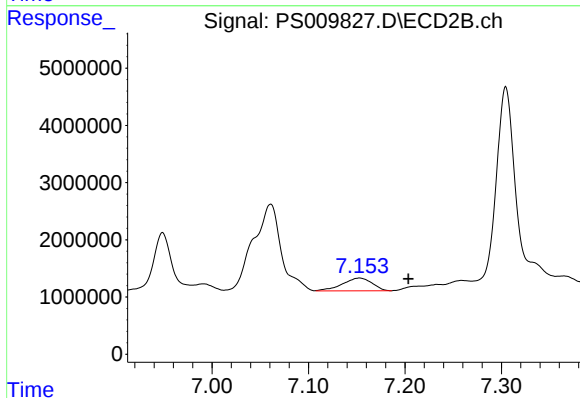


#6 MCP

R.T.: 7.153 min
Delta R.T.: -0.051 min
Response: 4784801
Conc: 2.63 ug/ml

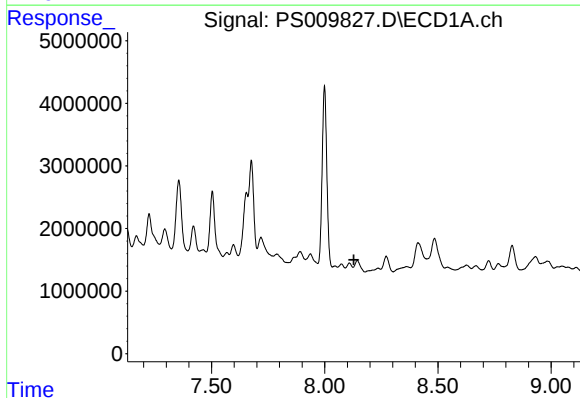


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

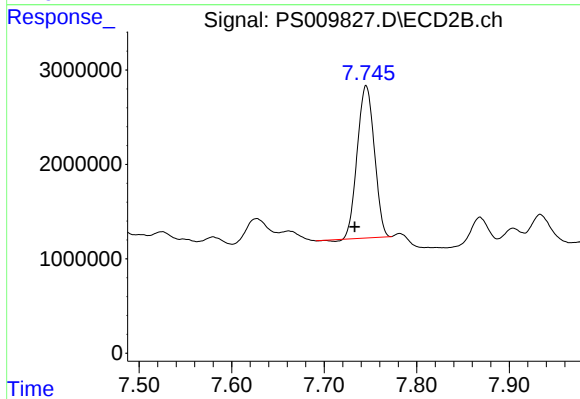


#8 DICHLORPROP

R.T.: 7.745 min
Delta R.T.: 0.012 min
Response: 20611871
Conc: 37.15 ng/ml

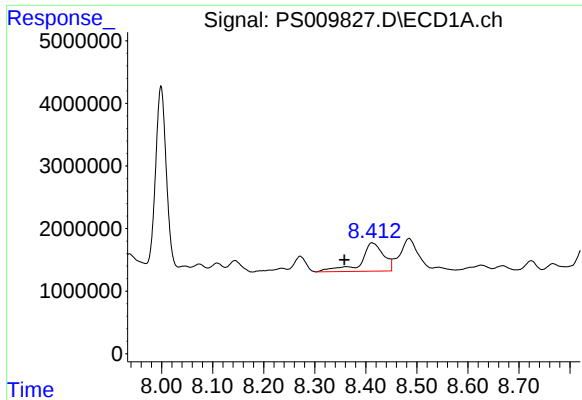


#9 2,4-D

R.T.: 8.413 min
Delta R.T.: 0.055 min
Response: 13986786
Conc: 26.53 ng/ml

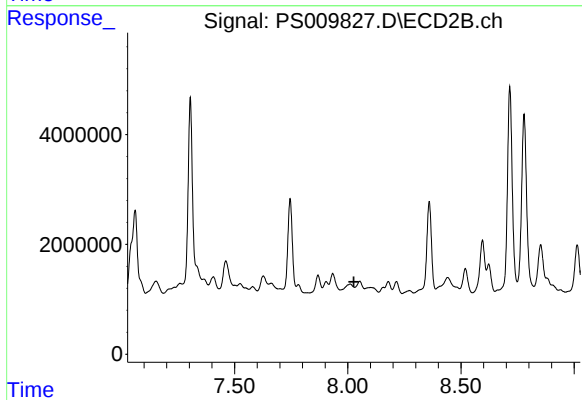


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

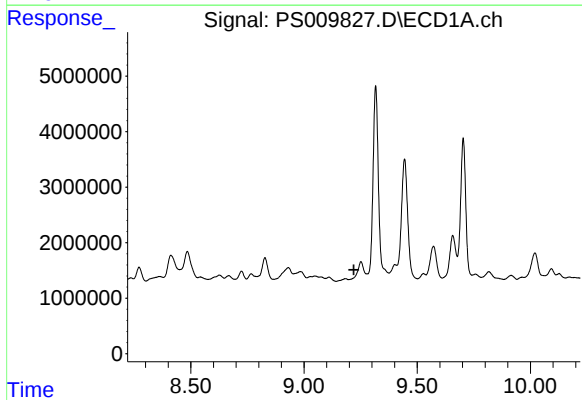


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

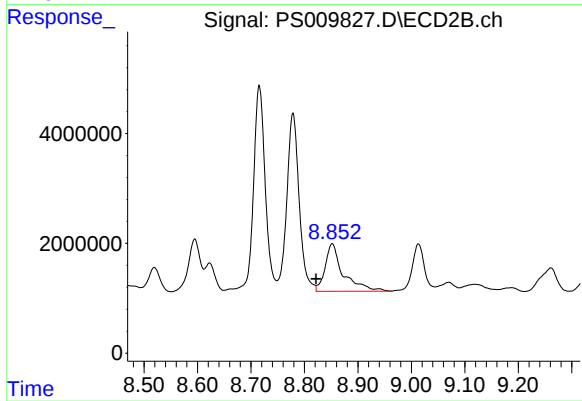


#11 2,4,5-TP (SILVEX)

R.T.: 8.852 min
Delta R.T.: 0.030 min
Response: 20274562
Conc: 6.80 ng/ml

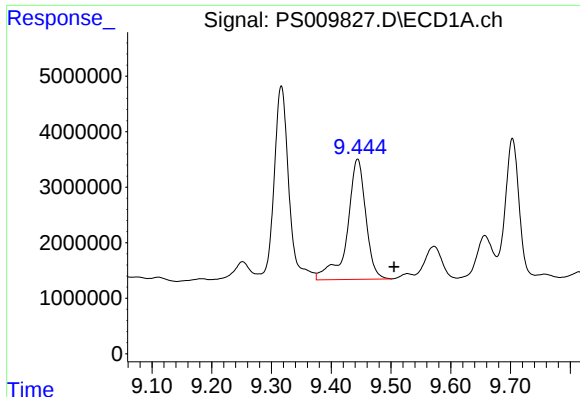


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 46659772
Conc: 18.34 ng/ml

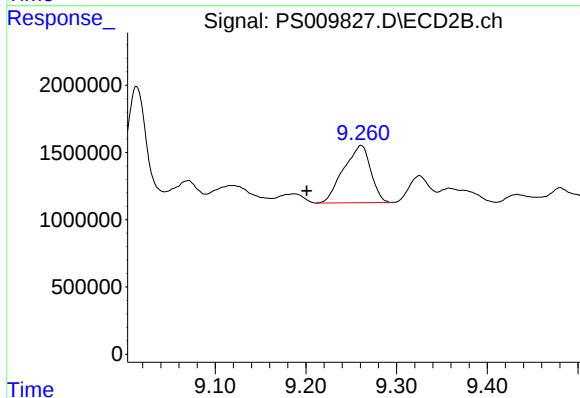


#12 2,4,5-T

R.T.: 9.261 min
Delta R.T.: 0.060 min
Response: 8893089
Conc: 3.01 ng/ml

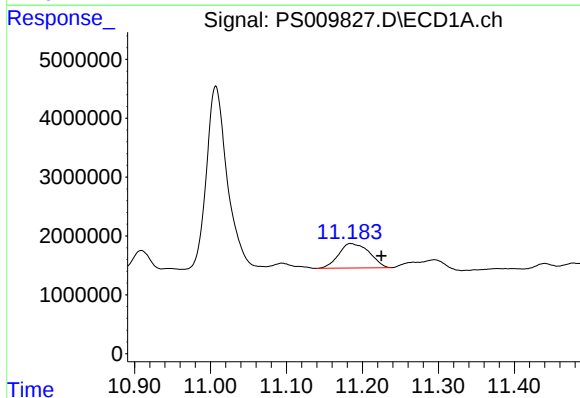


#14 DINOSEB

R.T.: 11.185 min
Delta R.T.: -0.040 min
Response: 11609094
Conc: 5.68 ng/ml

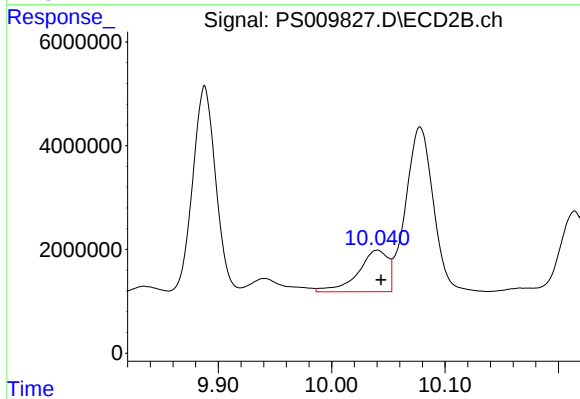


#14 DINOSEB

R.T.: 10.040 min
Delta R.T.: -0.003 min
Response: 14746973
Conc: 6.71 ng/ml

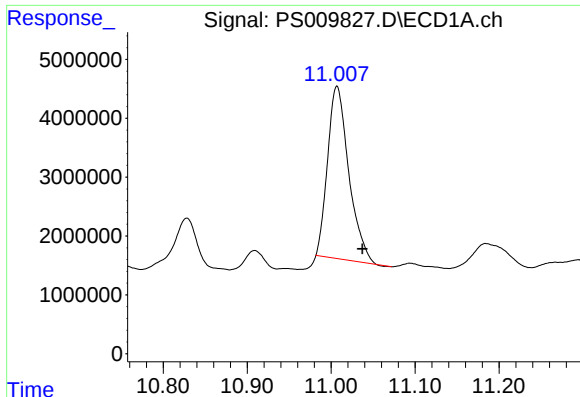


#15 Picloram

R.T.: 11.007 min
Delta R.T.: -0.030 min
Response: 51323948
Conc: 16.91 ng/ml

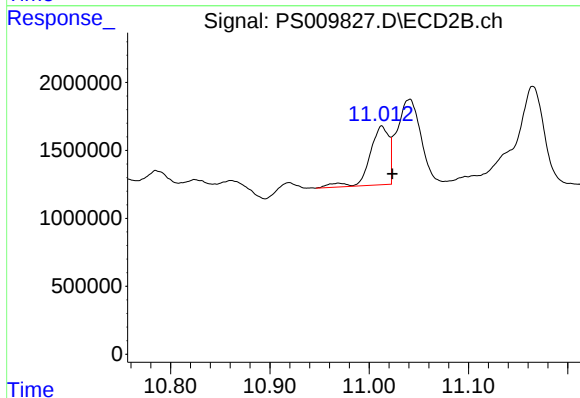


#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.010 min
Response: 5806332
Conc: 1.43 ng/ml

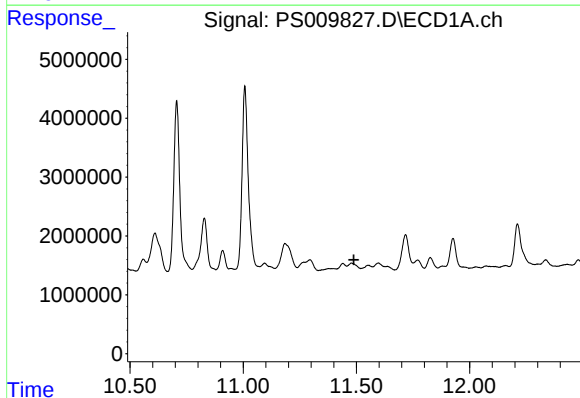

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

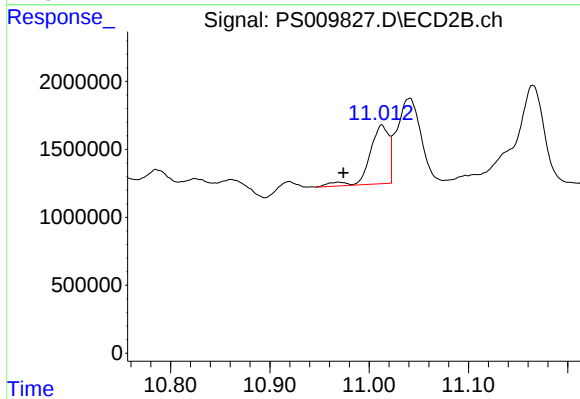

#16 DCPA

R.T.: 11.013 min
Delta R.T.: 0.039 min
Response: 5806332
Conc: 1.50 ng/ml