

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
 Data File : PS009830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 14:29
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:52:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.239	6.927	275.4E6	264.7E6	456.036	534.572
Target Compounds							
8) T	DICHLORPROP	0.000	7.749	0	2426754	N.D.	4.822
12) T	2,4,5-T	0.000	9.189	0	770016	N.D.	<MDL
15) T	Picloram	0.000	11.012	0	4576105	N.D.	1.345
16) T	DCPA	0.000	11.012	0	4576105	N.D.	1.365


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041720\
Data File : PS009830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 14:29
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:52:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

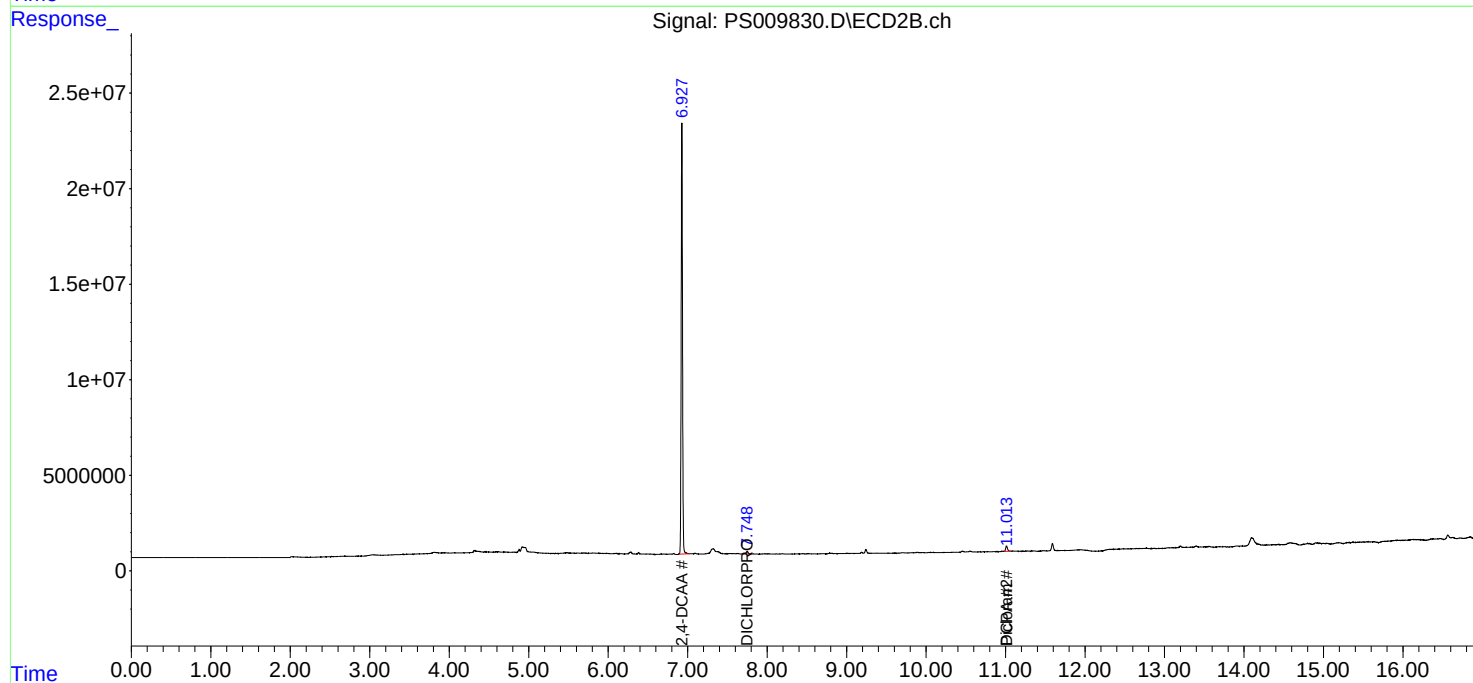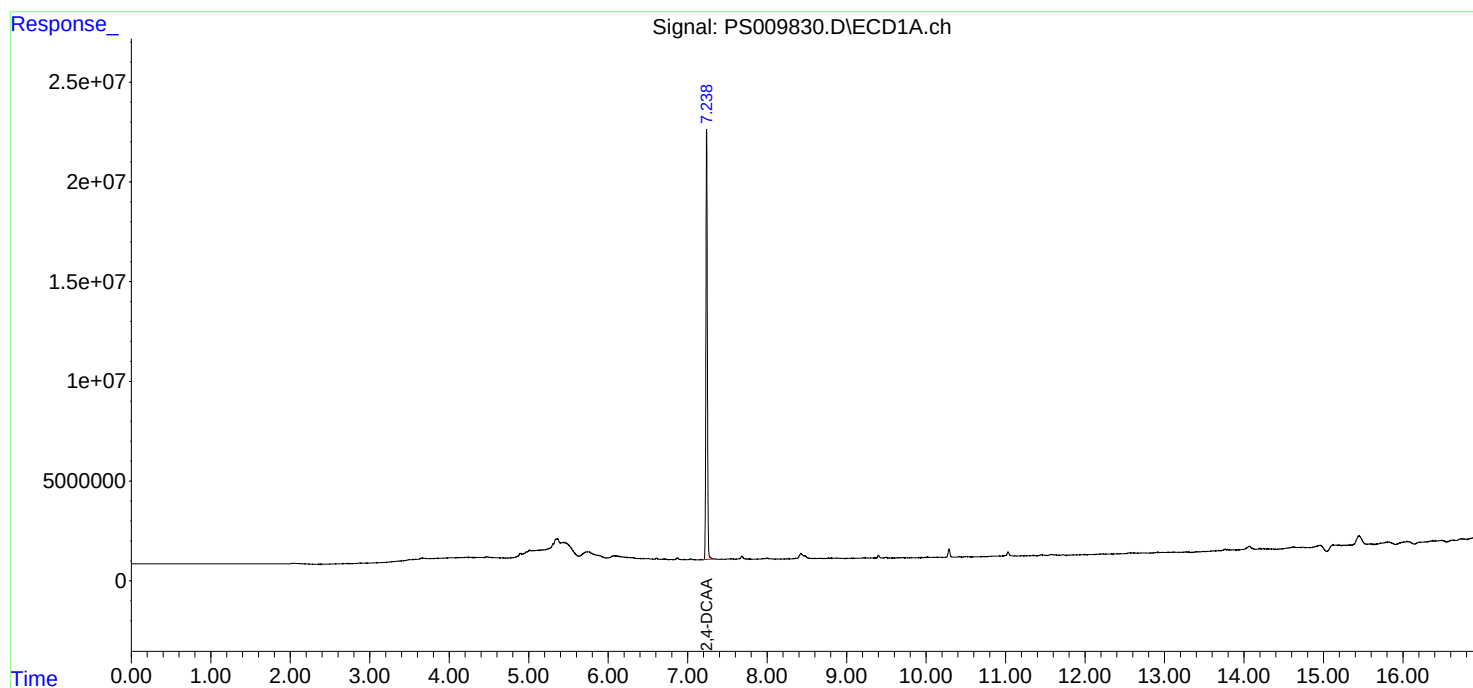

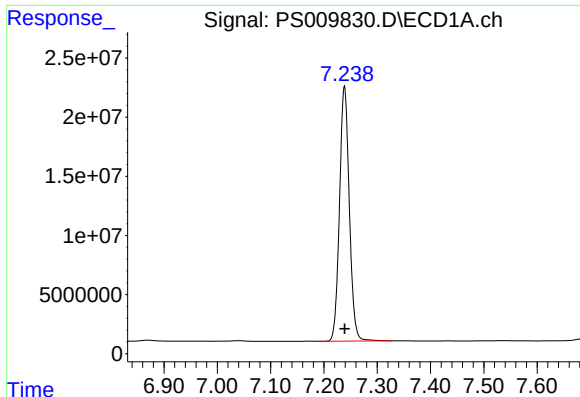


#4 2,4-DCAA

R.T.: 7.239 min
Delta R.T.: 0.000 min
Response: 275361600
Conc: 456.04 ng/ml

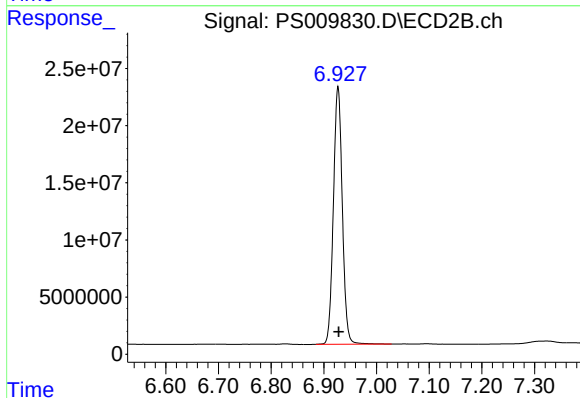


#4 2,4-DCAA

R.T.: 6.927 min
Delta R.T.: -0.001 min
Response: 264746918
Conc: 534.57 ng/ml

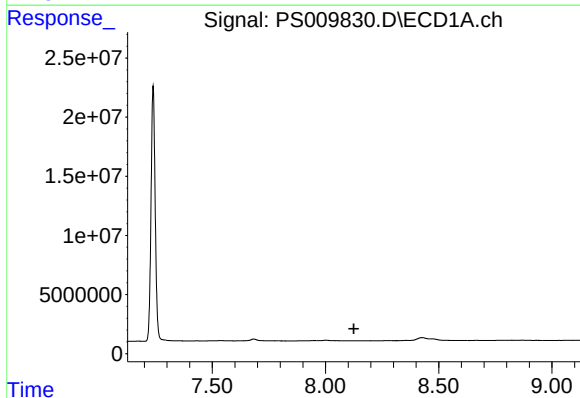


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

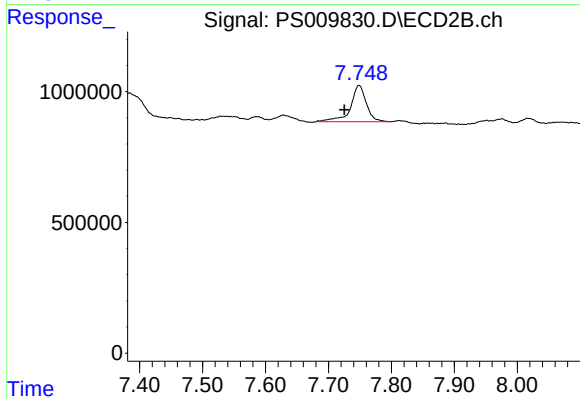


#8 DICHLORPROP

R.T.: 7.749 min
Delta R.T.: 0.023 min
Response: 2426754
Conc: 4.82 ng/ml

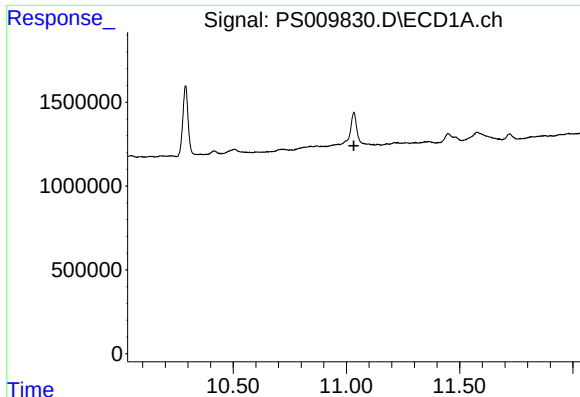


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.033 min
Response: 0
Conc: N.D.

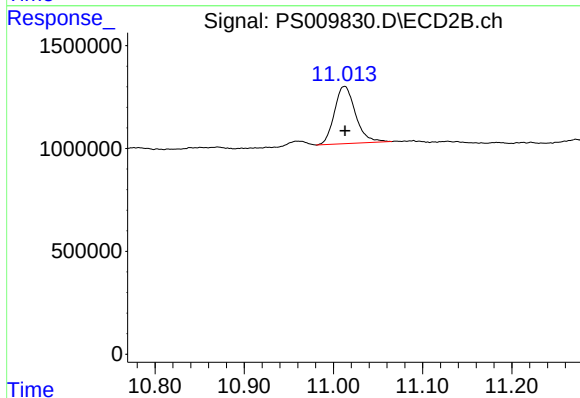


#15 Picloram

R.T.: 11.012 min
Delta R.T.: 0.000 min
Response: 4576105
Conc: 1.35 ng/ml

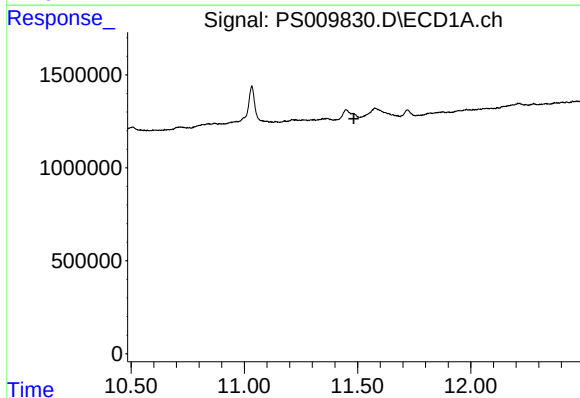

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.484 min
Response: 0
Conc: N.D.

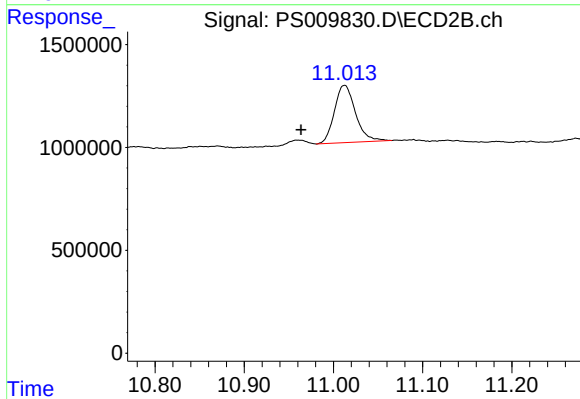

#16 DCPA

R.T.: 11.012 min
Delta R.T.: 0.049 min
Response: 4576105
Conc: 1.36 ng/ml