

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041724\
 Data File : PS026459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2024 21:22
 Operator : AR\AJ
 Sample : P2127-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SP-2-FRONT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/19/2024
 Supervised By :Ankita Jodhani 04/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 03:42:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041724.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 17 17:31:42 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.053	7.536	777.6E6	180.6E6	286.742m	227.647m
Target Compounds							
13) T	2,4-DB	9.886	10.604	178.5E6	59358107	95.701	141.444m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041724\
Data File : PS026459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2024 21:22
Operator : AR\AJ
Sample : P2127-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SP-2-FRONT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/19/2024
Supervised By : Ankita Jodhani 04/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 03:42:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041724.M
Quant Title : 8080.M
QLast Update : Wed Apr 17 17:31:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

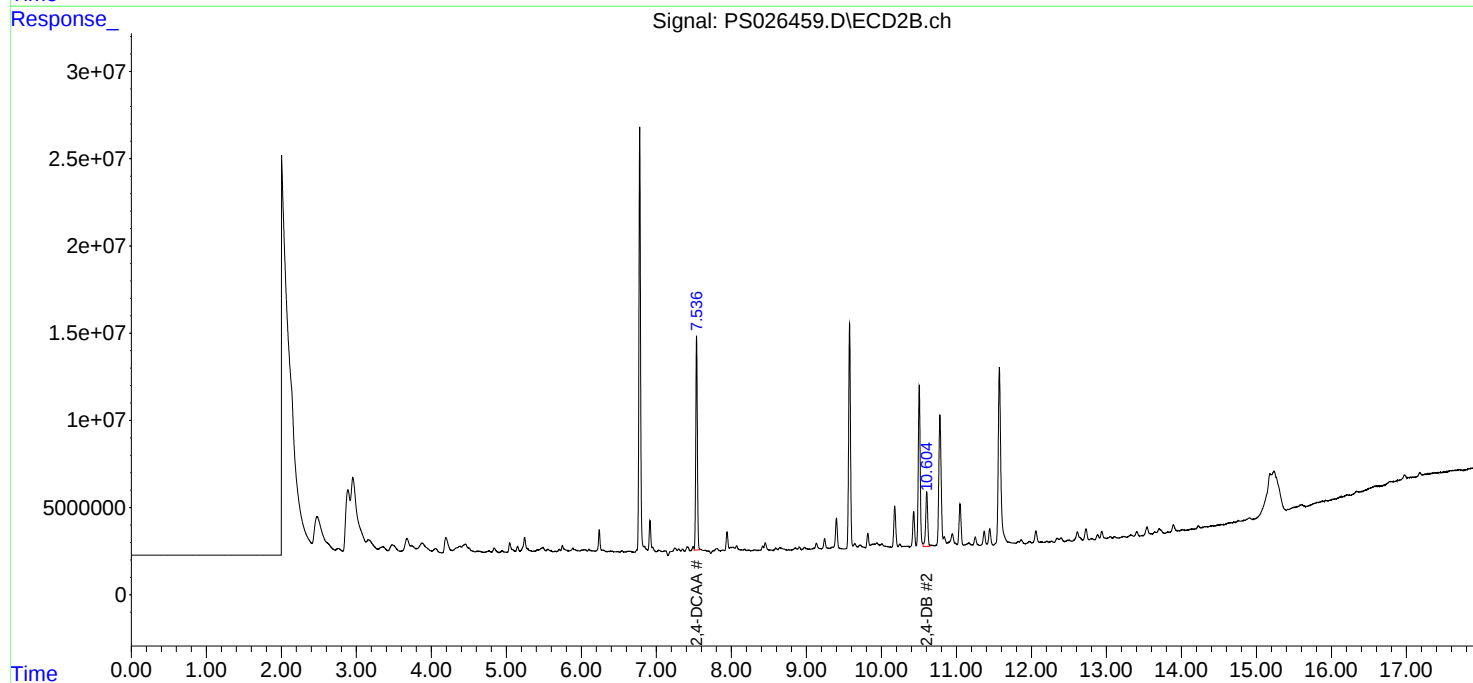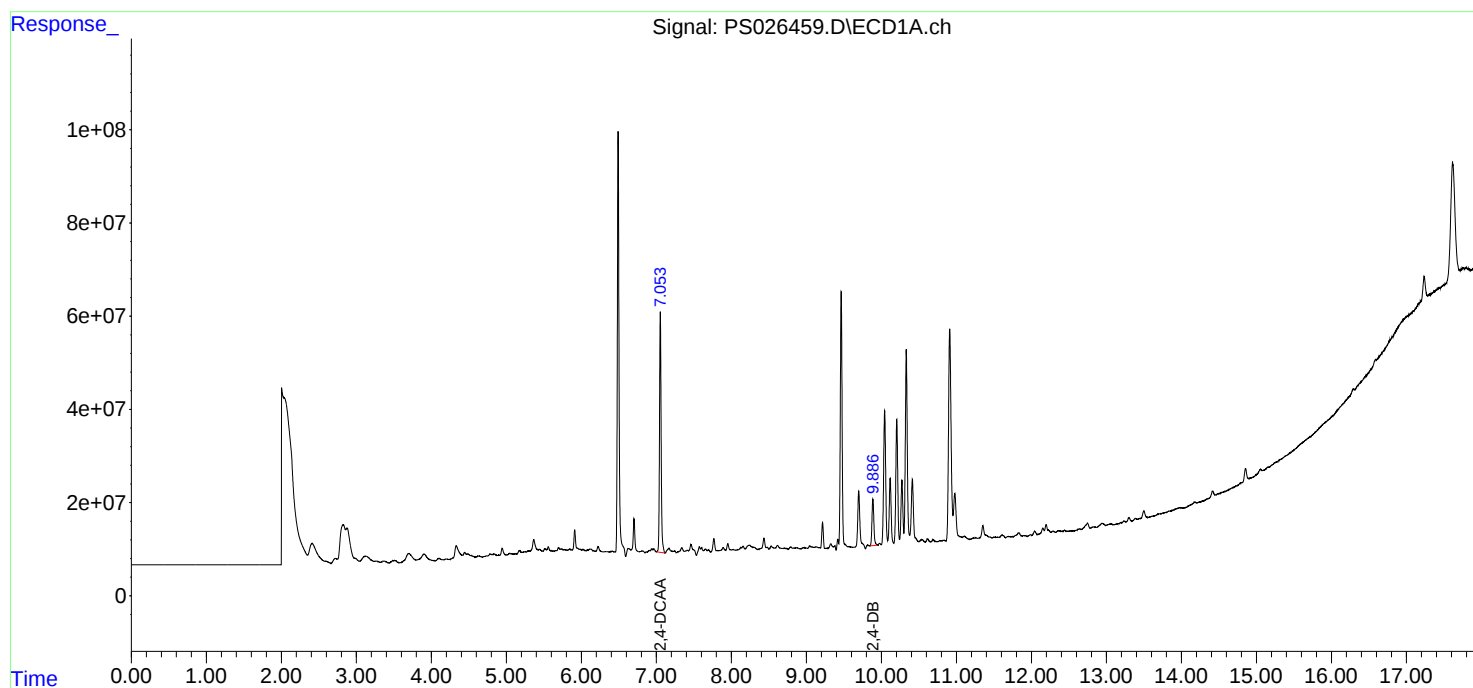

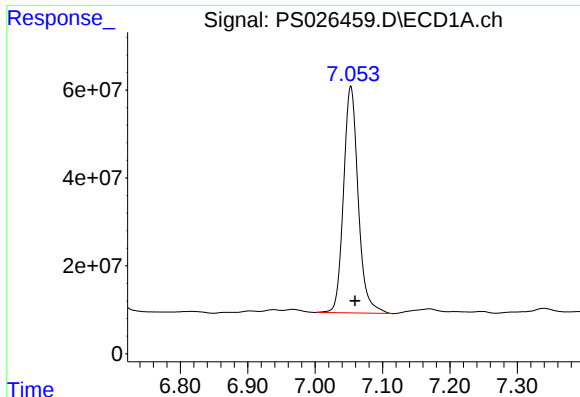


#4 2,4-DCAA

R.T.: 7.053 min
Delta R.T.: -0.007 min
Response: 777594346
Conc: 286.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
SP-2-FRONT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/19/2024
Supervised By :Ankita Jodhani 04/19/2024

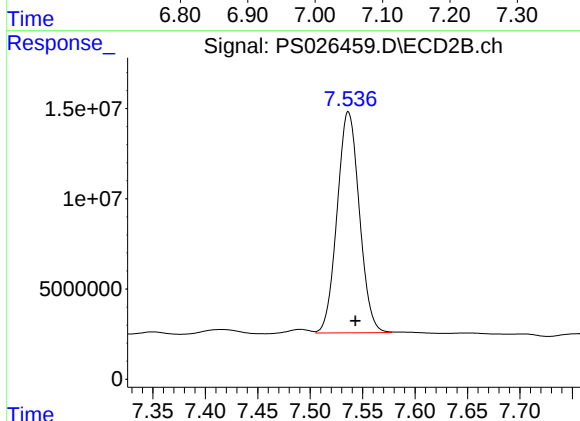


#4 2,4-DCAA

R.T.: 7.536 min
Delta R.T.: -0.007 min
Response: 180630235
Conc: 227.65 ng/ml m

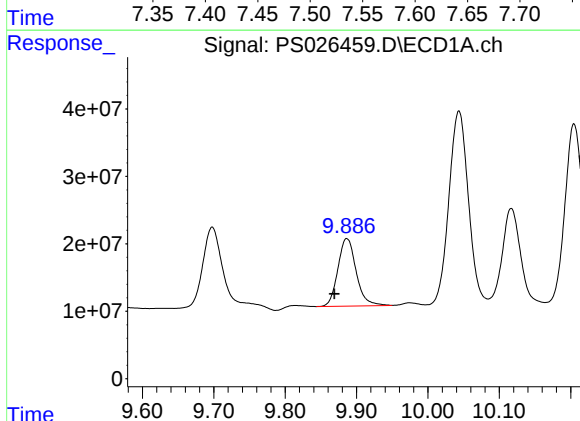

#13 2,4-DB

R.T.: 9.886 min
Delta R.T.: 0.017 min
Response: 178484296
Conc: 95.70 ng/ml

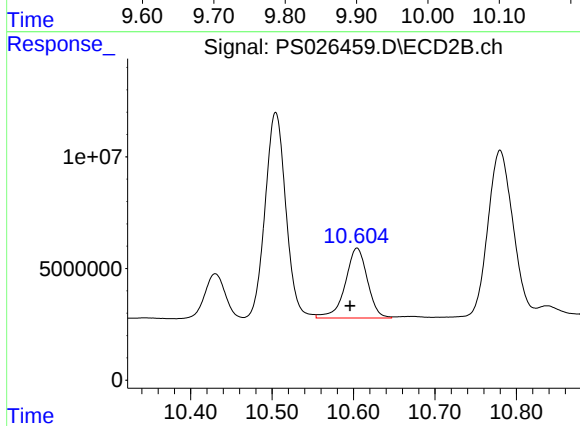

#13 2,4-DB

R.T.: 10.604 min
Delta R.T.: 0.008 min
Response: 59358107
Conc: 141.44 ng/ml m