

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041724\
 Data File : PS026460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2024 21:46
 Operator : AR\AJ
 Sample : P2127-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SP-2-BACK

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/19/2024
 Supervised By :Ankita Jodhani 04/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 03:43:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041724.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 17 17:31:42 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.052	7.537	771.9E6	179.3E6	284.625m	225.971m
Target Compounds							
13) T	2,4-DB	9.887	10.605	177.7E6	49700660	95.284	118.431

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041724\
Data File : PS026460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2024 21:46
Operator : AR\AJ
Sample : P2127-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SP-2-BACK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/19/2024
Supervised By : Ankita Jodhani 04/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 03:43:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041724.M
Quant Title : 8080.M
QLast Update : Wed Apr 17 17:31:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

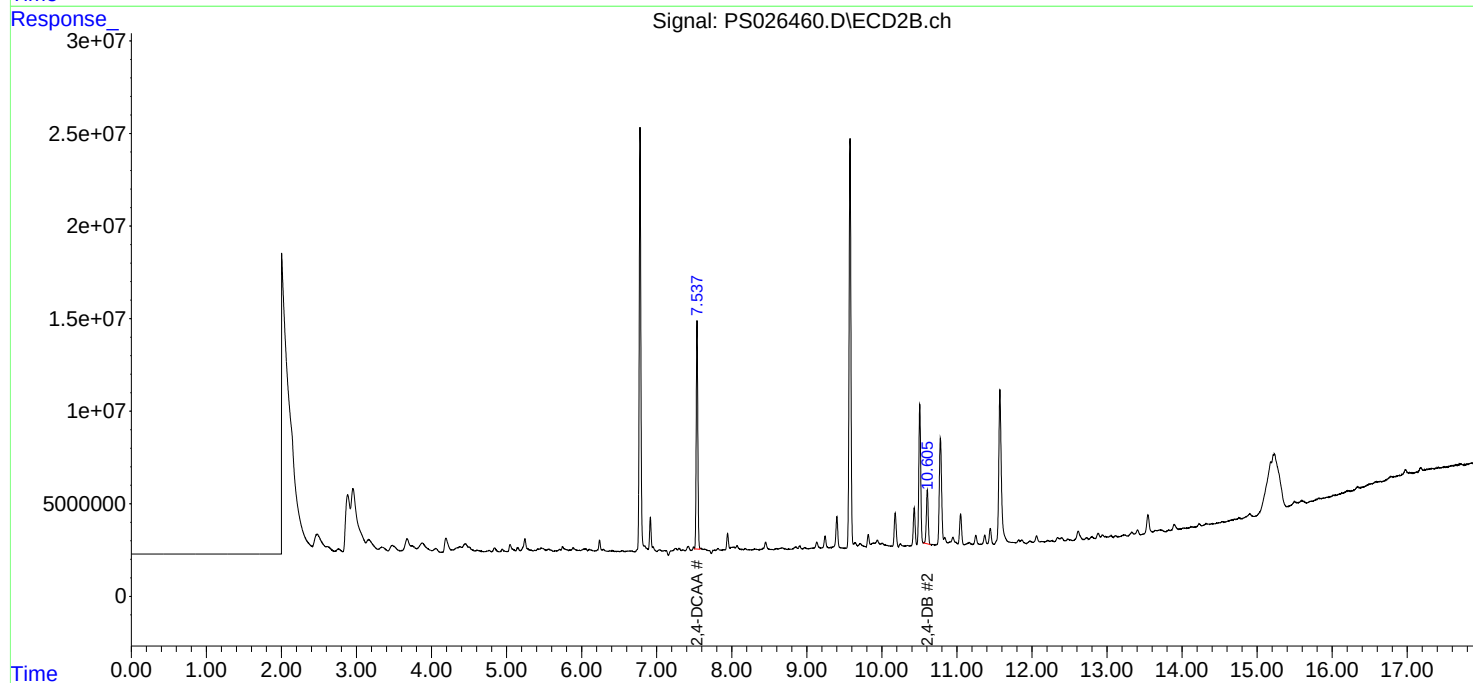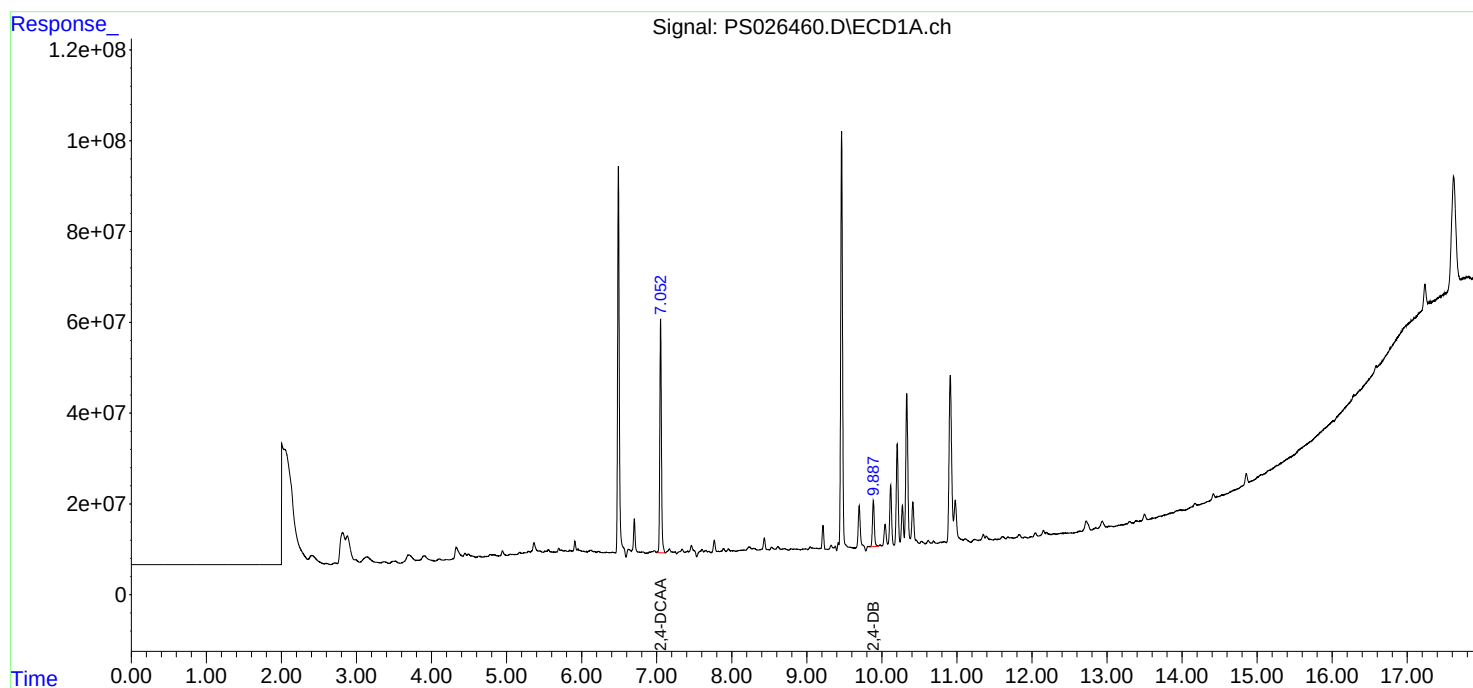

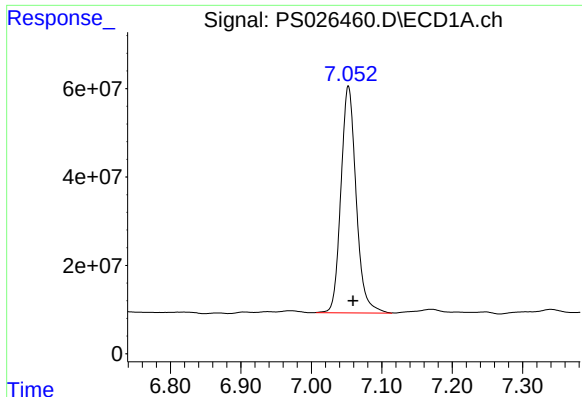


#4 2,4-DCAA

R.T.: 7.052 min
Delta R.T.: -0.007 min
Response: 771852575
Conc: 284.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
SP-2-BACK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/19/2024
Supervised By :Ankita Jodhani 04/19/2024

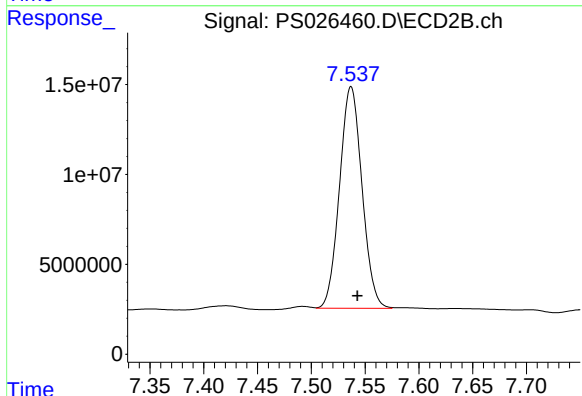


#4 2,4-DCAA

R.T.: 7.537 min
Delta R.T.: -0.007 min
Response: 179300889
Conc: 225.97 ng/ml m

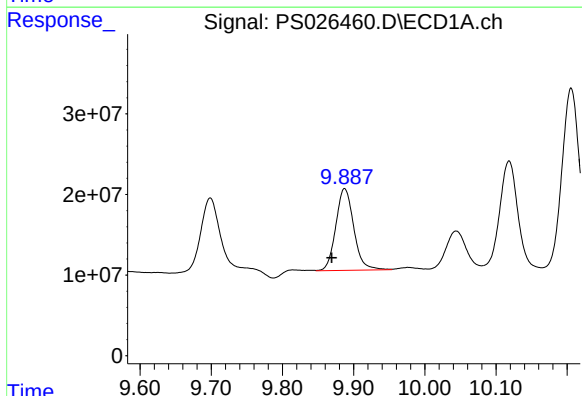

#13 2,4-DB

R.T.: 9.887 min
Delta R.T.: 0.018 min
Response: 177707355
Conc: 95.28 ng/ml

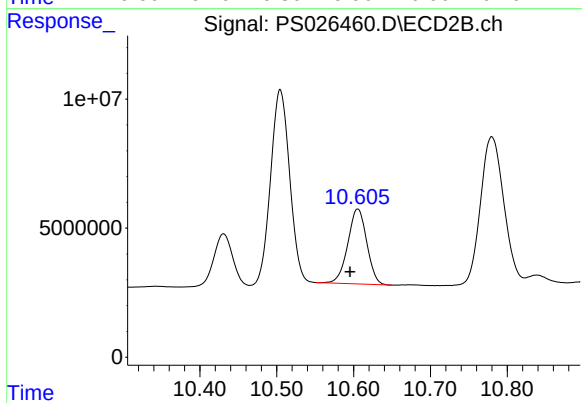

#13 2,4-DB

R.T.: 10.605 min
Delta R.T.: 0.010 min
Response: 49700660
Conc: 118.43 ng/ml