

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041819\
 Data File : PS004128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2019 07:42
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 01:42:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	11.180	10.813	16560522	2829127	34.130	6.160	#
Target Compounds								
3) T	4-Nitroph...	10.848	0.000	5513811	0	21.829	N.D.	#
8) T	DICHLORPROP	12.775	0.000	3817788	0	7.886	N.D.	#
13) T	2,4-DB	15.448	0.000	1151779	0	3.698	N.D.	#
15) T	Picloram	0.000	16.637	0	7766838	N.D.	2.269	
16) T	DCPA	17.328	16.558	3993705	2526647	1.109	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041819\
Data File : PS004128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2019 07:42
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 01:42:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

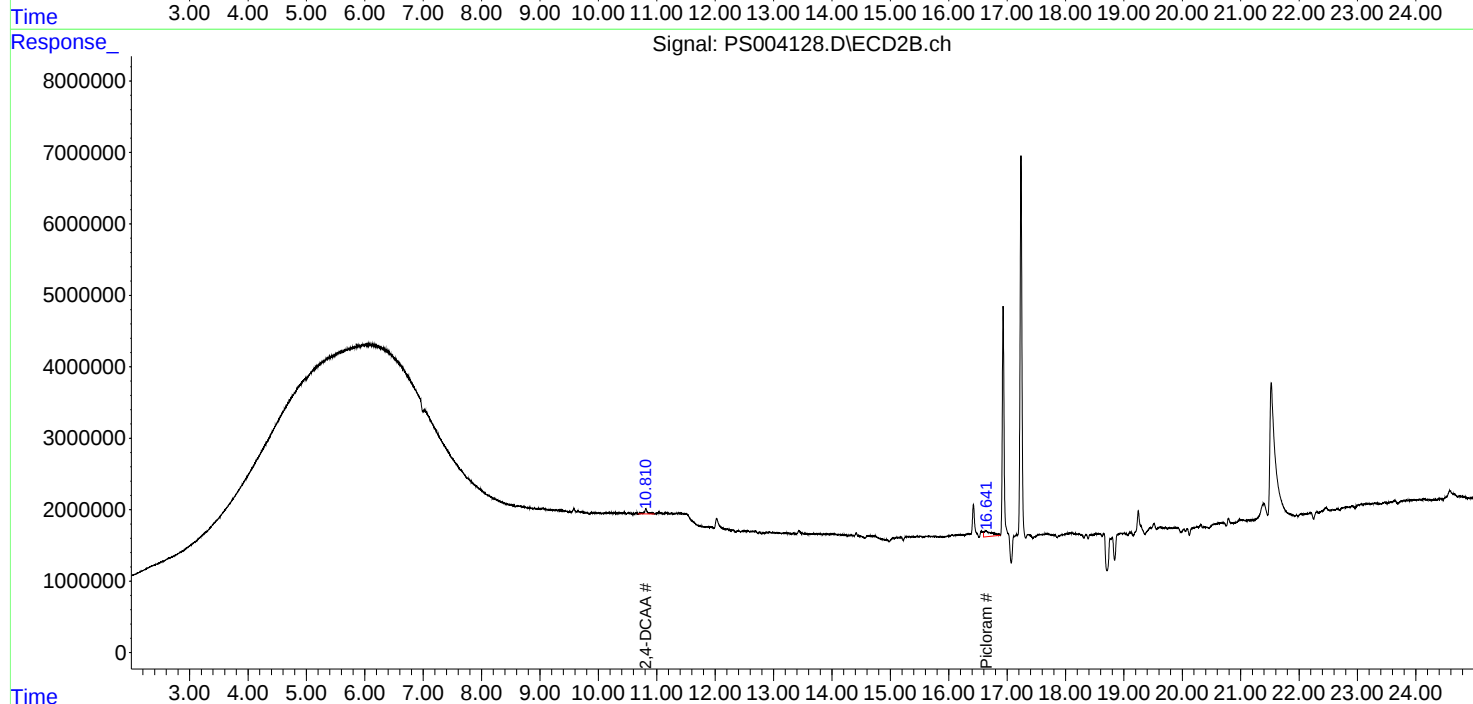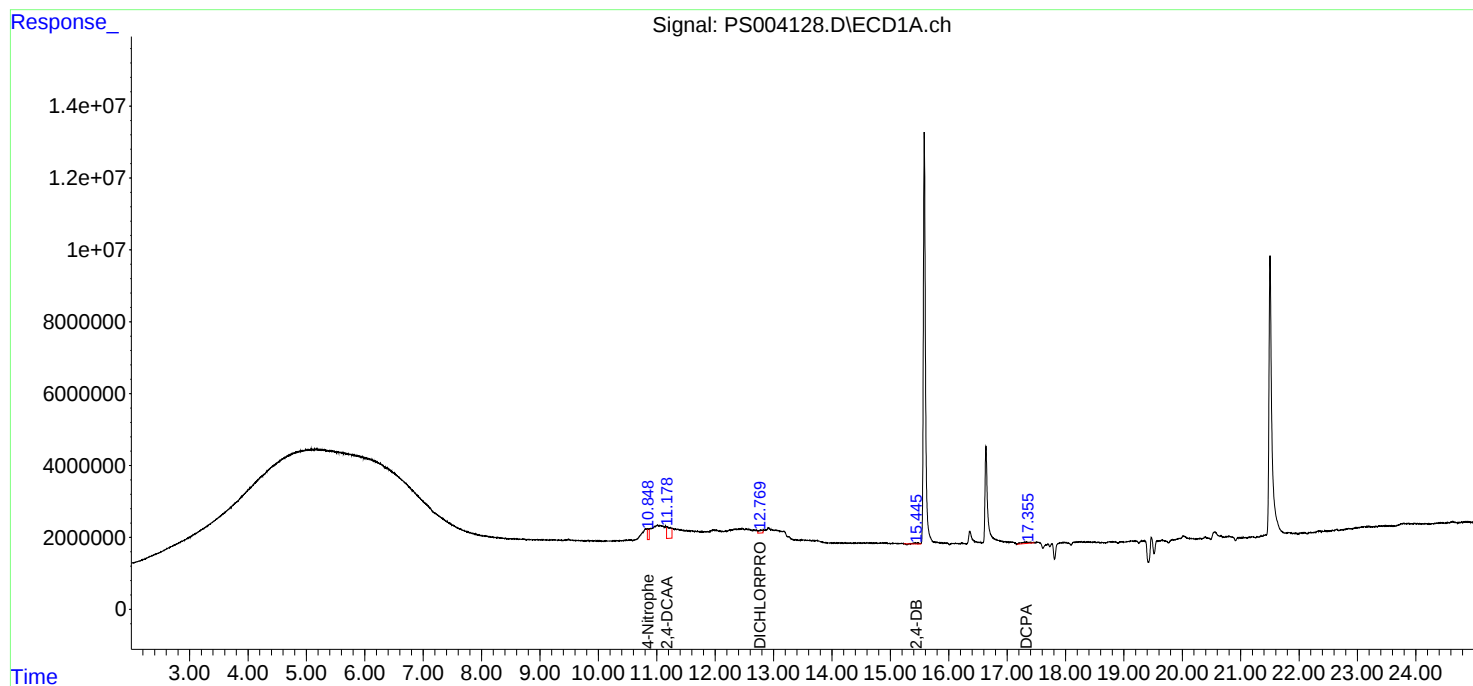


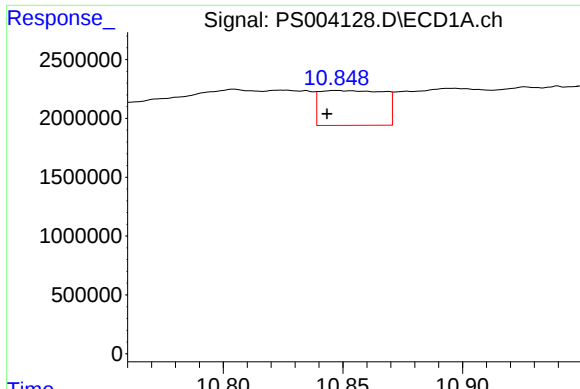

#3 4-Nitrophenol


R.T.: 10.848 min
Delta R.T.: 0.005 min
Response: 5513811
Conc: 21.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

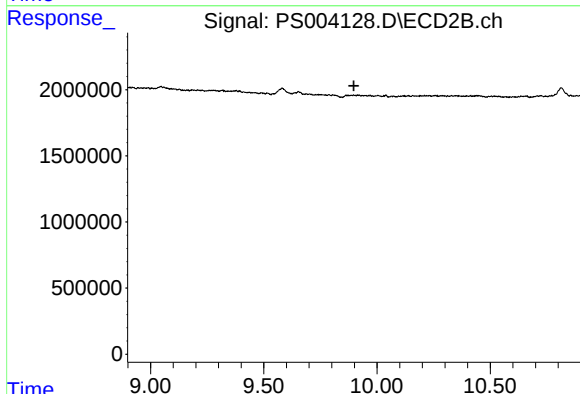


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.898 min
Response: 0
Conc: N.D.

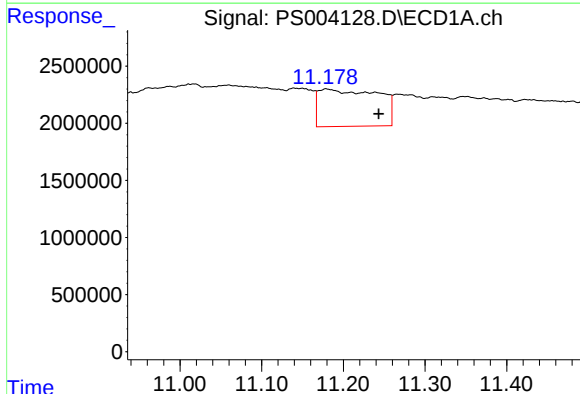


#4 2,4-DCAA

R.T.: 11.180 min
Delta R.T.: -0.064 min
Response: 16560522
Conc: 34.13 ng/ml

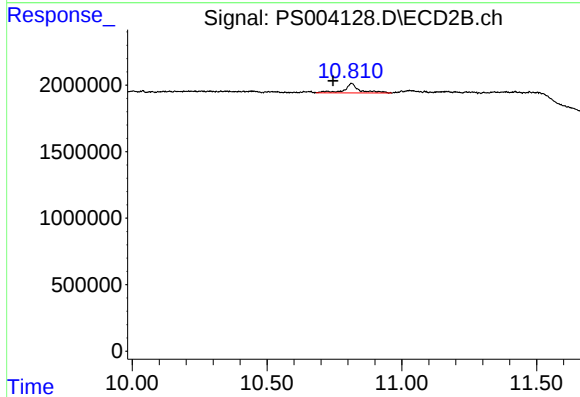

#4 2,4-DCAA


R.T.: 10.813 min
Delta R.T.: 0.068 min
Response: 2829127
Conc: 6.16 ng/ml

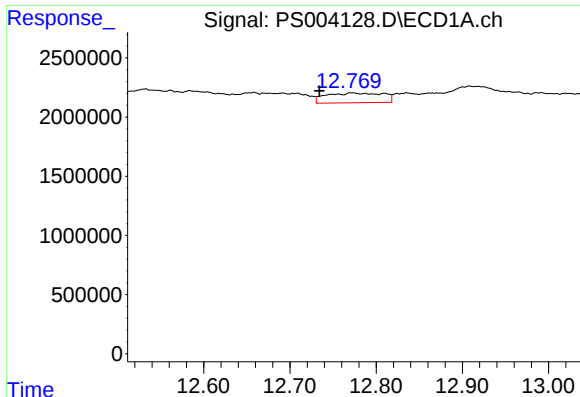

#8 DICHLORPROP


R.T.: 12.775 min
Delta R.T.: 0.040 min
Response: 3817788
Conc: 7.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

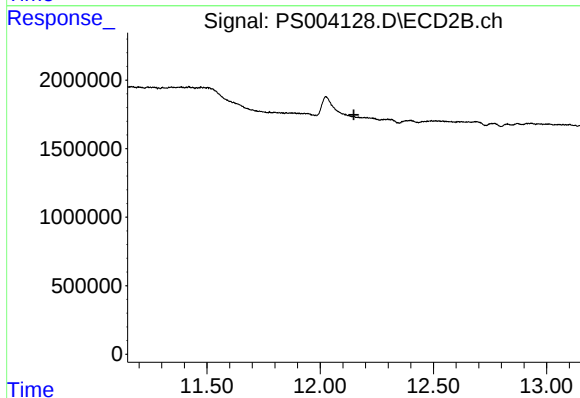


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.149 min
Response: 0
Conc: N.D.

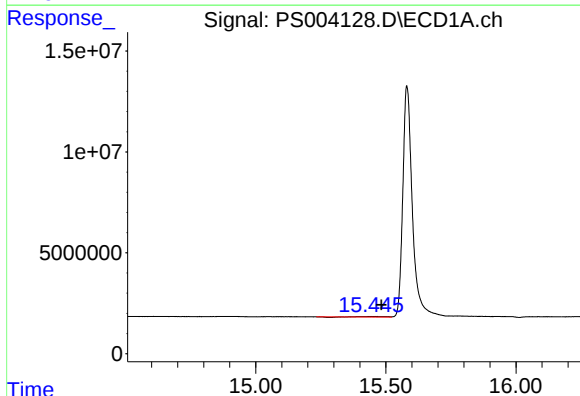


#13 2,4-DB

R.T.: 15.448 min
Delta R.T.: -0.036 min
Response: 1151779
Conc: 3.70 ng/ml

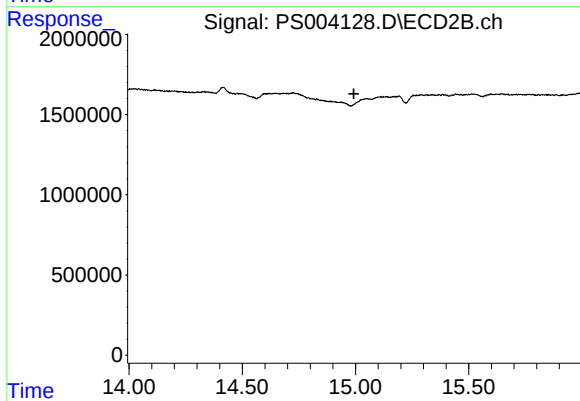

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 14.993 min
Response: 0
Conc: N.D.

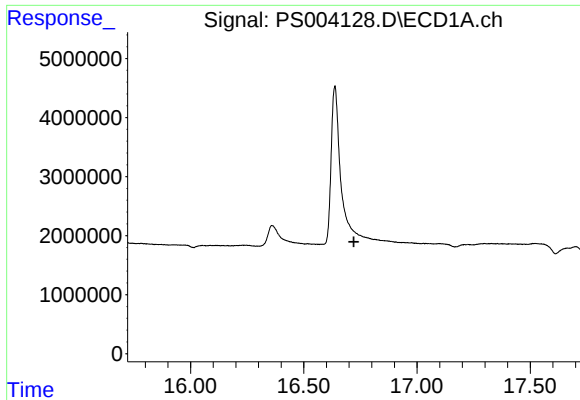

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.721 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

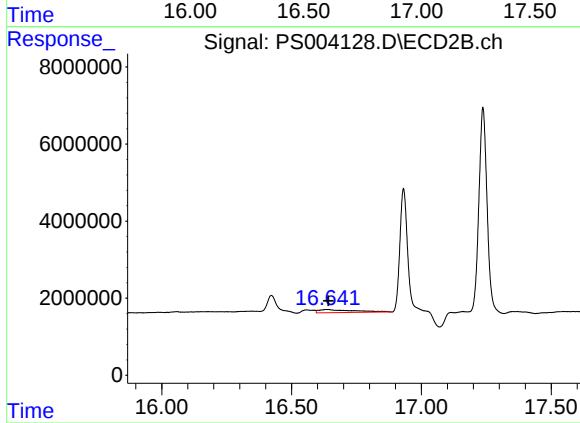


#15 Picloram

R.T.: 16.637 min
Delta R.T.: -0.005 min
Response: 7766838
Conc: 2.27 ng/ml

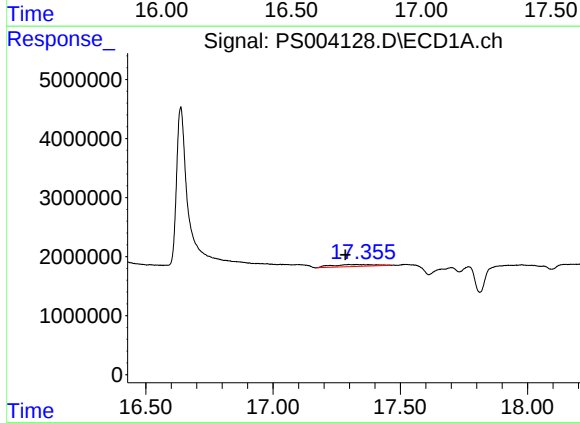

#16 DCPA

R.T.: 17.328 min
Delta R.T.: 0.044 min
Response: 3993705
Conc: 1.11 ng/ml

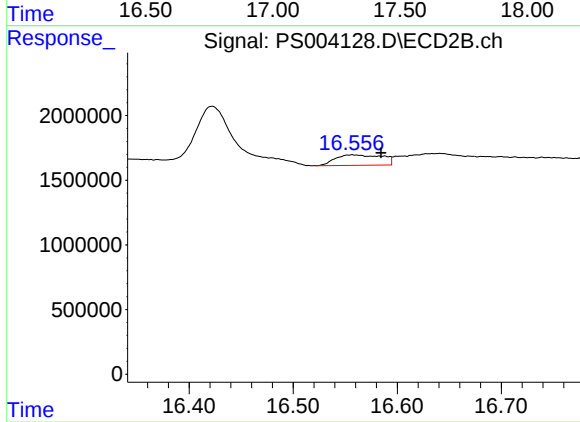

#16 DCPA

R.T.: 16.558 min
Delta R.T.: -0.026 min
Response: 2526647
Conc: N.D.