

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041819\
 Data File : PS004135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2019 11:53
 Operator : EI\SJ
 Sample : MDL-BL-WATER-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 01:44:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.225	10.739	211.0E6	163.7E6	434.821	356.505
Target Compounds							
7) T	MCPA	12.194	11.618	179088	5267027	<MDL	2.895 #
8) T	DICHLORPROP	12.729	0.000	10217443	0	21.106	N.D. #
15) T	Picloram	16.781	0.000	678883	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041819\
Data File : PS004135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2019 11:53
Operator : EI\SJ
Sample : MDL-BL-WATER-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 01:44:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

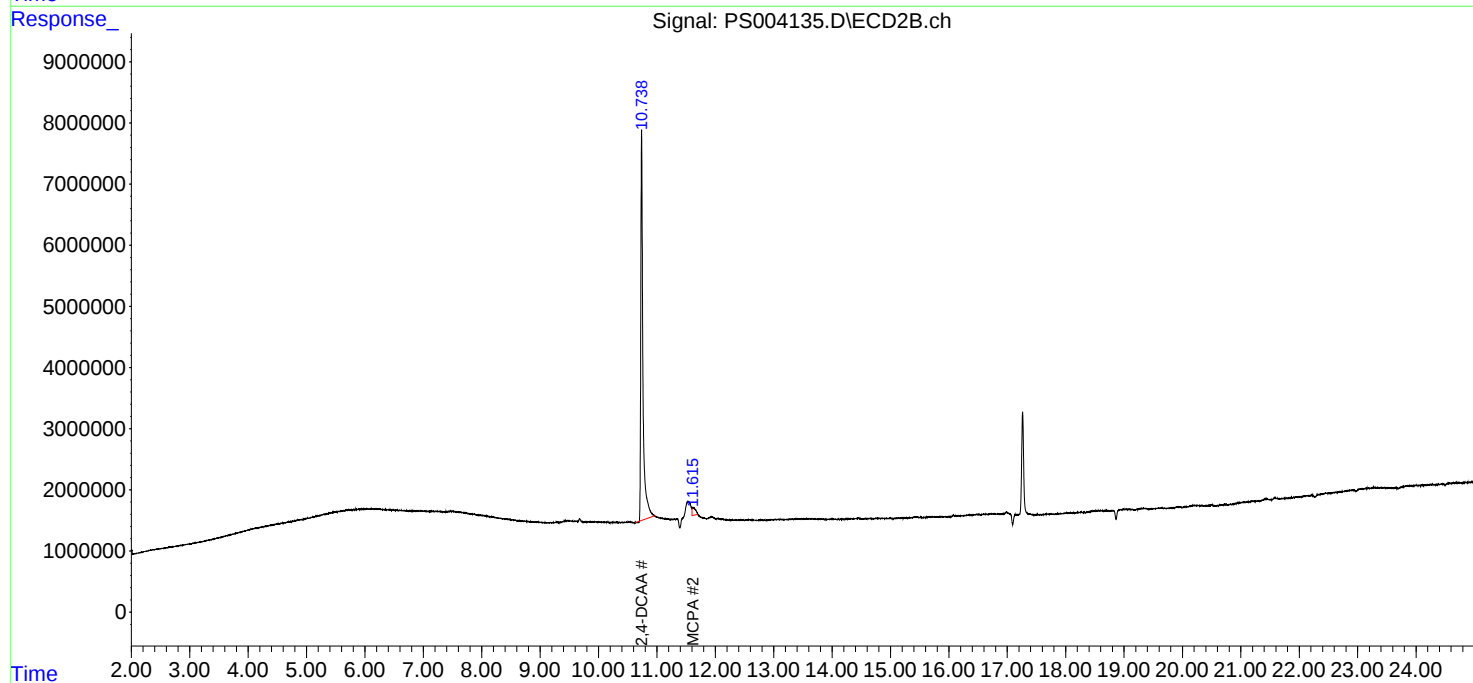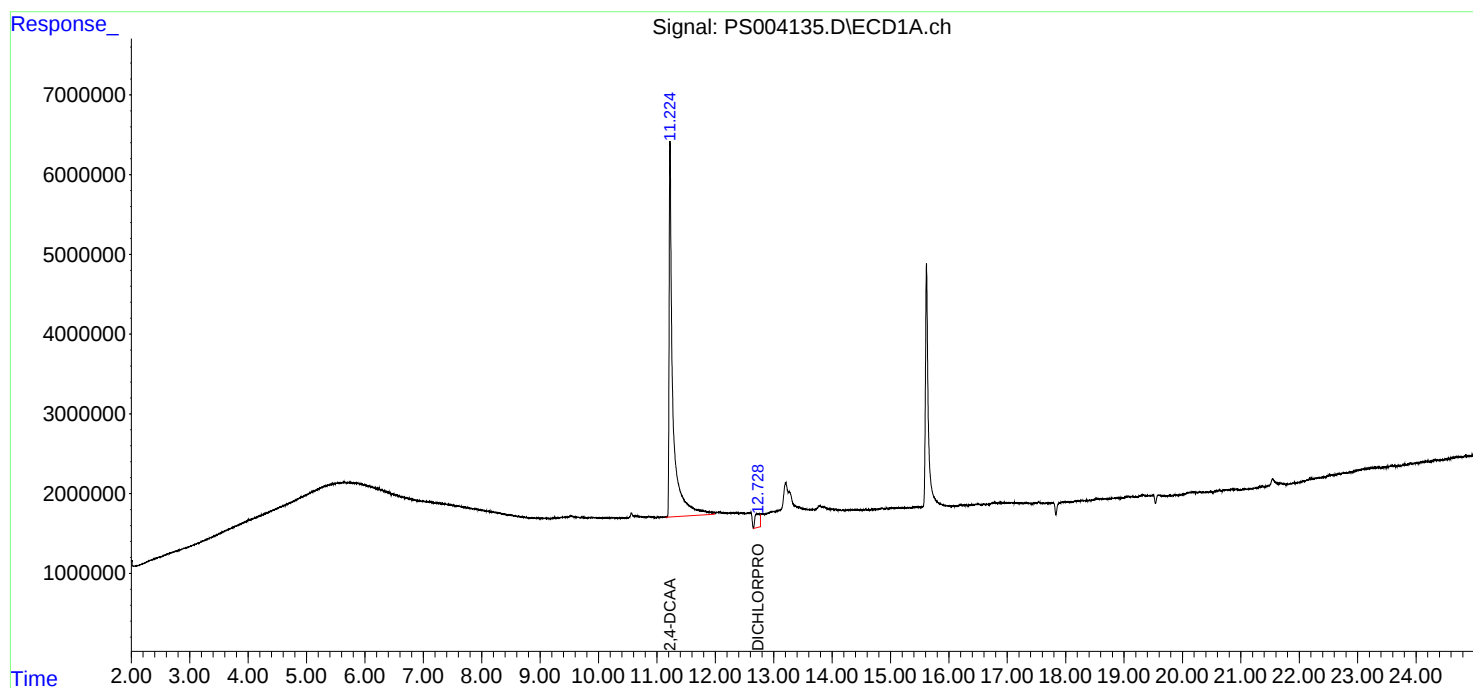


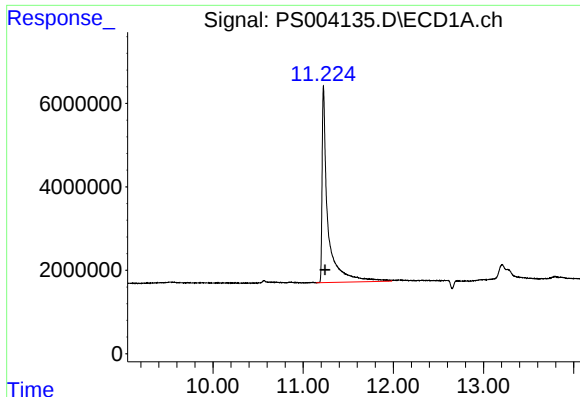

#4 2,4-DCAA


R.T.: 11.225 min
Delta R.T.: -0.018 min
Response: 210981694
Conc: 434.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

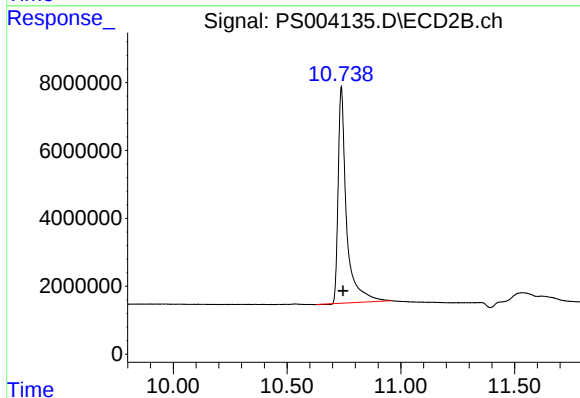


#4 2,4-DCAA

R.T.: 10.739 min
Delta R.T.: -0.007 min
Response: 163722036
Conc: 356.50 ng/ml

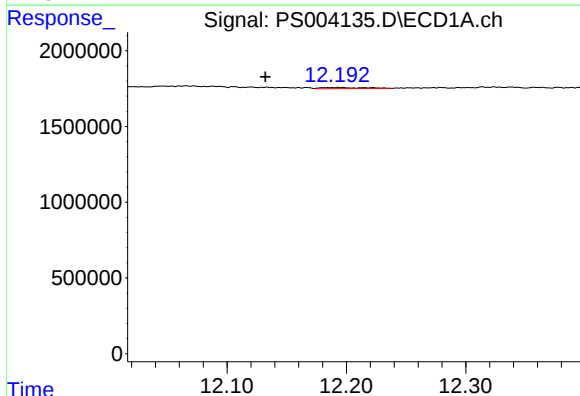


#7 MCPA

R.T.: 12.194 min
Delta R.T.: 0.062 min
Response: 179088
Conc: N.D.

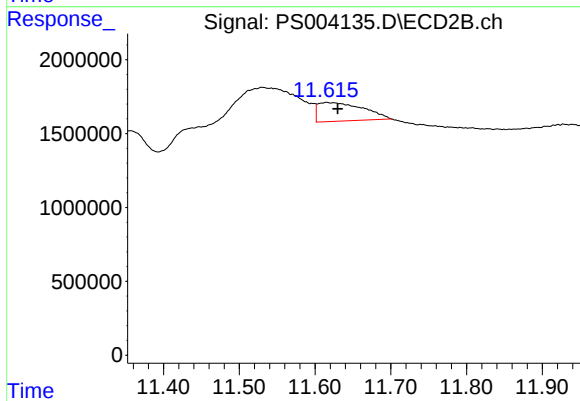

#7 MCPA


R.T.: 11.618 min
Delta R.T.: -0.012 min
Response: 5267027
Conc: 2.89 ug/ml

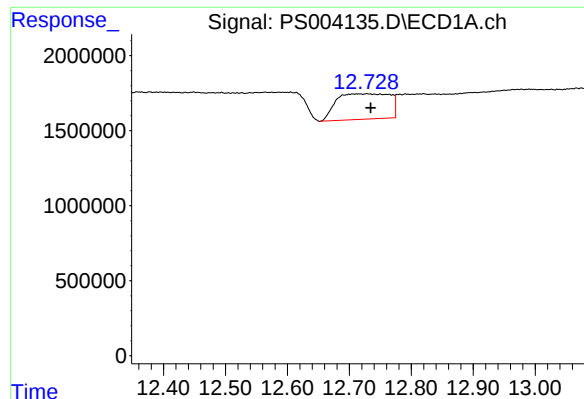

#8 DICHLORPROP

R.T.: 12.729 min
Delta R.T.: -0.005 min
Response: 10217443
Conc: 21.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

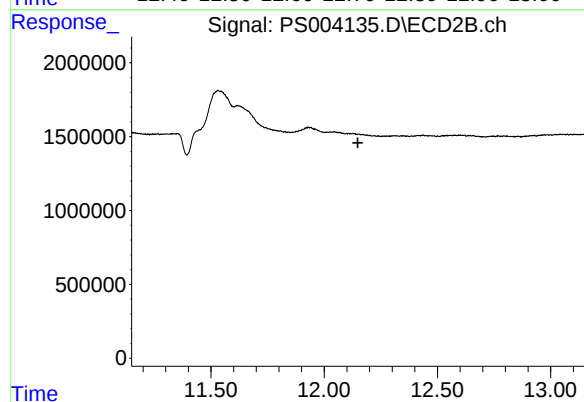

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.149 min
Response: 0
Conc: N.D.