

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041822\
 Data File : PS019022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 13:04
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 17:39:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3)	T	4-Nitroph...	7.013	0.000	29154	0	<MDL N.D. #
8)	T	DICHLORPROP	8.091	0.000	4470975	0	1.255 N.D. #
11)	T	2,4,5-TP ...	9.230	8.628f	12894038	2425318	<MDL <MDL #
12)	T	2,4,5-T	9.493	9.106f	5099316	3275202	<MDL <MDL #
13)	T	2,4-DB	0.000	9.549	0	42489680	N.D. 76.653
14)	T	DINOSEB	11.248f	0.000	63244670	0	4.133 N.D. #
15)	T	Picloram	10.994	10.870	39881862	22563879	1.488 3.811 #
16)	T	DCPA	11.531f	10.870f	11288847	22563879	<MDL 3.942 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041822\
Data File : PS019022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 13:04
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 17:39:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

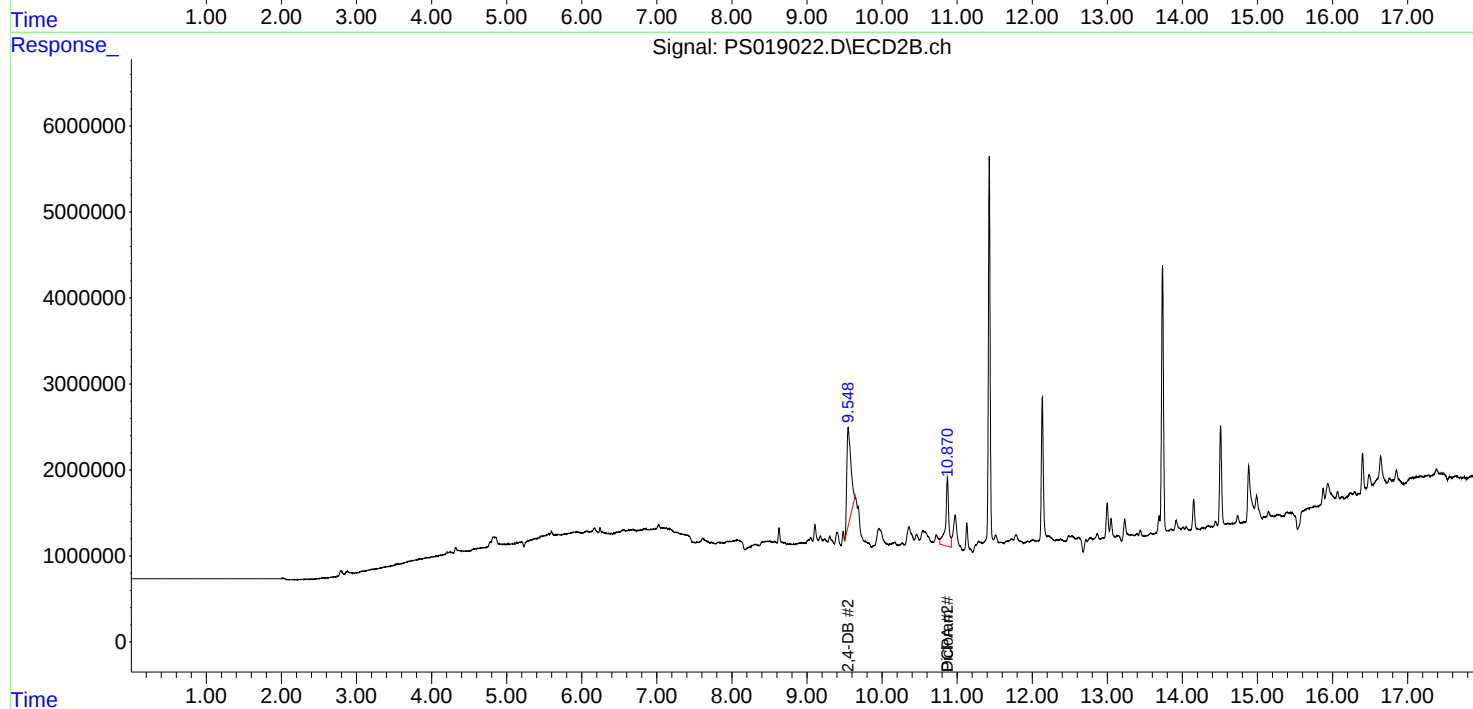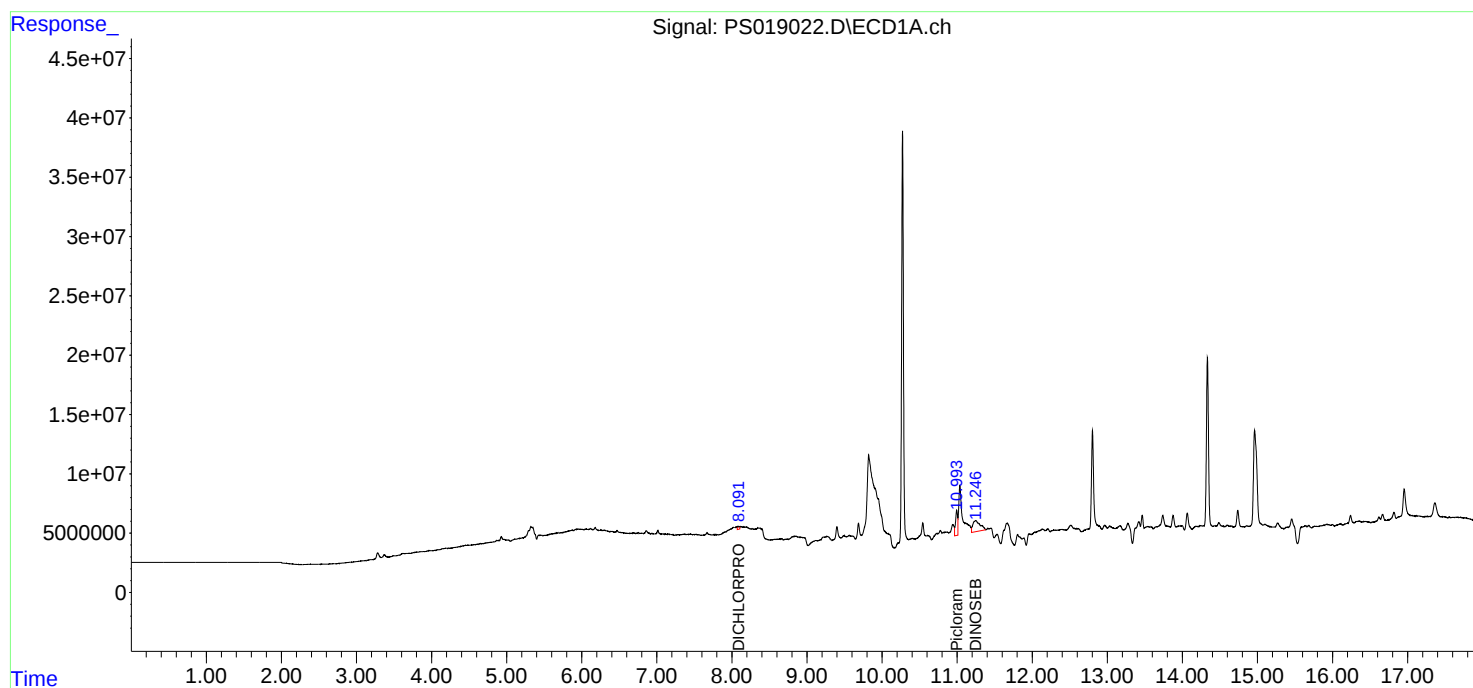


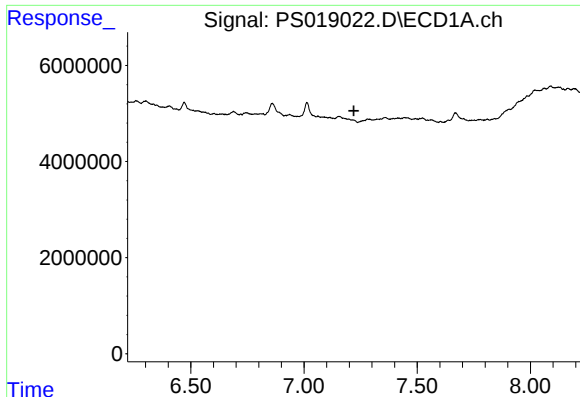

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

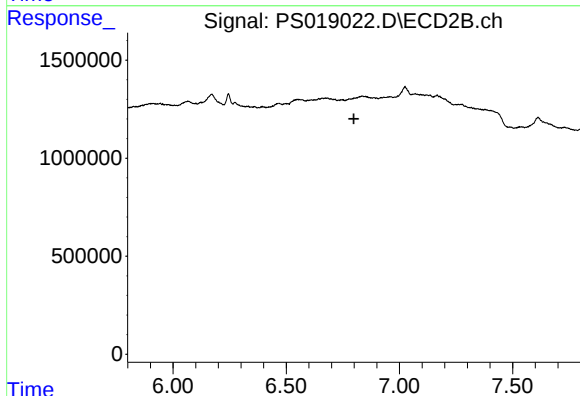


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.799 min
Response: 0
Conc: N.D.

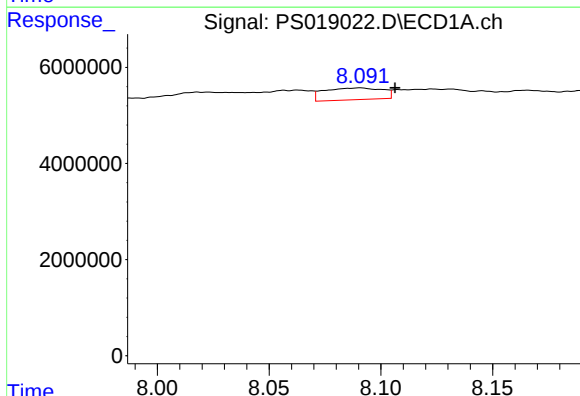


#8 DICHLORPROP

R.T.: 8.091 min
Delta R.T.: -0.016 min
Response: 4470975
Conc: 1.26 ng/ml

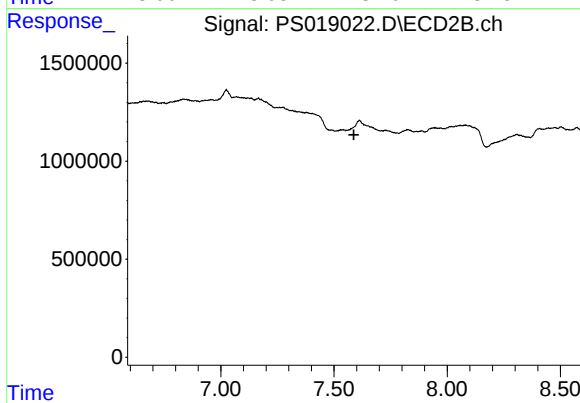

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.588 min
Response: 0
Conc: N.D.

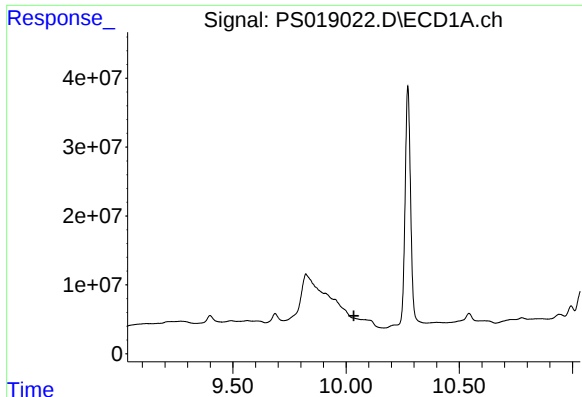

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

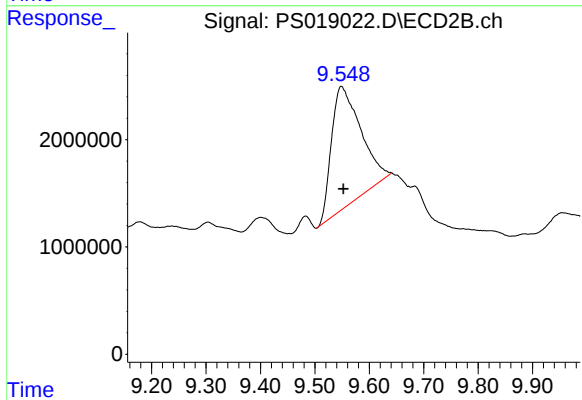


#13 2,4-DB

R.T.: 9.549 min
Delta R.T.: -0.004 min
Response: 42489680
Conc: 76.65 ng/ml

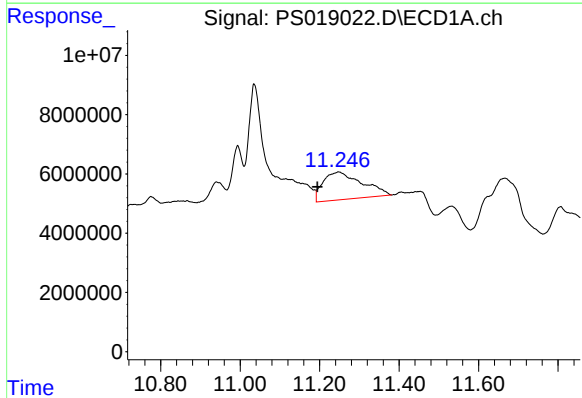


#14 DINOSEB

R.T.: 11.248 min
Delta R.T.: 0.054 min
Response: 63244670
Conc: 4.13 ng/ml

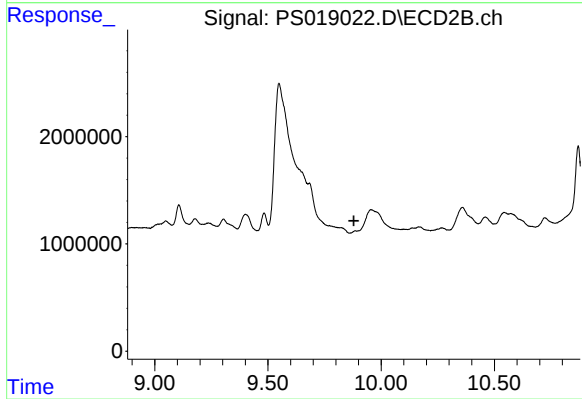

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.880 min
Response: 0
Conc: N.D.

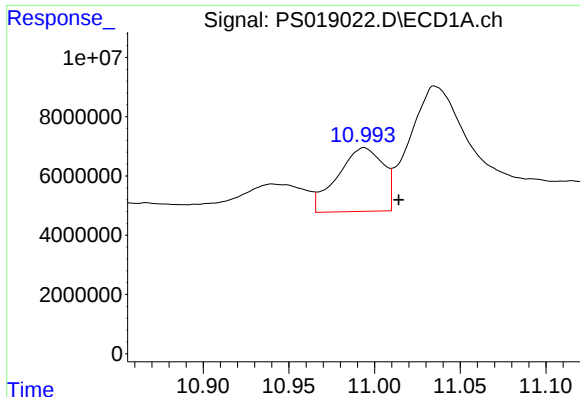

#15 Picloram


R.T.: 10.994 min
Delta R.T.: -0.020 min
Response: 39881862
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

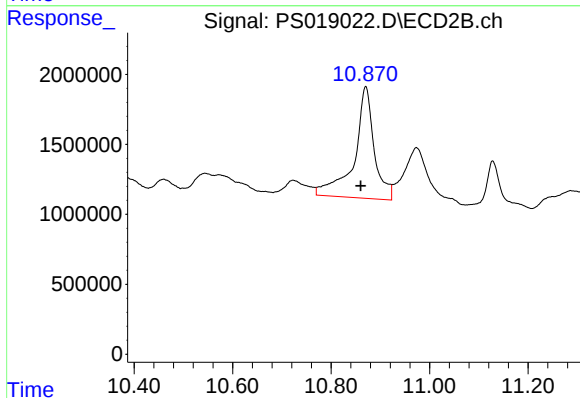


#15 Picloram

R.T.: 10.870 min
Delta R.T.: 0.010 min
Response: 22563879
Conc: 3.81 ng/ml

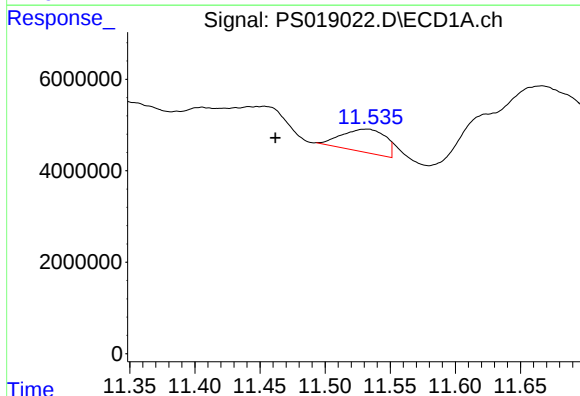

#16 DCPA

R.T.: 11.531 min
Delta R.T.: 0.070 min
Response: 11288847
Conc: N.D.

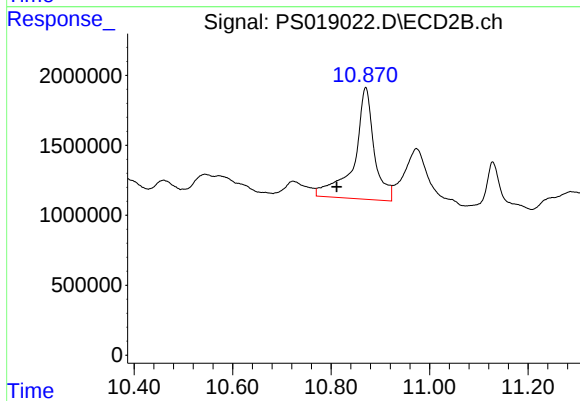

#16 DCPA

R.T.: 10.870 min
Delta R.T.: 0.059 min
Response: 22563879
Conc: 3.94 ng/ml