

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041822\
 Data File : PS019042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 22:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 03:36:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.798	1340.0E6	367.6E6	358.277	506.484 #
Target Compounds							
8) T	DICHLORPROP	0.000	7.613	0	5154242	N.D.	6.168
10) T	Pentachlo...	8.653	0.000	1172306	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.261f	8.627f	28026728	5340825	1.407	1.134
12) T	2,4,5-T	9.484	9.105f	9583409	2682725	<MDL	<MDL #
13) T	2,4-DB	9.995	0.000	41436466	0	11.766	N.D. #
14) T	DINOSEB	11.218	0.000	238.4E6	0	15.582	N.D. #
15) T	Picloram	11.027	10.870	60561861	14538171	2.260	2.455
16) T	DCPA	0.000	10.870f	0	14538171	N.D.	2.540



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041822\
Data File : PS019042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 22:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 03:36:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

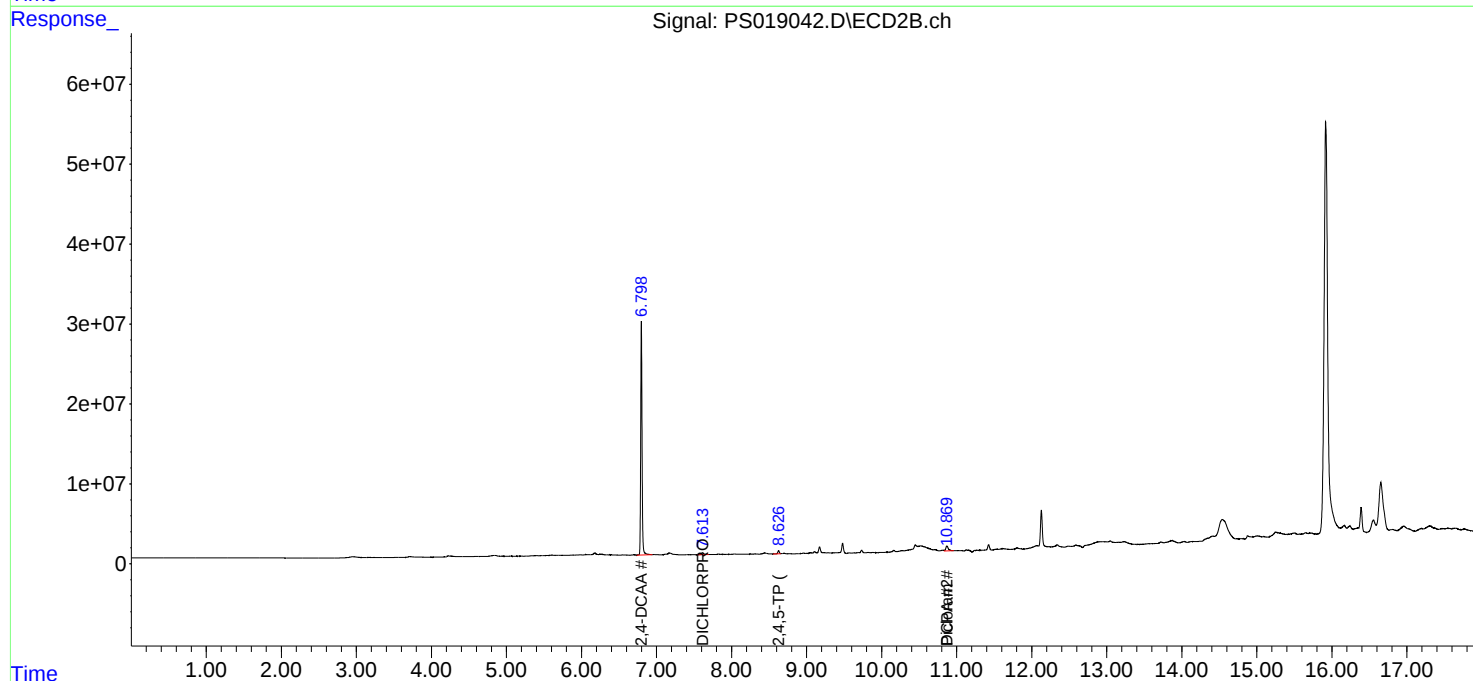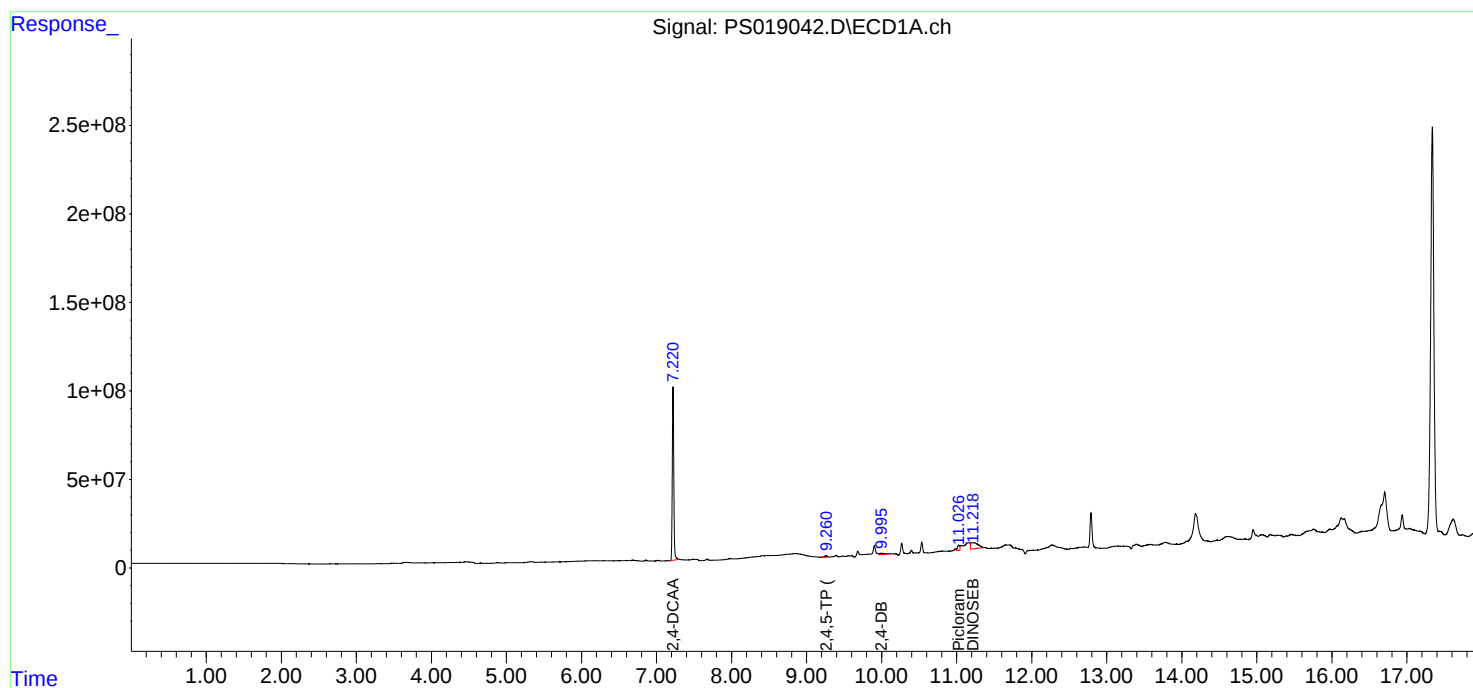


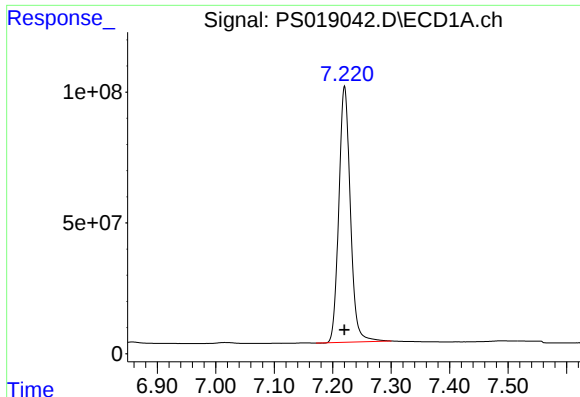

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 1339973310
Conc: 358.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

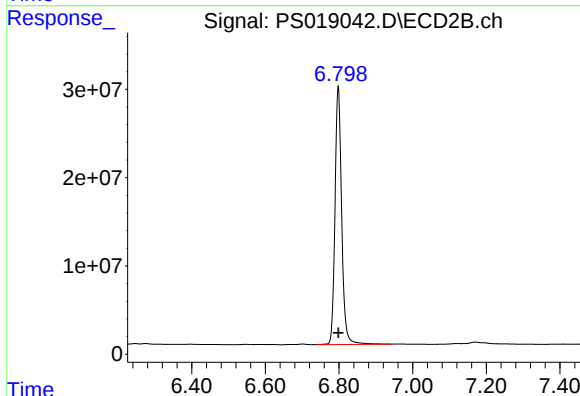


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 367645031
Conc: 506.48 ng/ml

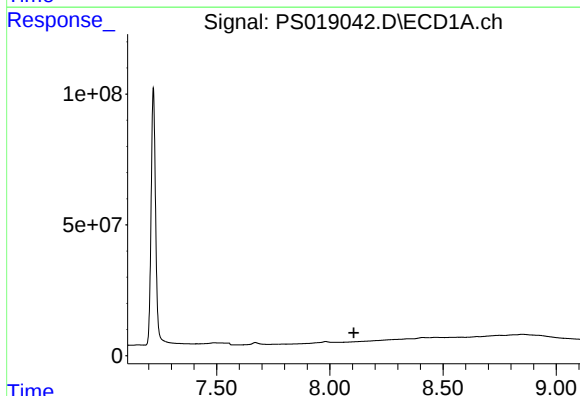


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.106 min
Response: 0
Conc: N.D.

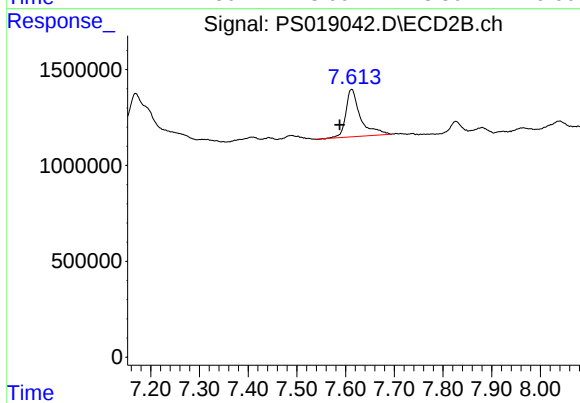

#8 DICHLORPROP


R.T.: 7.613 min
Delta R.T.: 0.024 min
Response: 5154242
Conc: 6.17 ng/ml

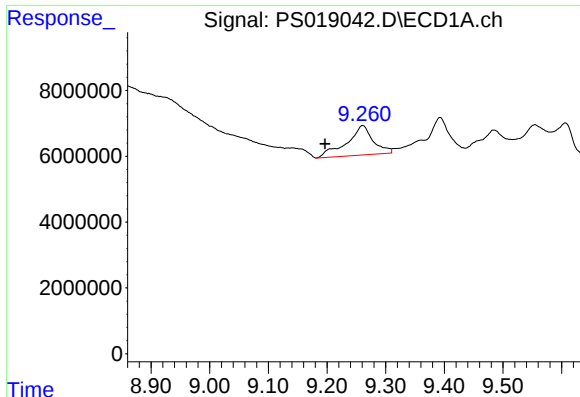

#11 2,4,5-TP (SILVEX)


R.T.: 9.261 min
Delta R.T.: 0.064 min
Response: 28026728
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

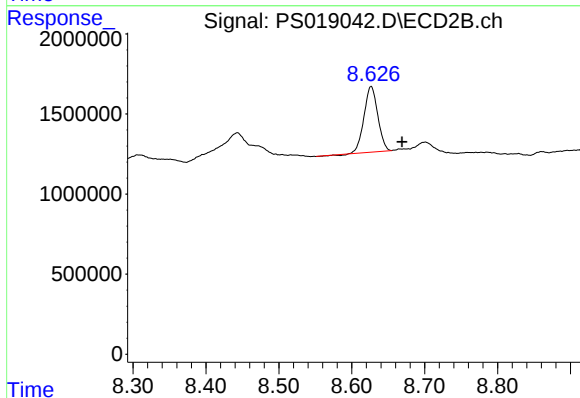


#11 2,4,5-TP (SILVEX)

R.T.: 8.627 min
Delta R.T.: -0.042 min
Response: 5340825
Conc: 1.13 ng/ml

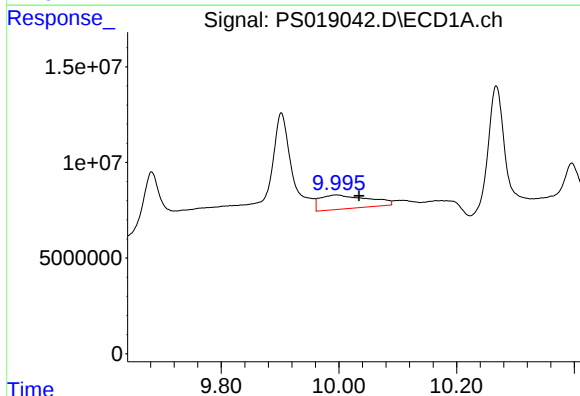


#13 2,4-DB

R.T.: 9.995 min
Delta R.T.: -0.039 min
Response: 41436466
Conc: 11.77 ng/ml

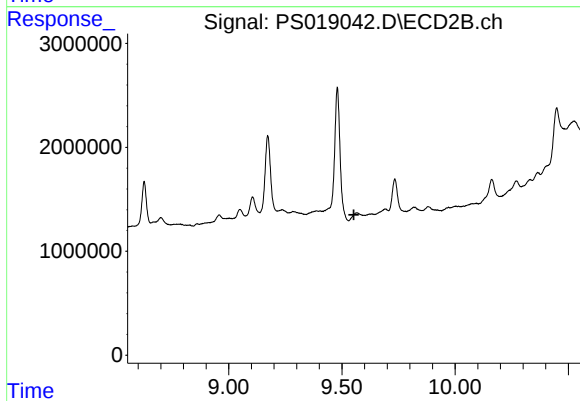

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.553 min
Response: 0
Conc: N.D.

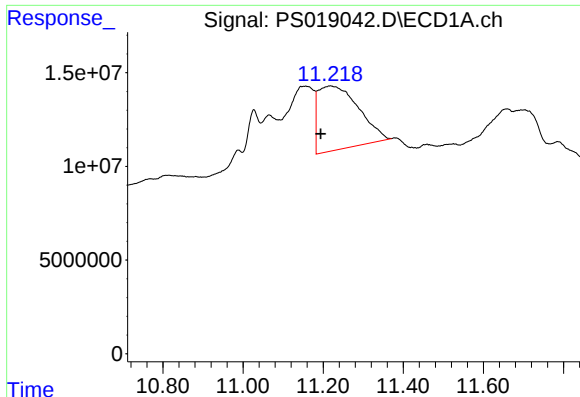

#14 DINOSEB


R.T.: 11.218 min
Delta R.T.: 0.024 min
Response: 238422611
Conc: 15.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

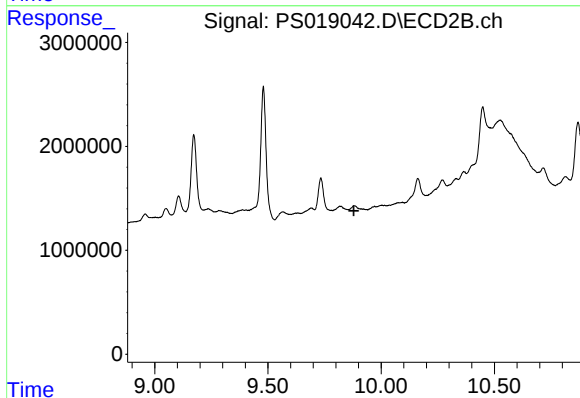


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

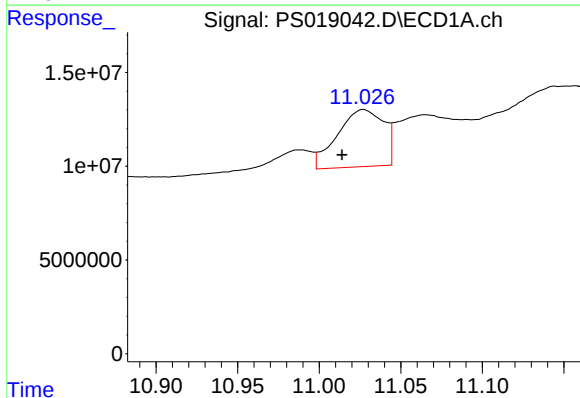


#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.013 min
Response: 60561861
Conc: 2.26 ng/ml

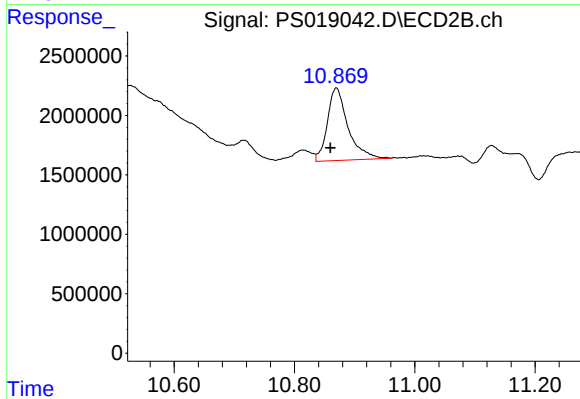

#15 Picloram


R.T.: 10.870 min
Delta R.T.: 0.010 min
Response: 14538171
Conc: 2.46 ng/ml

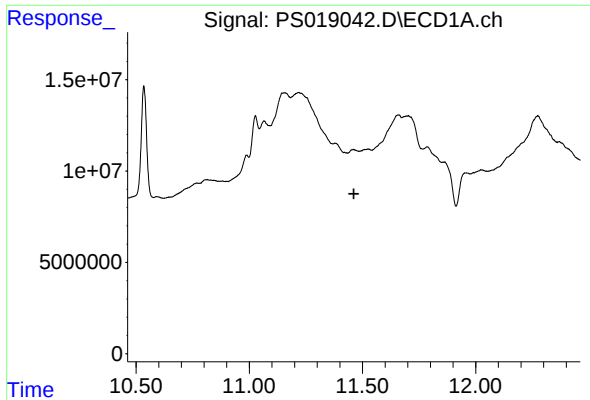

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

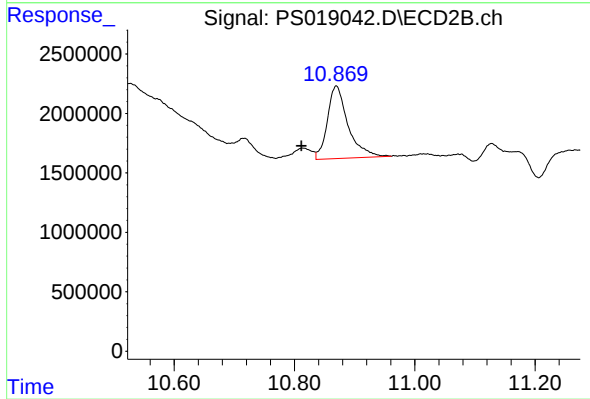

#16 DCPA

R.T.: 10.870 min
Delta R.T.: 0.058 min
Response: 14538171
Conc: 2.54 ng/ml