

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041822\
 Data File : PS019054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 05:18
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 06:04:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.798	1589.7E6	376.1E6	425.051	518.123
Target Compounds							
11) T	2,4,5-TP ...	9.157f	8.627f	14772894	5023428	<MDL	1.067 #
12) T	2,4,5-T	9.484	9.051	4602393	12053139	<MDL	2.791 #
13) T	2,4-DB	10.026	0.000	8682406	0	2.465	N.D. #
14) T	DINOSEB	11.143f	0.000	22026184	0	1.440	N.D. #
15) T	Picloram	11.025	10.868	26944685	10326750	1.006	1.744 #
16) T	DCPA	11.469	10.821	46958671	1220981	2.047	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041822\
Data File : PS019054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 05:18
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 06:04:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

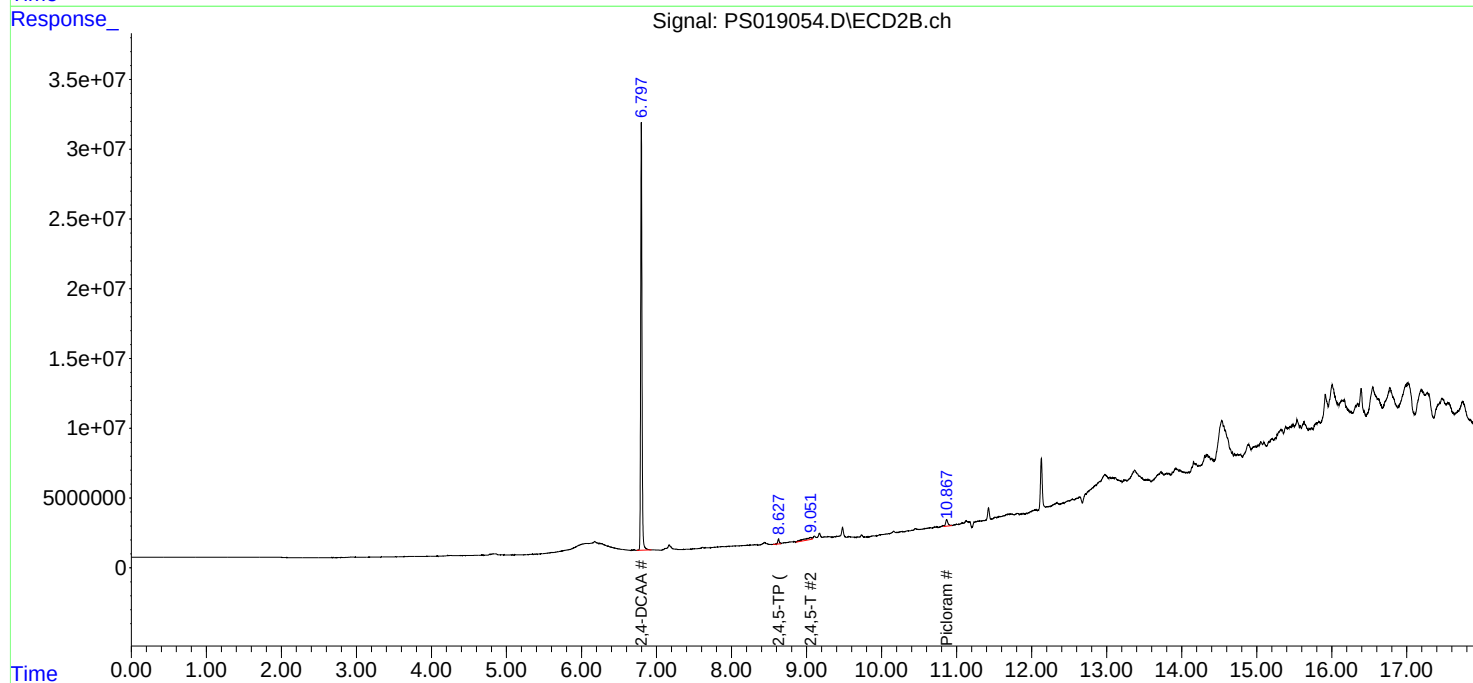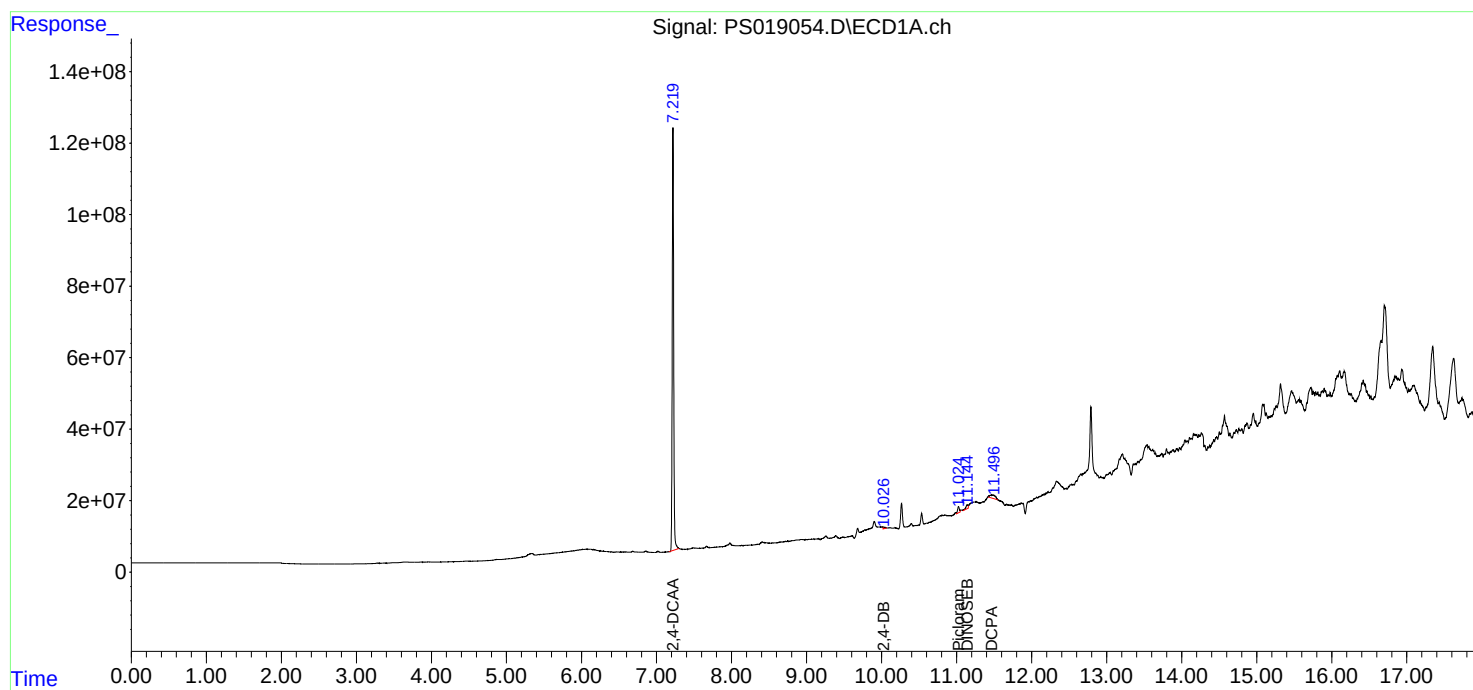


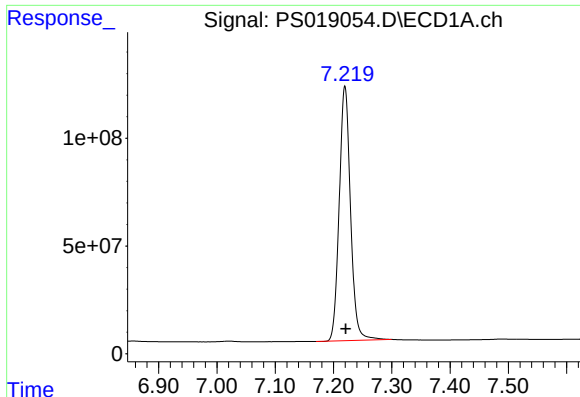

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: -0.001 min
Response: 1589713923
Conc: 425.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

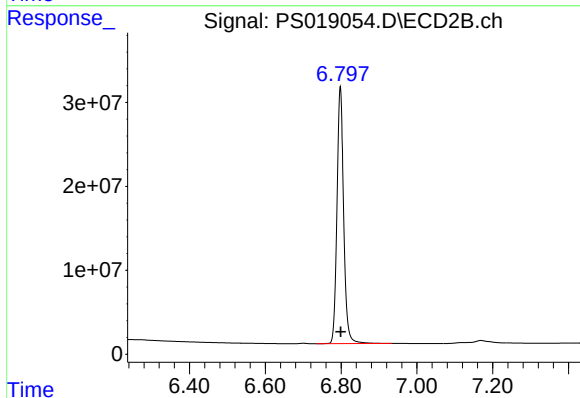


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 376093544
Conc: 518.12 ng/ml

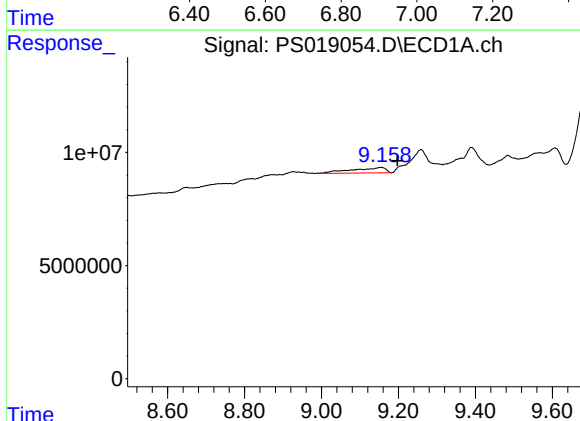


#11 2,4,5-TP (SILVEX)

R.T.: 9.157 min
Delta R.T.: -0.040 min
Response: 14772894
Conc: N.D.

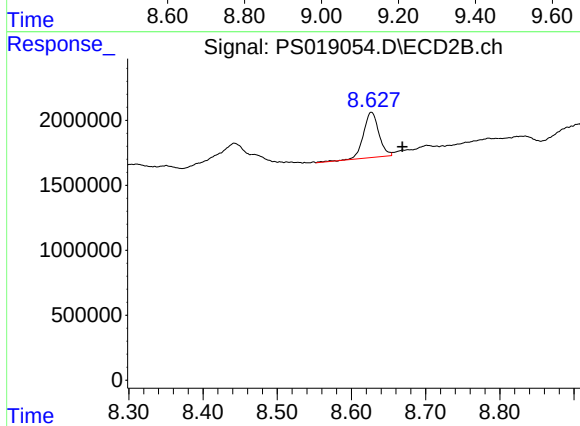

#11 2,4,5-TP (SILVEX)


R.T.: 8.627 min
Delta R.T.: -0.042 min
Response: 5023428
Conc: 1.07 ng/ml

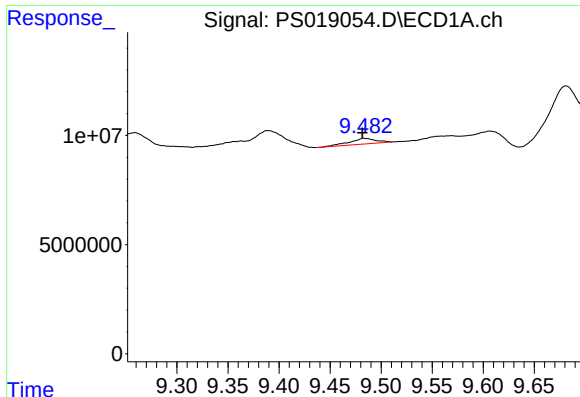

#12 2,4,5-T


R.T.: 9.484 min
Delta R.T.: 0.002 min
Response: 4602393
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

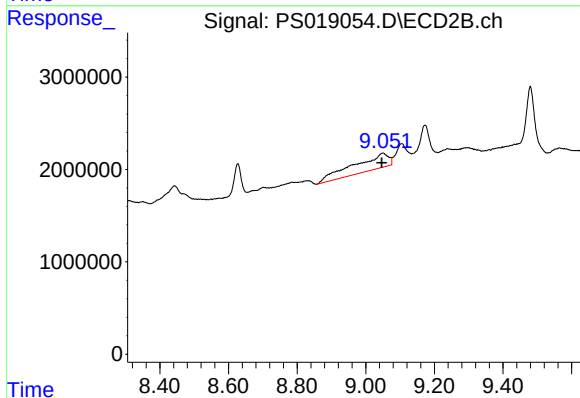


#12 2,4,5-T

R.T.: 9.051 min
Delta R.T.: 0.004 min
Response: 12053139
Conc: 2.79 ng/ml

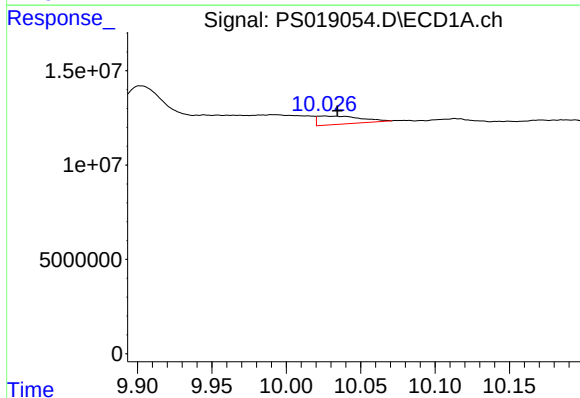


#13 2,4-DB

R.T.: 10.026 min
Delta R.T.: -0.009 min
Response: 8682406
Conc: 2.47 ng/ml

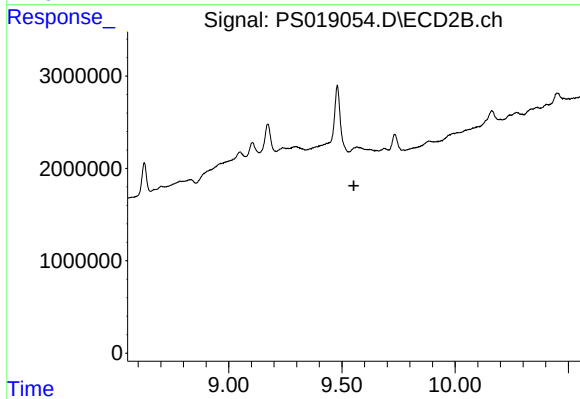

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.553 min
Response: 0
Conc: N.D.

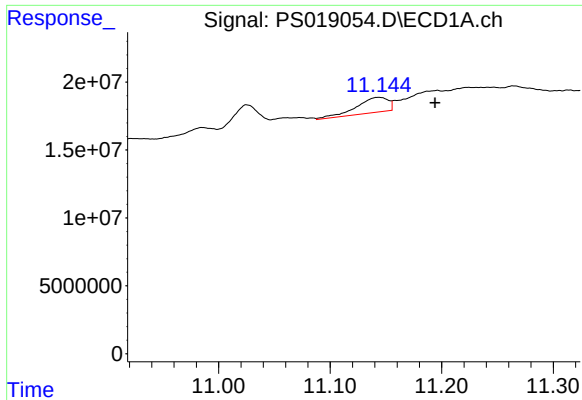

#14 DINOSEB


R.T.: 11.143 min
Delta R.T.: -0.051 min
Response: 22026184
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

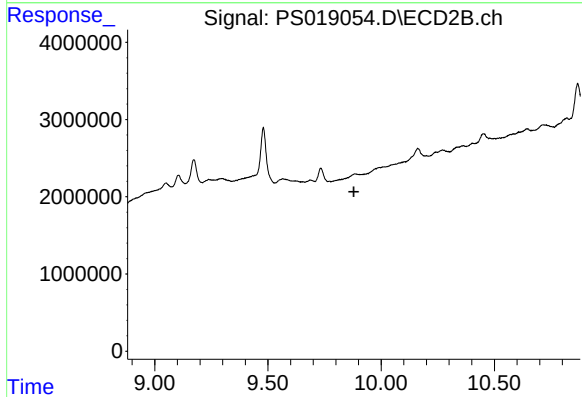


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

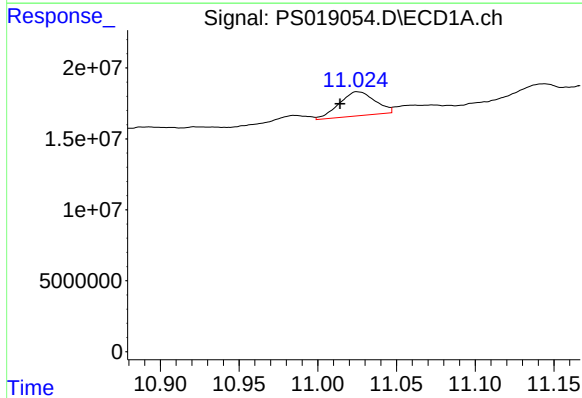


#15 Picloram

R.T.: 11.025 min
Delta R.T.: 0.011 min
Response: 26944685
Conc: 1.01 ng/ml

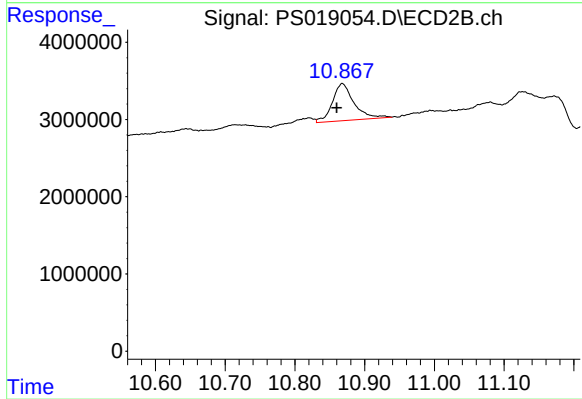

#15 Picloram


R.T.: 10.868 min
Delta R.T.: 0.008 min
Response: 10326750
Conc: 1.74 ng/ml

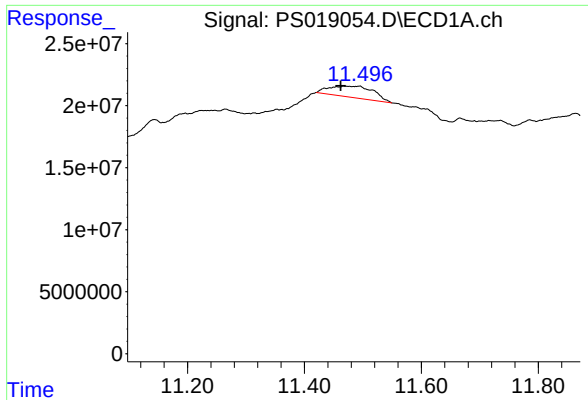

#16 DCPA

R.T.: 11.469 min
Delta R.T.: 0.007 min
Response: 46958671
Conc: 2.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

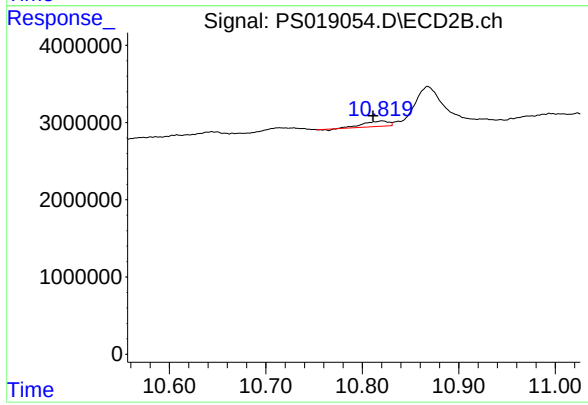

#16 DCPA

R.T.: 10.821 min
Delta R.T.: 0.009 min
Response: 1220981
Conc: N.D.