

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041822\
 Data File : PS019061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 13:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 14:41:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.797	1668.9E6	377.9E6	446.218	520.631
Target Compounds							
9) T	2,4-D	8.340	0.000	29155454	0	7.104	N.D. #
11) T	2,4,5-TP ...	0.000	8.627f	0	5388202	N.D.	1.144
12) T	2,4,5-T	9.486	9.101f	6059324	24112364	<MDL	5.584 #
13) T	2,4-DB	10.033	0.000	13040625	0	3.703	N.D. #
14) T	DINOSEB	11.150f	0.000	81824271	0	5.348	N.D. #
15) T	Picloram	11.028	10.865	49895634	42468244	1.862	7.172 #
16) T	DCPA	11.518f	10.865f	19512339	42468244	<MDL	7.420 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041822\
Data File : PS019061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 13:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 14:41:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

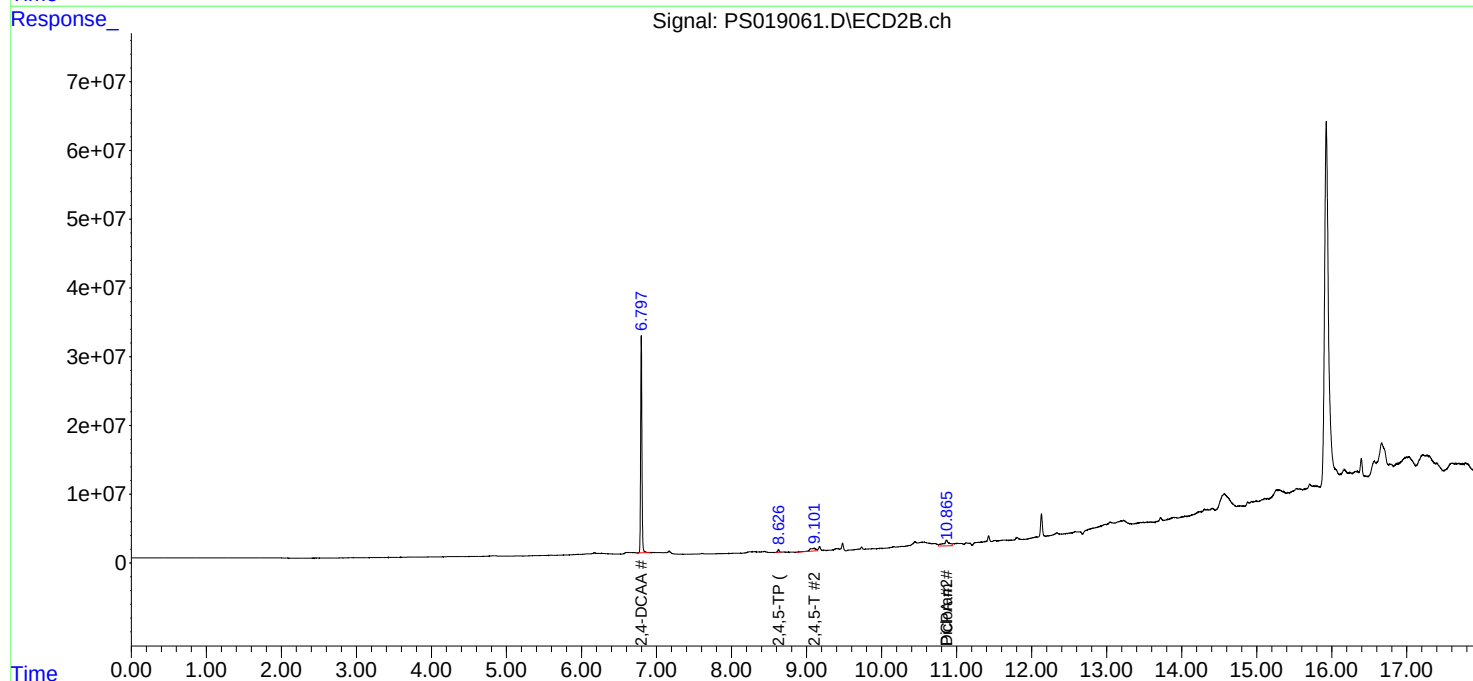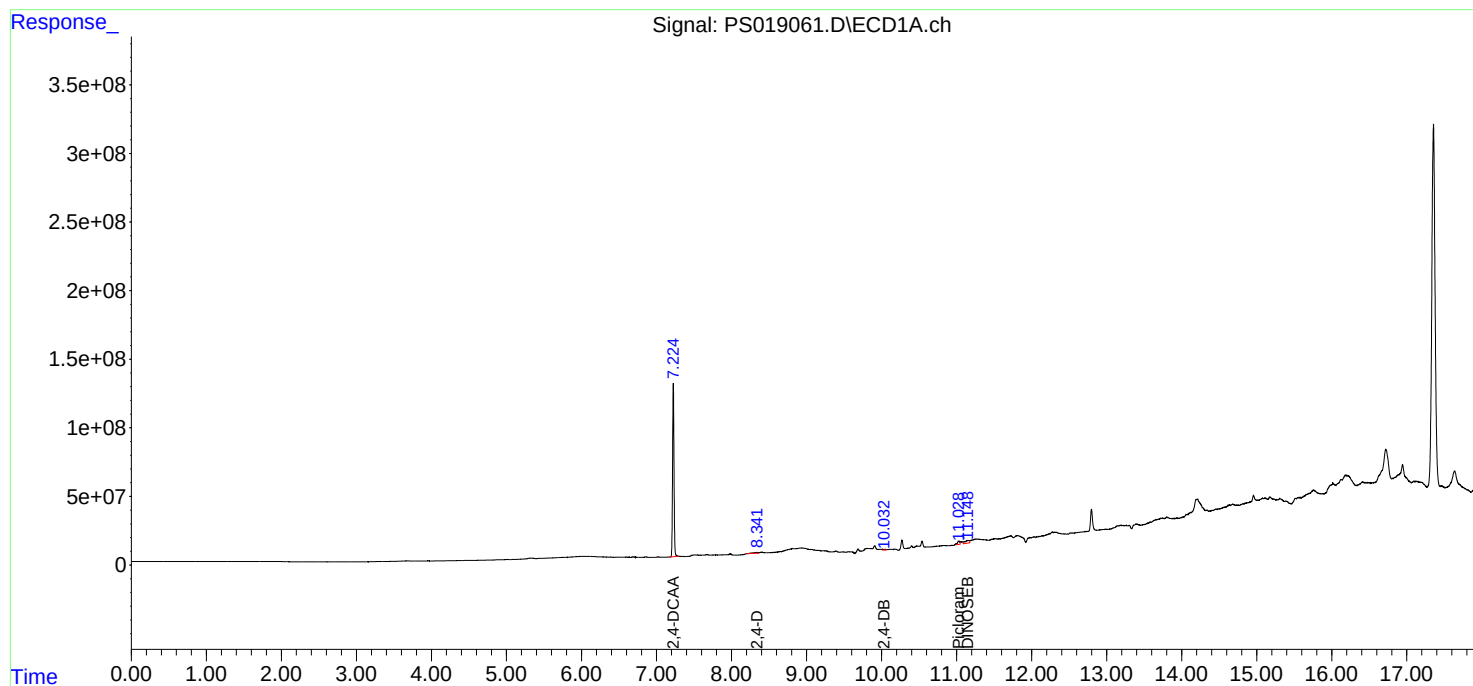


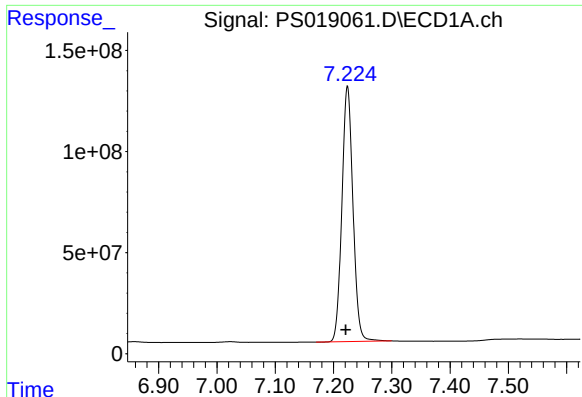

#4 2,4-DCAA


R.T.: 7.224 min
Delta R.T.: 0.003 min
Response: 1668877693
Conc: 446.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

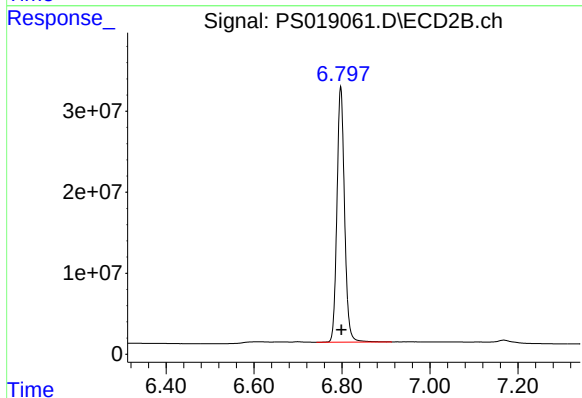


#4 2,4-DCAA

R.T.: 6.797 min
Delta R.T.: -0.002 min
Response: 377914208
Conc: 520.63 ng/ml

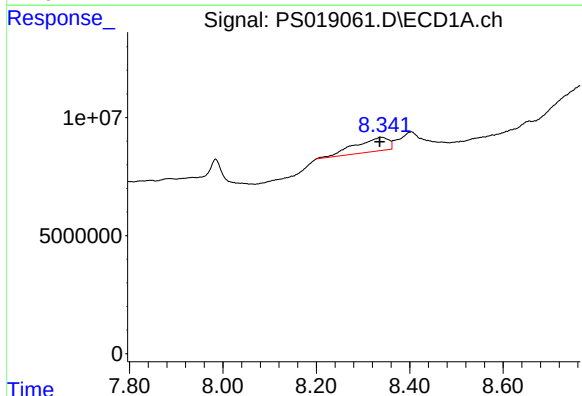


#9 2,4-D

R.T.: 8.340 min
Delta R.T.: 0.004 min
Response: 29155454
Conc: 7.10 ng/ml

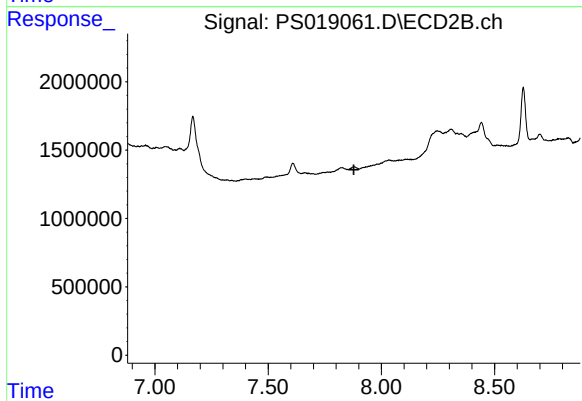

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.879 min
Response: 0
Conc: N.D.

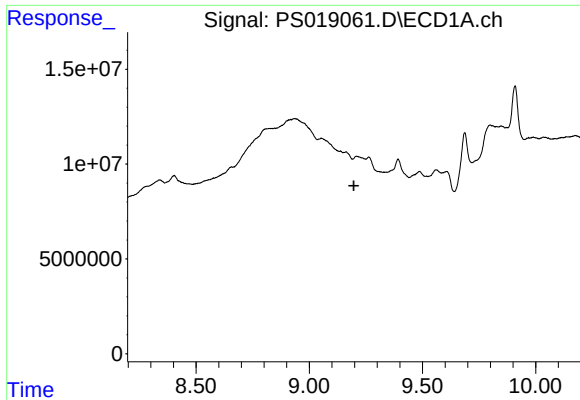

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

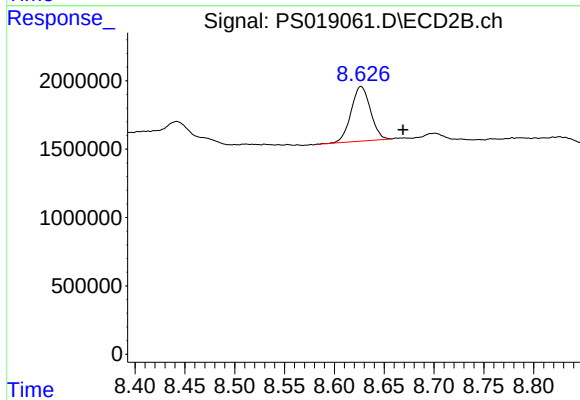


#11 2,4,5-TP (SILVEX)

R.T.: 8.627 min
Delta R.T.: -0.042 min
Response: 5388202
Conc: 1.14 ng/ml

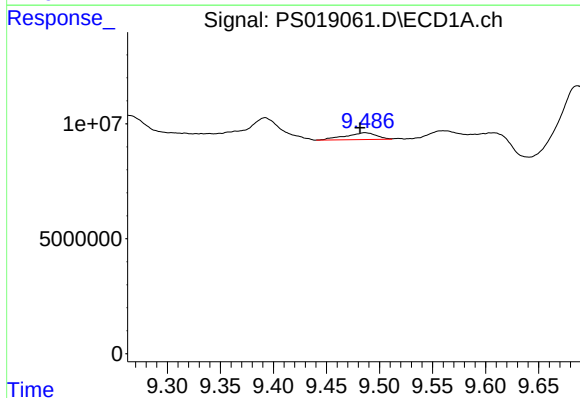


#12 2,4,5-T

R.T.: 9.486 min
Delta R.T.: 0.005 min
Response: 6059324
Conc: N.D.

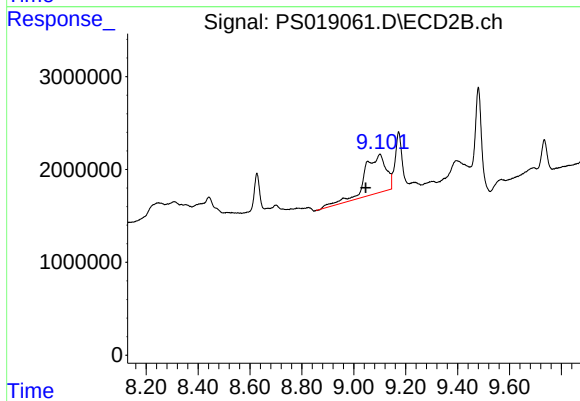

#12 2,4,5-T


R.T.: 9.101 min
Delta R.T.: 0.055 min
Response: 24112364
Conc: 5.58 ng/ml

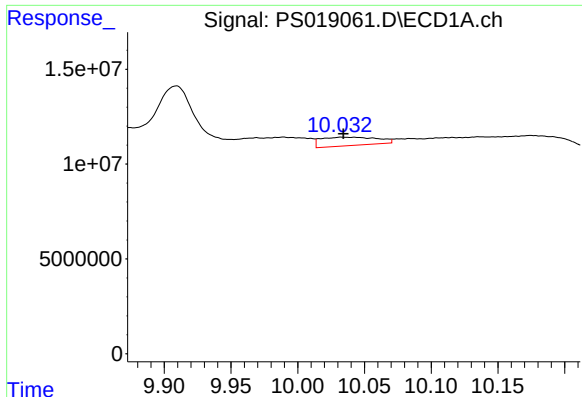

#13 2,4-DB


R.T.: 10.033 min
Delta R.T.: -0.002 min
Response: 13040625
Conc: 3.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

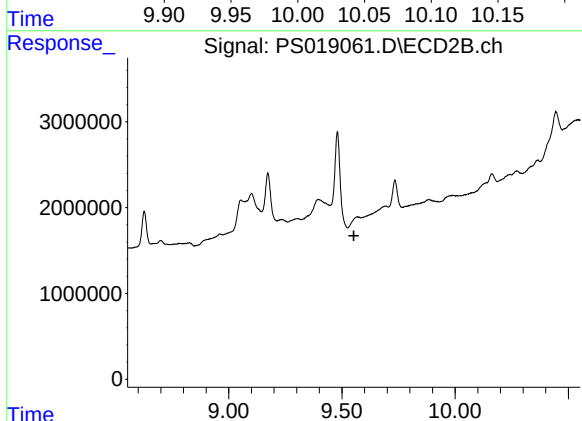


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.553 min
Response: 0
Conc: N.D.

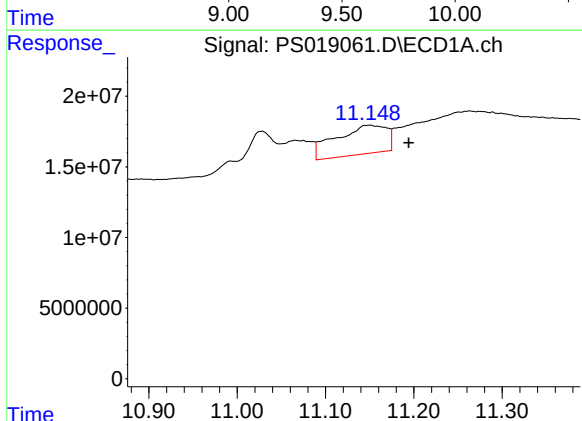


#14 DINOSEB

R.T.: 11.150 min
Delta R.T.: -0.044 min
Response: 81824271
Conc: 5.35 ng/ml

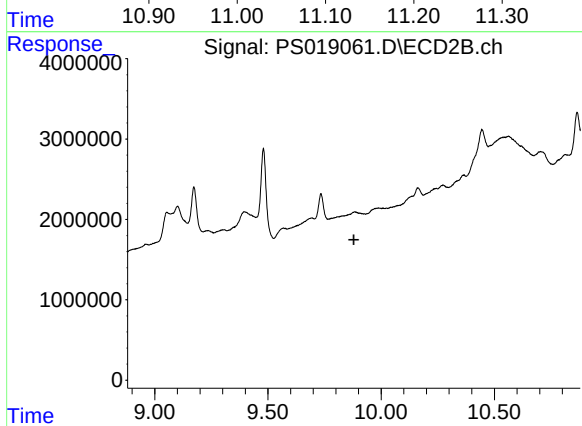

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

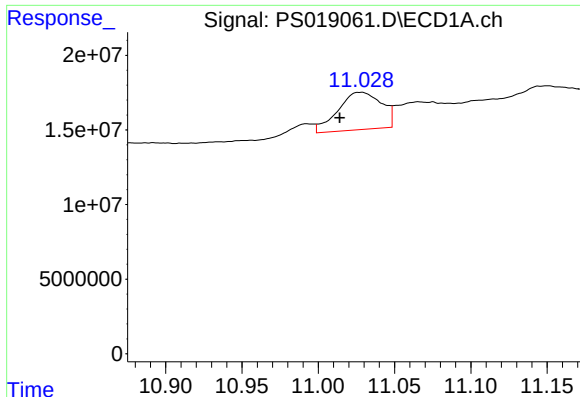

#15 Picloram


R.T.: 11.028 min
Delta R.T.: 0.014 min
Response: 49895634
Conc: 1.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

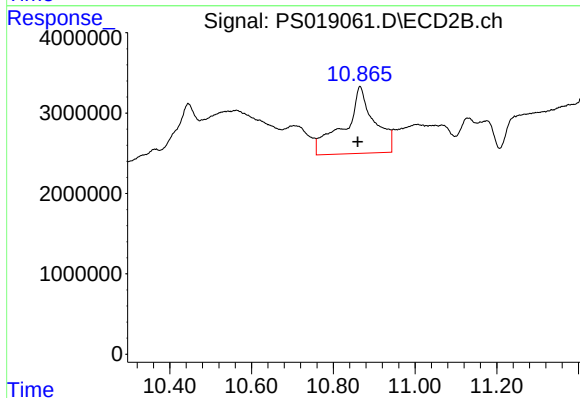


#15 Picloram

R.T.: 10.865 min
Delta R.T.: 0.006 min
Response: 42468244
Conc: 7.17 ng/ml

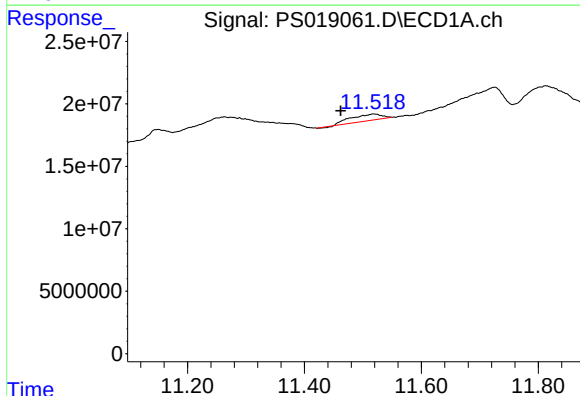

#16 DCPA

R.T.: 11.518 min
Delta R.T.: 0.056 min
Response: 19512339
Conc: N.D.

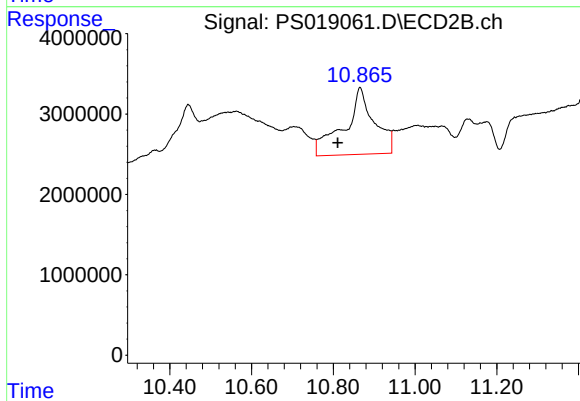

#16 DCPA

R.T.: 10.865 min
Delta R.T.: 0.054 min
Response: 42468244
Conc: 7.42 ng/ml