

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041825\
 Data File : PS029859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2025 12:58
 Operator : AR\AJ
 Sample : Q1825-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-10

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/19/2025
 Supervised By :mohammad ahmed 04/22/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 00:32:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040225.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 02 23:52:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.944	7.471	349.9E6	124.7E6	171.633m	182.953
Target Compounds						
8) T DICHLORPROP	7.819	8.373	322.8E6	121.2E6	146.779	125.451m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041825\
Data File : PS029859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2025 12:58
Operator : AR\AJ
Sample : Q1825-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/19/2025
Supervised By : mohammad ahmed 04/22/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 00:32:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040225.M
Quant Title : 8080.M
QLast Update : Wed Apr 02 23:52:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

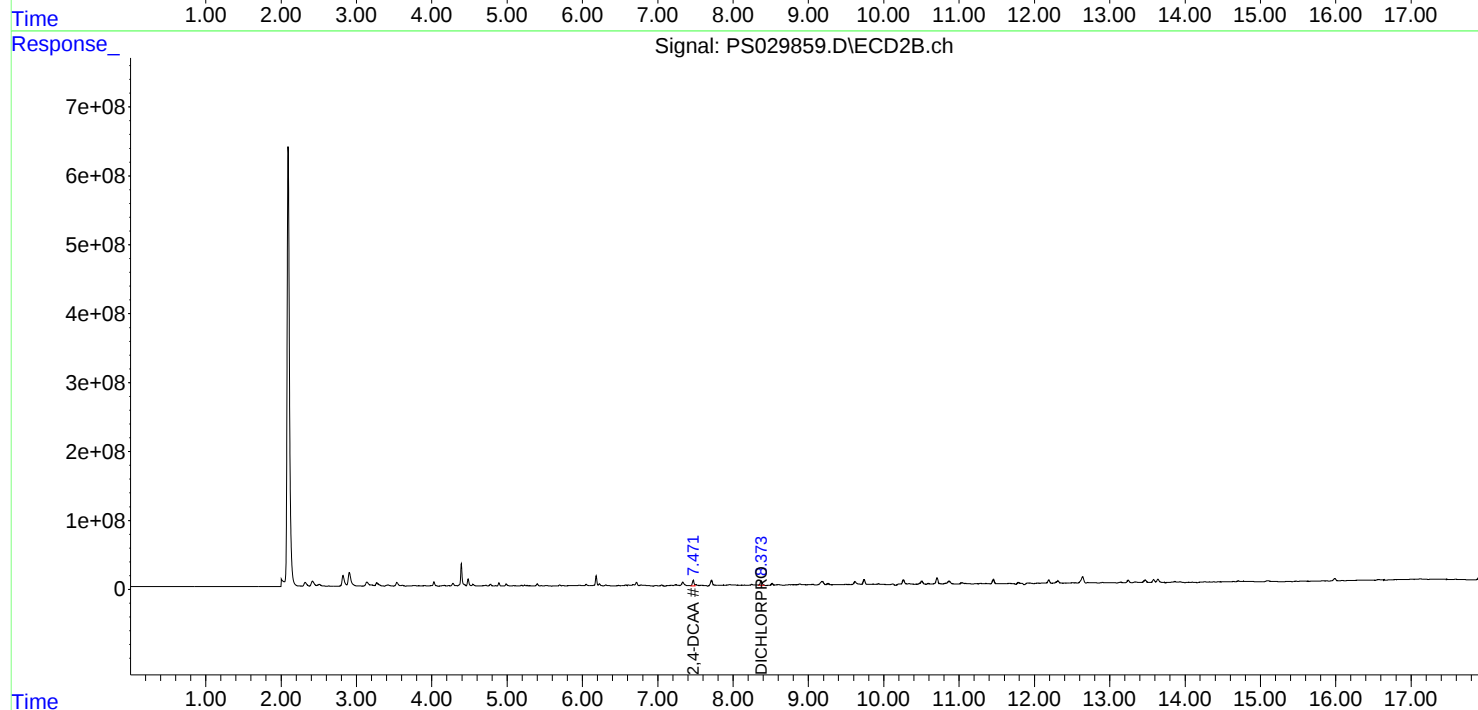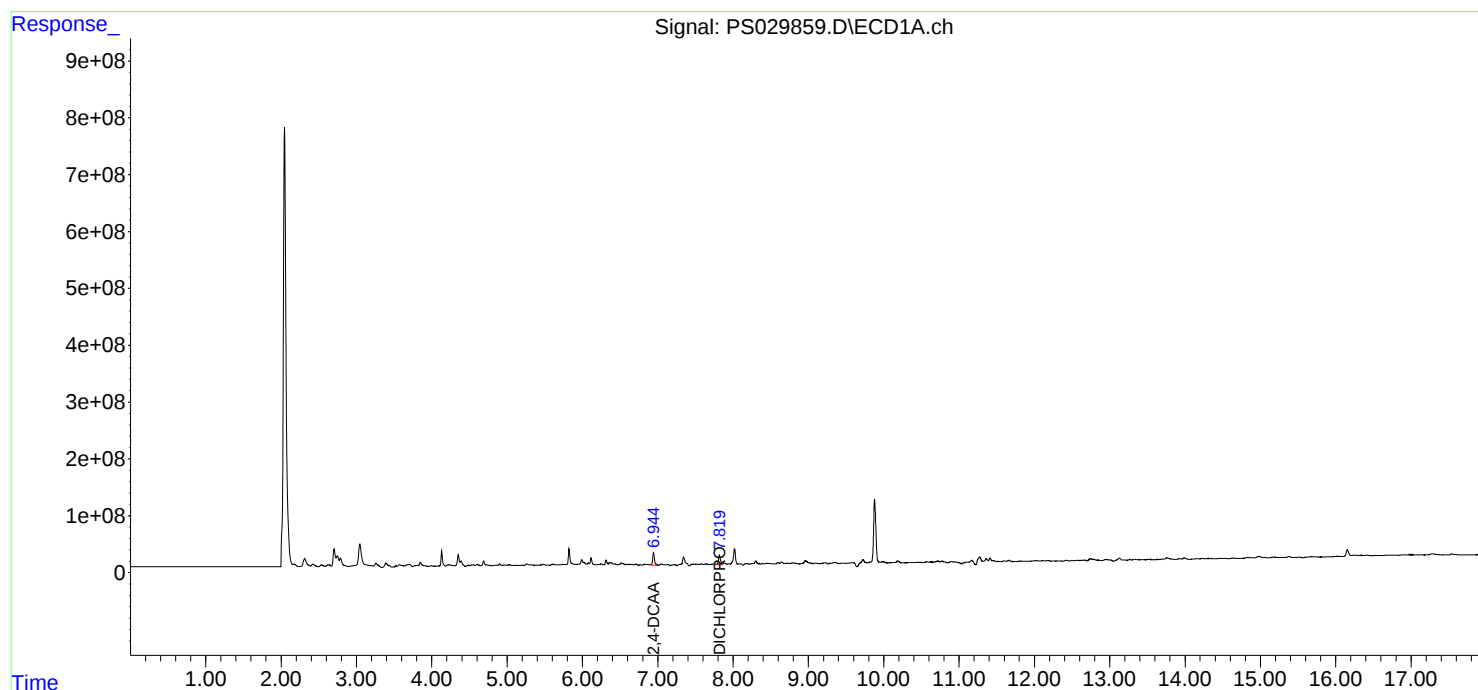

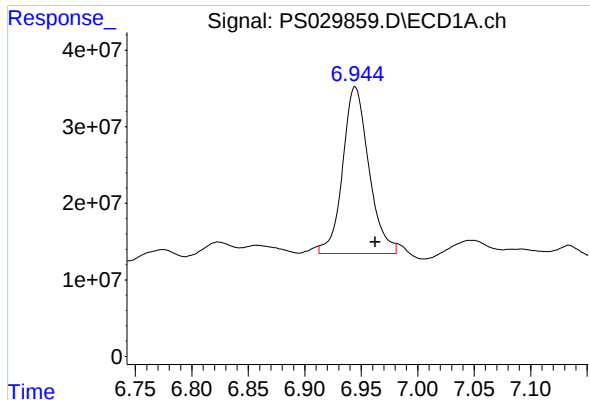


#4 2,4-DCAA

R.T.: 6.944 min
Delta R.T.: -0.019 min
Response: 349930664
Conc: 171.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/19/2025
Supervised By :mohammad ahmed 04/22/2025

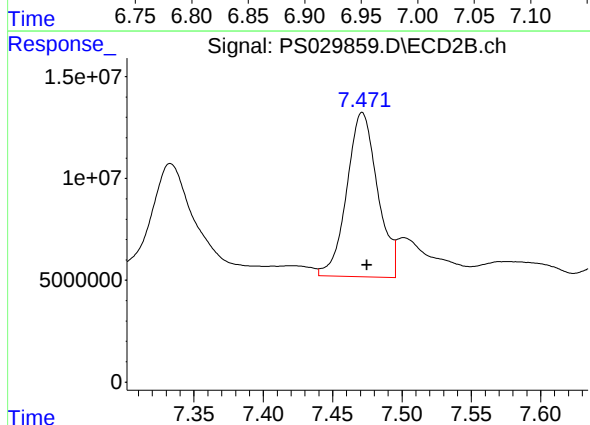


#4 2,4-DCAA

R.T.: 7.471 min
Delta R.T.: -0.004 min
Response: 124684530
Conc: 182.95 ng/ml

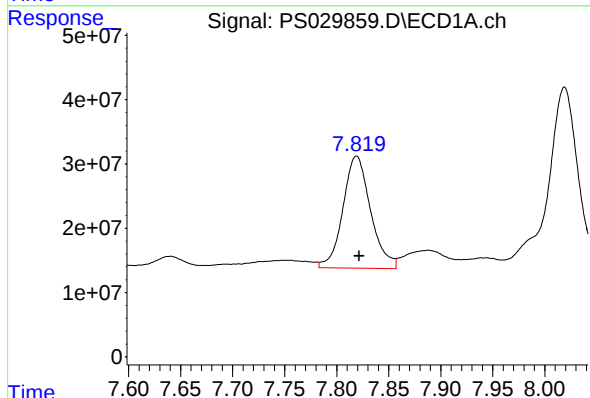

#8 DICHLORPROP

R.T.: 7.819 min
Delta R.T.: -0.003 min
Response: 322832203
Conc: 146.78 ng/ml

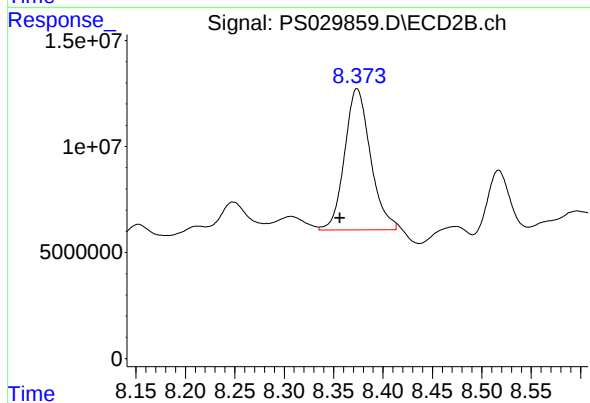

#8 DICHLORPROP

R.T.: 8.373 min
Delta R.T.: 0.017 min
Response: 121205222
Conc: 125.45 ng/ml m