

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
 Data File : PS004155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2019 07:21
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:54:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2)	T	3,5-DICHL...	9.675	0.000	384143	0	<MDL N.D. #
6)	T	MCP	11.937	0.000	593482	0	<MDL N.D. #
14)	T	DINOSEB	16.916	0.000	71233516	0	28.432 N.D. #
15)	T	Picloram	0.000	16.629	0	8661077	N.D. 2.530
16)	T	DCPA	17.279	16.629	17649388	8661077	4.903 2.725 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
Data File : PS004155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 07:21
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:54:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

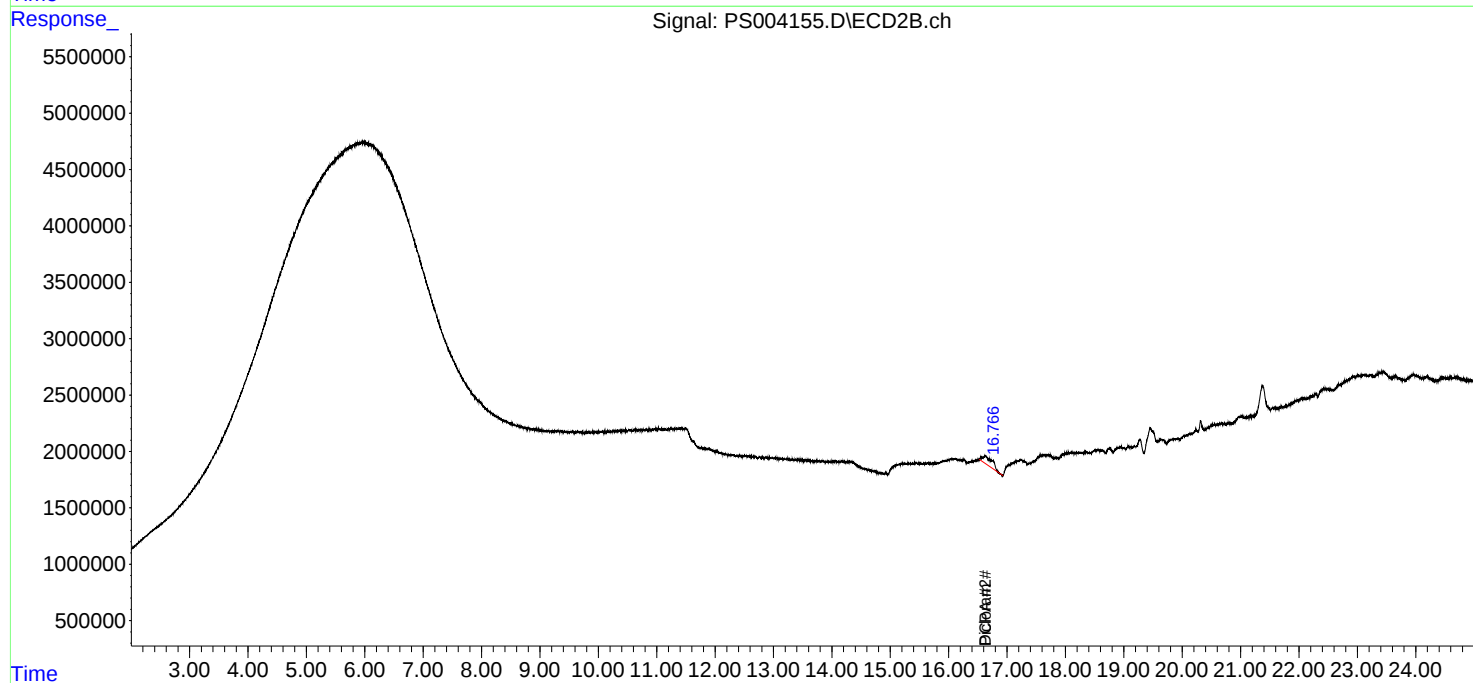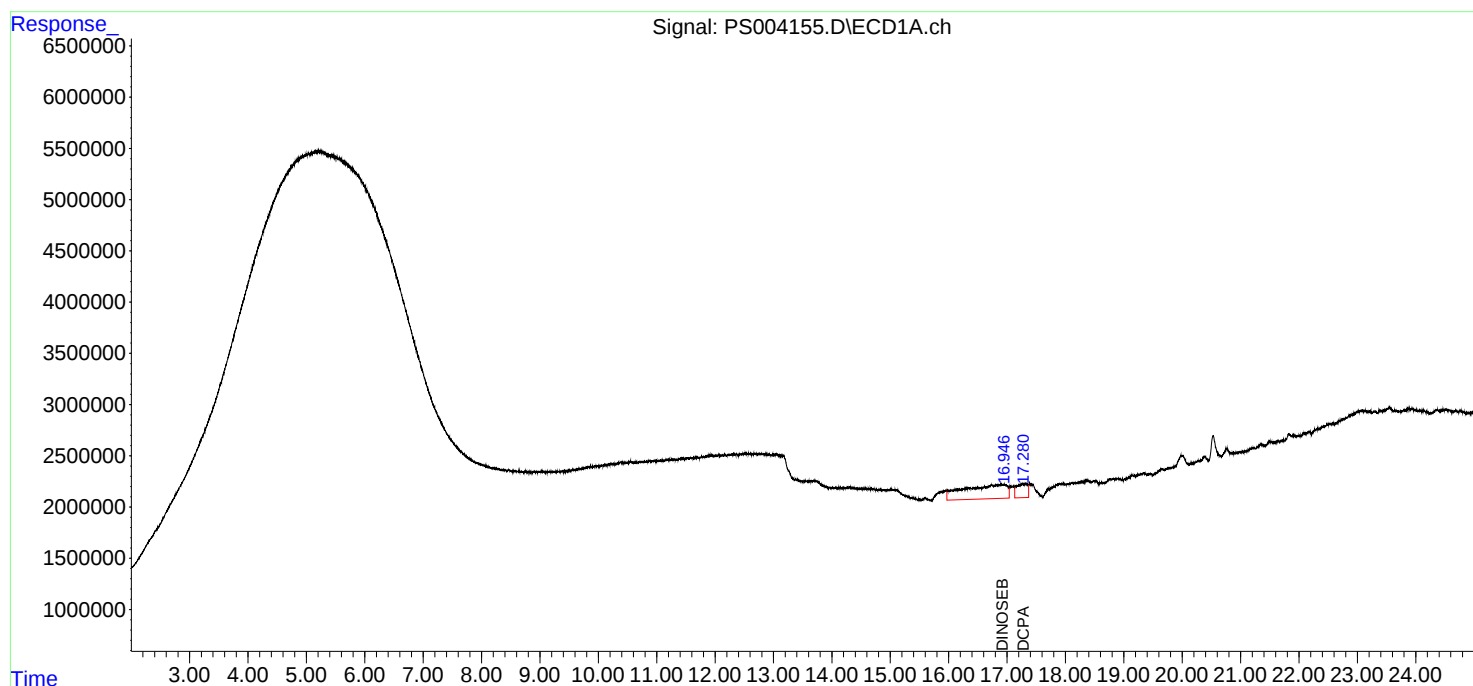


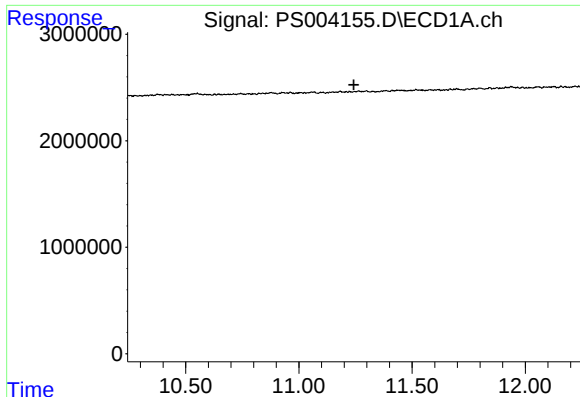

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

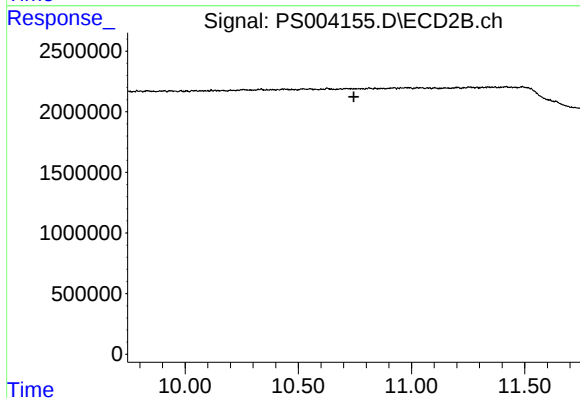


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 10.746 min
Response: 0
Conc: N.D.

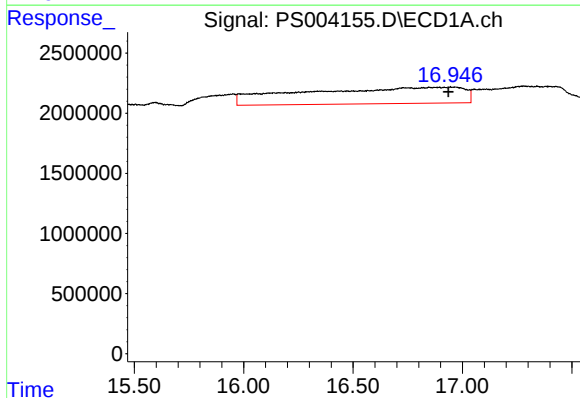


#14 DINOSEB

R.T.: 16.916 min
Delta R.T.: -0.020 min
Response: 71233516
Conc: 28.43 ng/ml

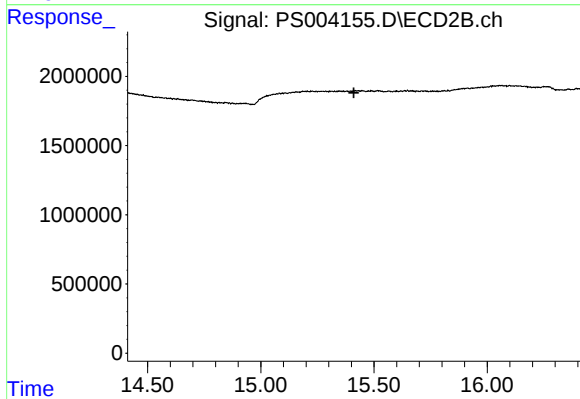

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 15.411 min
Response: 0
Conc: N.D.

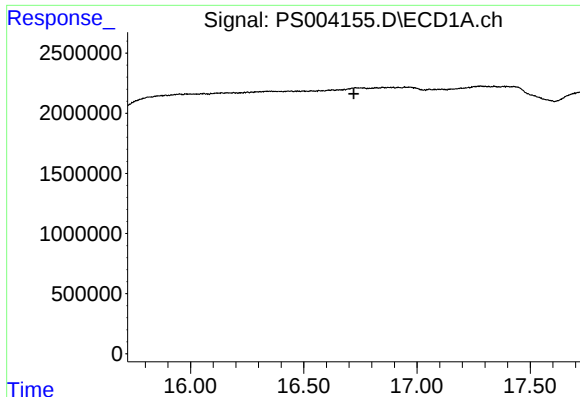

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.721 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

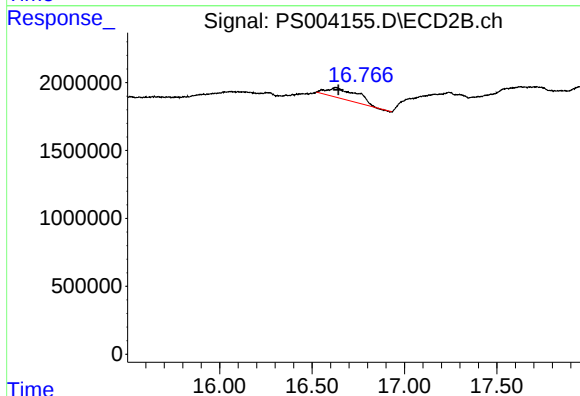


#15 Picloram

R.T.: 16.629 min
Delta R.T.: -0.014 min
Response: 8661077
Conc: 2.53 ng/ml

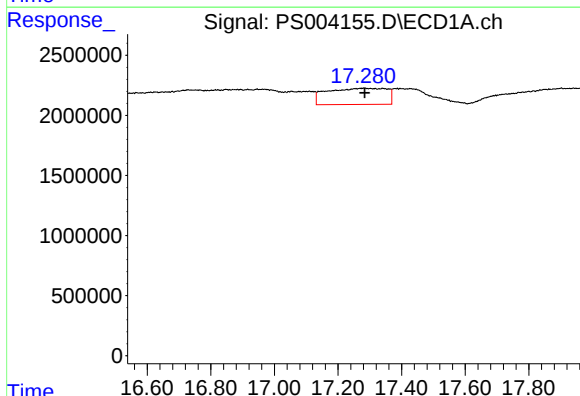

#16 DCPA

R.T.: 17.279 min
Delta R.T.: -0.004 min
Response: 17649388
Conc: 4.90 ng/ml

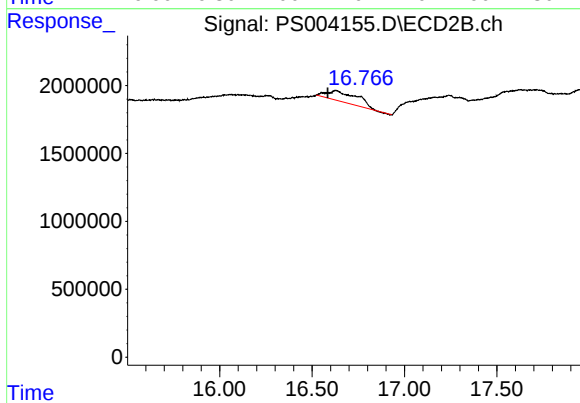

#16 DCPA

R.T.: 16.629 min
Delta R.T.: 0.044 min
Response: 8661077
Conc: 2.72 ng/ml