

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
 Data File : PS004166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2019 16:06
 Operator : EI\SJ
 Sample : MDL-BL-WATER-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:57:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.239	10.746	291.1E6	237.7E6	600.017	517.488
Target Compounds							
6) T	MCP	11.945	0.000	238734	0	<MDL	N.D. #
8) T	DICHLORPROP	12.758	0.000	5195439	0	10.732	N.D. #
10) T	Pentachlo...	13.463	0.000	1557135	0	<MDL	N.D. #
14) T	DINOSEB	16.943	0.000	782102	0	<MDL	N.D. #
15) T	Picloram	16.777	0.000	2884672	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
Data File : PS004166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 16:06
Operator : EI\SJ
Sample : MDL-BL-WATER-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:57:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

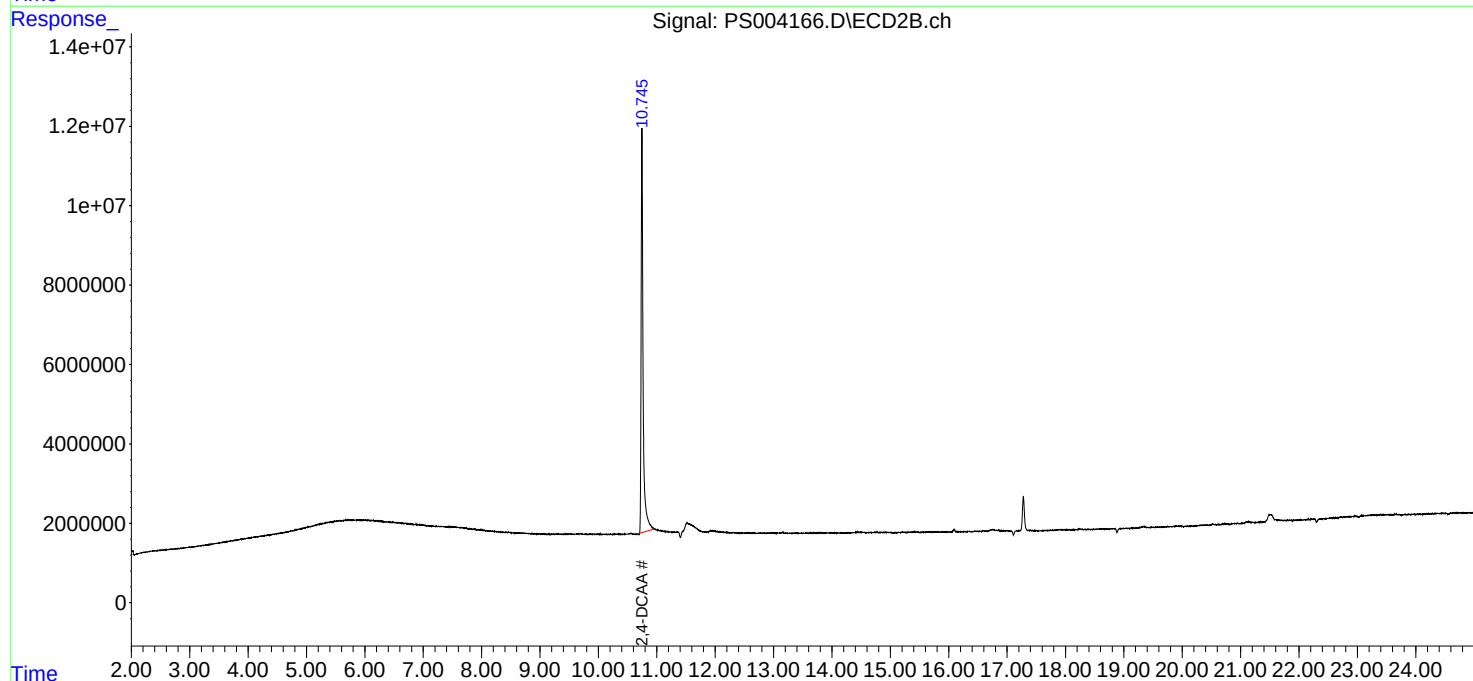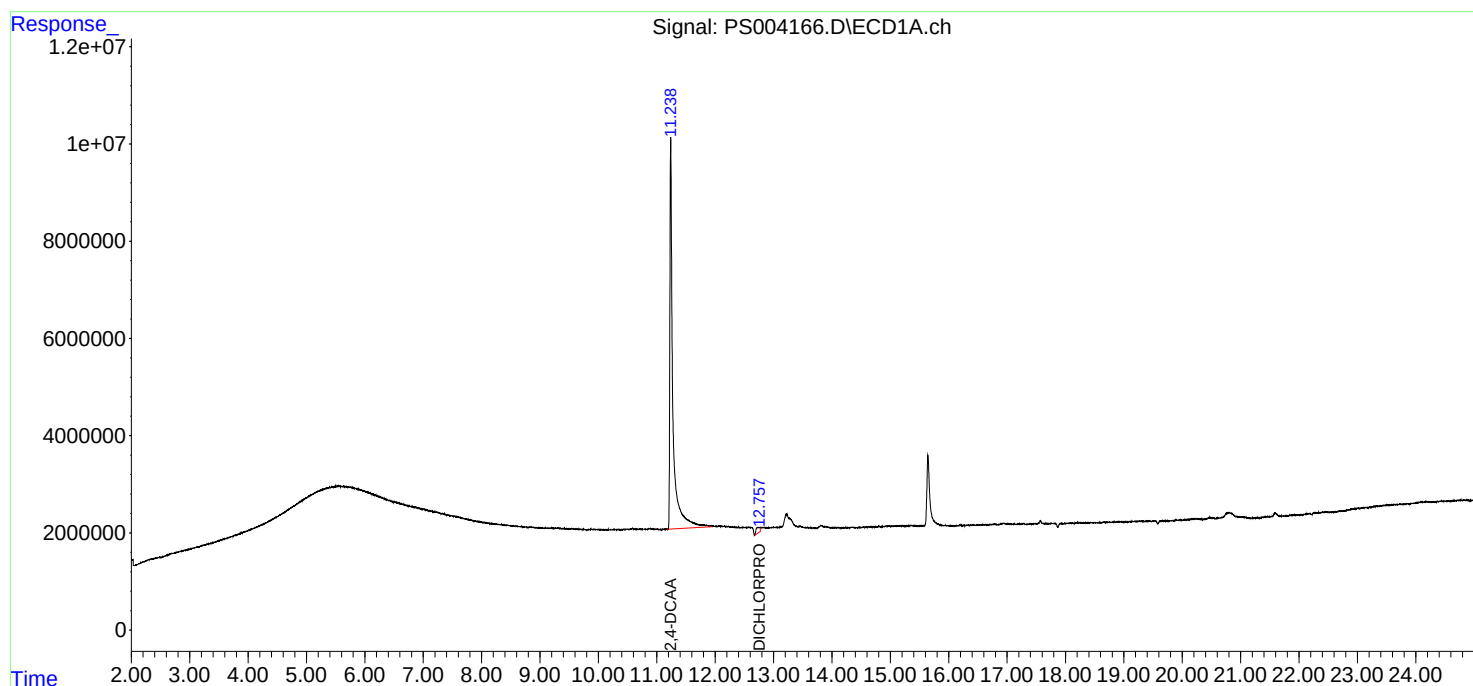


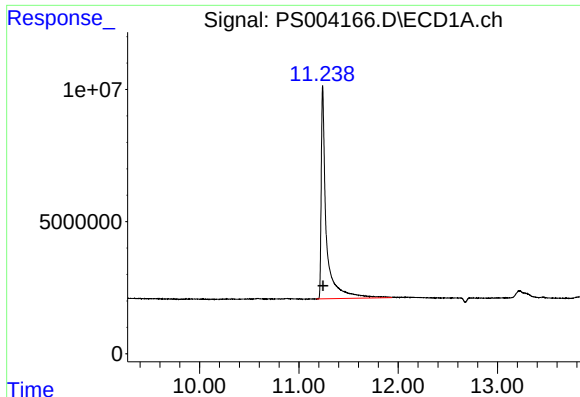

#4 2,4-DCAA


R.T.: 11.239 min
Delta R.T.: -0.005 min
Response: 291136858
Conc: 600.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-01

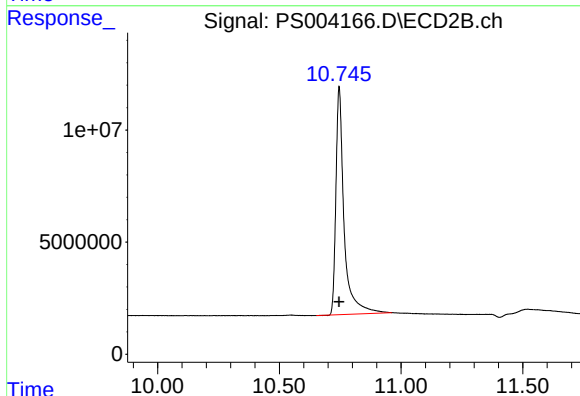


#4 2,4-DCAA

R.T.: 10.746 min
Delta R.T.: 0.000 min
Response: 237652286
Conc: 517.49 ng/ml

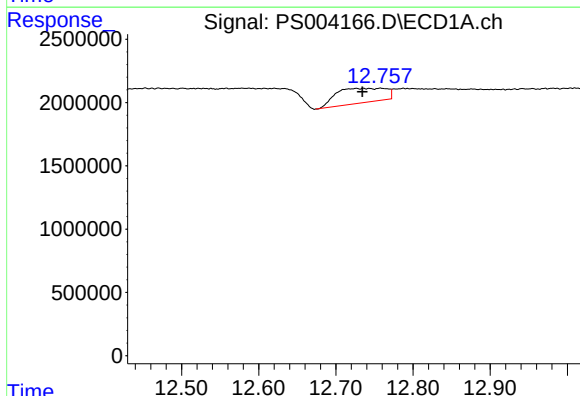

#8 DICHLORPROP

R.T.: 12.758 min
Delta R.T.: 0.024 min
Response: 5195439
Conc: 10.73 ng/ml

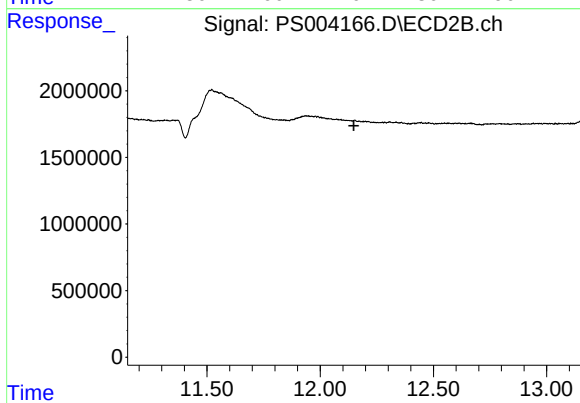

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.149 min
Response: 0
Conc: N.D.