

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
 Data File : PS004168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2019 17:10
 Operator : EI\SJ
 Sample : MDL-BL-WATER-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:58:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.229	10.730	202.6E6	165.4E6	417.566	360.130
Target Compounds							
3) T	4-Nitroph...	10.864	0.000	2290345	0	9.067	N.D. #
14) T	DINOSEB	16.937	0.000	7616687	0	3.040	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
Data File : PS004168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 17:10
Operator : EI\SJ
Sample : MDL-BL-WATER-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:58:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

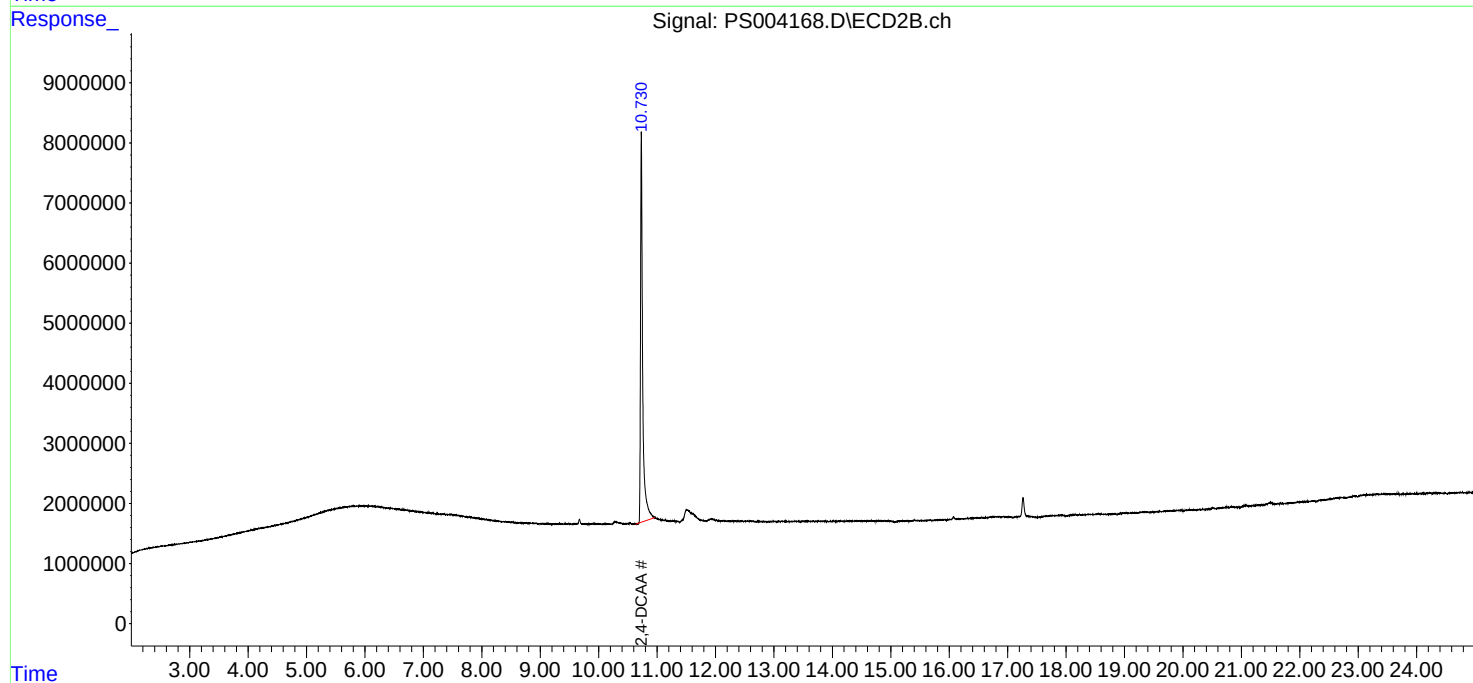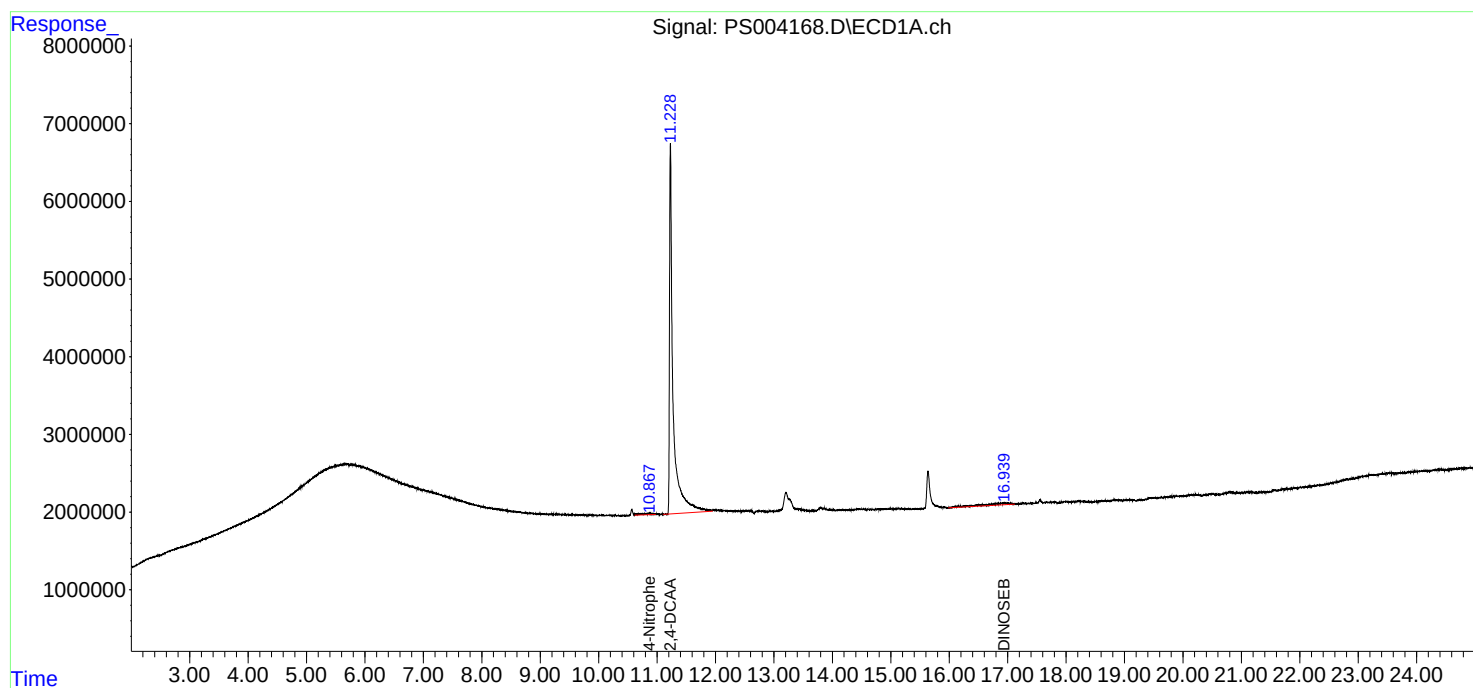


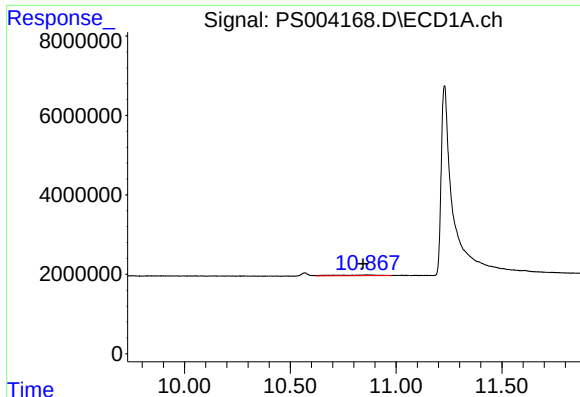

#3 4-Nitrophenol


R.T.: 10.864 min
Delta R.T.: 0.021 min
Response: 2290345
Conc: 9.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-02

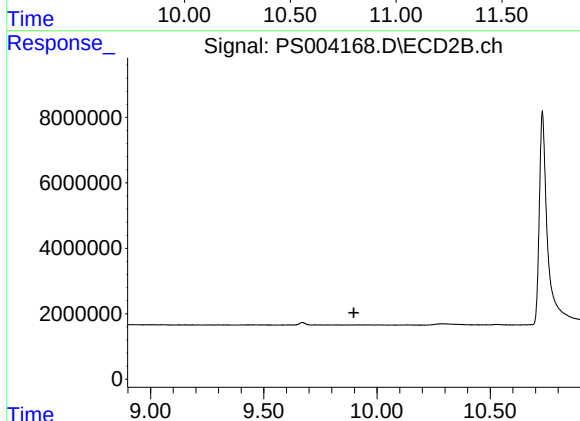


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.898 min
Response: 0
Conc: N.D.

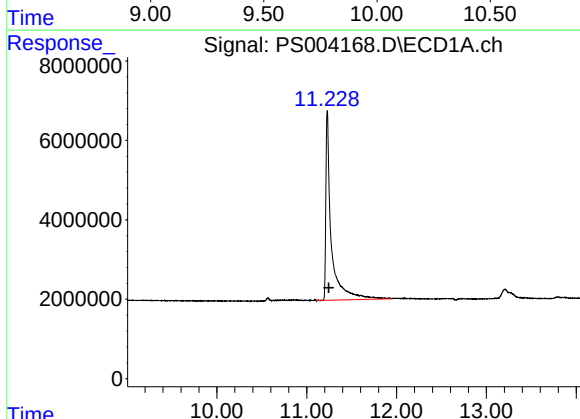


#4 2,4-DCAA

R.T.: 11.229 min
Delta R.T.: -0.015 min
Response: 202609078
Conc: 417.57 ng/ml

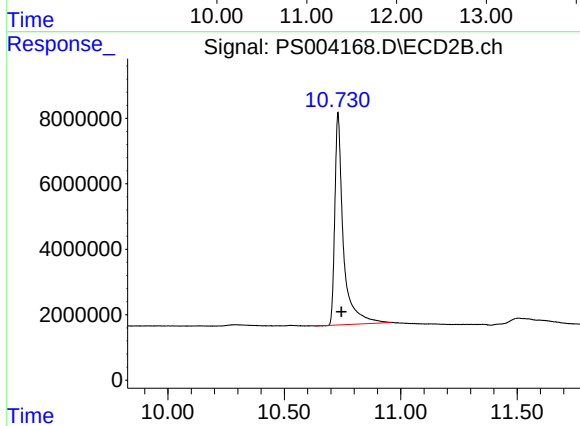

#4 2,4-DCAA


R.T.: 10.730 min
Delta R.T.: -0.015 min
Response: 165386887
Conc: 360.13 ng/ml

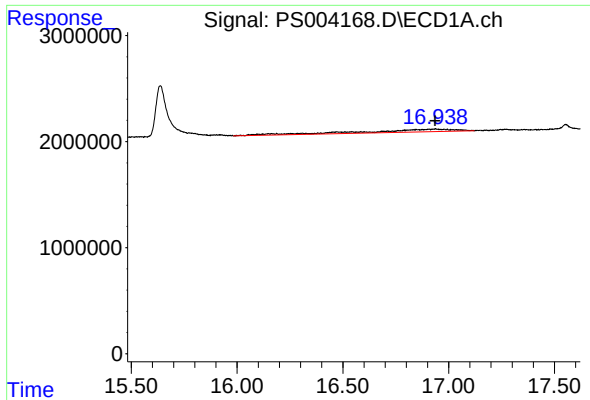

#14 DINOSEB

R.T.: 16.937 min
Delta R.T.: 0.001 min
Response: 7616687
Conc: 3.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-02

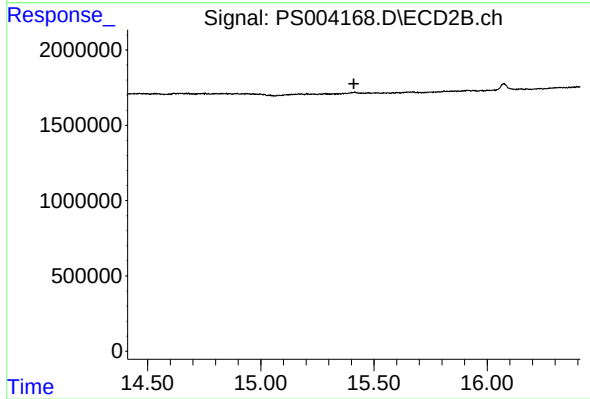

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.411 min
Response: 0
Conc: N.D.