

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
 Data File : PS004170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2019 18:14
 Operator : EI\SJ
 Sample : MDL-BL-WATER-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:58:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.210	10.713	206.8E6	167.3E6	426.290	364.365
Target Compounds							
3) T	4-Nitroph...	10.837	0.000	1784573	0	7.065	N.D. #
7) T	MCPA	0.000	11.585	0	5197421	N.D.	2.856
16) T	DCPA	17.251	0.000	8677452	0	2.411	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
Data File : PS004170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 18:14
Operator : EI\SJ
Sample : MDL-BL-WATER-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:58:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

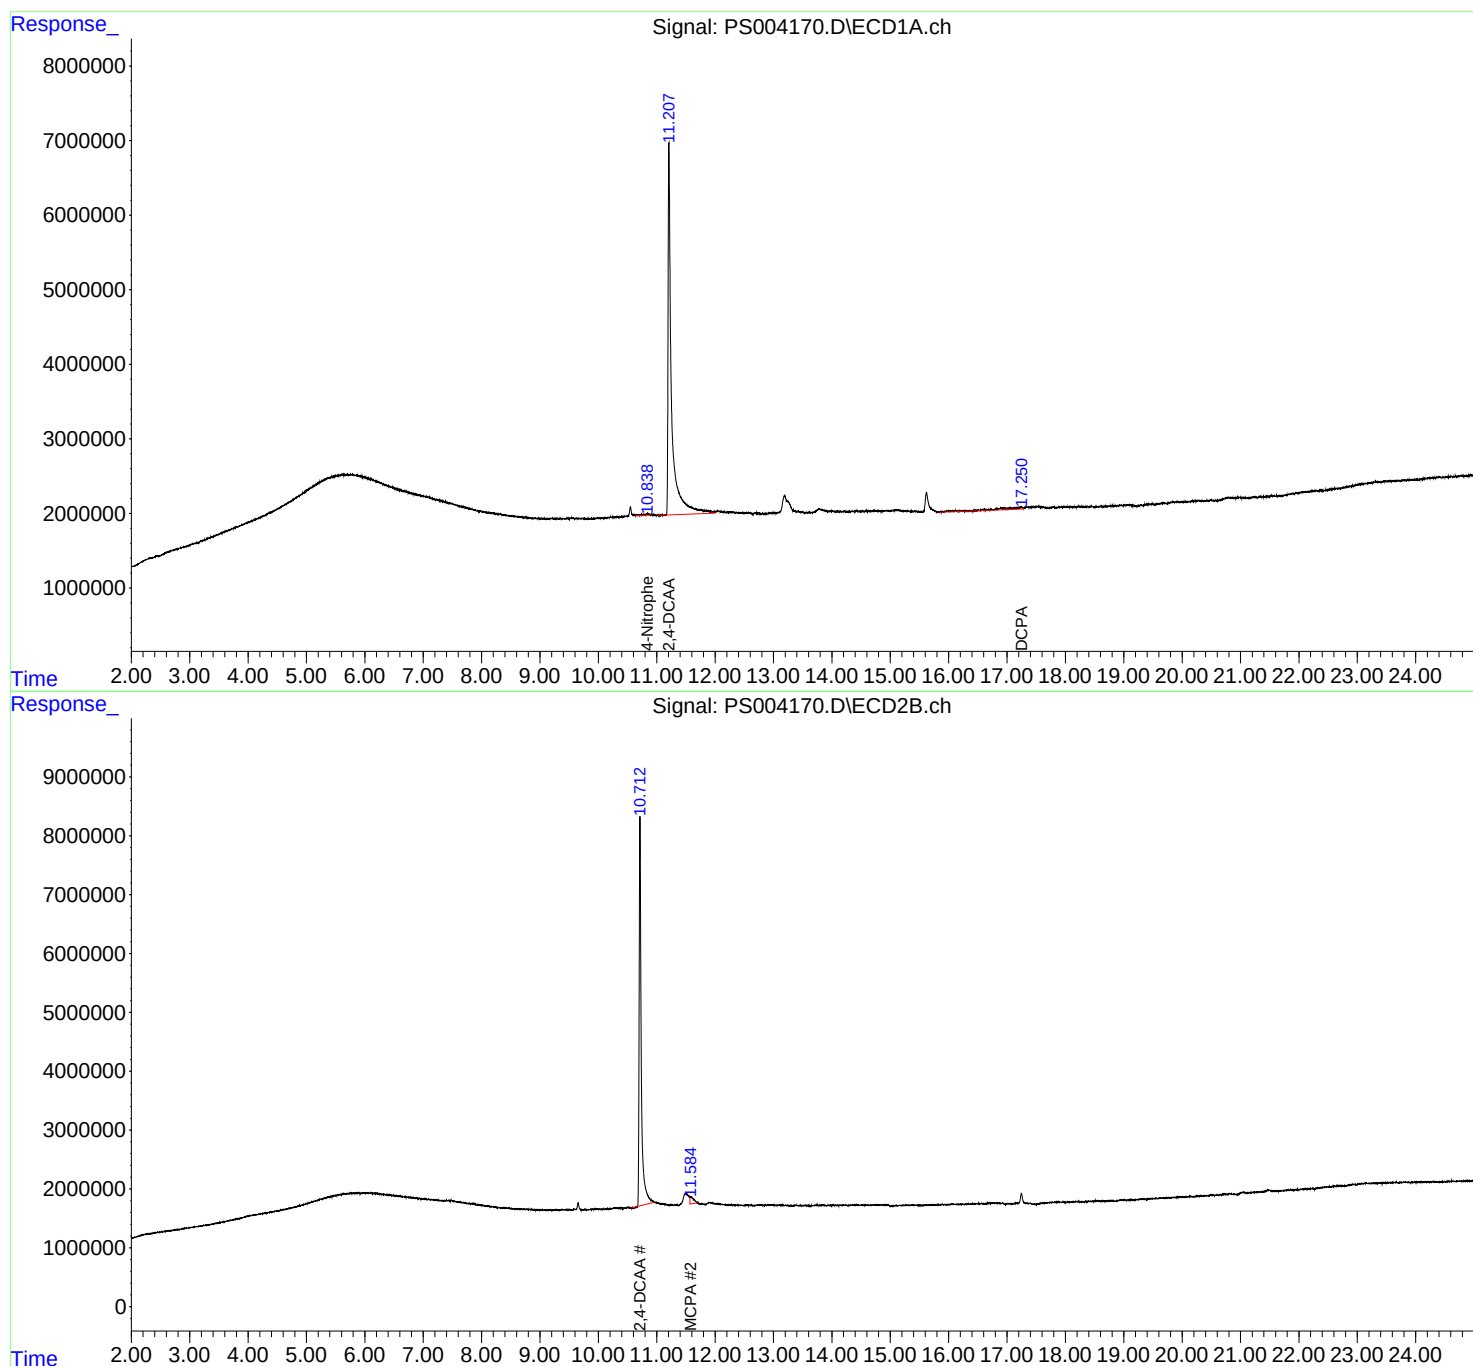


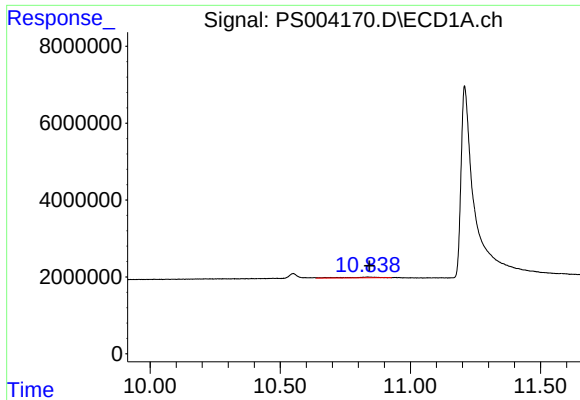

#3 4-Nitrophenol


R.T.: 10.837 min
Delta R.T.: -0.006 min
Response: 1784573
Conc: 7.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-03

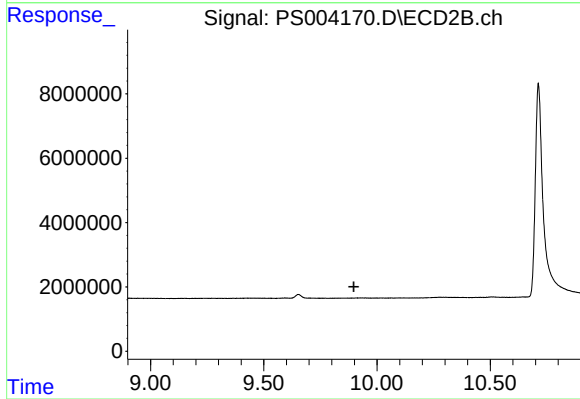


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.898 min
Response: 0
Conc: N.D.

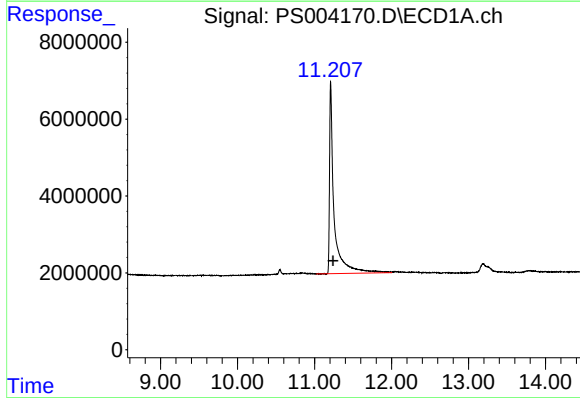


#4 2,4-DCAA

R.T.: 11.210 min
Delta R.T.: -0.034 min
Response: 206842195
Conc: 426.29 ng/ml

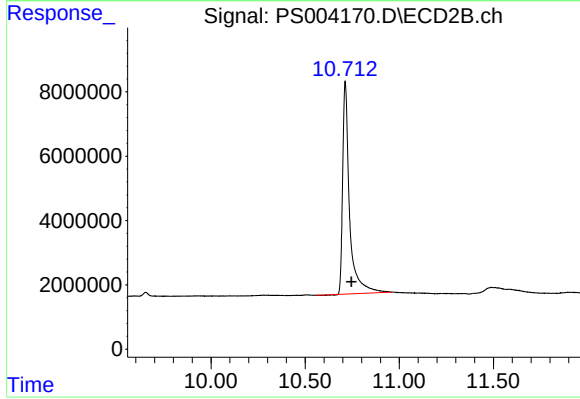

#4 2,4-DCAA


R.T.: 10.713 min
Delta R.T.: -0.033 min
Response: 167331730
Conc: 364.37 ng/ml

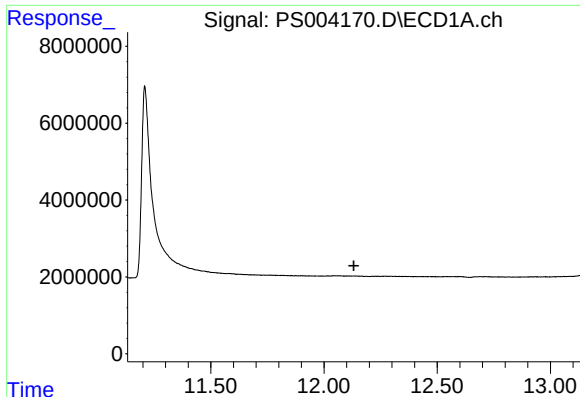

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-03

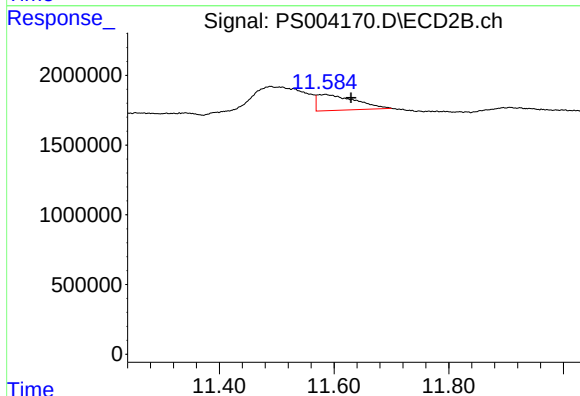


#7 MCPA

R.T.: 11.585 min
Delta R.T.: -0.045 min
Response: 5197421
Conc: 2.86 ug/ml

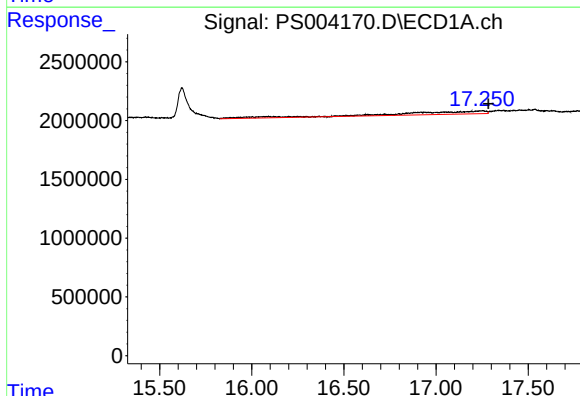

#16 DCPA

R.T.: 17.251 min
Delta R.T.: -0.033 min
Response: 8677452
Conc: 2.41 ng/ml

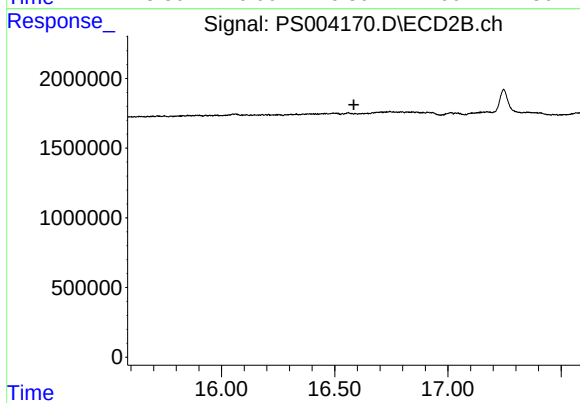

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 16.584 min
Response: 0
Conc: N.D.