

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
 Data File : PS004172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2019 19:17
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:59:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.206	10.712	291.0E6	231.5E6	599.746	504.006
Target Compounds							
7) T	MCPA	0.000	11.574	0	5220137	N.D.	2.869
10) T	Pentachlo...	13.422	0.000	570447	0	<MDL	N.D. #
16) T	DCPA	17.240	0.000	4497277	0	1.249	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041919\
Data File : PS004172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 19:17
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:59:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

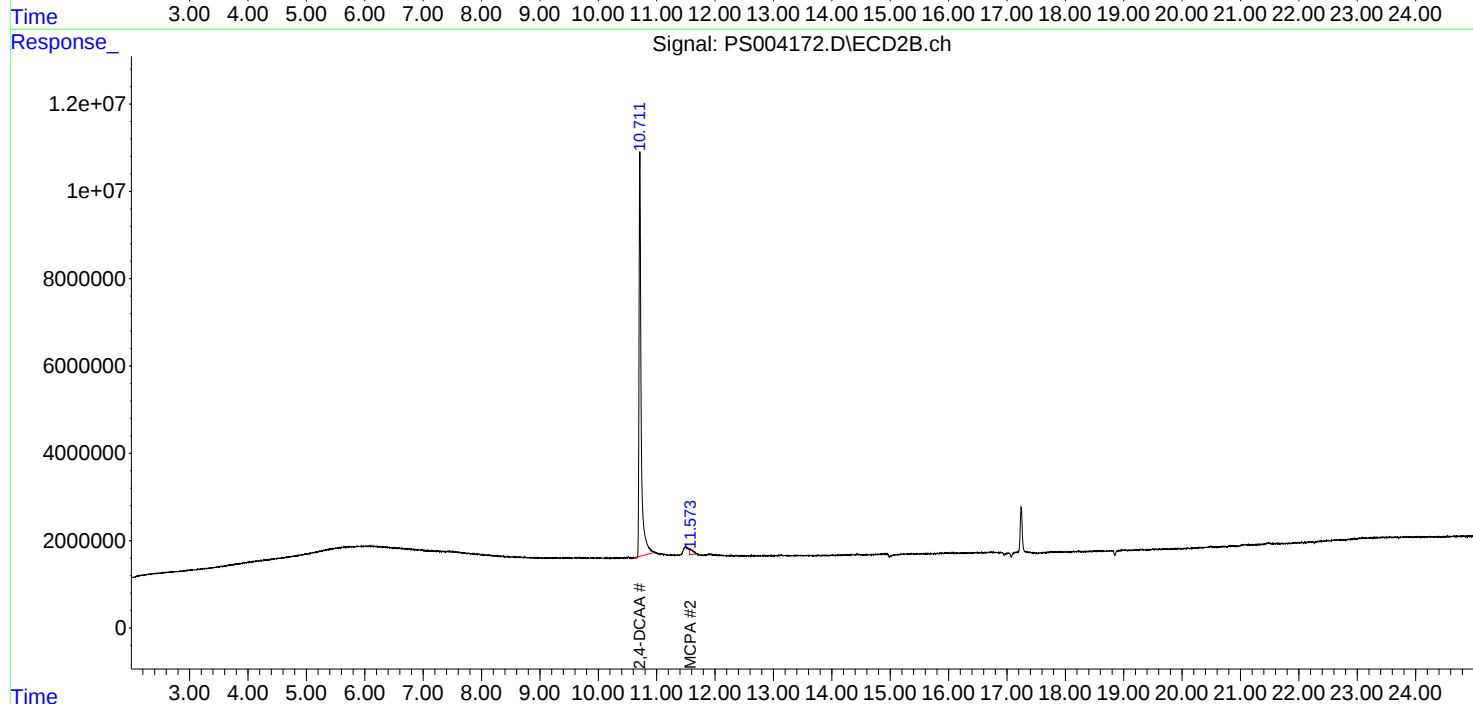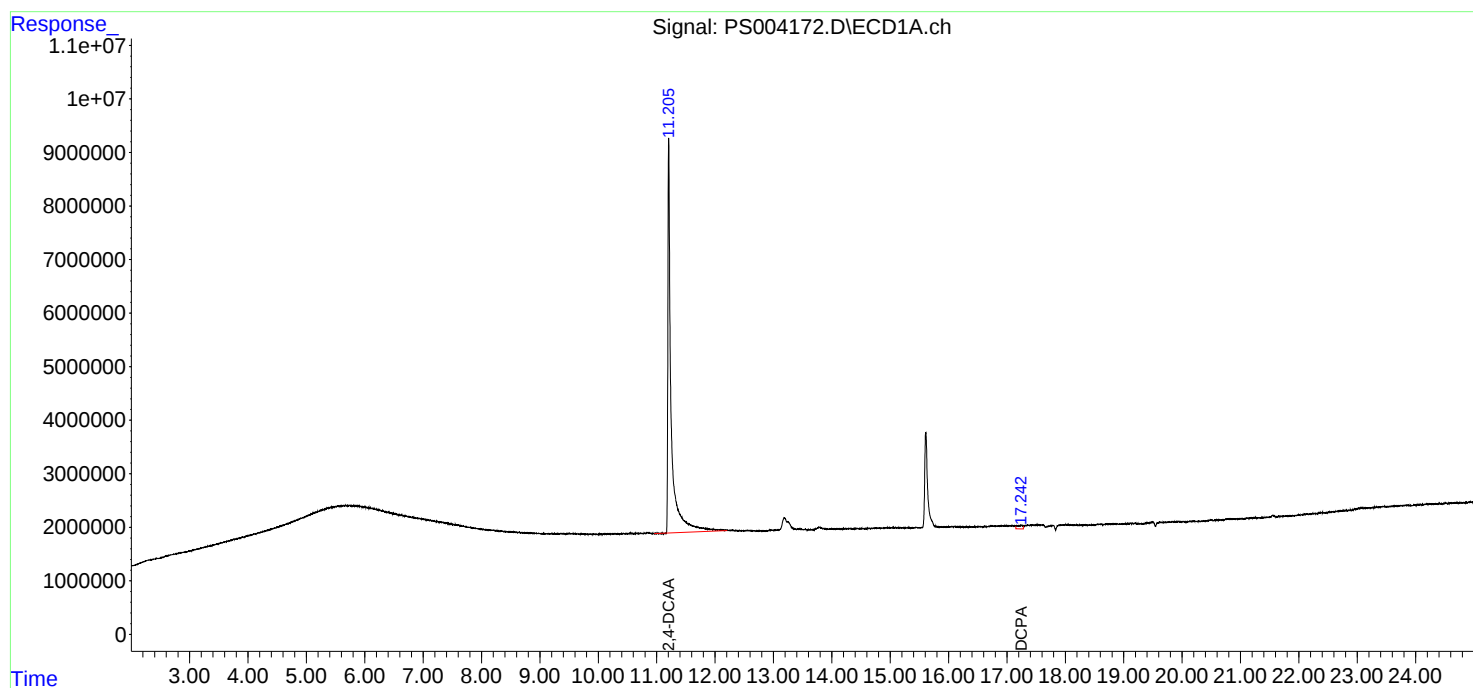


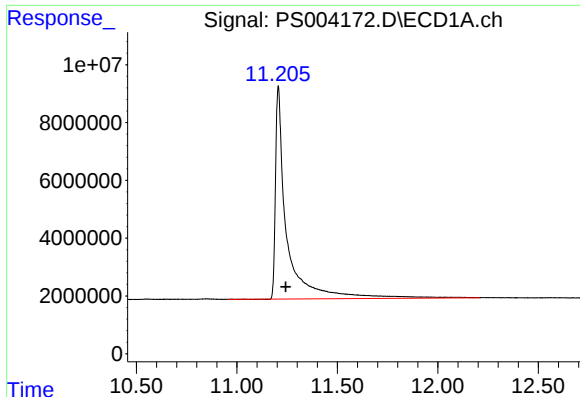

#4 2,4-DCAA


R.T.: 11.206 min
Delta R.T.: -0.037 min
Response: 291005568
Conc: 599.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

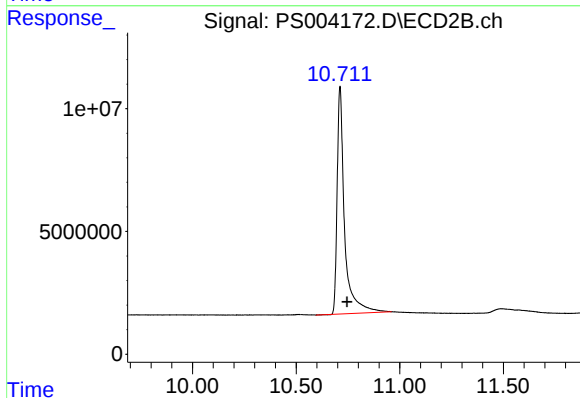


#4 2,4-DCAA

R.T.: 10.712 min
Delta R.T.: -0.034 min
Response: 231460854
Conc: 504.01 ng/ml

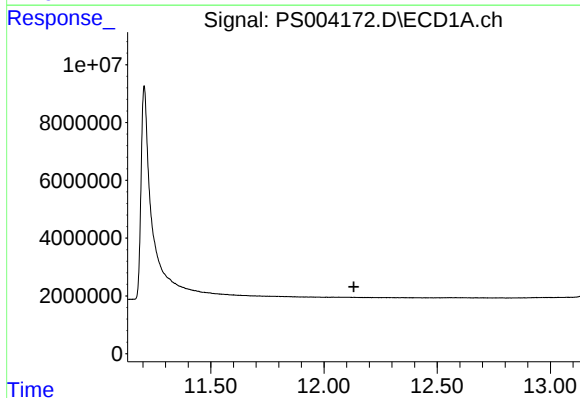


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.132 min
Response: 0
Conc: N.D.

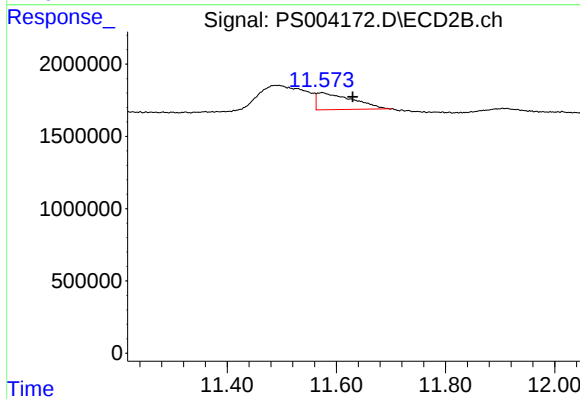

#7 MCPA


R.T.: 11.574 min
Delta R.T.: -0.056 min
Response: 5220137
Conc: 2.87 ug/ml

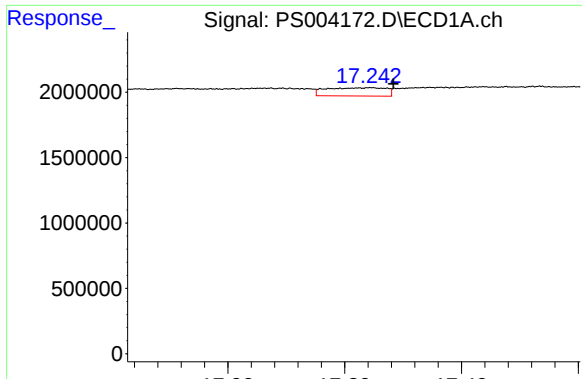

#16 DCPA

R.T.: 17.240 min
Delta R.T.: -0.043 min
Response: 4497277
Conc: 1.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

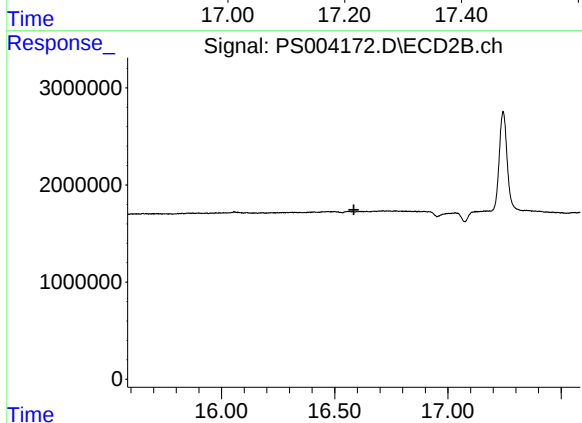

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.584 min
Response: 0
Conc: N.D.