

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041922\
 Data File : PS019063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 17:51
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 01:59:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.472f	0.000	12216983	0	2.457	N.D. #
3) T	4-Nitroph...	7.007f	0.000	3059452	0	2.336	N.D. #
5) T	DICAMBA	0.000	7.025f	0	1526216	N.D.	<MDL
6) T	MCP	0.000	7.025f	0	1526216	N.D.	<MDL
7) T	MCPA	7.684f	0.000	5977573	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.261f	8.629f	9508991	2849905	<MDL	<MDL #
12) T	2,4,5-T	9.488	9.113f	4775752	3927401	<MDL	<MDL #
13) T	2,4-DB	0.000	9.483f	0	6377059	N.D.	11.504
14) T	DINOSEB	11.148f	0.000	26920954	0	1.759	N.D. #
15) T	Picloram	11.038	10.877	116.4E6	20525122	4.345	3.466
16) T	DCPA	0.000	10.877f	0	20525122	N.D.	3.586


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041922\
Data File : PS019063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 17:51
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 01:59:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

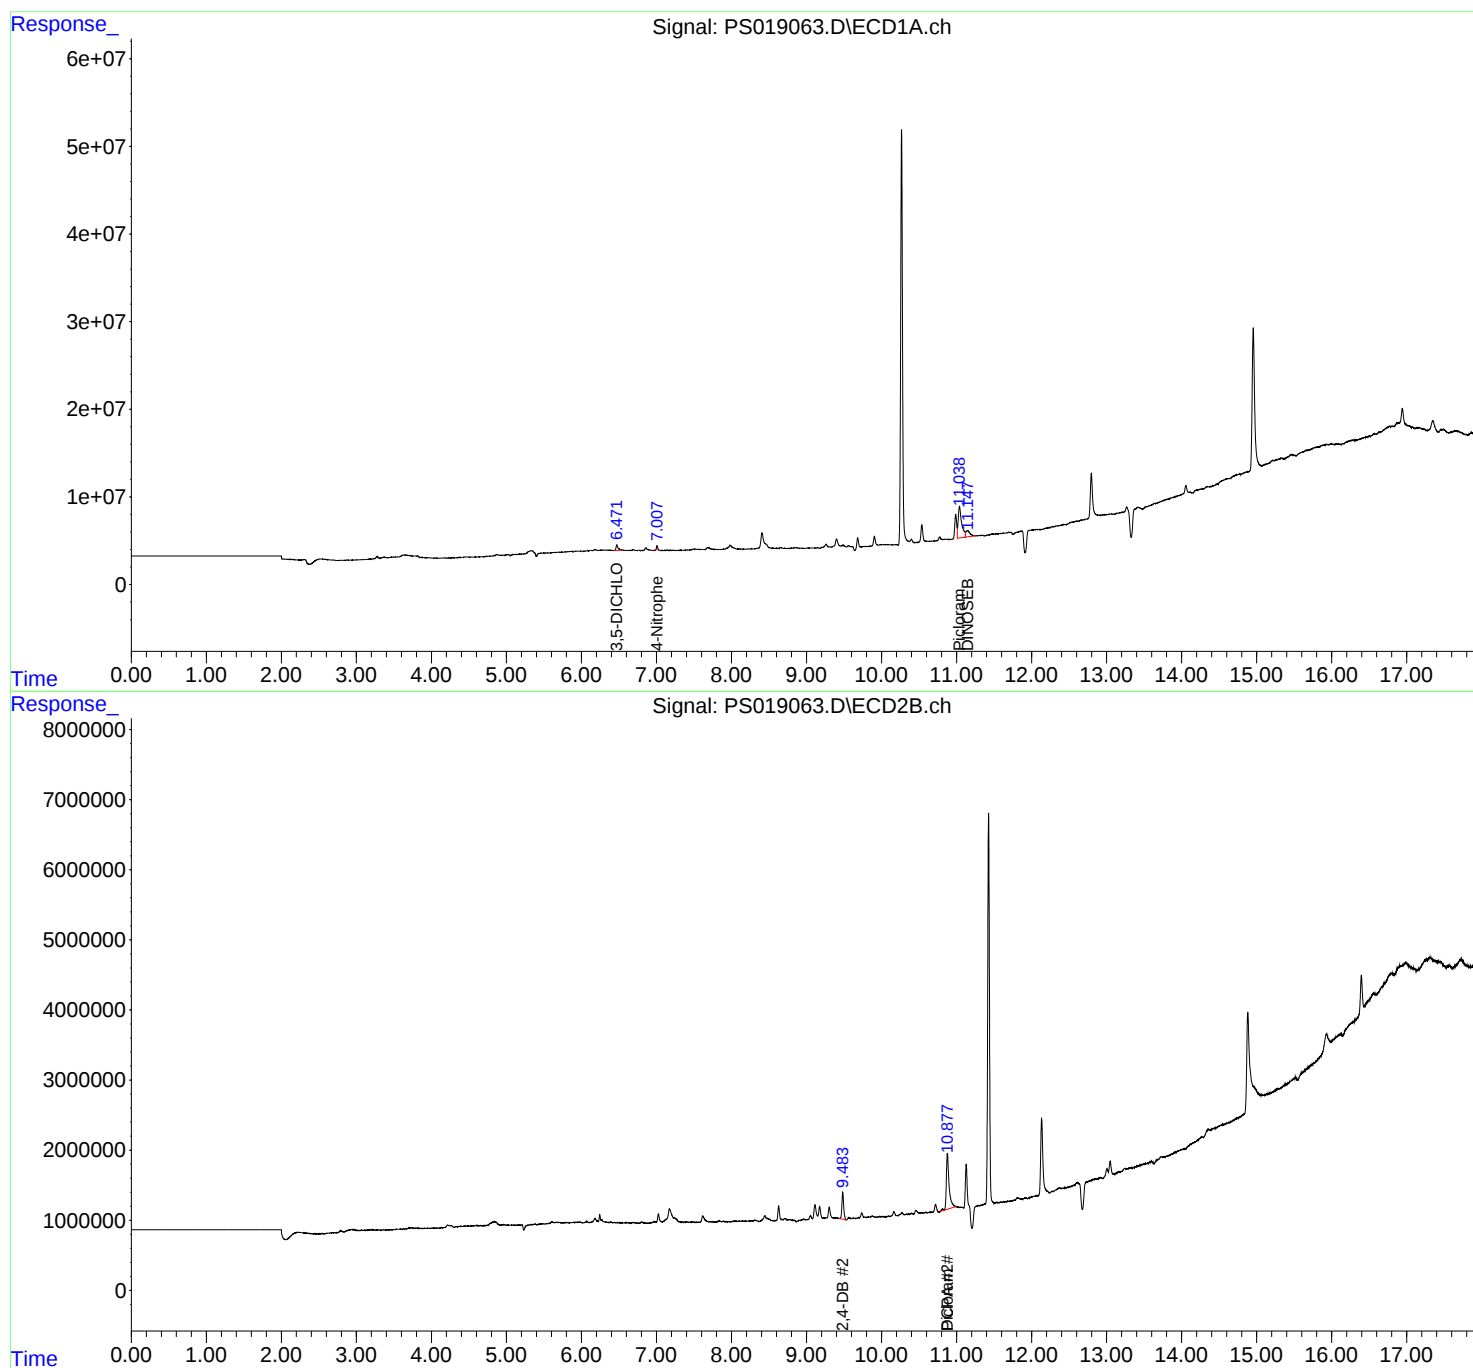


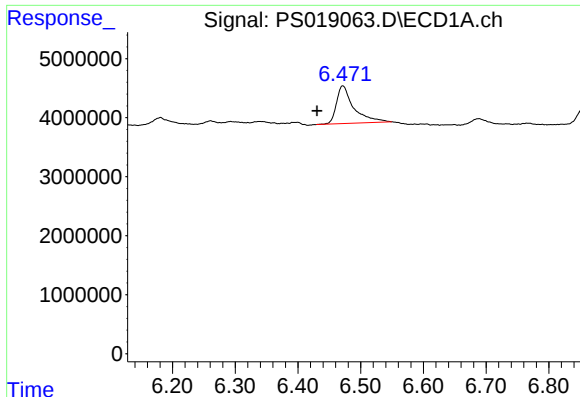

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.472 min
Delta R.T.: 0.041 min
Response: 12216983
Conc: 2.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

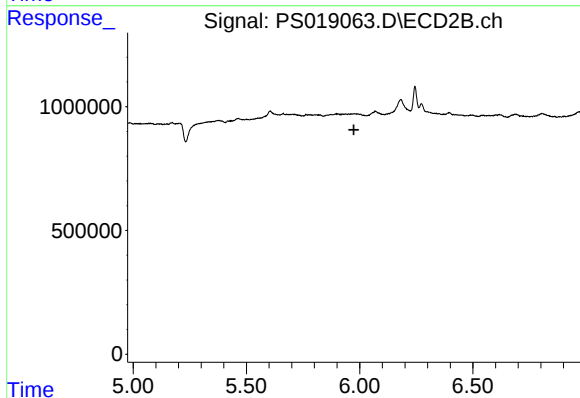


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.975 min
Response: 0
Conc: N.D.

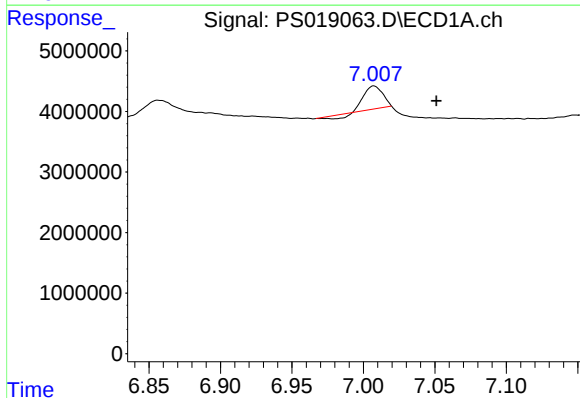


#3 4-Nitrophenol

R.T.: 7.007 min
Delta R.T.: -0.044 min
Response: 3059452
Conc: 2.34 ng/ml

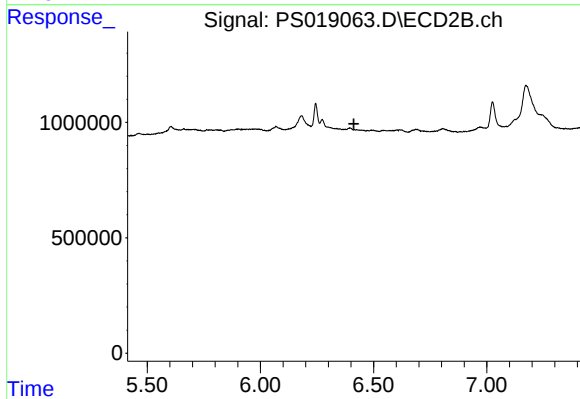

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.413 min
Response: 0
Conc: N.D.

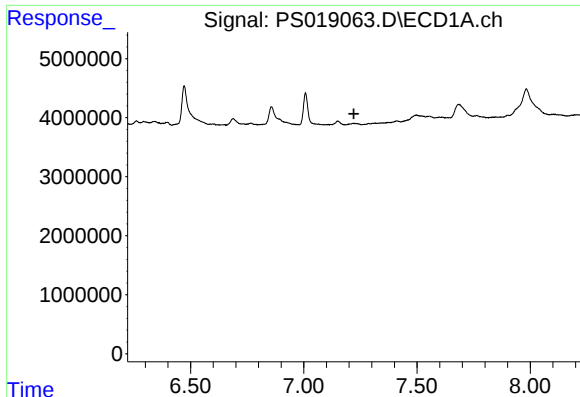

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

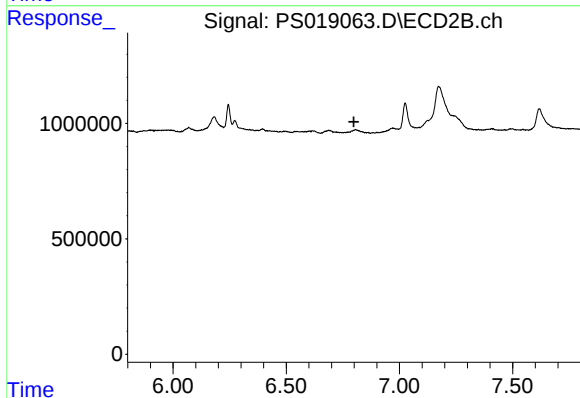


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

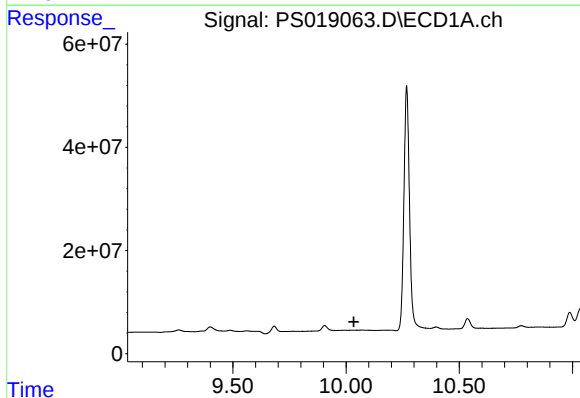


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.034 min
Response: 0
Conc: N.D.

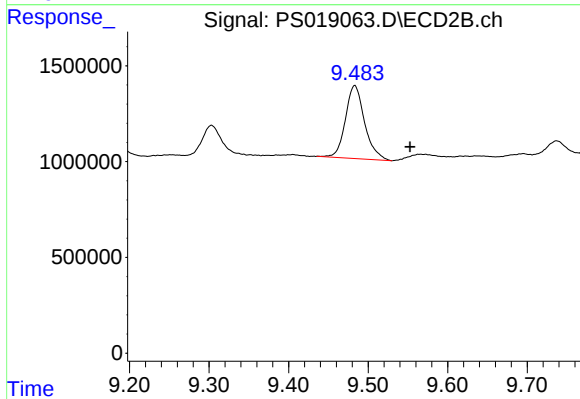

#13 2,4-DB


R.T.: 9.483 min
Delta R.T.: -0.069 min
Response: 6377059
Conc: 11.50 ng/ml

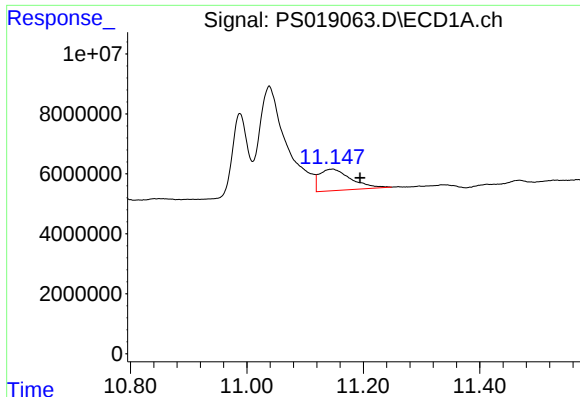

#14 DINoseb


R.T.: 11.148 min
Delta R.T.: -0.047 min
Response: 26920954
Conc: 1.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

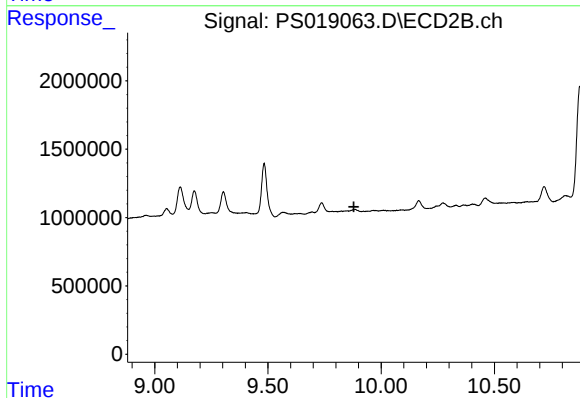


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

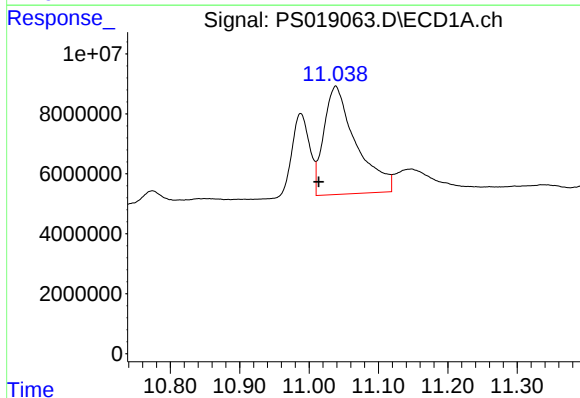


#15 Picloram

R.T.: 11.038 min
Delta R.T.: 0.024 min
Response: 116423736
Conc: 4.34 ng/ml

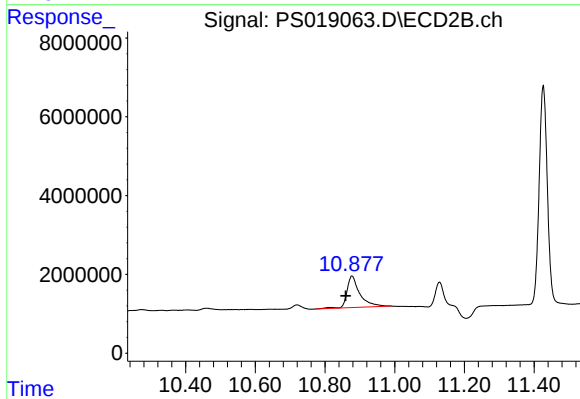

#15 Picloram


R.T.: 10.877 min
Delta R.T.: 0.017 min
Response: 20525122
Conc: 3.47 ng/ml

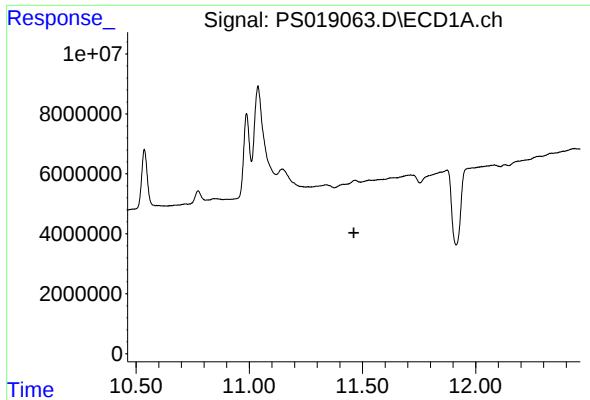

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

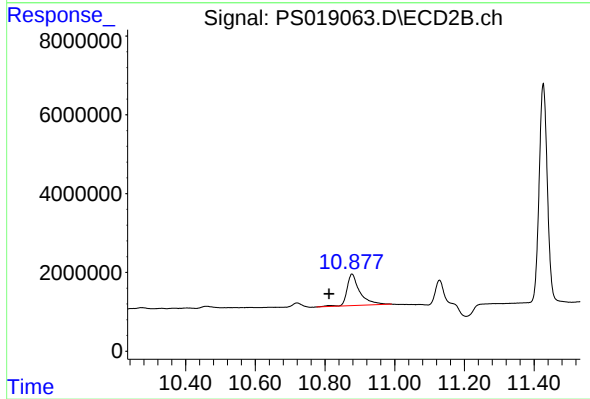

#16 DCPA

R.T.: 10.877 min
Delta R.T.: 0.066 min
Response: 20525122
Conc: 3.59 ng/ml