

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041922\
 Data File : PS019076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 01:01
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:04:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.798	1630.6E6	388.2E6	435.986	534.868
Target Compounds							
8) T	DICHLORPROP	0.000	7.612	0	1424819	N.D.	1.705
10) T	Pentachlo...	8.651	0.000	1566300	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.257f	8.627f	39719294	4853222	1.995	1.031 #
12) T	2,4,5-T	9.482	9.049	7602547	2083599	<MDL	<MDL #
13) T	2,4-DB	9.989f	0.000	25581994	0	7.264	N.D. #
14) T	DINOSEB	11.232	0.000	255.5E6	0	16.697	N.D. #
15) T	Picloram	11.024	10.867	47364219	11429365	1.768	1.930
16) T	DCPA	0.000	10.867f	0	11429365	N.D.	1.997



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041922\
Data File : PS019076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 01:01
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:04:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

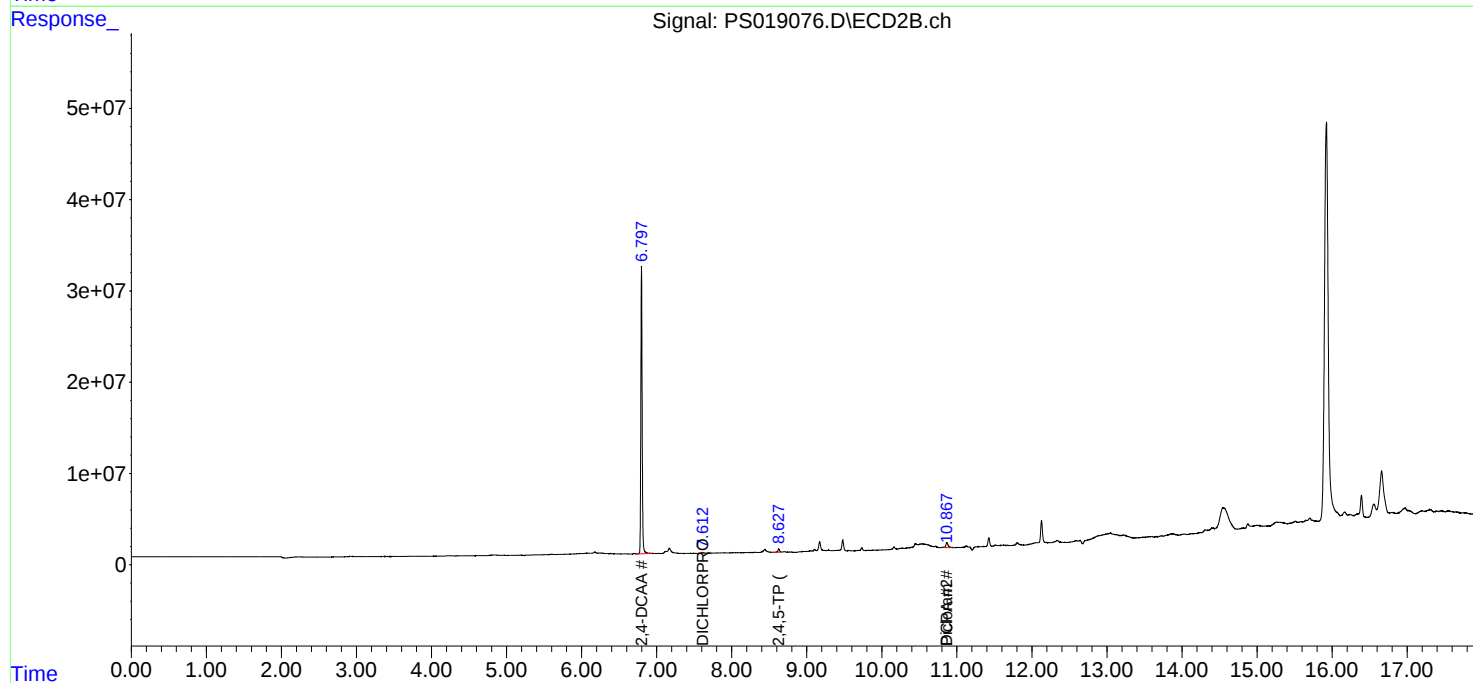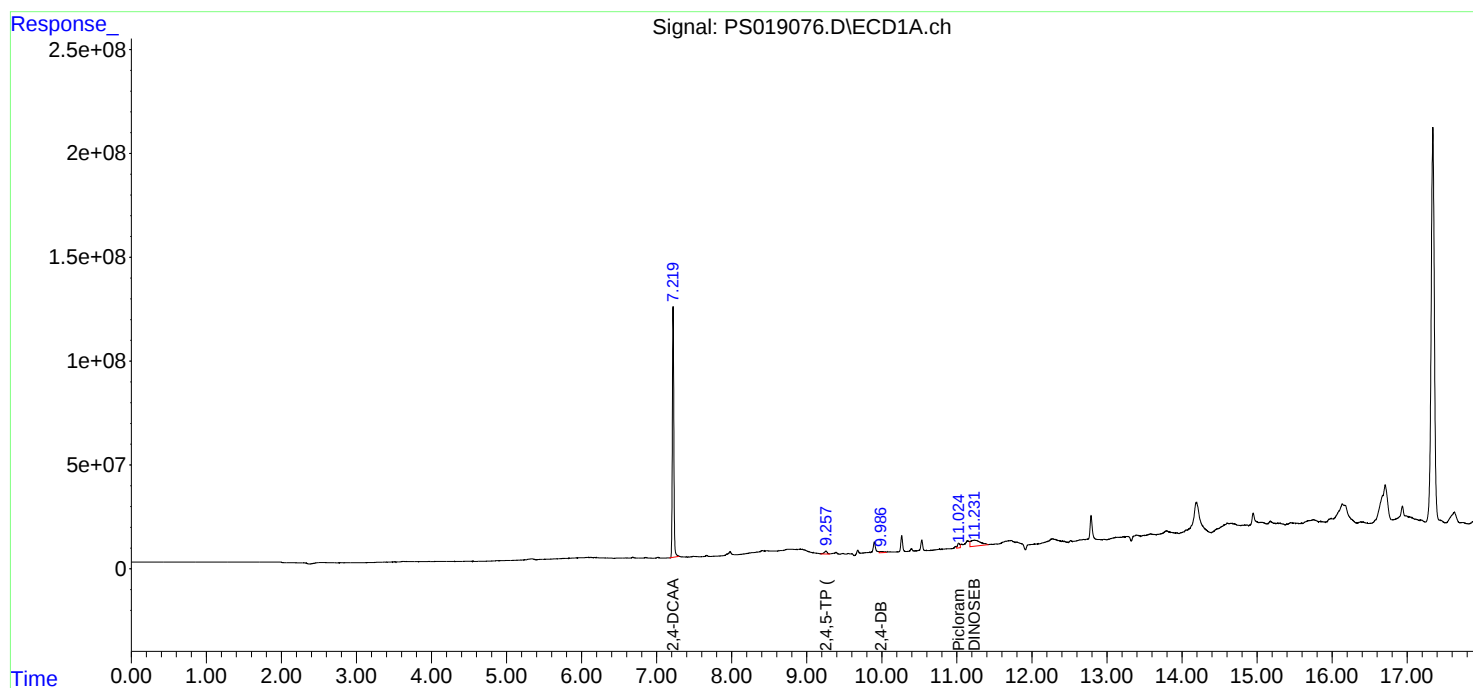


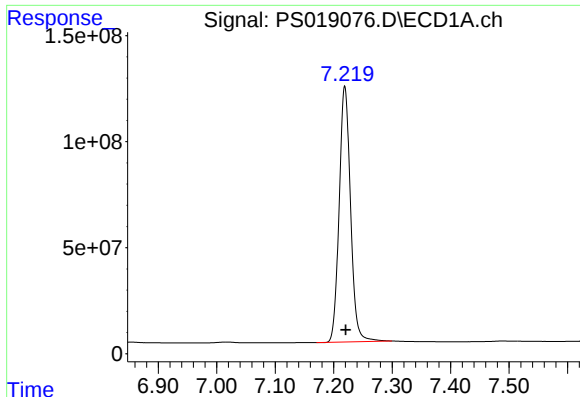

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.002 min
Response: 1630610711
Conc: 435.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

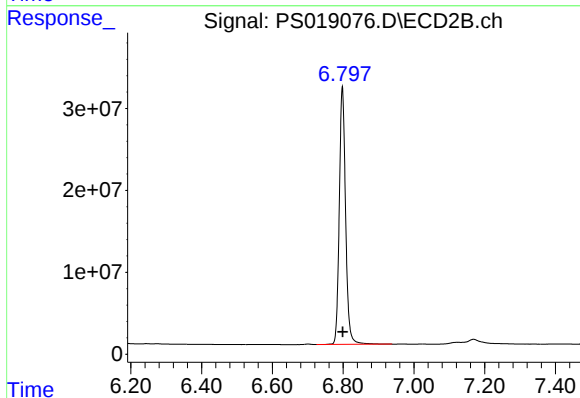


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 388248086
Conc: 534.87 ng/ml

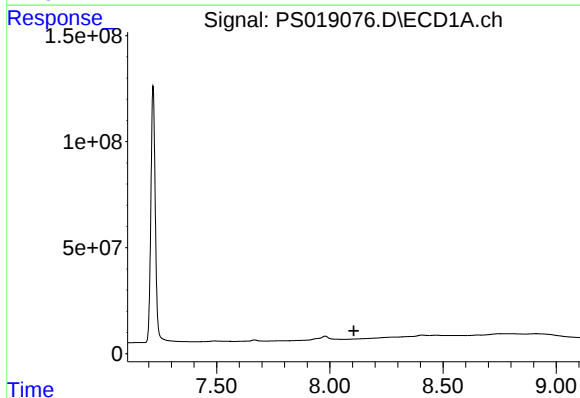


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.106 min
Response: 0
Conc: N.D.

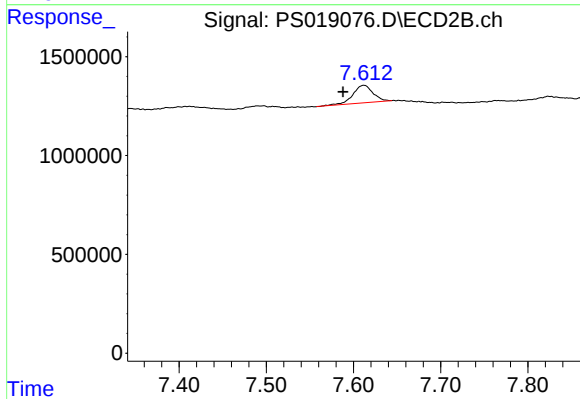

#8 DICHLORPROP


R.T.: 7.612 min
Delta R.T.: 0.024 min
Response: 1424819
Conc: 1.71 ng/ml

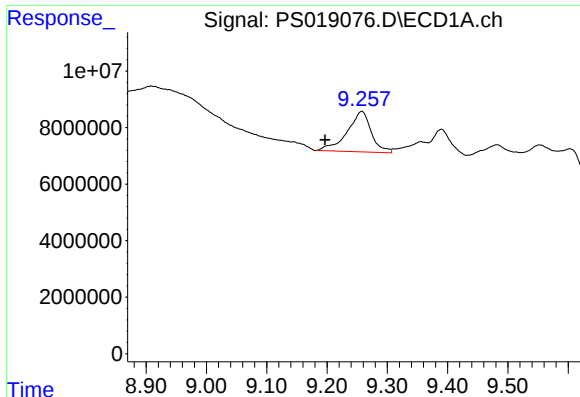

#11 2,4,5-TP (SILVEX)


R.T.: 9.257 min
Delta R.T.: 0.060 min
Response: 39719294
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

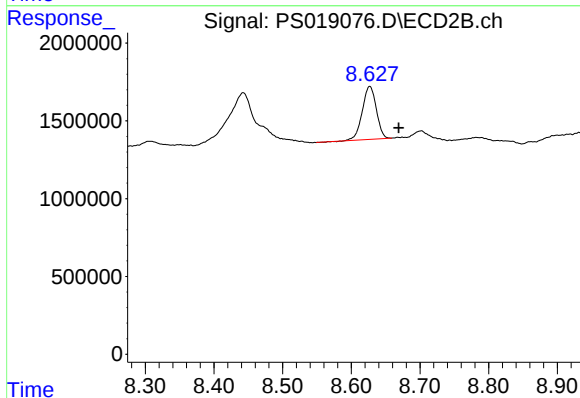


#11 2,4,5-TP (SILVEX)

R.T.: 8.627 min
Delta R.T.: -0.042 min
Response: 4853222
Conc: 1.03 ng/ml

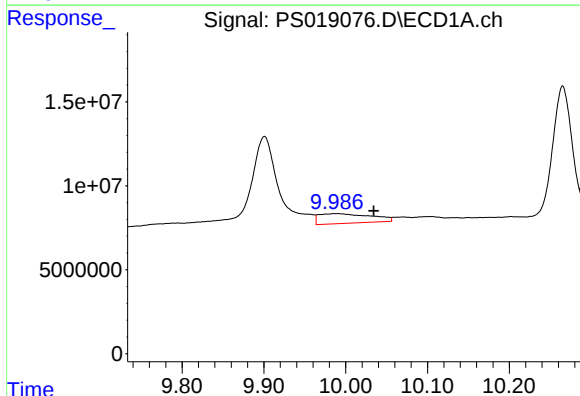


#13 2,4-DB

R.T.: 9.989 min
Delta R.T.: -0.046 min
Response: 25581994
Conc: 7.26 ng/ml

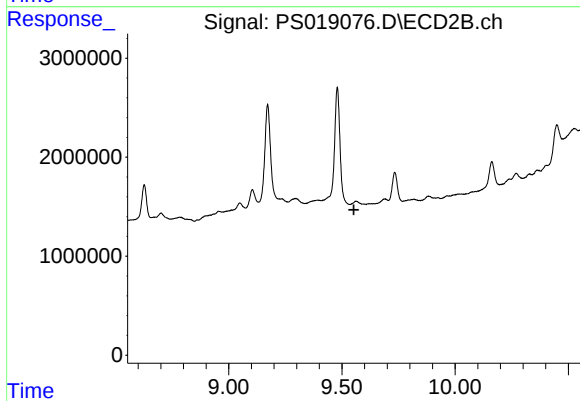

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.553 min
Response: 0
Conc: N.D.

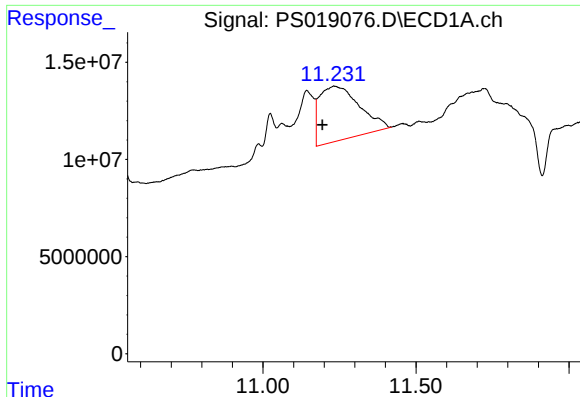

#14 DINOSEB


R.T.: 11.232 min
Delta R.T.: 0.038 min
Response: 255480979
Conc: 16.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

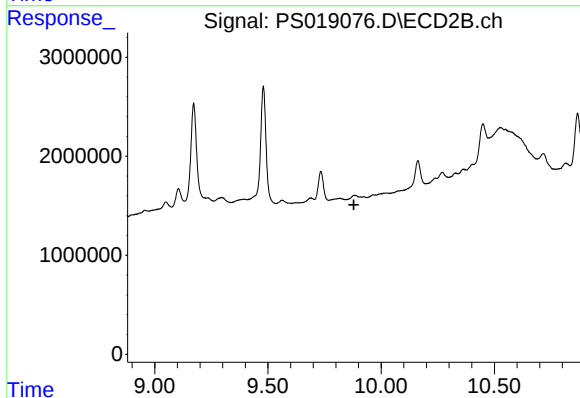


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

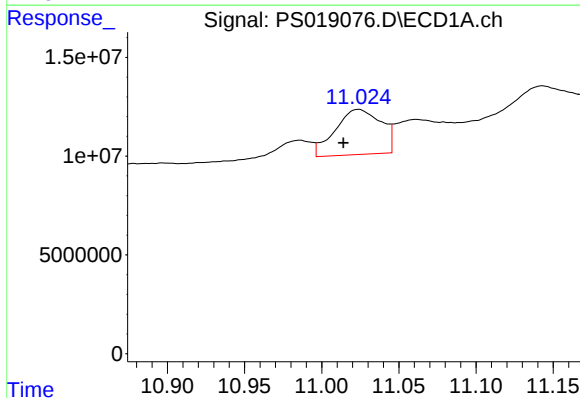


#15 Picloram

R.T.: 11.024 min
Delta R.T.: 0.010 min
Response: 47364219
Conc: 1.77 ng/ml

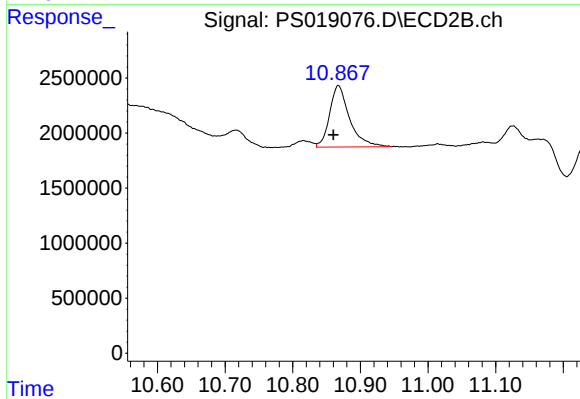

#15 Picloram


R.T.: 10.867 min
Delta R.T.: 0.008 min
Response: 11429365
Conc: 1.93 ng/ml

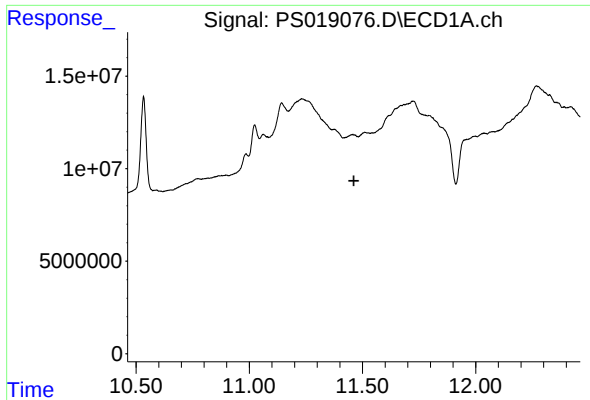

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

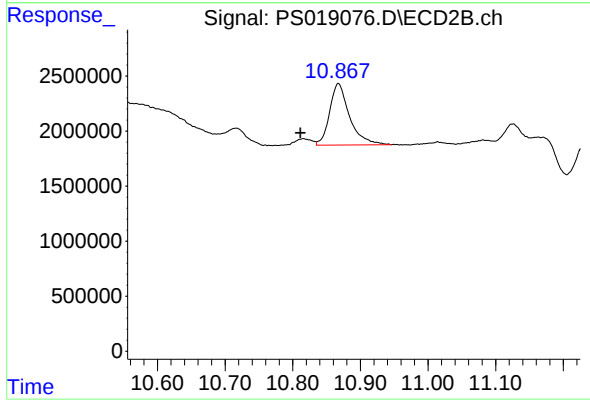

#16 DCPA

R.T.: 10.867 min
Delta R.T.: 0.056 min
Response: 11429365
Conc: 2.00 ng/ml