

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041922\
 Data File : PS019082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 05:23
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 06:14:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.798	1687.7E6	387.8E6	451.259	534.255
Target Compounds							
9) T	2,4-D	8.343	0.000	6364995	0	1.551	N.D. #
10) T	Pentachlo...	8.648	0.000	3876403	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.257f	8.626f	40852277	7377298	2.051	1.567
12) T	2,4,5-T	9.481	9.049	21903096	3628363	1.102	<MDL #
13) T	2,4-DB	10.072	0.000	9164511	0	2.602	N.D. #
14) T	DINOSEB	11.198	0.000	65200812	0	4.261	N.D. #
15) T	Picloram	11.025	10.868	56330099	14294292	2.102	2.414
16) T	DCPA	11.519f	10.868f	3454676	14294292	<MDL	2.497 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041922\
Data File : PS019082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 05:23
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 06:14:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

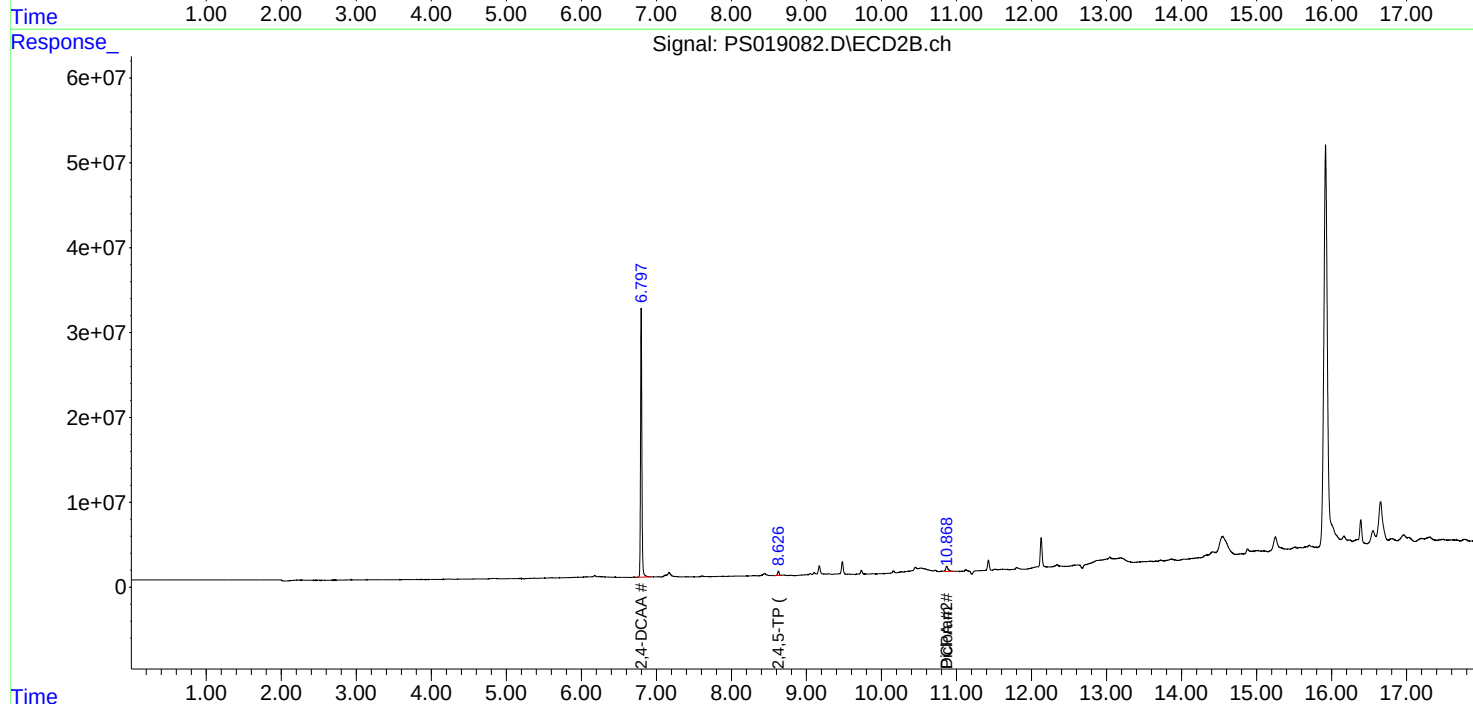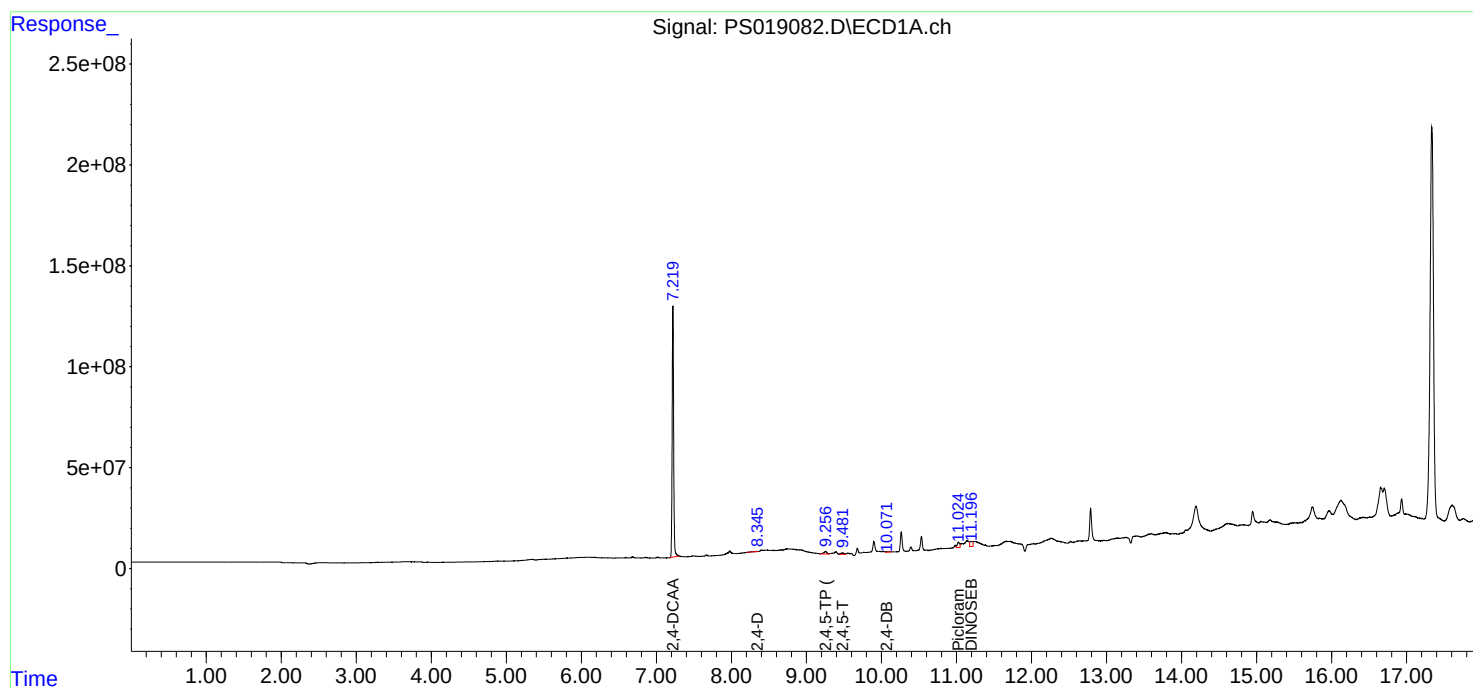


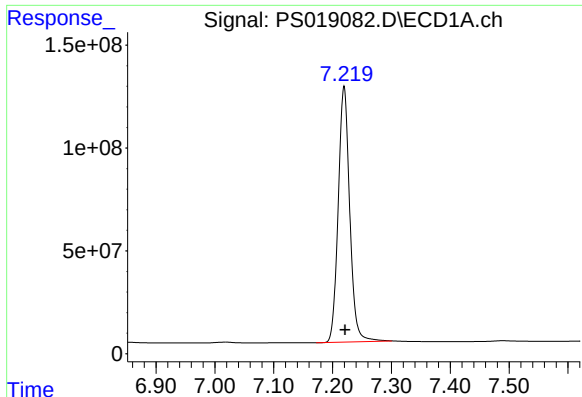

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: -0.002 min
Response: 1687733997
Conc: 451.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

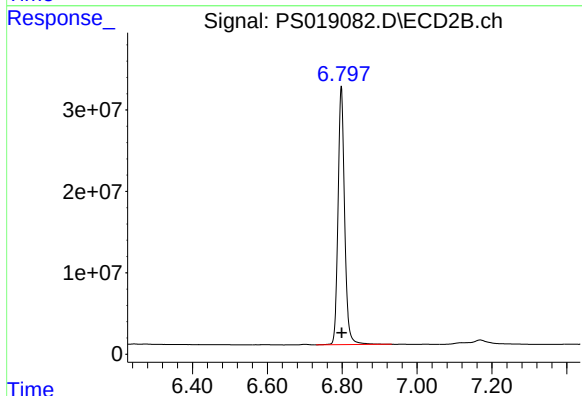


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: -0.001 min
Response: 387803395
Conc: 534.25 ng/ml

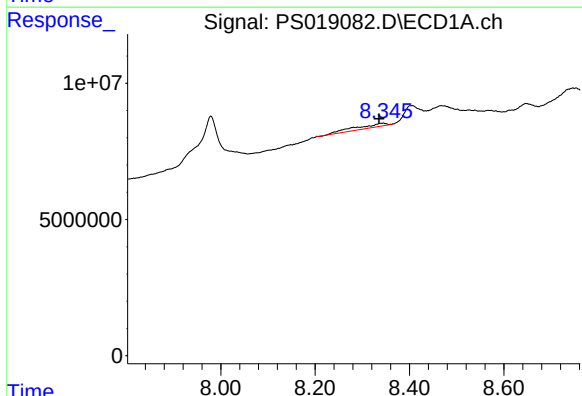


#9 2,4-D

R.T.: 8.343 min
Delta R.T.: 0.008 min
Response: 6364995
Conc: 1.55 ng/ml

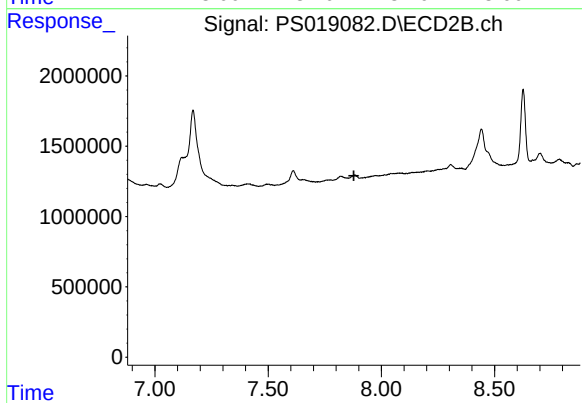

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.879 min
Response: 0
Conc: N.D.

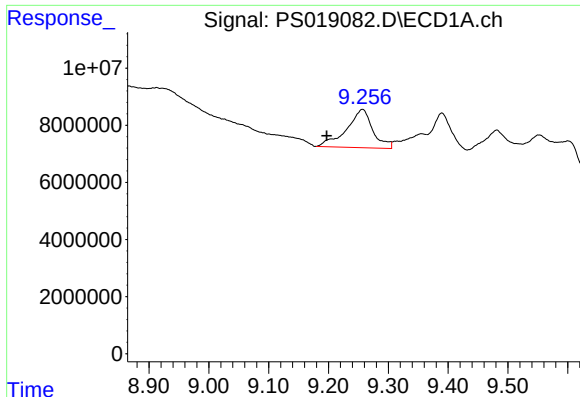

#11 2,4,5-TP (SILVEX)


R.T.: 9.257 min
Delta R.T.: 0.060 min
Response: 40852277
Conc: 2.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

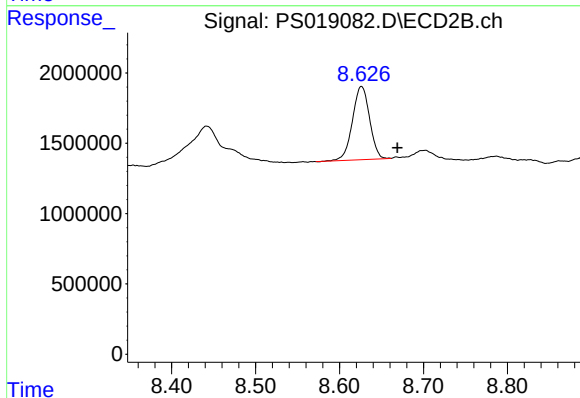


#11 2,4,5-TP (SILVEX)

R.T.: 8.626 min
Delta R.T.: -0.043 min
Response: 7377298
Conc: 1.57 ng/ml

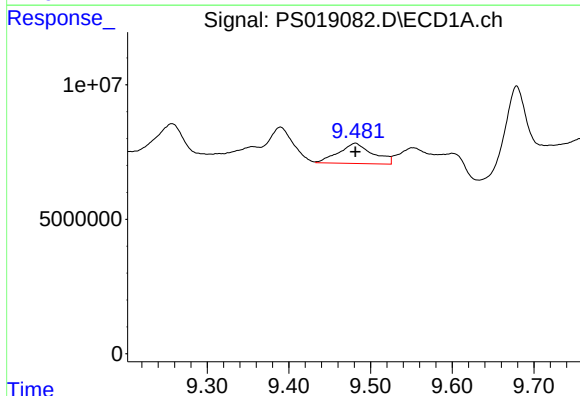


#12 2,4,5-T

R.T.: 9.481 min
Delta R.T.: 0.000 min
Response: 21903096
Conc: 1.10 ng/ml

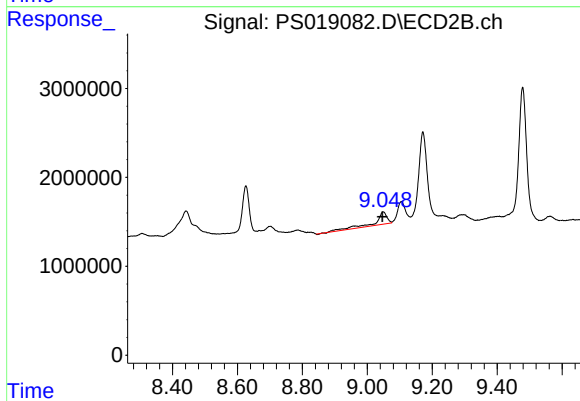

#12 2,4,5-T


R.T.: 9.049 min
Delta R.T.: 0.002 min
Response: 3628363
Conc: N.D.

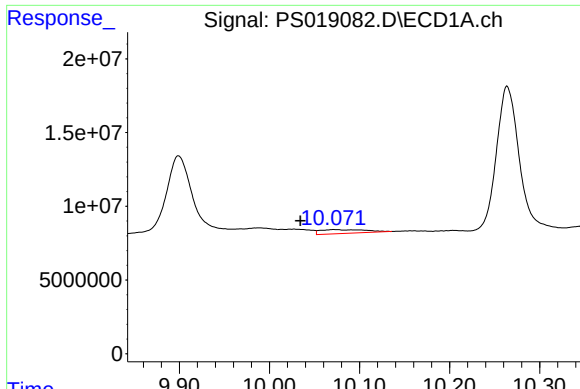

#13 2,4-DB


R.T.: 10.072 min
Delta R.T.: 0.038 min
Response: 9164511
Conc: 2.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

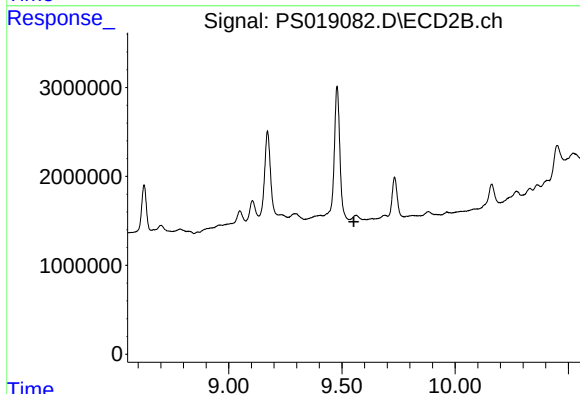


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.553 min
Response: 0
Conc: N.D.

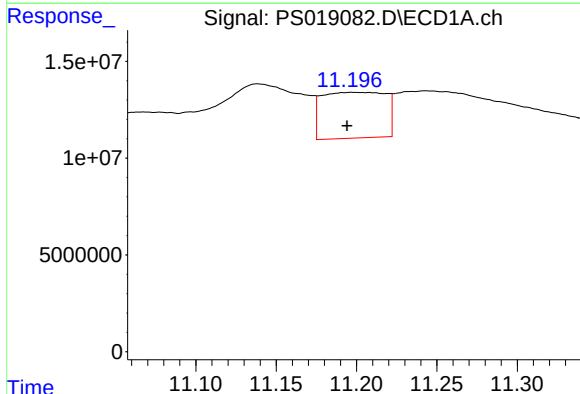


#14 DINOSEB

R.T.: 11.198 min
Delta R.T.: 0.004 min
Response: 65200812
Conc: 4.26 ng/ml

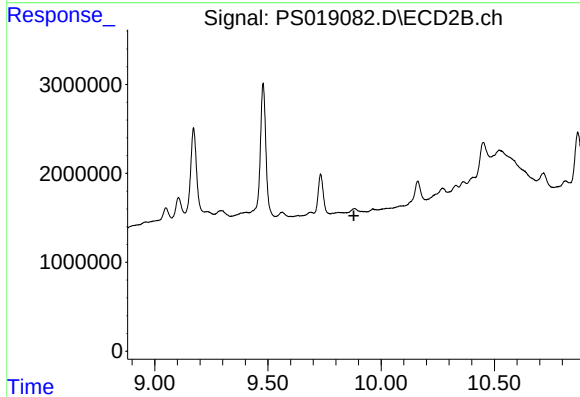

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

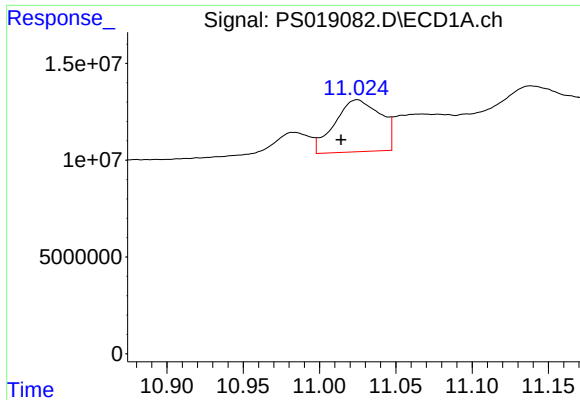

#15 Picloram


R.T.: 11.025 min
Delta R.T.: 0.011 min
Response: 56330099
Conc: 2.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

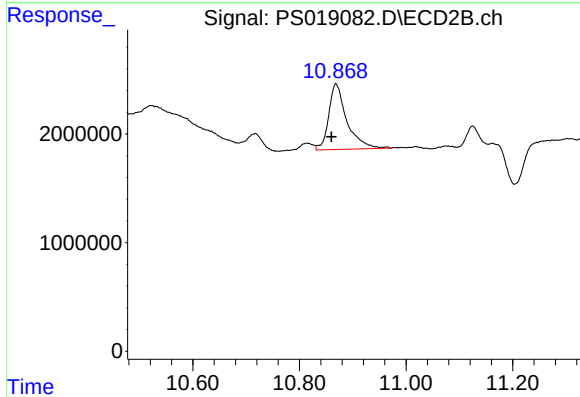


#15 Picloram

R.T.: 10.868 min
Delta R.T.: 0.008 min
Response: 14294292
Conc: 2.41 ng/ml

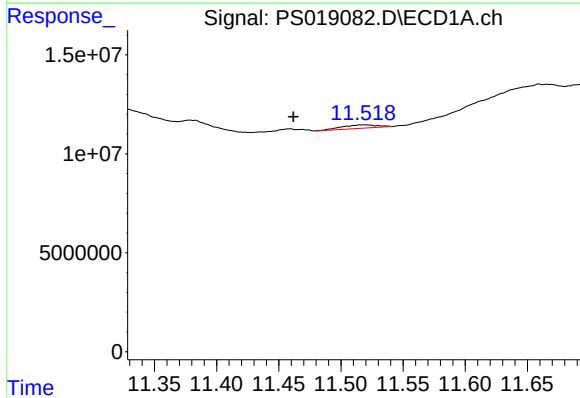

#16 DCPA

R.T.: 11.519 min
Delta R.T.: 0.057 min
Response: 3454676
Conc: N.D.

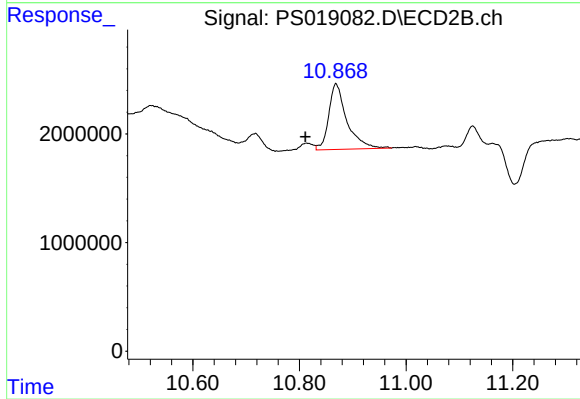

#16 DCPA

R.T.: 10.868 min
Delta R.T.: 0.057 min
Response: 14294292
Conc: 2.50 ng/ml