

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041924\
 Data File : PS026491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2024 17:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 17:46:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041924.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 19 12:45:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.316	7.804	1248.5E6	850.4E6	507.432	479.656
Target Compounds							
1) T	Dalapon	2.650f	2.749f	3029208	7597563	<MDL	2.683 #
2) T	3,5-DICHL...	6.457	6.738	577122	1477872	<MDL	<MDL #
3) T	4-Nitroph...	7.106	7.299f	8692959	1951650	5.358	1.624 #
5) T	DICAMBA	7.515	7.997	-248732	1012196	N.D.	<MDL
6) T	MCPD	0.000	8.092f	0	662753	N.D.	<MDL
7) T	MCPA	7.854	0.000	646071	0	<MDL	N.D. #
8) T	DICHLORPROP	8.183f	0.000	4114800	0	1.402	N.D. #
9) T	2,4-D	0.000	9.047	0	39533	N.D.	<MDL
10) T	Pentachlo...	8.754	0.000	903768	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.332	9.932f	52508	6930200	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.382	0	1472766	N.D.	<MDL
13) T	2,4-DB	10.223	10.980f	60202	3309488	<MDL	2.071 #
14) T	DINOSEB	11.417	0.000	2370417	0	<MDL	N.D. #
15) T	Picloram	11.202f	12.407f	11583911	780.1E6	<MDL	42.555 #
16) T	DCPA	11.688f	12.407f	7407790	780.1E6	<MDL	52.447 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041924\
Data File : PS026491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2024 17:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 17:46:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041924.M
Quant Title : 8080.M
QLast Update : Fri Apr 19 12:45:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

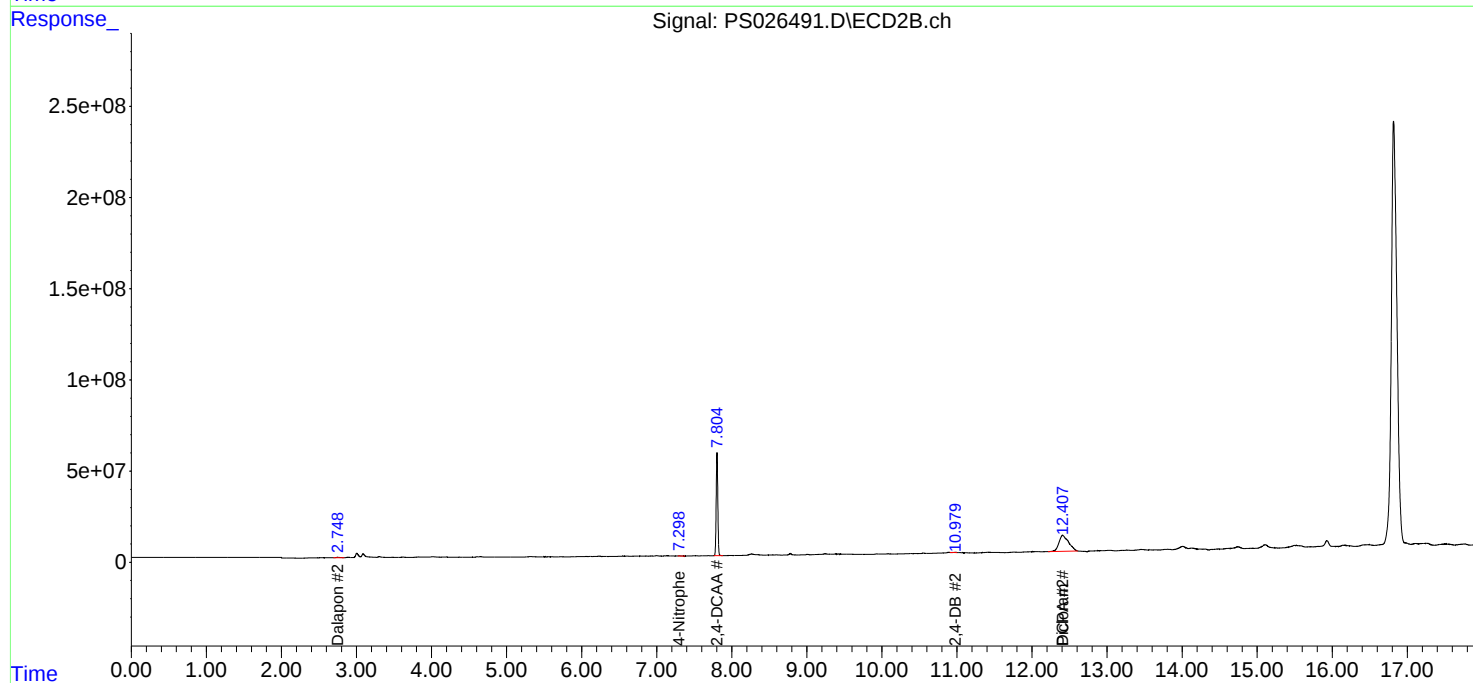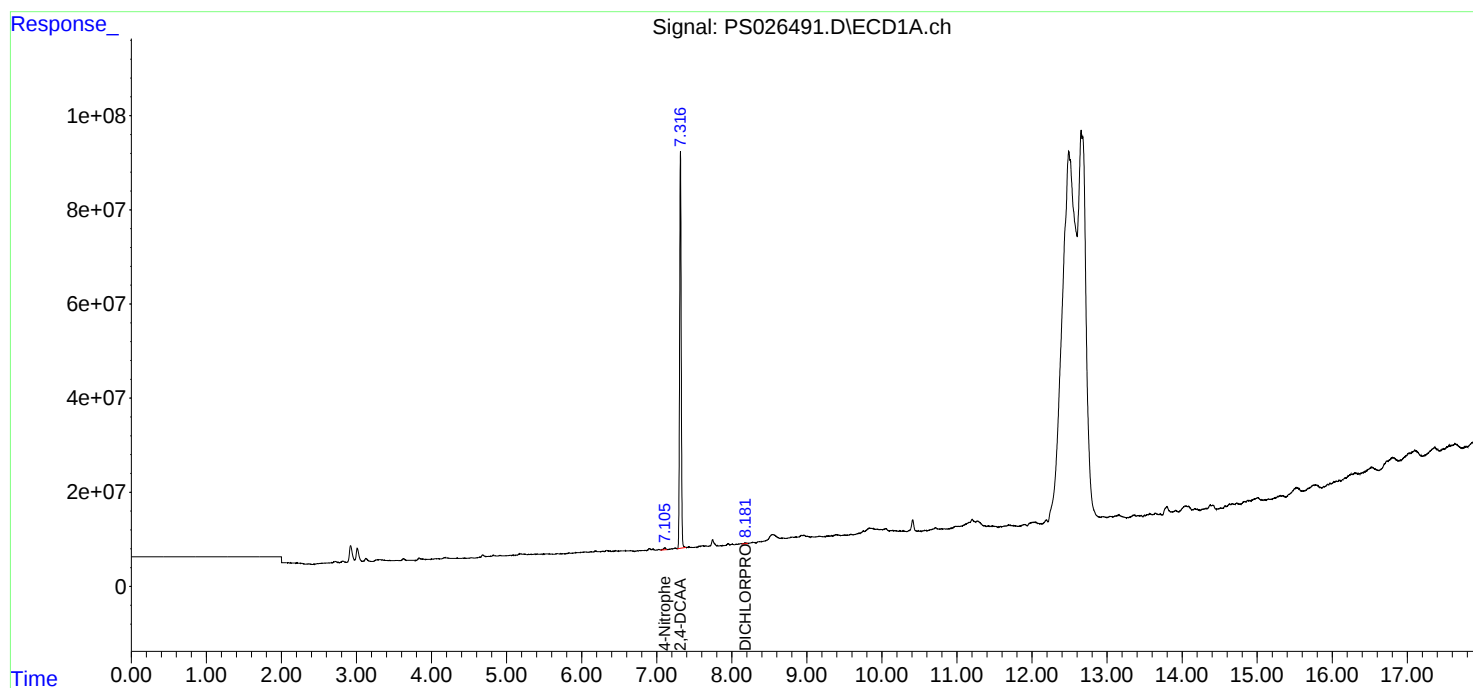


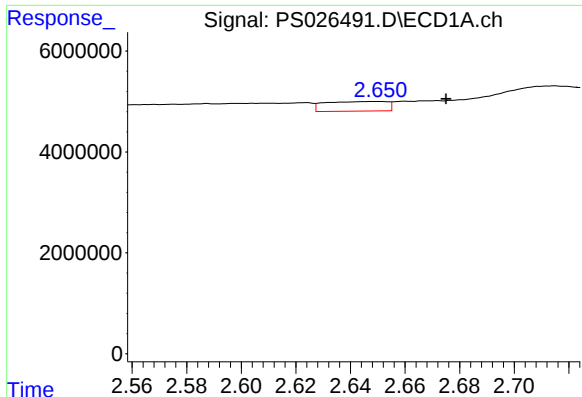

#1 Dalapon


R.T.: 2.650 min
Delta R.T.: -0.025 min
Response: 3029208
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

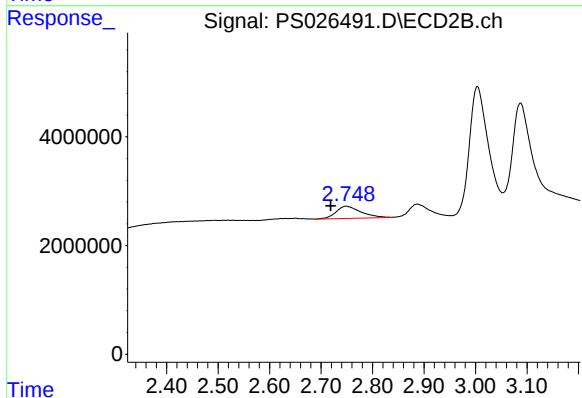


#1 Dalapon

R.T.: 2.749 min
Delta R.T.: 0.030 min
Response: 7597563
Conc: 2.68 ng/ml

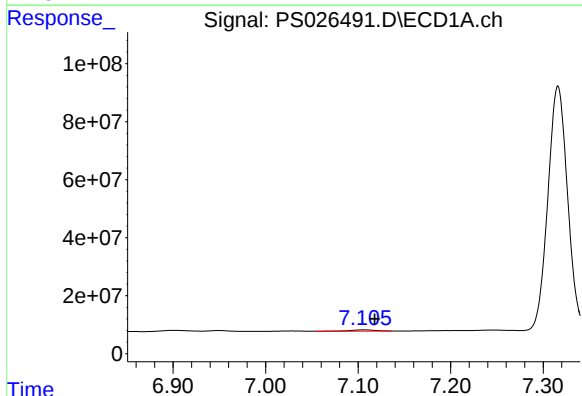


#3 4-Nitrophenol

R.T.: 7.106 min
Delta R.T.: -0.012 min
Response: 8692959
Conc: 5.36 ng/ml

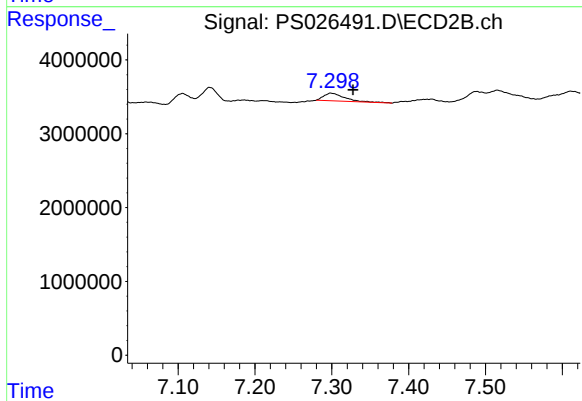

#3 4-Nitrophenol


R.T.: 7.299 min
Delta R.T.: -0.029 min
Response: 1951650
Conc: 1.62 ng/ml

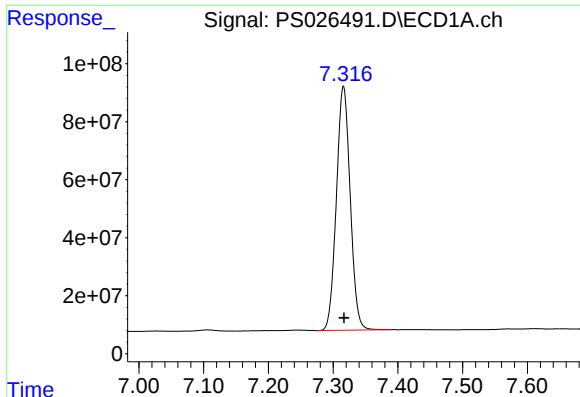

#4 2,4-DCAA


R.T.: 7.316 min
Delta R.T.: 0.000 min
Response: 1248484219
Conc: 507.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

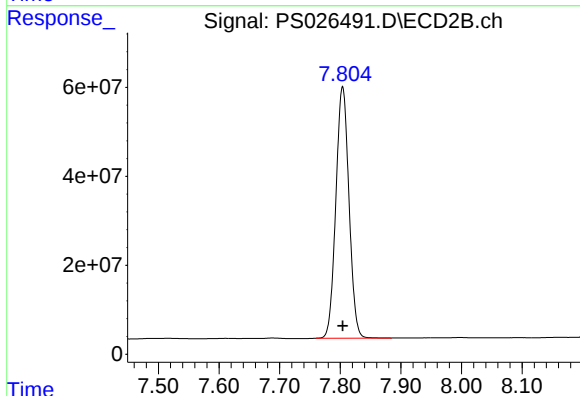


#4 2,4-DCAA

R.T.: 7.804 min
Delta R.T.: 0.000 min
Response: 850414969
Conc: 479.66 ng/ml

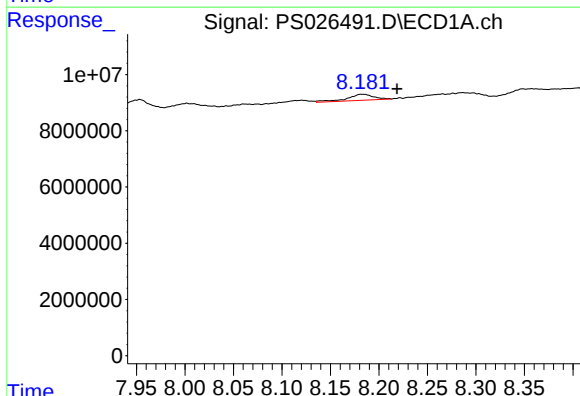


#8 DICHLORPROP

R.T.: 8.183 min
Delta R.T.: -0.036 min
Response: 4114800
Conc: 1.40 ng/ml

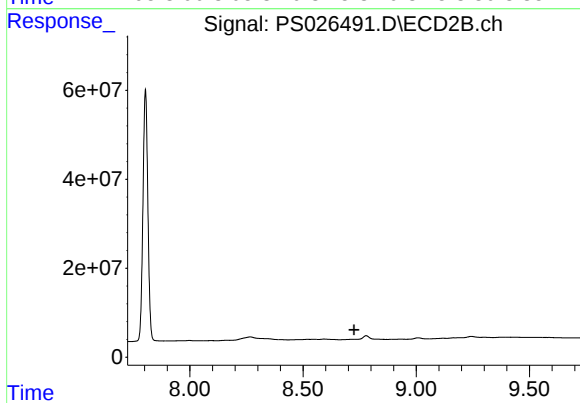

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.725 min
Response: 0
Conc: N.D.

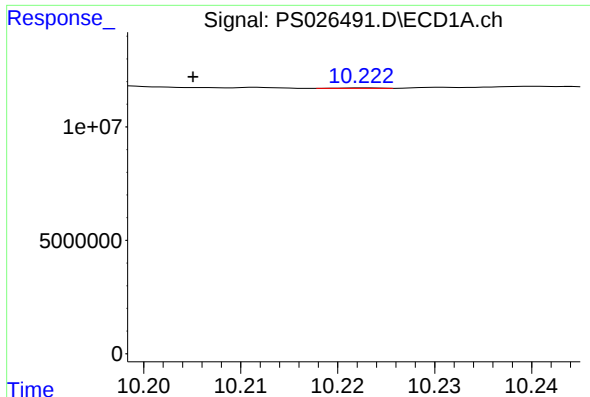

#13 2,4-DB


R.T.: 10.223 min
Delta R.T.: 0.018 min
Response: 60202
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

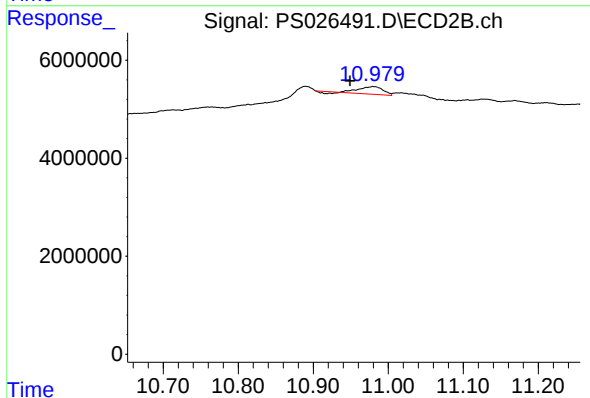


#13 2,4-DB

R.T.: 10.980 min
Delta R.T.: 0.031 min
Response: 3309488
Conc: 2.07 ng/ml

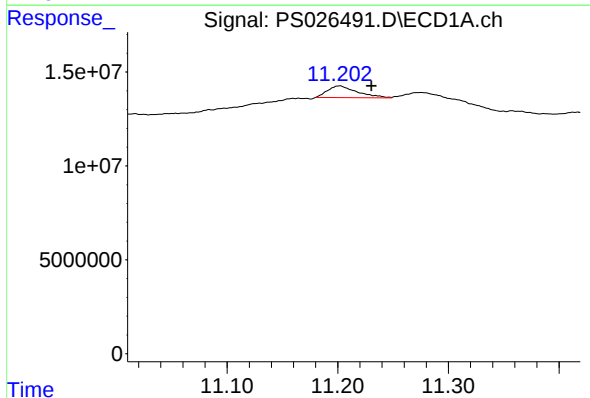


#15 Picloram

R.T.: 11.202 min
Delta R.T.: -0.029 min
Response: 11583911
Conc: N.D.

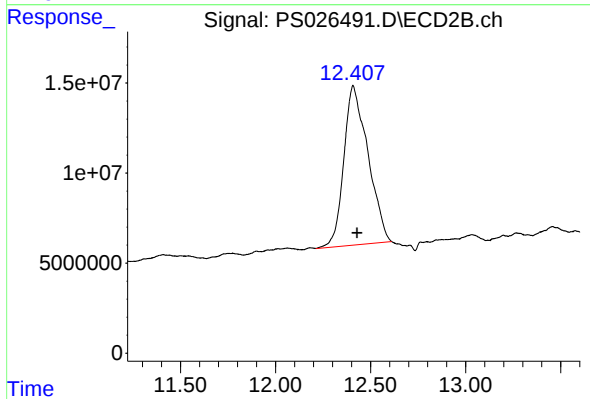

#15 Picloram


R.T.: 12.407 min
Delta R.T.: -0.021 min
Response: 780103102
Conc: 42.56 ng/ml

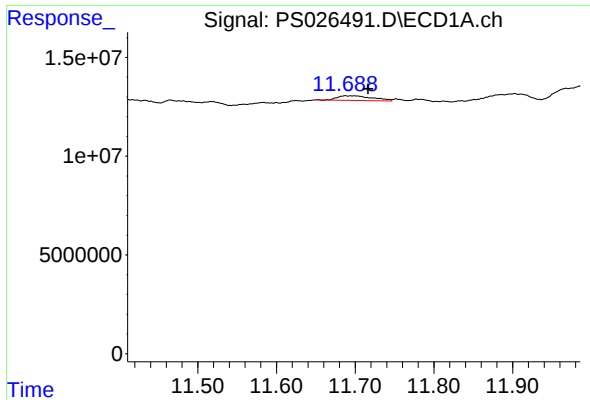

#16 DCPA

R.T.: 11.688 min
Delta R.T.: -0.029 min
Response: 7407790
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

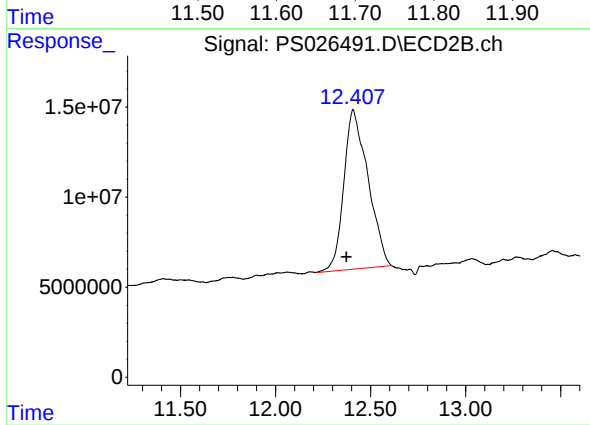

#16 DCPA

R.T.: 12.407 min
Delta R.T.: 0.033 min
Response: 780103102
Conc: 52.45 ng/ml