

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041924\
 Data File : PS026483.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2024 14:03
 Operator : AR\AJ
 Sample : P2151-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WATER-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/22/2024
 Supervised By :Ankita Jodhani 04/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 14:23:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041924.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 19 12:45:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.316	7.803	1091.5E6	710.2E6	443.631	400.563m
------	----------	-------	-------	----------	---------	---------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041924\
Data File : PS026483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2024 14:03
Operator : AR\AJ
Sample : P2151-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
WATER-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/22/2024
Supervised By :Ankita Jodhani 04/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 14:23:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041924.M
Quant Title : 8080.M
QLast Update : Fri Apr 19 12:45:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

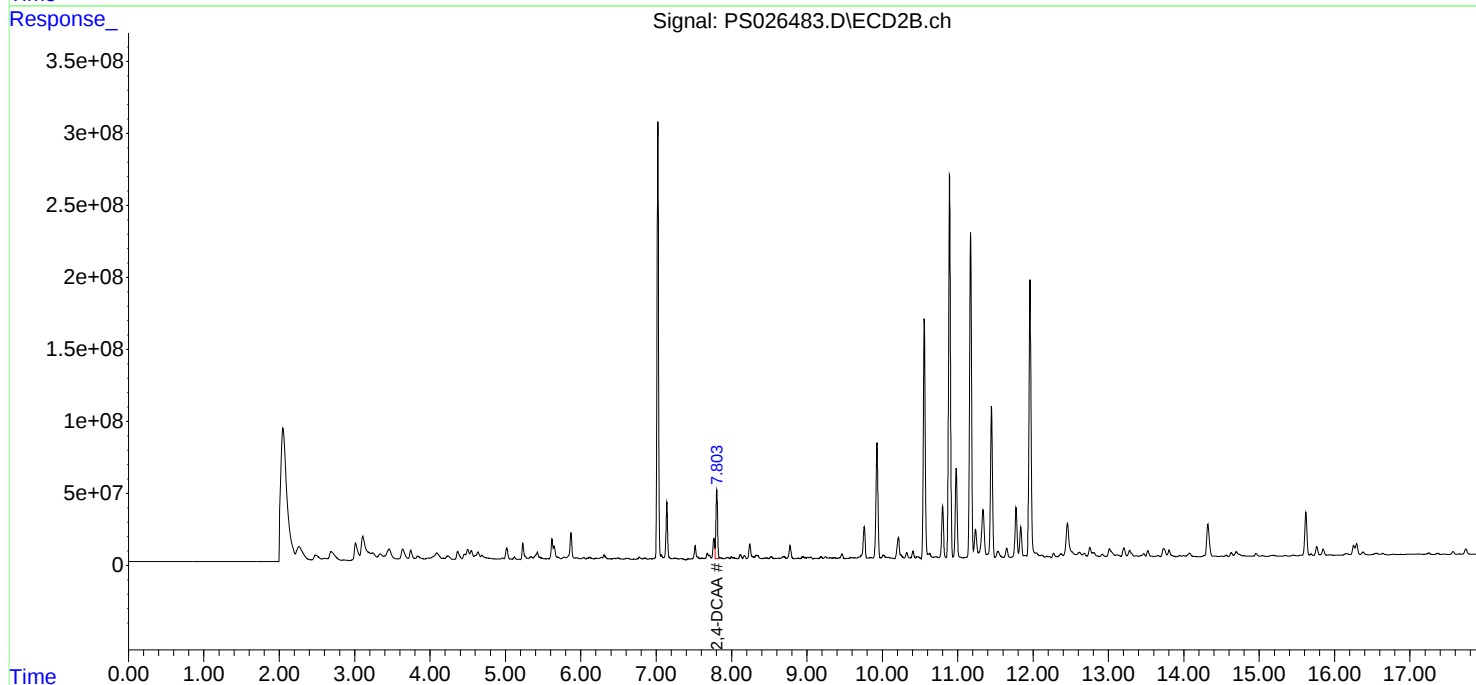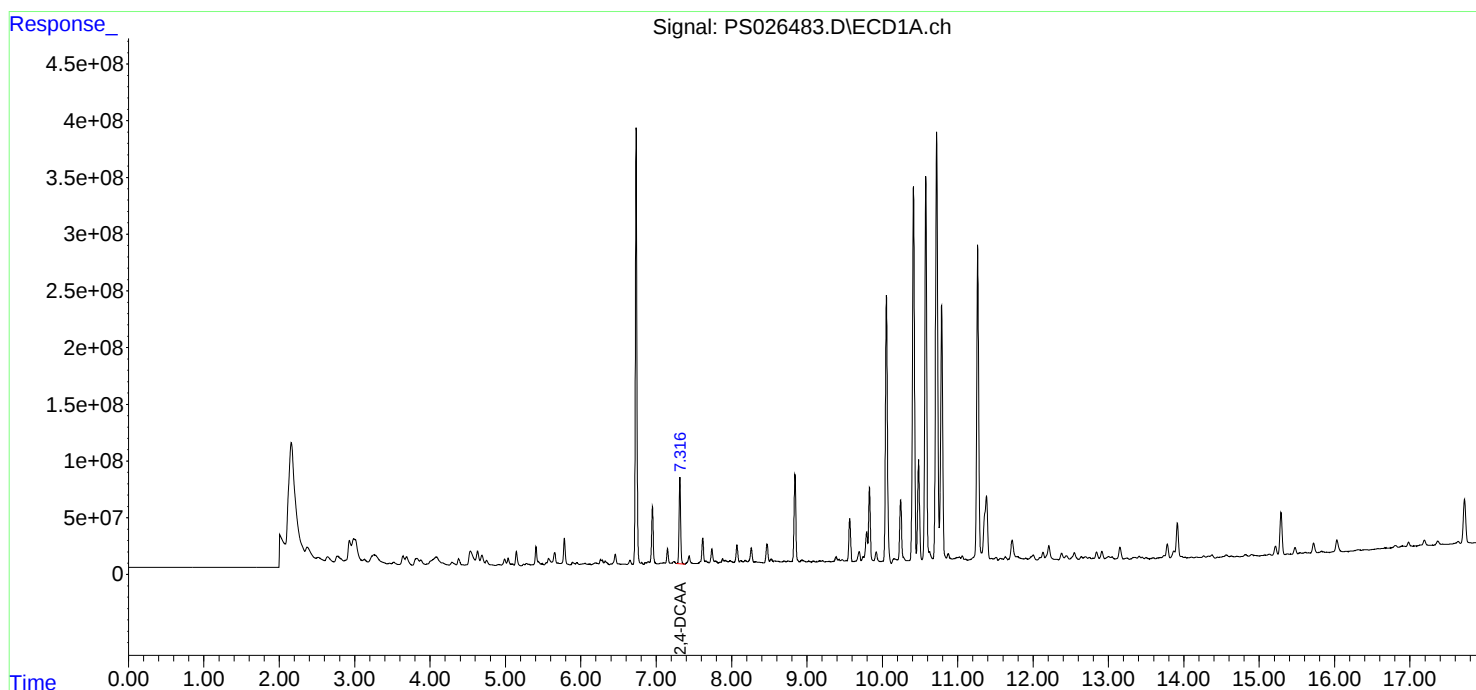

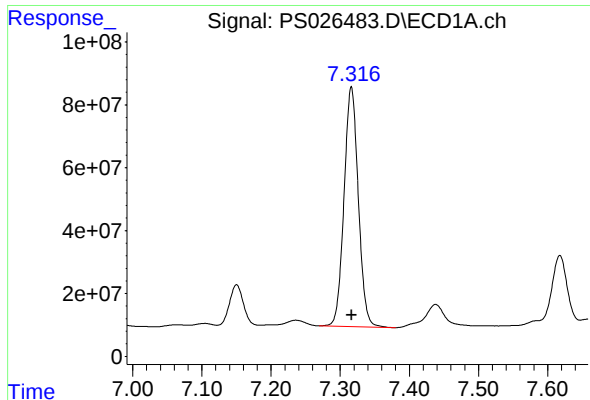


#4 2,4-DCAA

R.T.: 7.316 min
Delta R.T.: 0.000 min
Response: 1091509455
Conc: 443.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
WATER-COMP

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/22/2024
Supervised By :Ankita Jodhani 04/22/2024

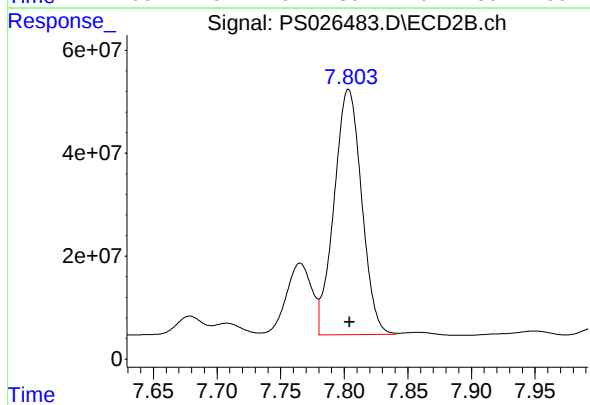

#4 2,4-DCAA

R.T.: 7.803 min
Delta R.T.: -0.001 min
Response: 710186068
Conc: 400.56 ng/ml