

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042020\
 Data File : PS009865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2020 13:50
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 00:49:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.926	0	1846216	N.D.	3.728
Target Compounds							
2) T	3,5-DICHL...	6.489	0.000	431.4E6	0	524.635	N.D. #
5) T	DICAMBA	0.000	7.088	0	5276895	N.D.	2.653
6) T	MCP	0.000	7.155	0	413.8E6	N.D.	251.430
8) T	DICHLORPROP	0.000	7.744	0	6753469	N.D.	13.418
9) T	2,4-D	8.337	0.000	67834604	0	118.141	N.D. #
10) T	Pentachlo...	0.000	8.445	0	2226008	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.806	0	2456948	N.D.	<MDL
12) T	2,4,5-T	0.000	9.188	0	2124160	N.D.	<MDL
13) T	2,4-DB	0.000	9.711	0	7045281	N.D.	19.870
14) T	DINOSEB	0.000	10.024	0	742104	N.D.	<MDL
15) T	Picloram	11.002	11.011	88843734	18700583	28.677	5.498 #
16) T	DCPA	0.000	10.956	0	3091549	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042020\
Data File : PS009865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2020 13:50
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 00:49:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

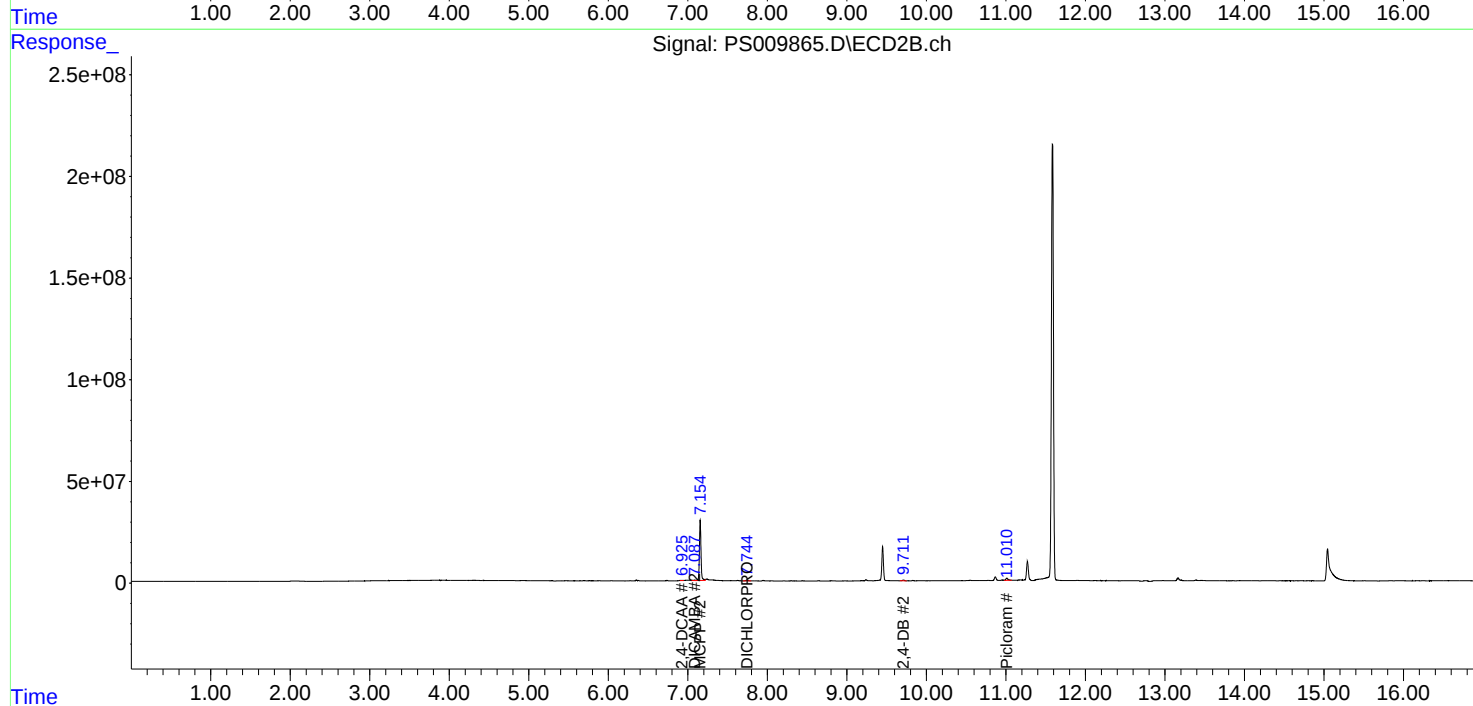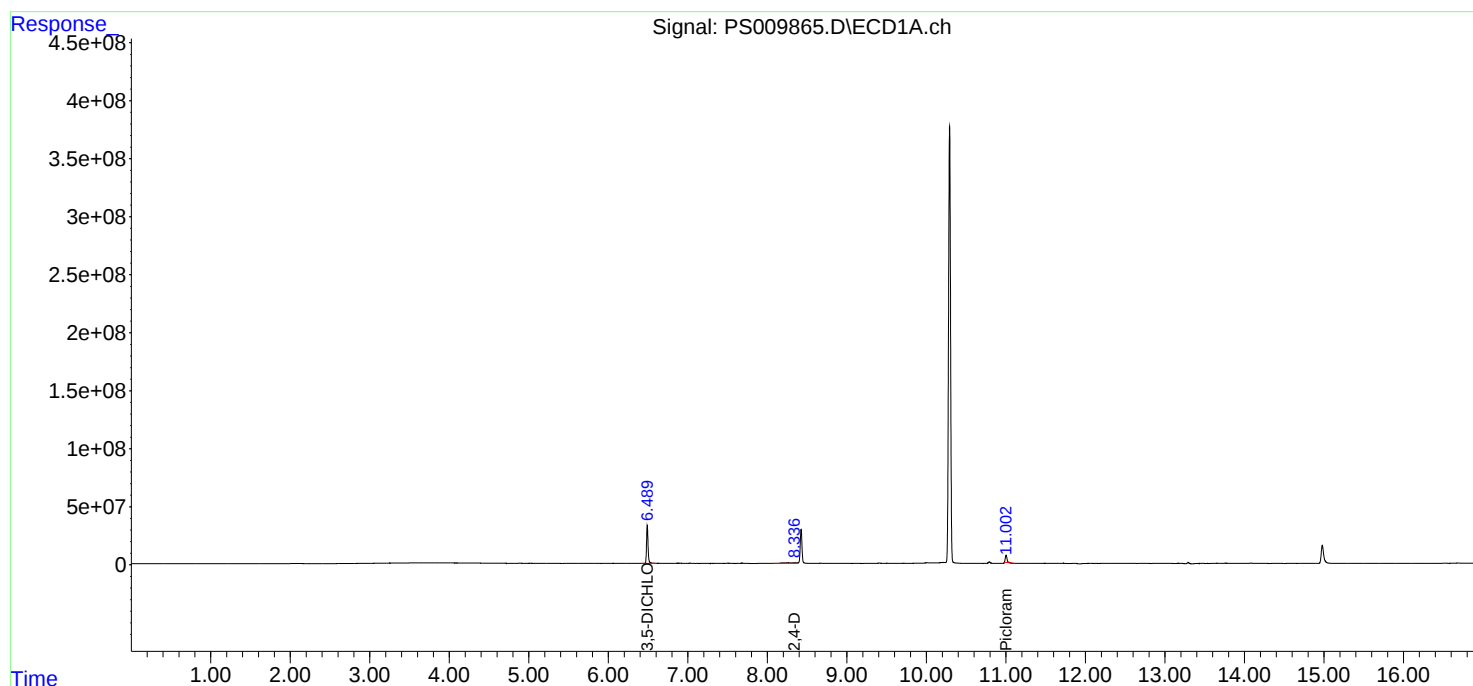


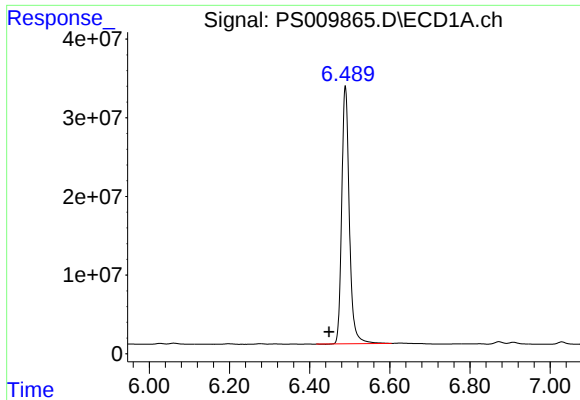

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.489 min
Delta R.T.: 0.041 min
Response: 431421606
Conc: 524.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

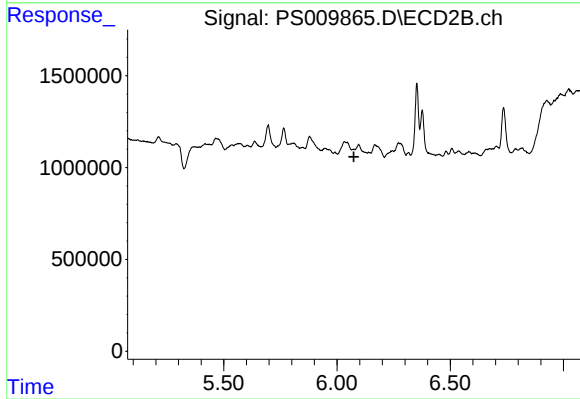


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.075 min
Response: 0
Conc: N.D.

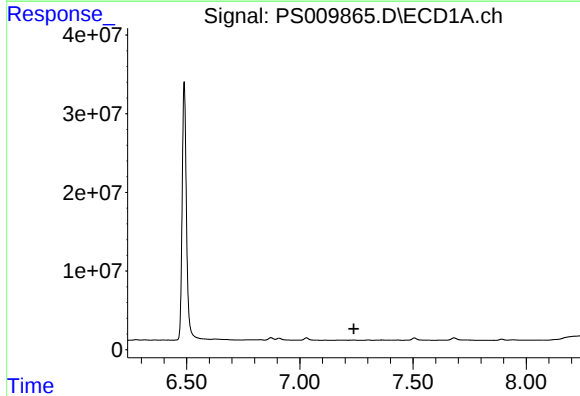


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.239 min
Response: 0
Conc: N.D.

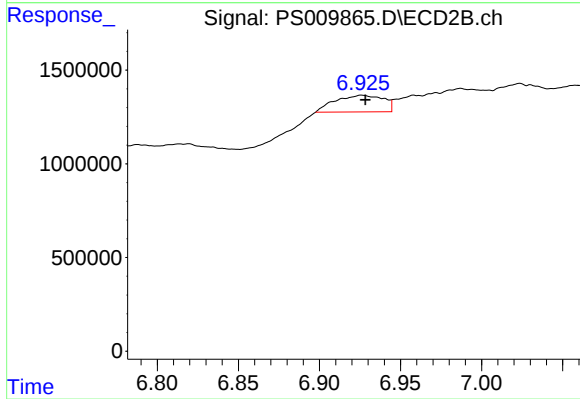

#4 2,4-DCAA


R.T.: 6.926 min
Delta R.T.: -0.002 min
Response: 1846216
Conc: 3.73 ng/ml

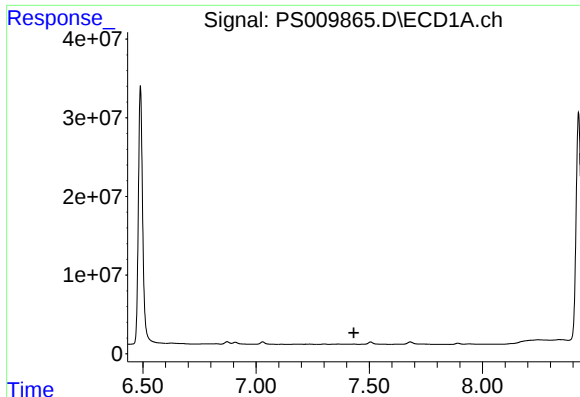

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

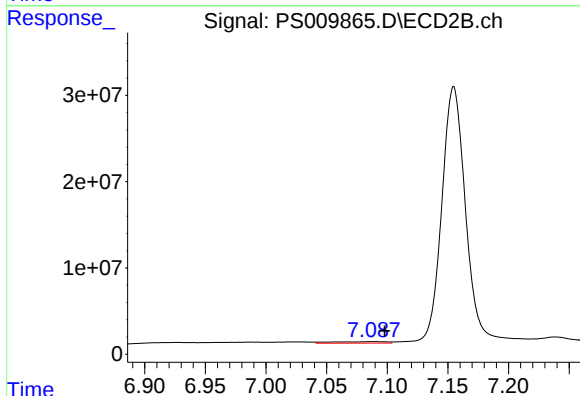


#5 DICAMBA

R.T.: 7.088 min
Delta R.T.: -0.010 min
Response: 5276895
Conc: 2.65 ng/ml

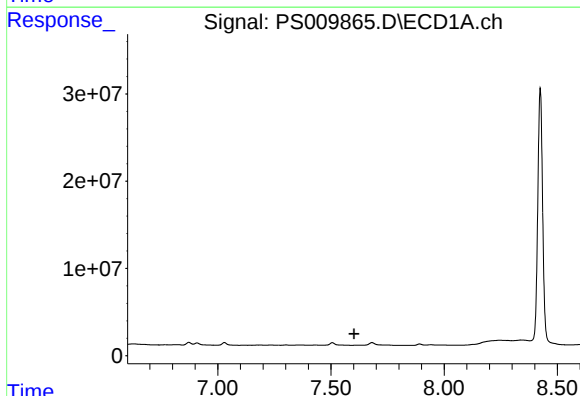


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.602 min
Response: 0
Conc: N.D.

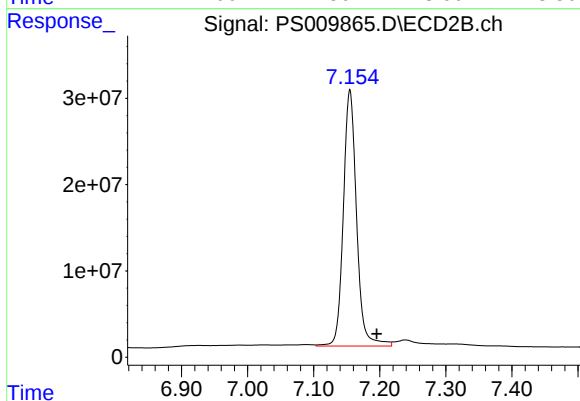

#6 MCP


R.T.: 7.155 min
Delta R.T.: -0.041 min
Response: 413847837
Conc: 251.43 ug/ml

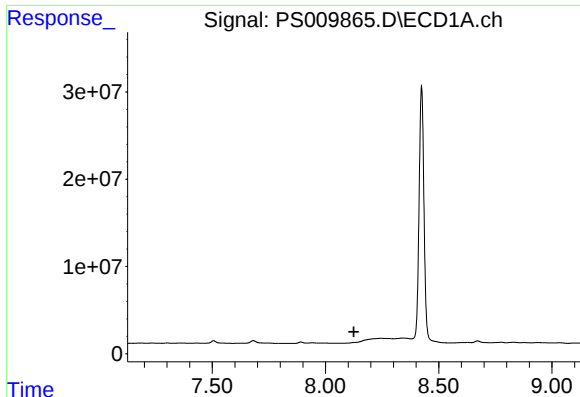

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

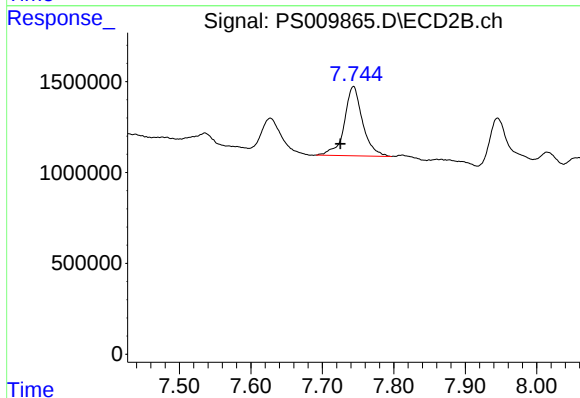


#8 DICHLORPROP

R.T.: 7.744 min
Delta R.T.: 0.018 min
Response: 6753469
Conc: 13.42 ng/ml

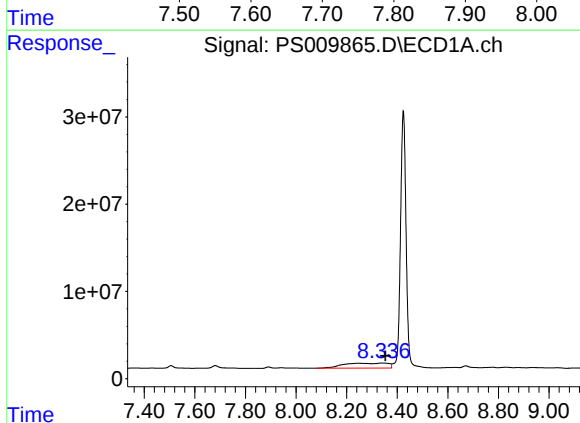


#9 2,4-D

R.T.: 8.337 min
Delta R.T.: -0.017 min
Response: 67834604
Conc: 118.14 ng/ml

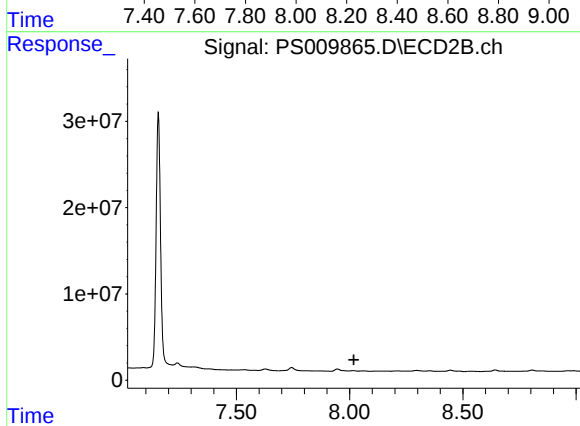

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.019 min
Response: 0
Conc: N.D.

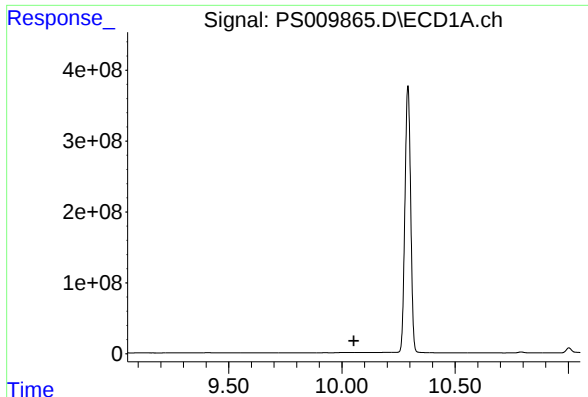

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

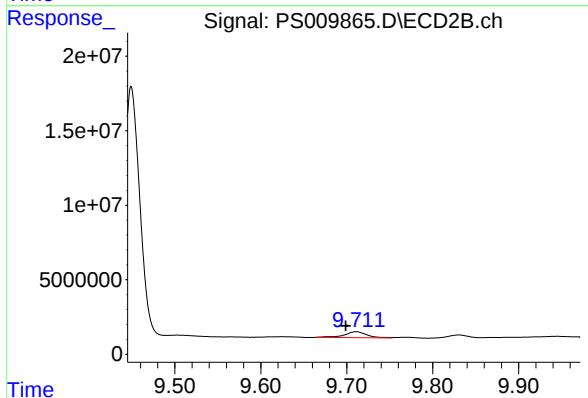


#13 2,4-DB

R.T.: 9.711 min
Delta R.T.: 0.013 min
Response: 7045281
Conc: 19.87 ng/ml

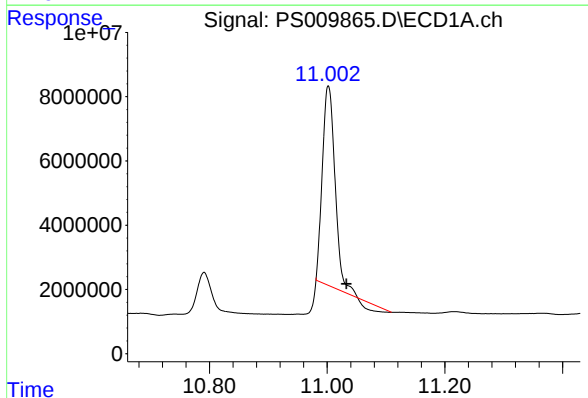

#15 Picloram

R.T.: 11.002 min
Delta R.T.: -0.030 min
Response: 88843734
Conc: 28.68 ng/ml

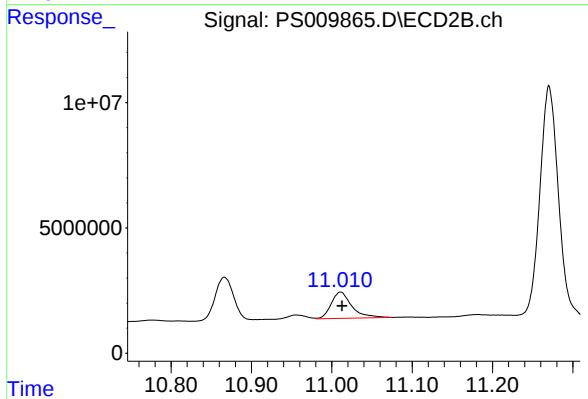

#15 Picloram

R.T.: 11.011 min
Delta R.T.: -0.002 min
Response: 18700583
Conc: 5.50 ng/ml