

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042020\
 Data File : PS009890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 02:16
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 04:22:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	6.922	326.5E6	321.9E6	540.749	649.931
Target Compounds							
5) T	DICAMBA	0.000	7.156	0	4187059	N.D.	2.105
6) T	MCPD	0.000	7.156	0	4187059	N.D.	2.544
8) T	DICHLORPROP	0.000	7.745	0	4302043	N.D.	8.547
9) T	2,4-D	8.421	0.000	17116772	0	29.811	N.D. #
11) T	2,4,5-TP ...	0.000	8.804	0	1826414	N.D.	<MDL
12) T	2,4,5-T	0.000	9.185	0	1531857	N.D.	<MDL
14) T	DINOSEB	0.000	10.024	0	947693	N.D.	<MDL
15) T	Picloram	10.997	11.010	11518831	1772174	3.718	<MDL #
16) T	DCPA	0.000	10.953	0	3669150	N.D.	1.094



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042020\
Data File : PS009890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 02:16
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 04:22:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

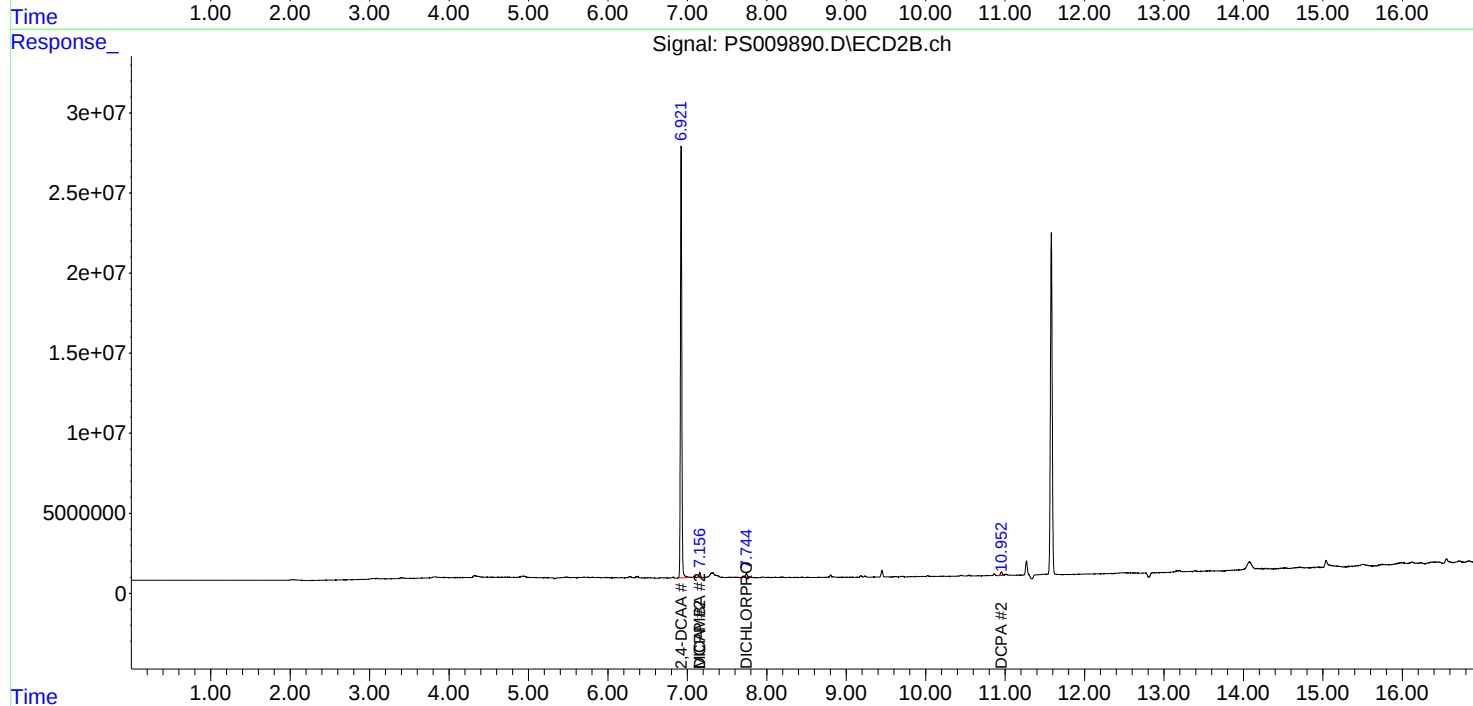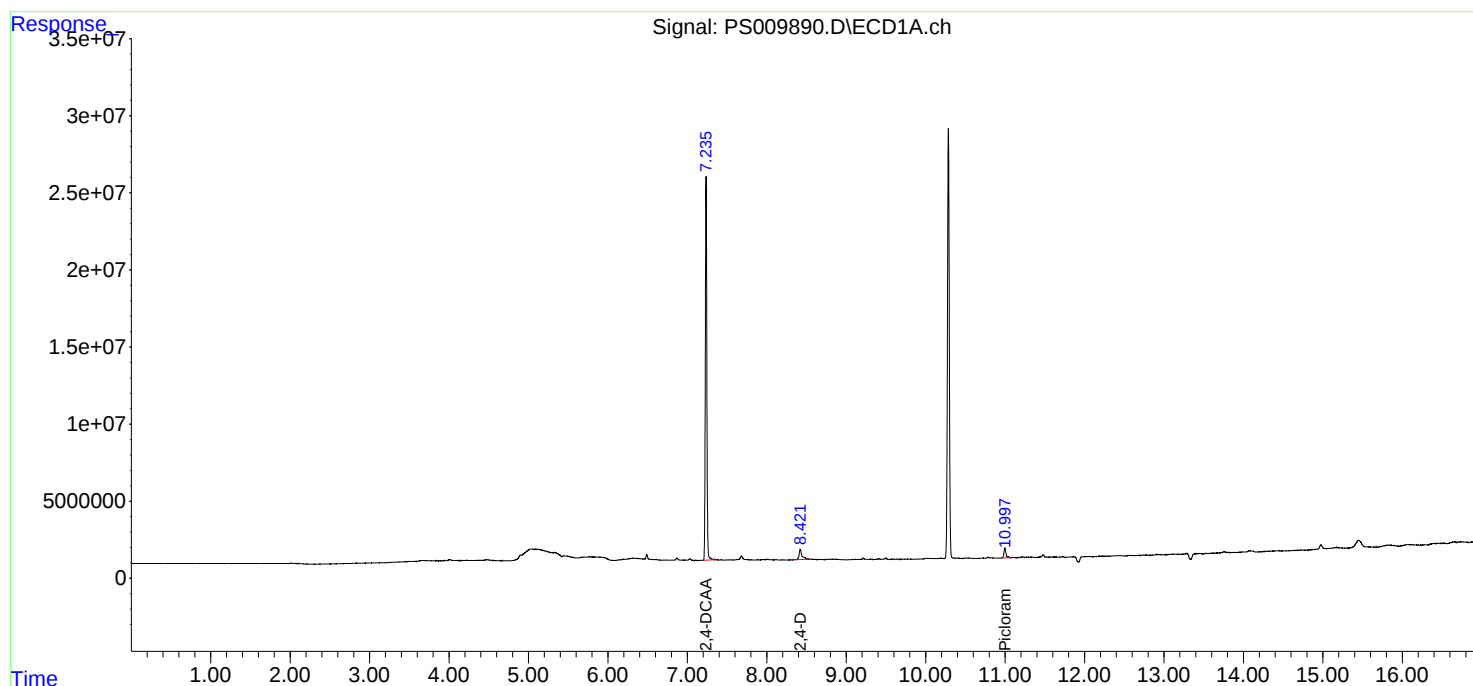


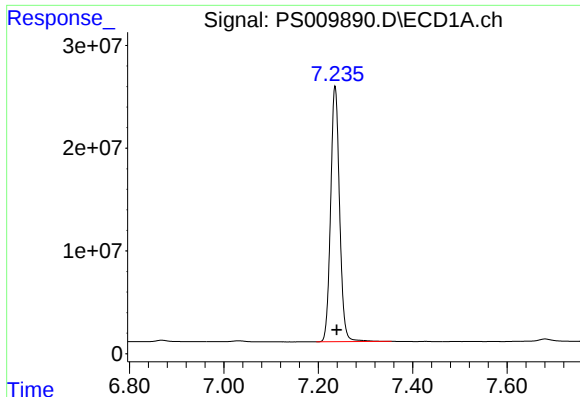

#4 2,4-DCAA


R.T.: 7.236 min
Delta R.T.: -0.003 min
Response: 326512545
Conc: 540.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

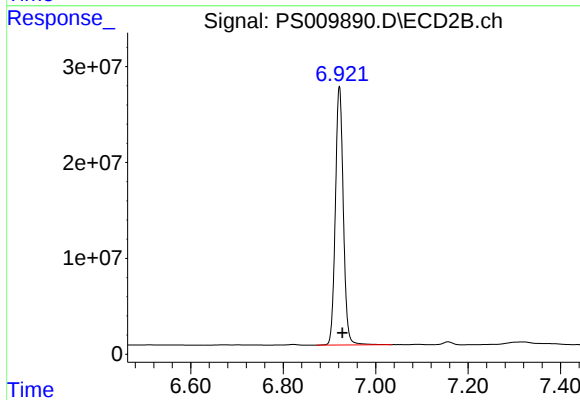


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.007 min
Response: 321878425
Conc: 649.93 ng/ml

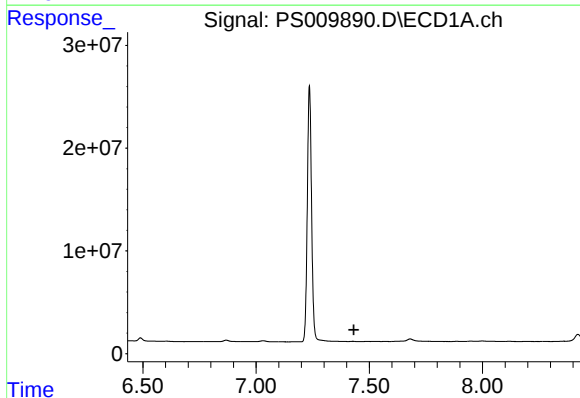


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

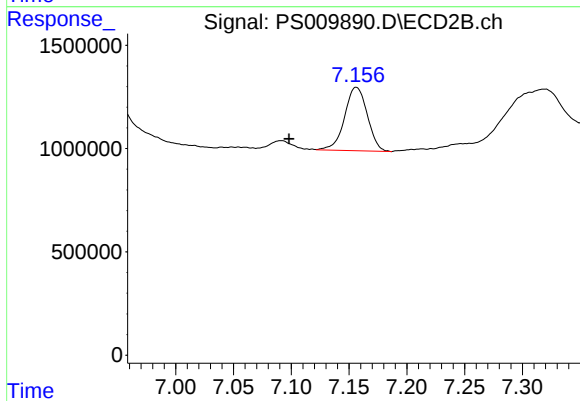

#5 DICAMBA


R.T.: 7.156 min
Delta R.T.: 0.058 min
Response: 4187059
Conc: 2.11 ng/ml

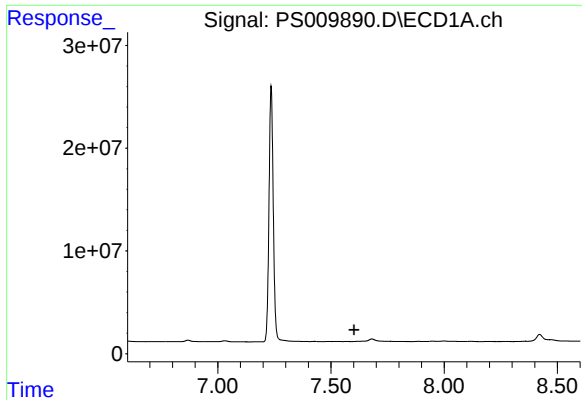

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

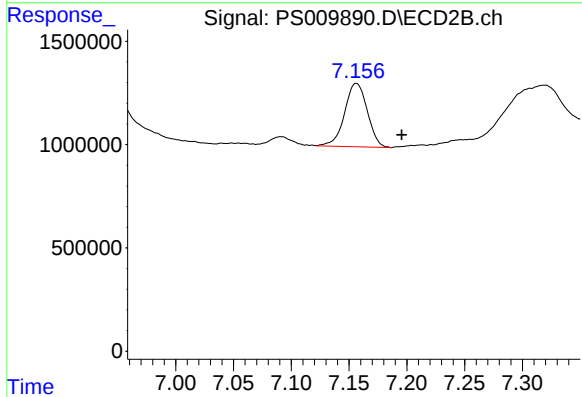


#6 MCP

R.T.: 7.156 min
Delta R.T.: -0.039 min
Response: 4187059
Conc: 2.54 ug/ml

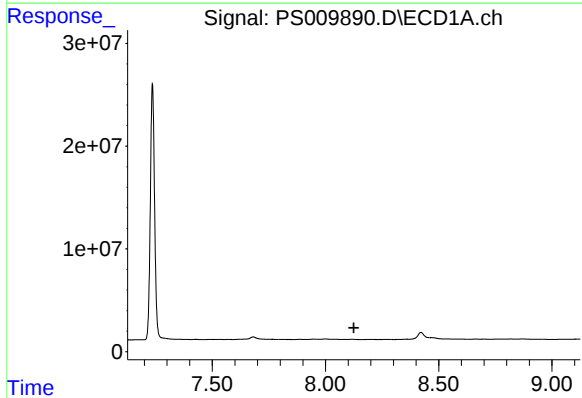


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

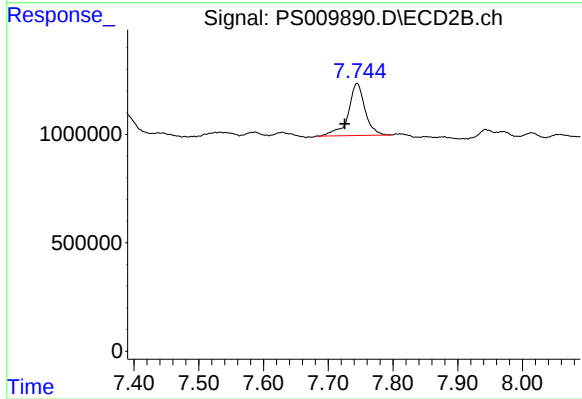

#8 DICHLORPROP


R.T.: 7.745 min
Delta R.T.: 0.019 min
Response: 4302043
Conc: 8.55 ng/ml

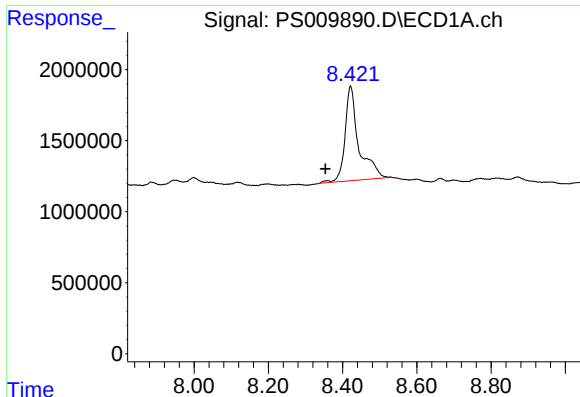

#9 2,4-D


R.T.: 8.421 min
Delta R.T.: 0.067 min
Response: 17116772
Conc: 29.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

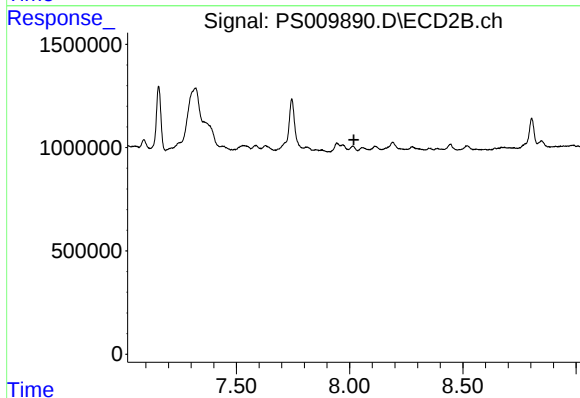


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.019 min
Response: 0
Conc: N.D.

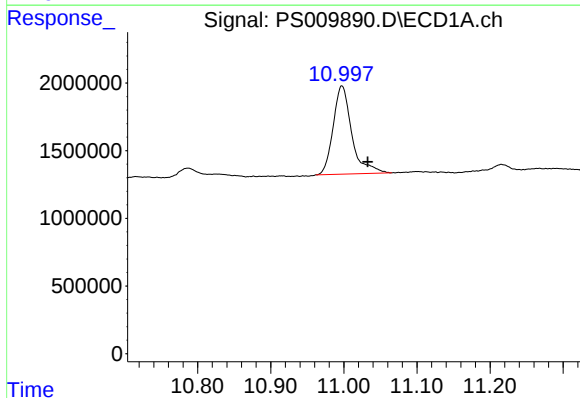


#15 Picloram

R.T.: 10.997 min
Delta R.T.: -0.035 min
Response: 11518831
Conc: 3.72 ng/ml

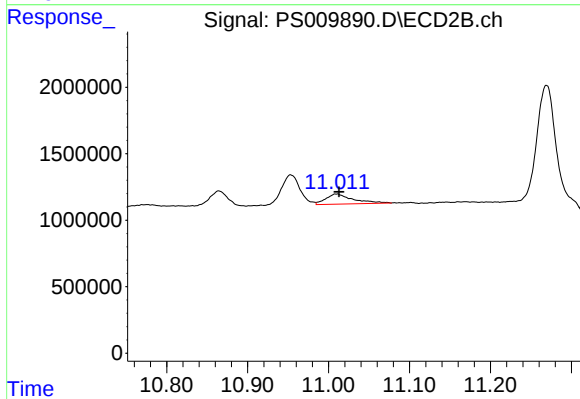

#15 Picloram


R.T.: 11.010 min
Delta R.T.: -0.003 min
Response: 1772174
Conc: N.D.

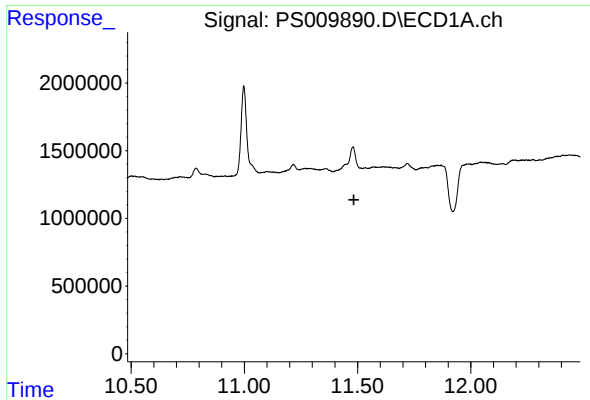

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

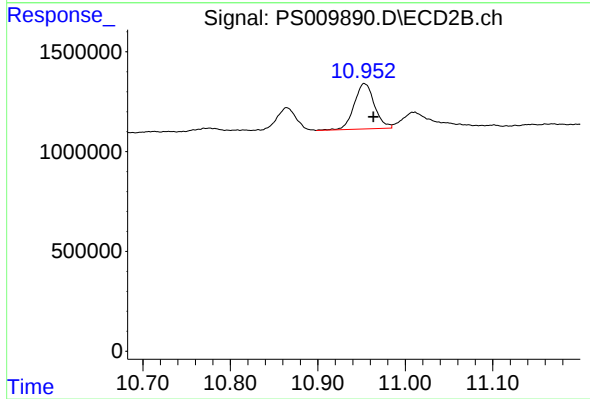

#16 DCPA

R.T.: 10.953 min
Delta R.T.: -0.010 min
Response: 3669150
Conc: 1.09 ng/ml