

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042020\
 Data File : PS009902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 07:15
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:01:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	6.922	334.8E6	331.7E6	554.403	669.863
Target Compounds							
5) T	DICAMBA	0.000	7.092	0	1099438	N.D.	<MDL
6) T	MCP	0.000	7.157	0	4719101	N.D.	2.867
8) T	DICHLORPROP	0.000	7.744	0	4735321	N.D.	9.408
9) T	2,4-D	8.422	0.000	10654269	0	18.555	N.D. #
11) T	2,4,5-TP ...	0.000	8.804	0	1473344	N.D.	<MDL
12) T	2,4,5-T	0.000	9.185	0	1174767	N.D.	<MDL
14) T	DINOSEB	0.000	10.025	0	768579	N.D.	<MDL
15) T	Picloram	10.998	11.008	13333040	2246781	4.304	<MDL #
16) T	DCPA	0.000	10.954	0	2332759	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042020\
Data File : PS009902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 07:15
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:01:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

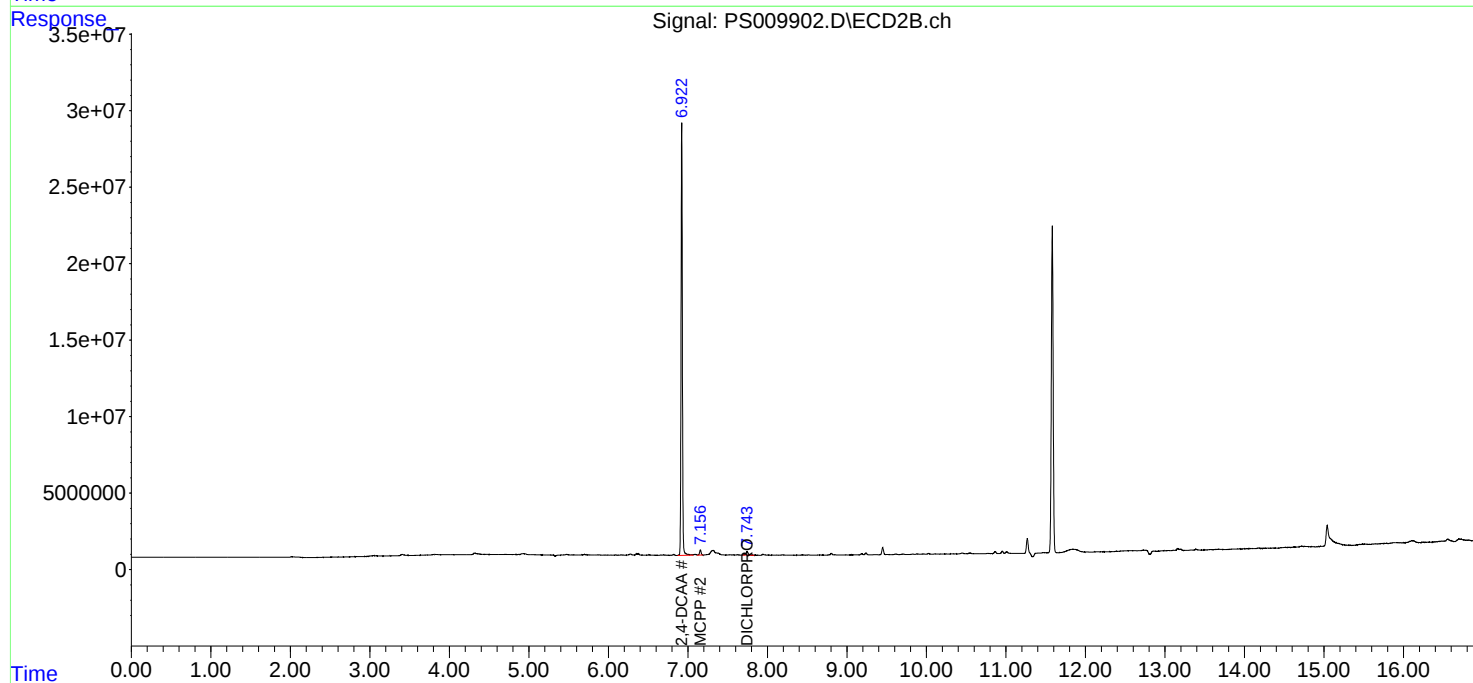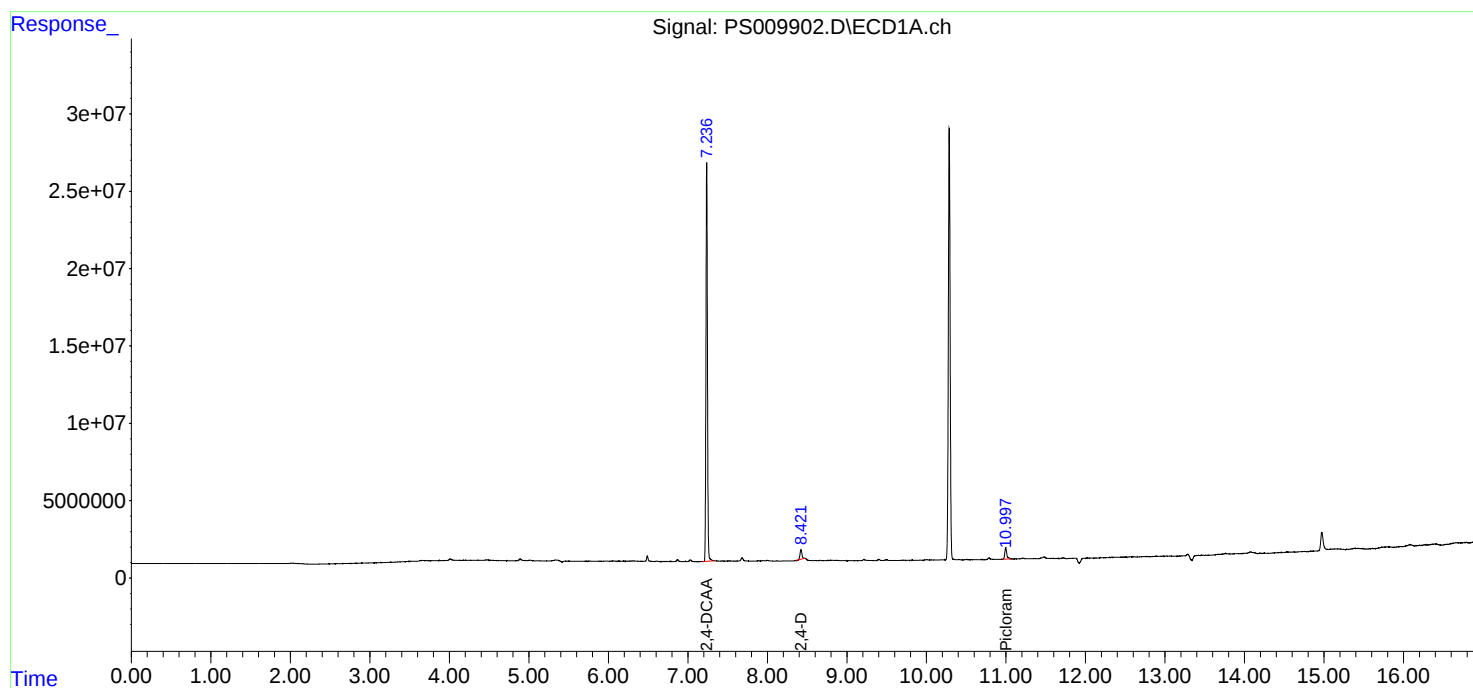


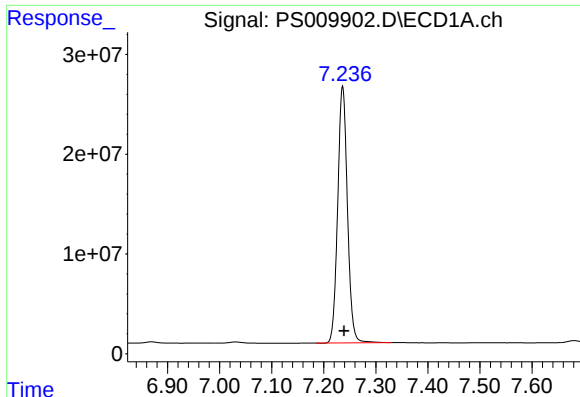

#4 2,4-DCAA


R.T.: 7.236 min
Delta R.T.: -0.003 min
Response: 334757123
Conc: 554.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

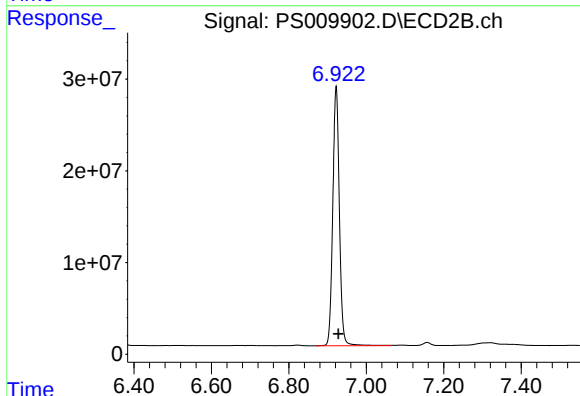


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.006 min
Response: 331749770
Conc: 669.86 ng/ml

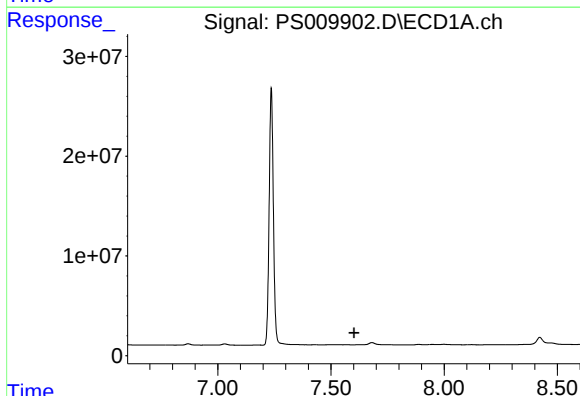


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.602 min
Response: 0
Conc: N.D.

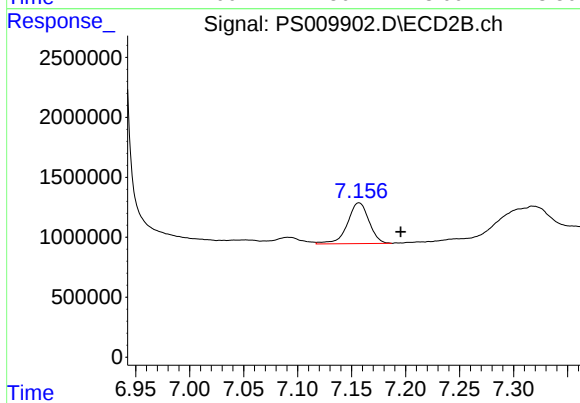

#6 MCP


R.T.: 7.157 min
Delta R.T.: -0.039 min
Response: 4719101
Conc: 2.87 ug/ml

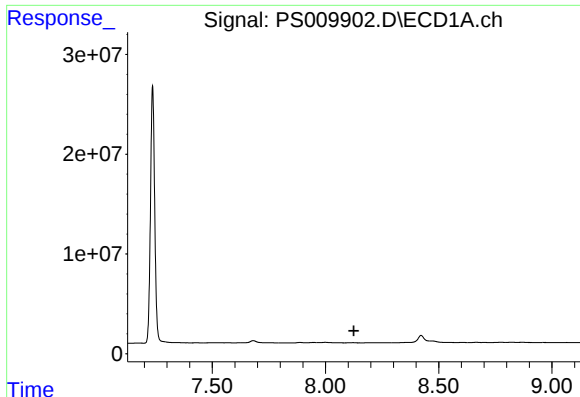

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

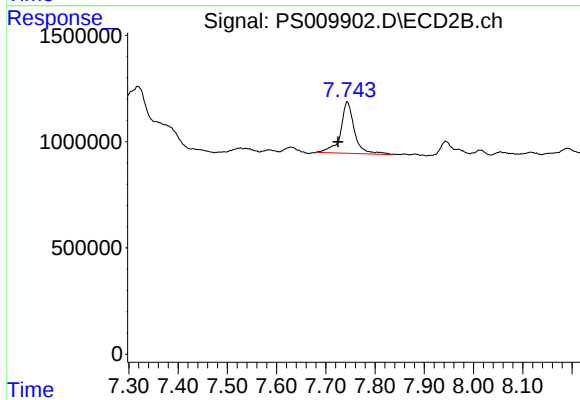


#8 DICHLORPROP

R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 4735321
Conc: 9.41 ng/ml

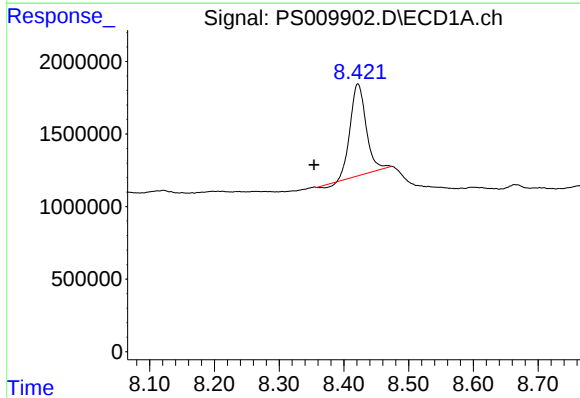


#9 2,4-D

R.T.: 8.422 min
Delta R.T.: 0.068 min
Response: 10654269
Conc: 18.56 ng/ml

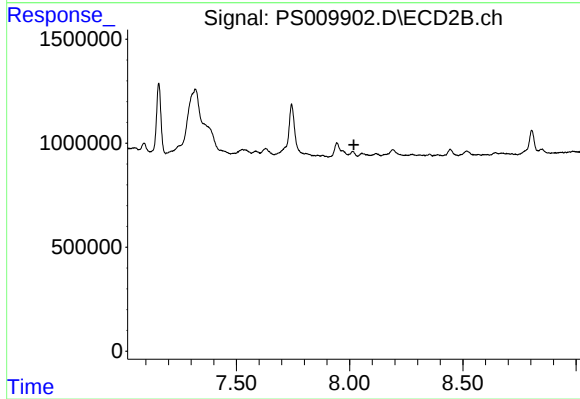

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.019 min
Response: 0
Conc: N.D.

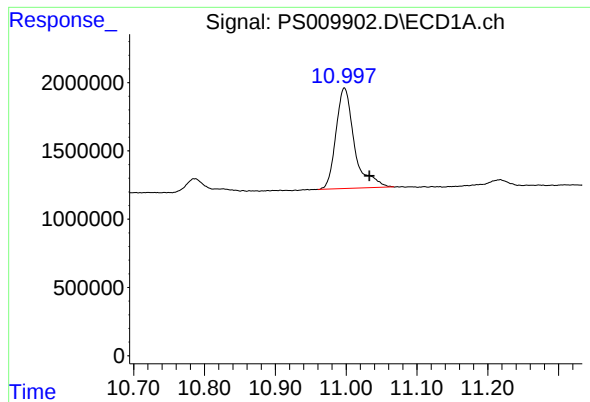

#15 Picloram

R.T.: 10.998 min
Delta R.T.: -0.035 min
Response: 13333040
Conc: 4.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

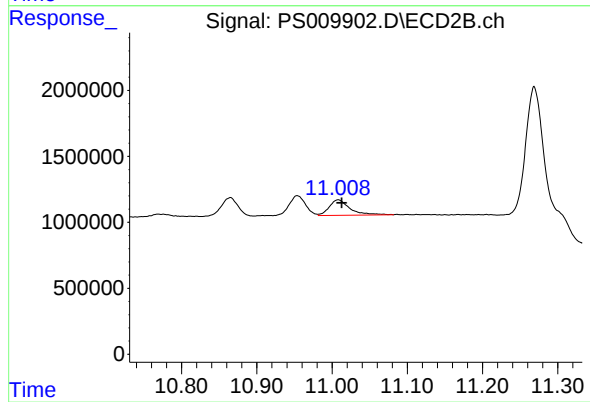

#15 Picloram

R.T.: 11.008 min
Delta R.T.: -0.005 min
Response: 2246781
Conc: N.D.