

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042021\
 Data File : PS014705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 15:11
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 15:22:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	6.884	728.7E6	266.4E6	479.053	572.305
Target Compounds							
6) T	MCP	7.557	0.000	6944968	0	1.595	N.D. #
7) T	MCPA	7.608f	0.000	13187271	0	2.119	N.D. #
8) T	DICHLORPROP	0.000	7.702	0	12478528	N.D.	24.719
11) T	2,4,5-TP ...	0.000	8.727	0	7220117	N.D.	2.643
12) T	2,4,5-T	9.383	0.000	4201840	0	<MDL	N.D. #
13) T	2,4-DB	9.931	9.659	32349653	22743529	21.258	65.568 #
14) T	DINOSEB	11.166f	0.000	25497957	0	3.957	N.D. #
15) T	Picloram	10.891	10.973	23247676	5697120	2.078	1.519 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042021\
Data File : PS014705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 15:11
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 15:22:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

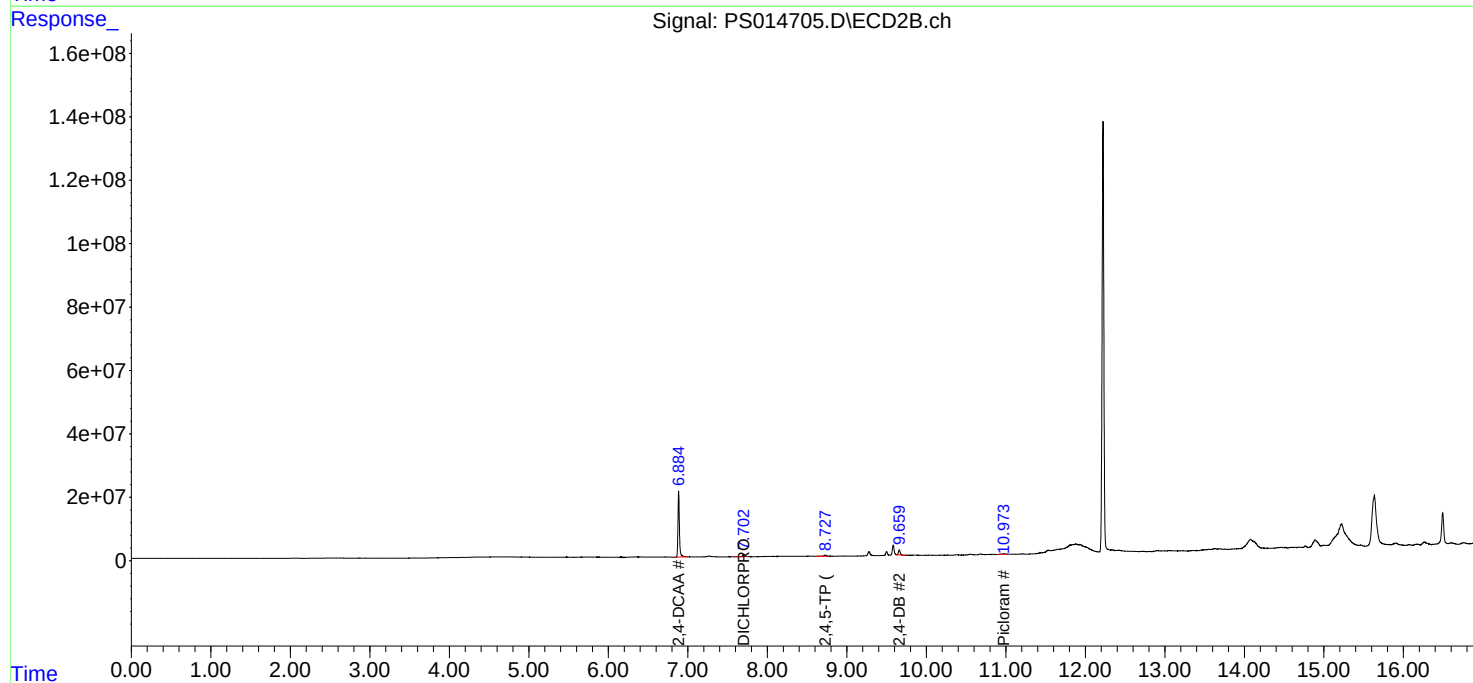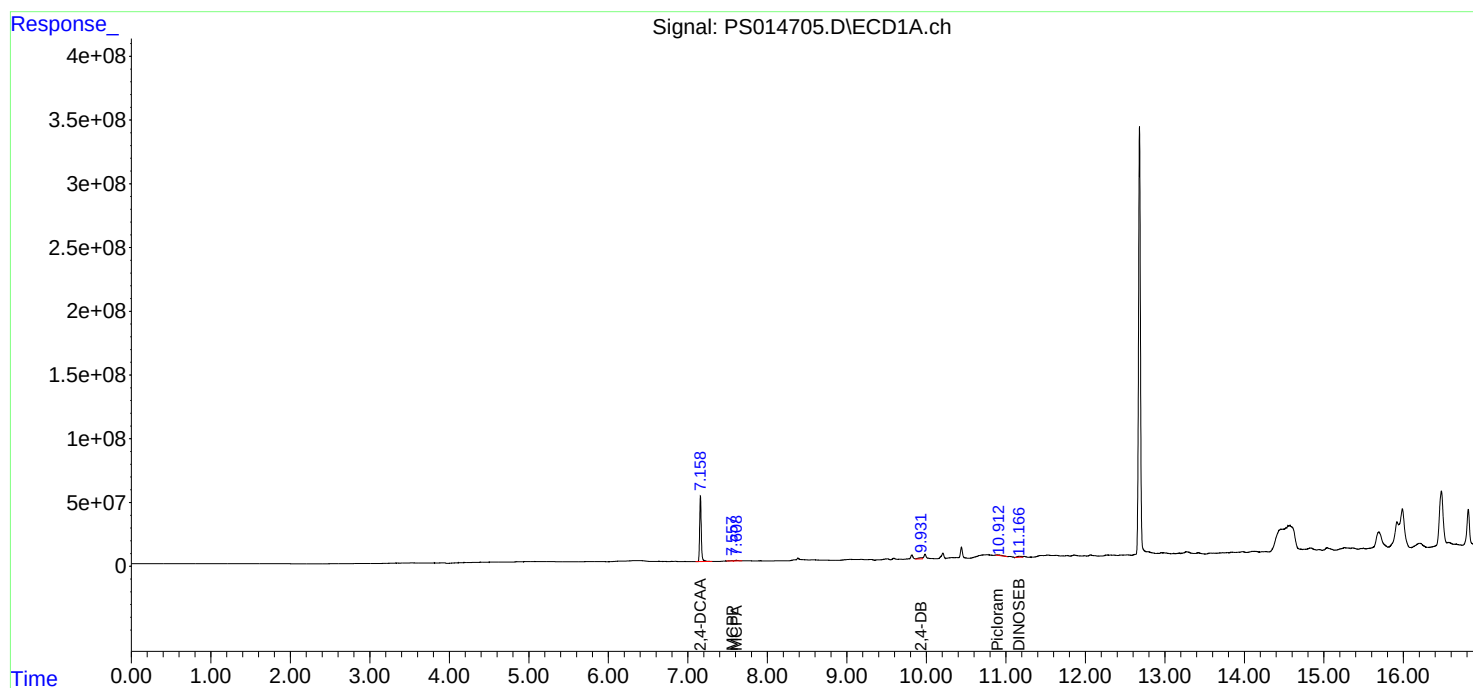


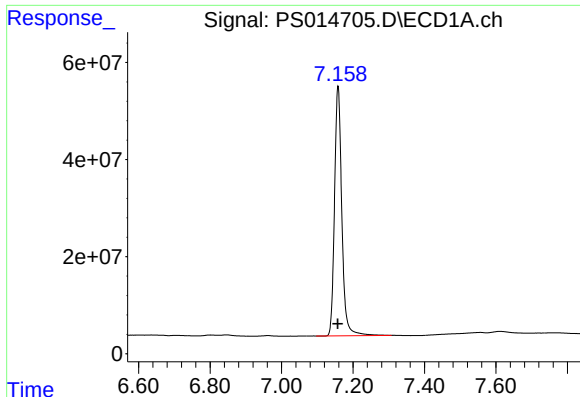

#4 2,4-DCAA


R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 728732904
Conc: 479.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

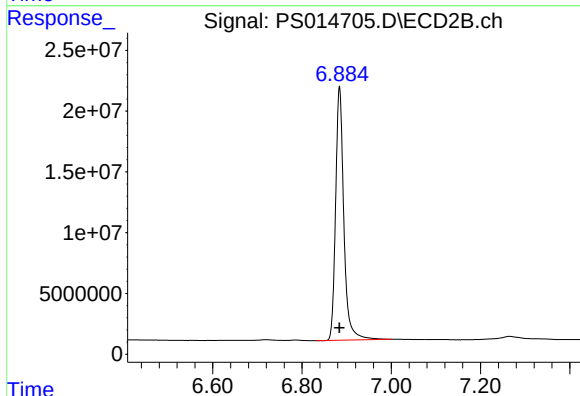


#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 266382073
Conc: 572.31 ng/ml

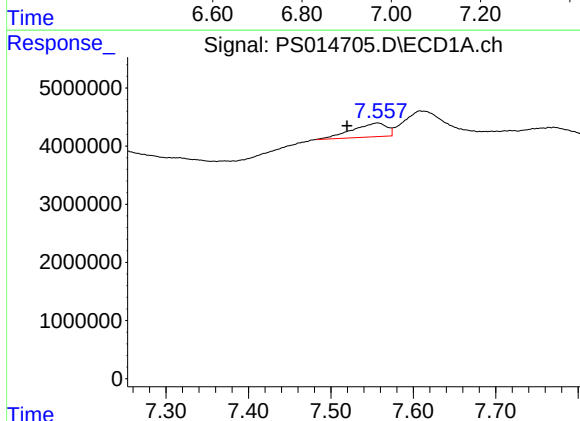


#6 MCP

R.T.: 7.557 min
Delta R.T.: 0.037 min
Response: 6944968
Conc: 1.60 ug/ml

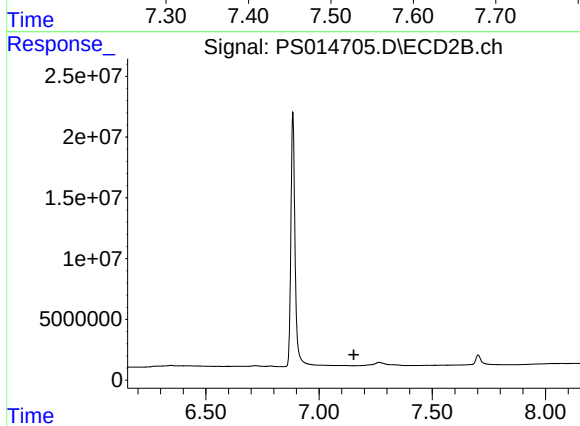

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

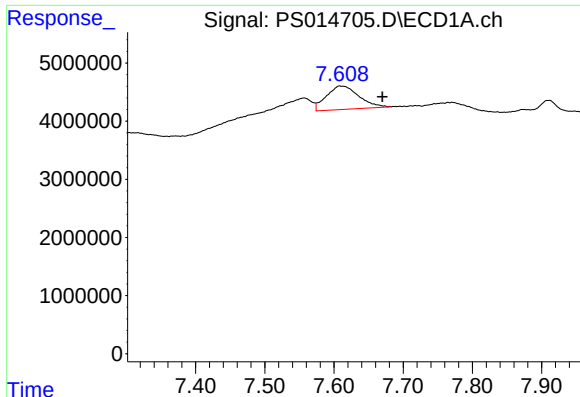

#7 MCPA


R.T.: 7.608 min
Delta R.T.: -0.062 min
Response: 13187271
Conc: 2.12 ug/ml

Instrument :
ECD_S
ClientSampleId :

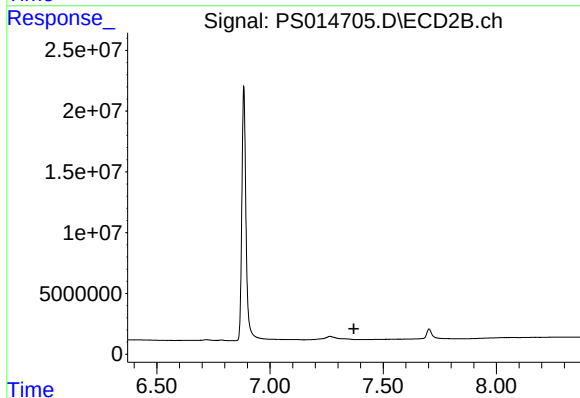


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.370 min
Response: 0
Conc: N.D.

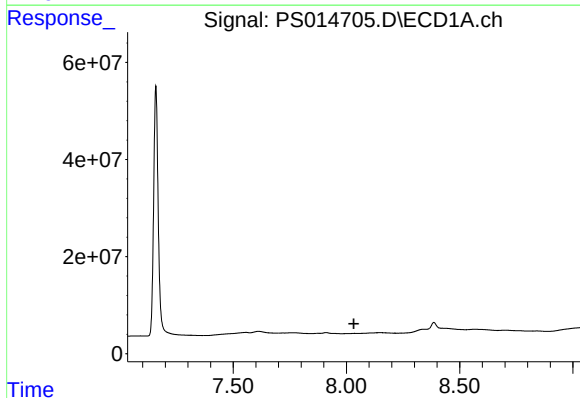


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

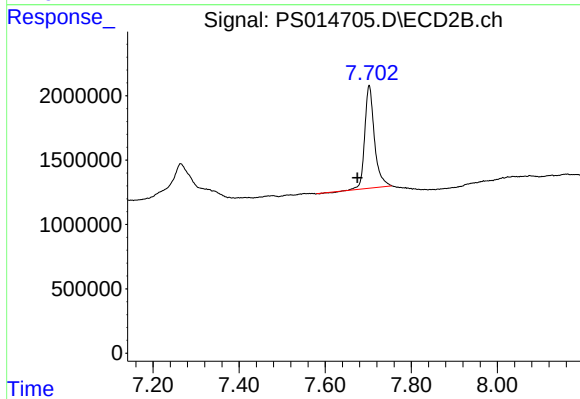

#8 DICHLORPROP


R.T.: 7.702 min
Delta R.T.: 0.027 min
Response: 12478528
Conc: 24.72 ng/ml

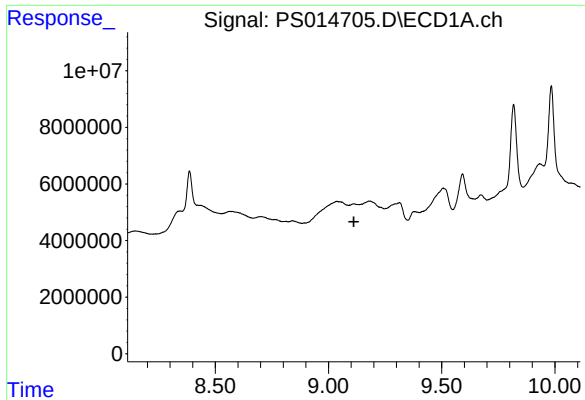

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

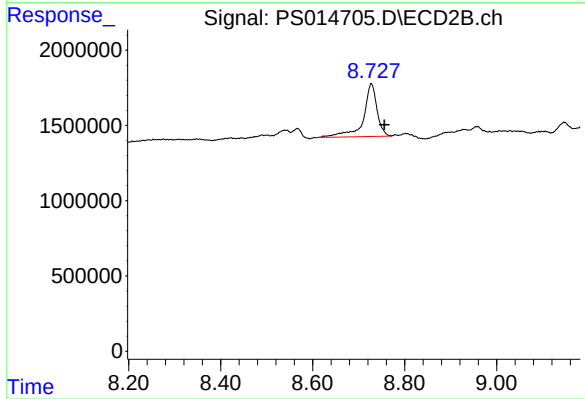


#11 2,4,5-TP (SILVEX)

R.T.: 8.727 min
Delta R.T.: -0.029 min
Response: 7220117
Conc: 2.64 ng/ml

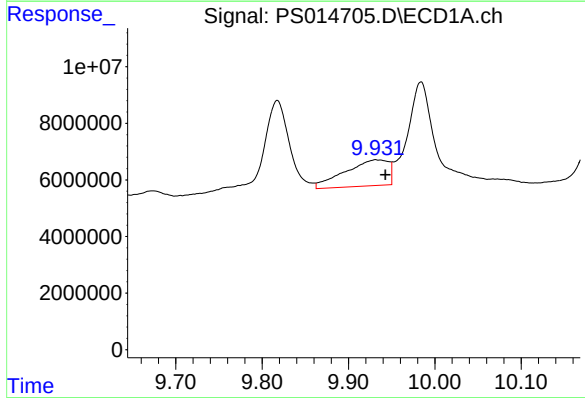


#13 2,4-DB

R.T.: 9.931 min
Delta R.T.: -0.012 min
Response: 32349653
Conc: 21.26 ng/ml

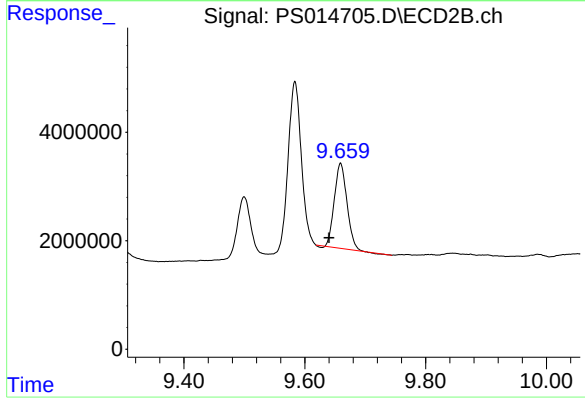

#13 2,4-DB


R.T.: 9.659 min
Delta R.T.: 0.019 min
Response: 22743529
Conc: 65.57 ng/ml

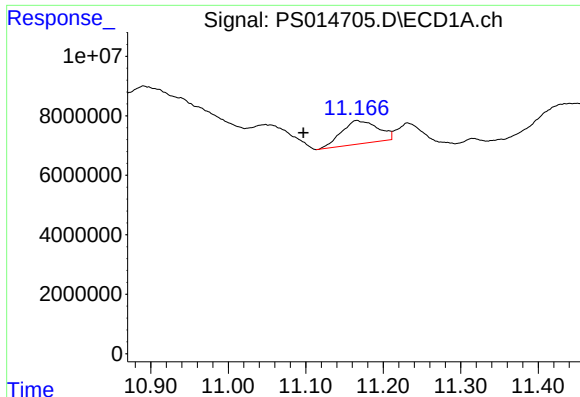

#14 DINOSEB


R.T.: 11.166 min
Delta R.T.: 0.069 min
Response: 25497957
Conc: 3.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

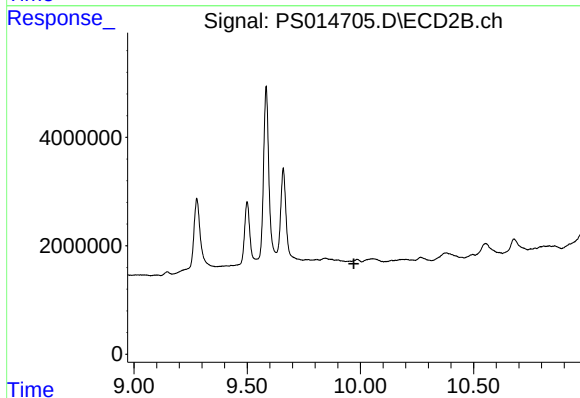


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

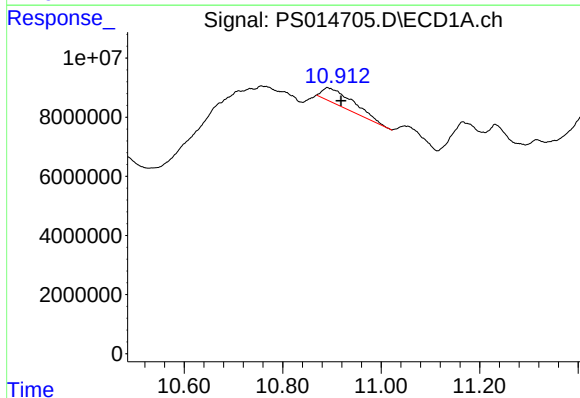

#15 Picloram

R.T.: 10.891 min
Delta R.T.: -0.028 min
Response: 23247676
Conc: 2.08 ng/ml

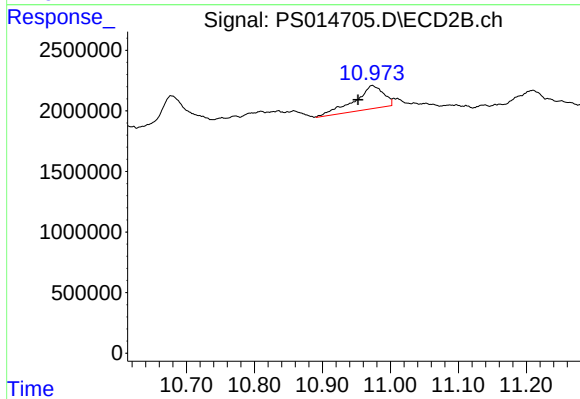

#15 Picloram

R.T.: 10.973 min
Delta R.T.: 0.021 min
Response: 5697120
Conc: 1.52 ng/ml