

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042021\
 Data File : PS014711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 17:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 18:05:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	6.884	730.3E6	268.2E6	480.071	576.140
Target Compounds							
6) T	MCPP	7.555	0.000	8298974	0	1.906	N.D. #
7) T	MCPA	7.607f	0.000	12912720	0	2.075	N.D. #
8) T	DICHLORPROP	0.000	7.701	0	17246011	N.D.	34.163
11) T	2,4,5-TP ...	9.113	8.728	3710929	11382383	<MDL	4.167 #
12) T	2,4,5-T	9.408	9.147	9635462	1911007	1.171	<MDL #
13) T	2,4-DB	9.938	9.659	34585214	26465438	22.727	76.297 #
15) T	Picloram	10.940	10.972	22769091	7988933	2.035	2.130
16) T	DCPA	0.000	10.899	0	1967644	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042021\
Data File : PS014711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 17:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 18:05:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

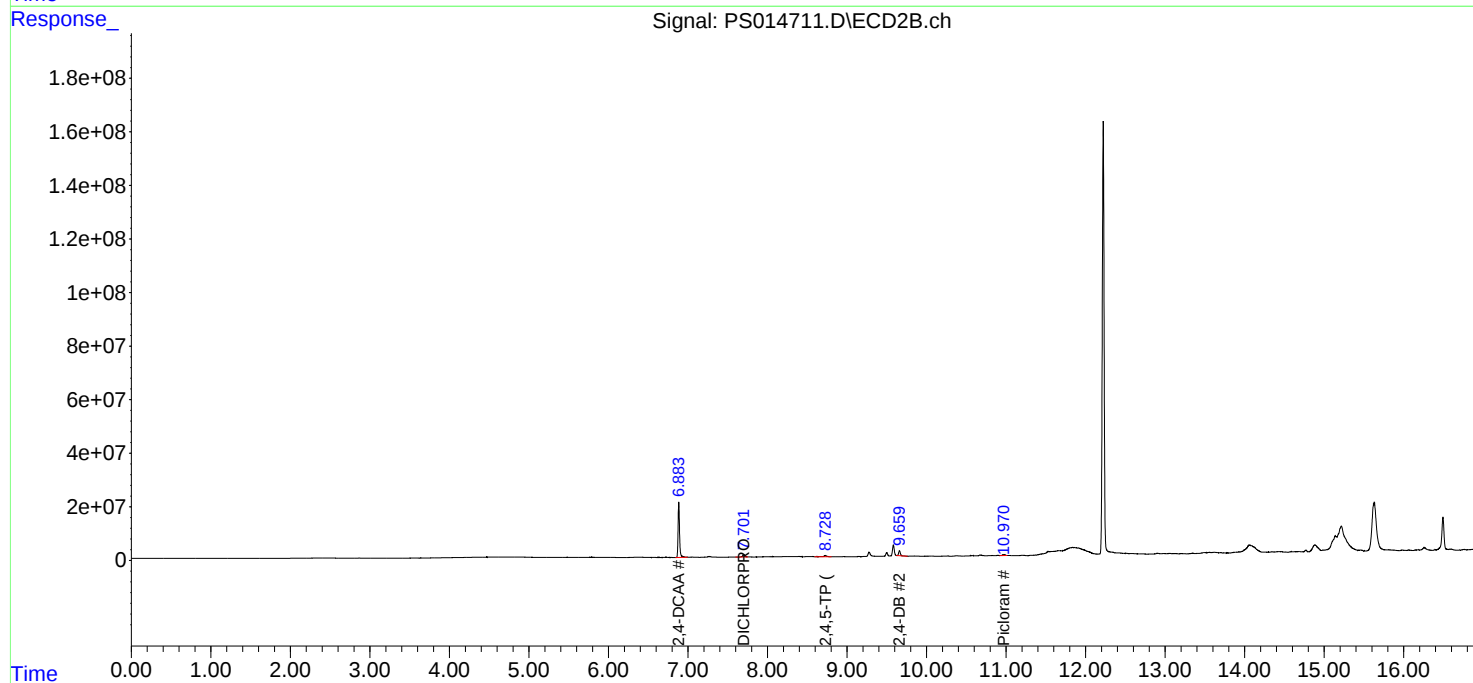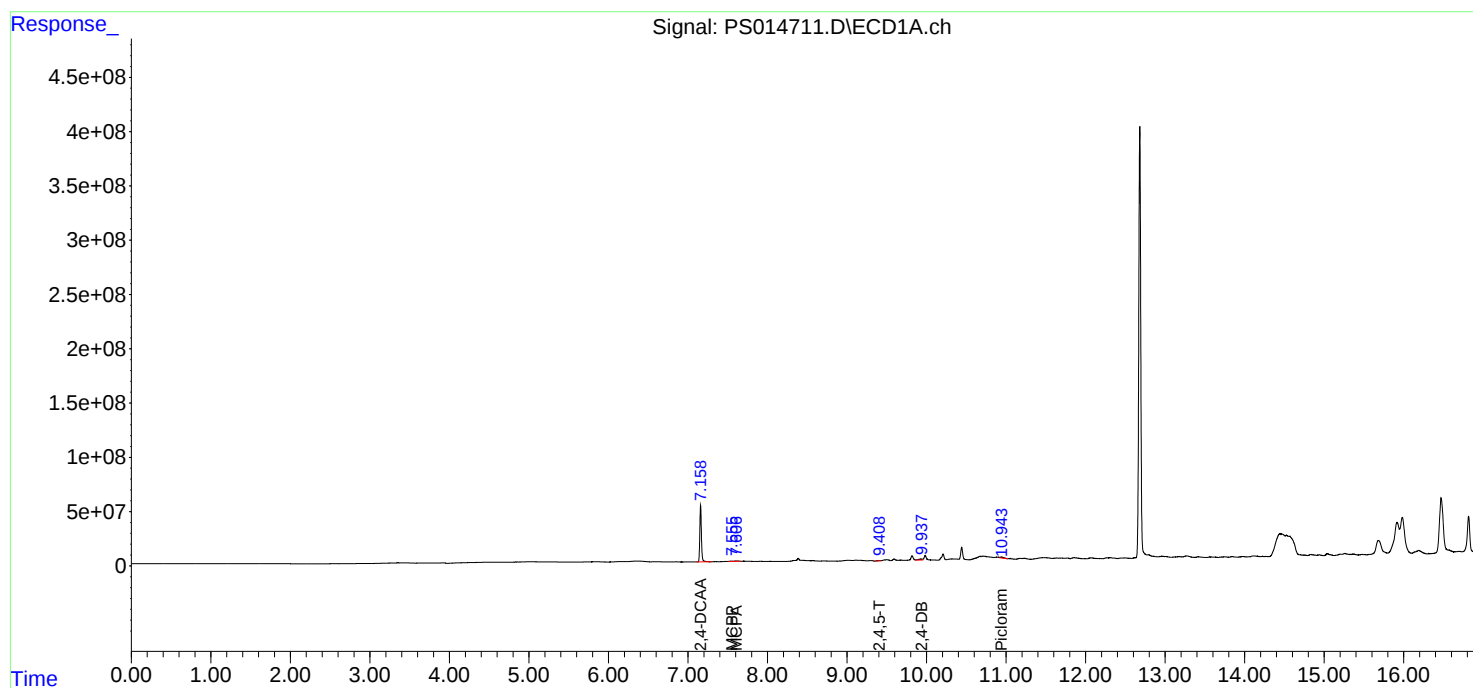


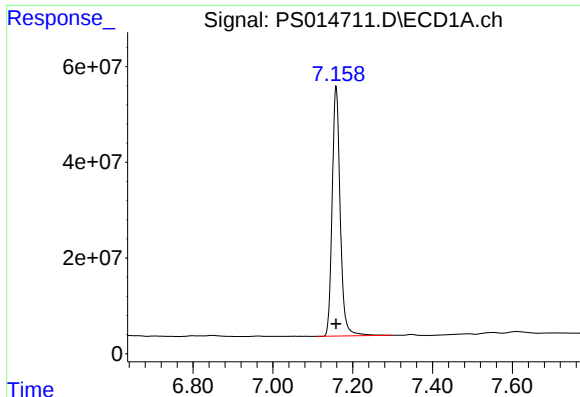

#4 2,4-DCAA


R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 730281974
Conc: 480.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

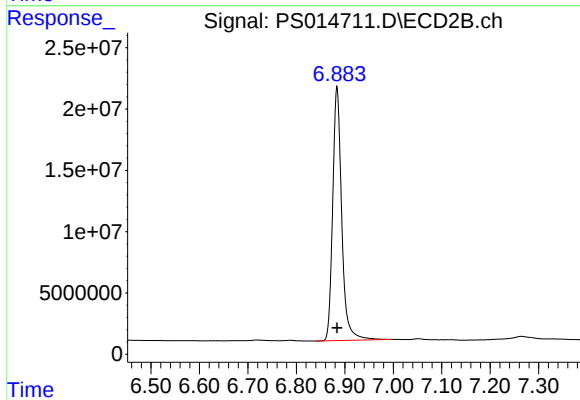


#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 268167293
Conc: 576.14 ng/ml

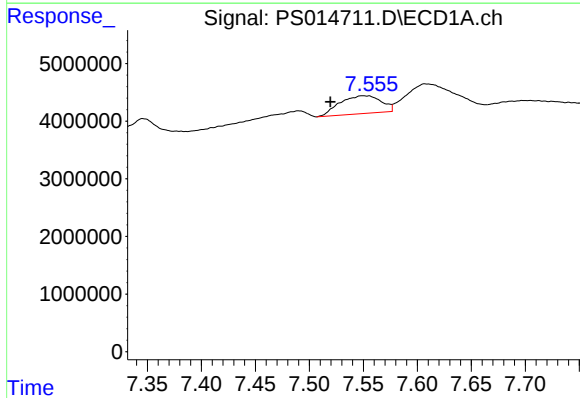


#6 MCP

R.T.: 7.555 min
Delta R.T.: 0.035 min
Response: 8298974
Conc: 1.91 ug/ml

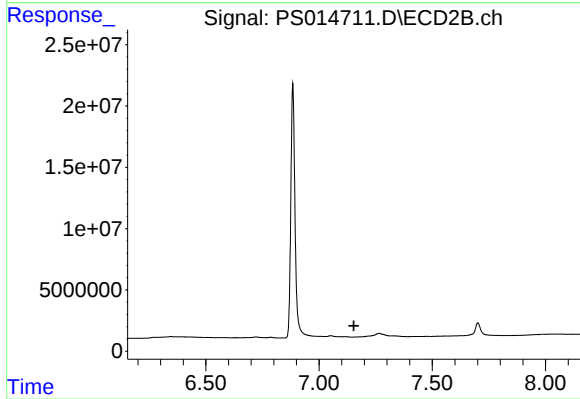

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

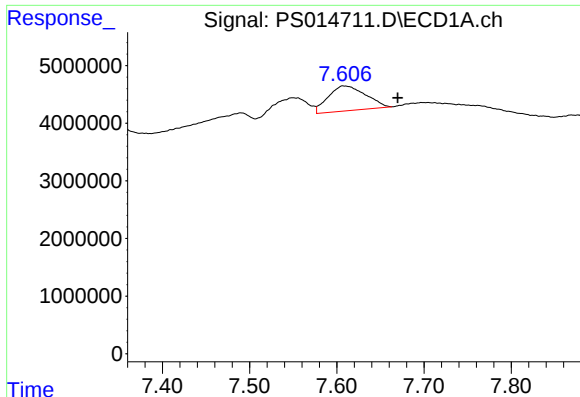

#7 MCPA


R.T.: 7.607 min
Delta R.T.: -0.063 min
Response: 12912720
Conc: 2.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

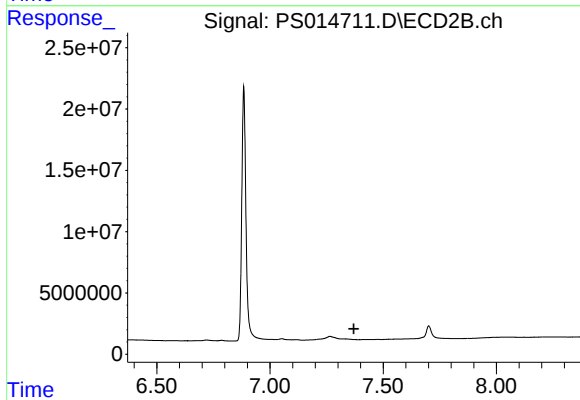


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.370 min
Response: 0
Conc: N.D.

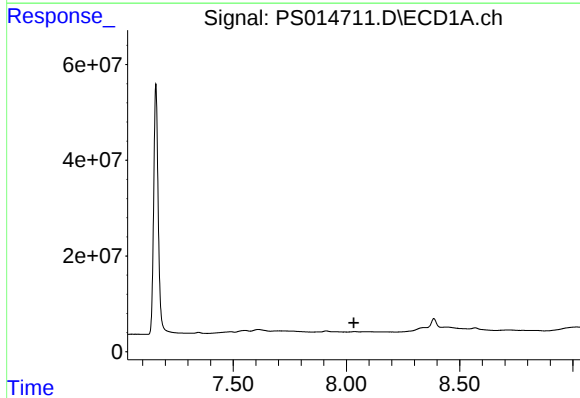


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

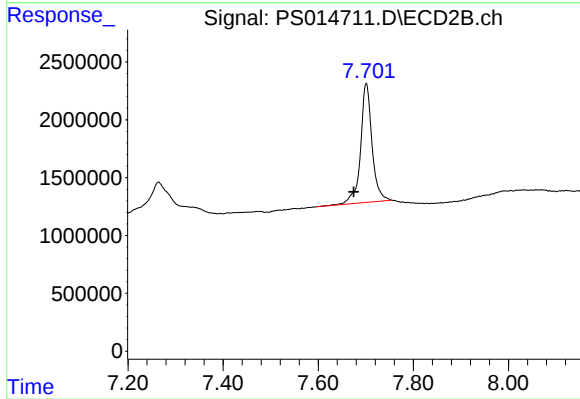

#8 DICHLORPROP


R.T.: 7.701 min
Delta R.T.: 0.026 min
Response: 17246011
Conc: 34.16 ng/ml

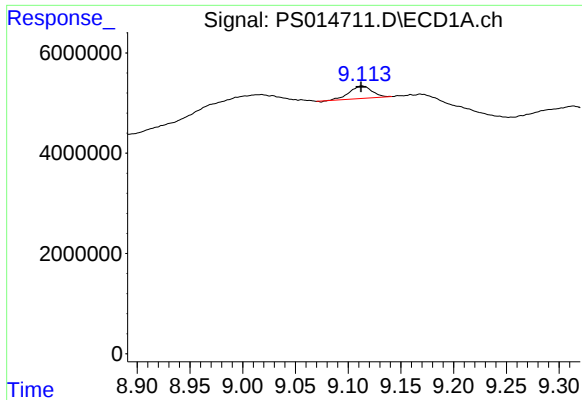

#11 2,4,5-TP (SILVEX)


R.T.: 9.113 min
Delta R.T.: 0.001 min
Response: 3710929
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

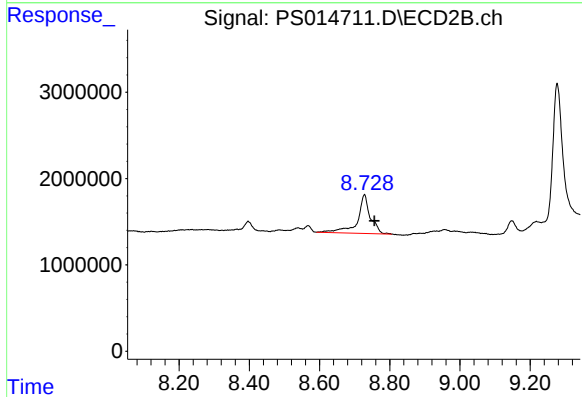


#11 2,4,5-TP (SILVEX)

R.T.: 8.728 min
Delta R.T.: -0.028 min
Response: 11382383
Conc: 4.17 ng/ml

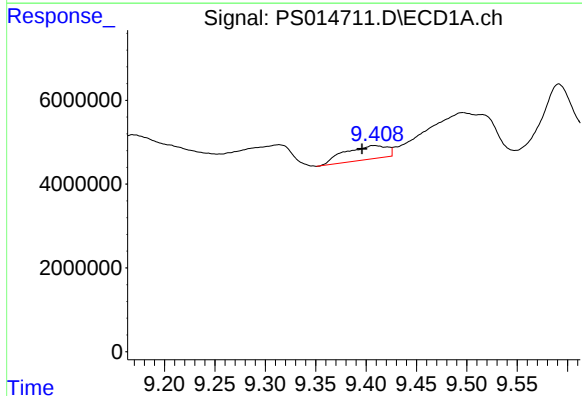


#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: 0.012 min
Response: 9635462
Conc: 1.17 ng/ml

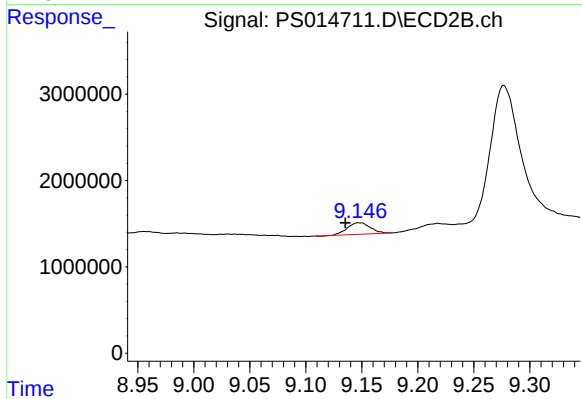

#12 2,4,5-T


R.T.: 9.147 min
Delta R.T.: 0.012 min
Response: 1911007
Conc: N.D.

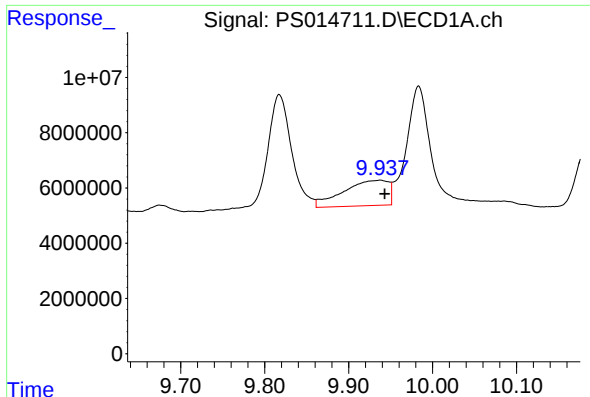

#13 2,4-DB


R.T.: 9.938 min
Delta R.T.: -0.005 min
Response: 34585214
Conc: 22.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

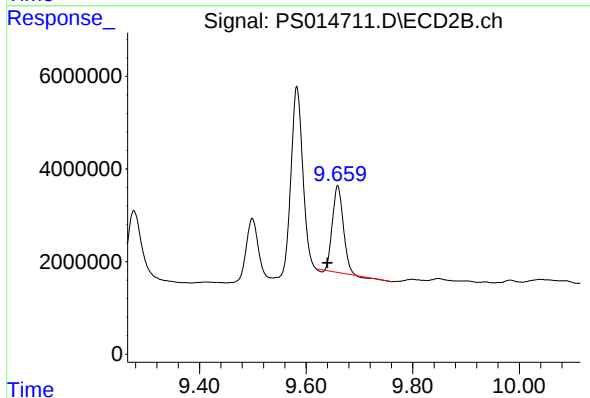


#13 2,4-DB

R.T.: 9.659 min
Delta R.T.: 0.019 min
Response: 26465438
Conc: 76.30 ng/ml

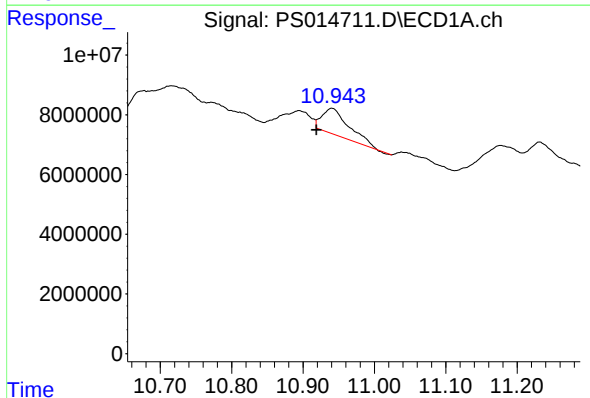

#15 Picloram

R.T.: 10.940 min
Delta R.T.: 0.021 min
Response: 22769091
Conc: 2.04 ng/ml

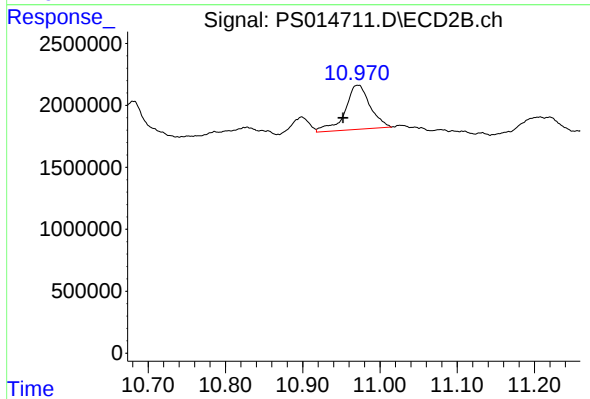

#15 Picloram

R.T.: 10.972 min
Delta R.T.: 0.019 min
Response: 7988933
Conc: 2.13 ng/ml