

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042022\
 Data File : PS019085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 09:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:02:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.798	1585.3E6	366.9E6	423.860	505.478
Target Compounds							
7) T	MCPA	7.675f	0.000	7011658	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.207	8.629	4252500	2647719	<MDL	<MDL #
12) T	2,4,5-T	9.488	9.115f	6257119	4963333	<MDL	1.149 #
14) T	DINOSEB	11.143f	0.000	37215904	0	2.432	N.D. #
15) T	Picloram	10.989	10.880	12246700	24623191	<MDL	4.159 #
16) T	DCPA	0.000	10.880f	0	24623191	N.D.	4.302



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042022\
Data File : PS019085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 09:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:02:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

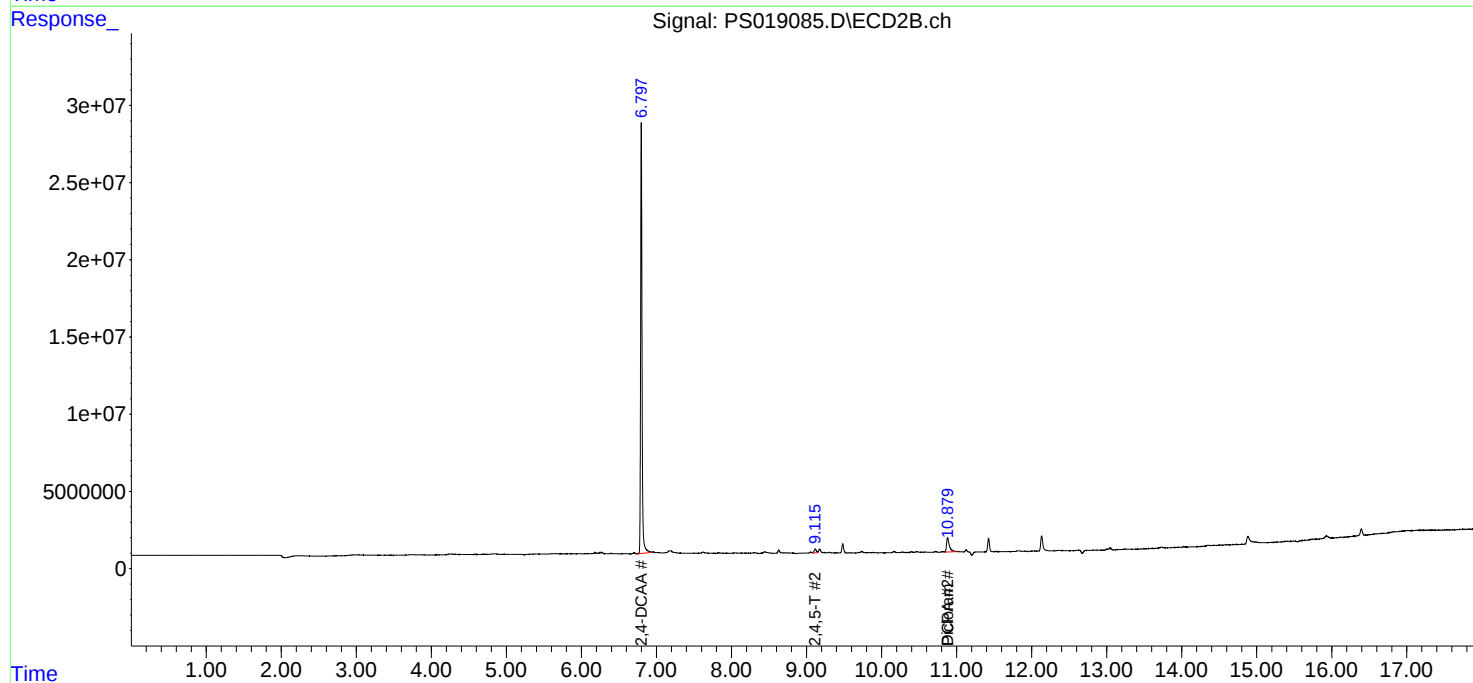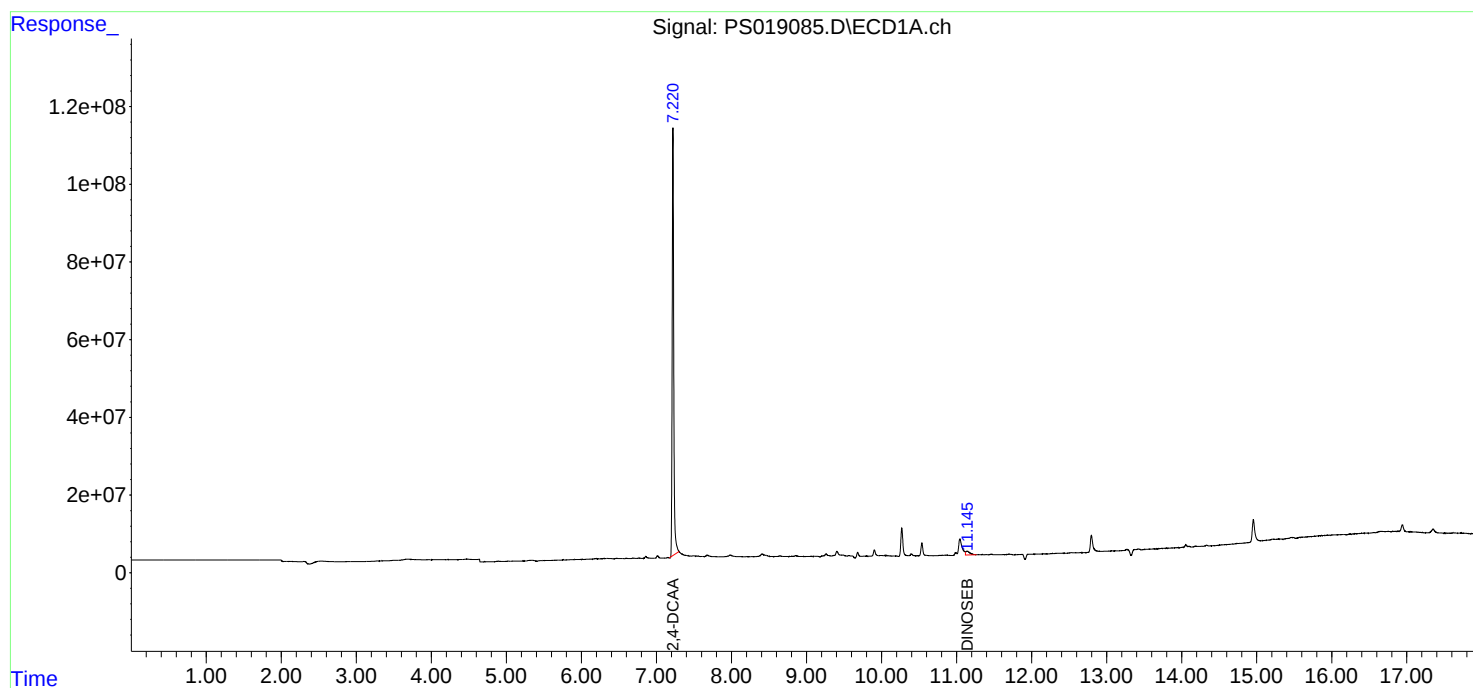


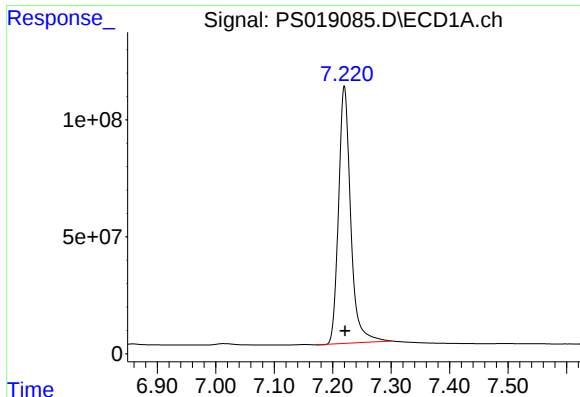

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: -0.001 min
Response: 1585259212
Conc: 423.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

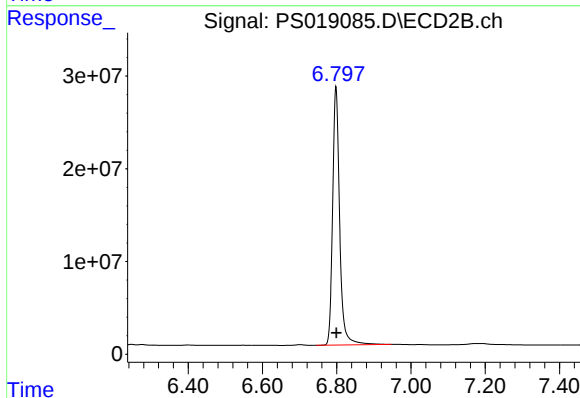


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 366914634
Conc: 505.48 ng/ml

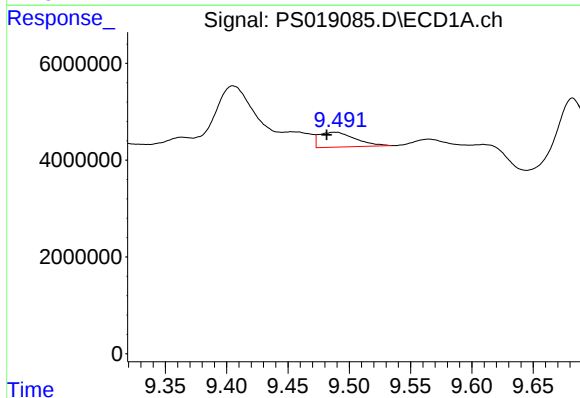


#12 2,4,5-T

R.T.: 9.488 min
Delta R.T.: 0.006 min
Response: 6257119
Conc: N.D.

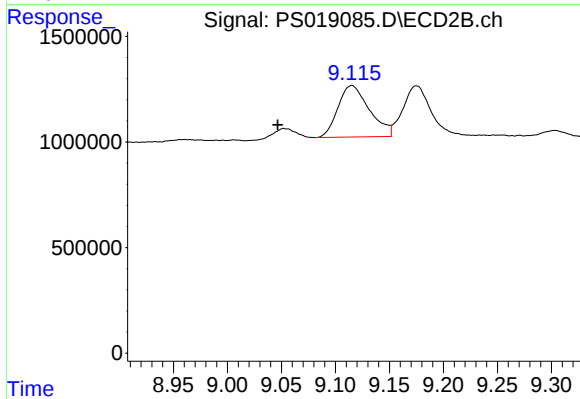

#12 2,4,5-T


R.T.: 9.115 min
Delta R.T.: 0.069 min
Response: 4963333
Conc: 1.15 ng/ml

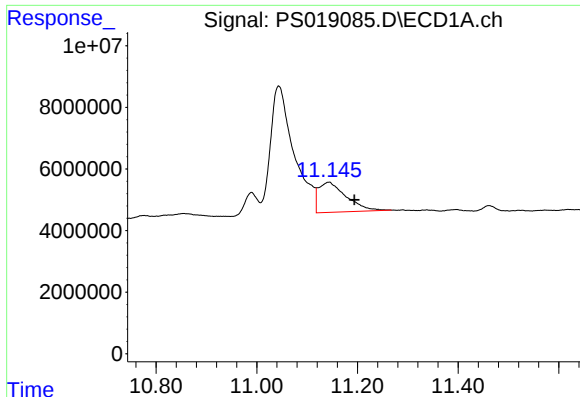

#14 DINOSEB


R.T.: 11.143 min
Delta R.T.: -0.051 min
Response: 37215904
Conc: 2.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

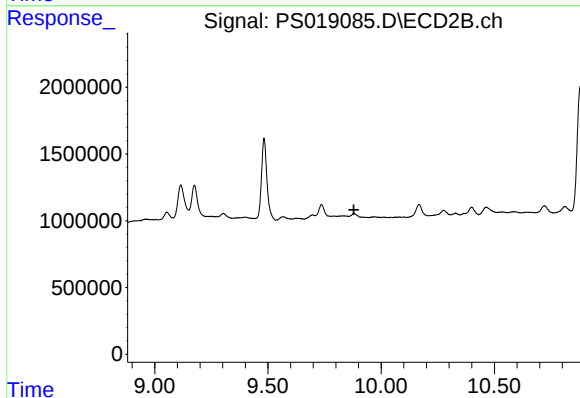


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

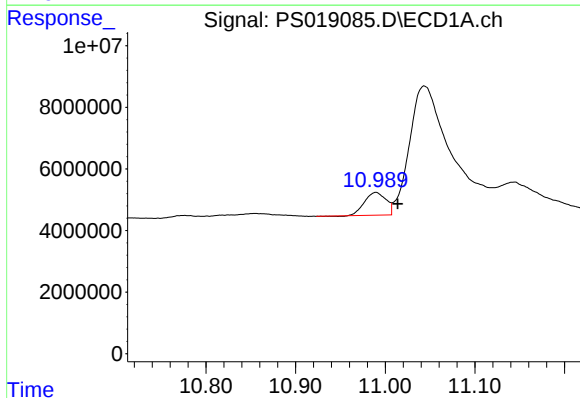


#15 Picloram

R.T.: 10.989 min
Delta R.T.: -0.025 min
Response: 12246700
Conc: N.D.

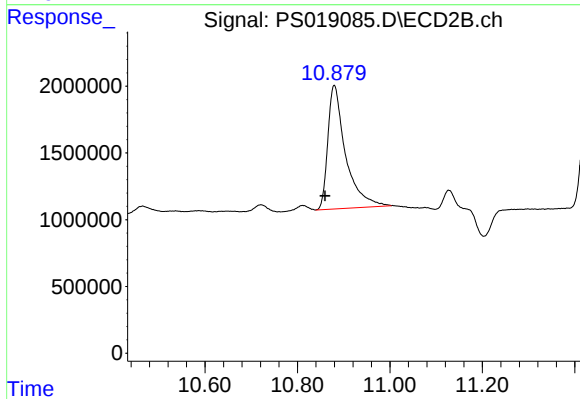

#15 Picloram


R.T.: 10.880 min
Delta R.T.: 0.020 min
Response: 24623191
Conc: 4.16 ng/ml

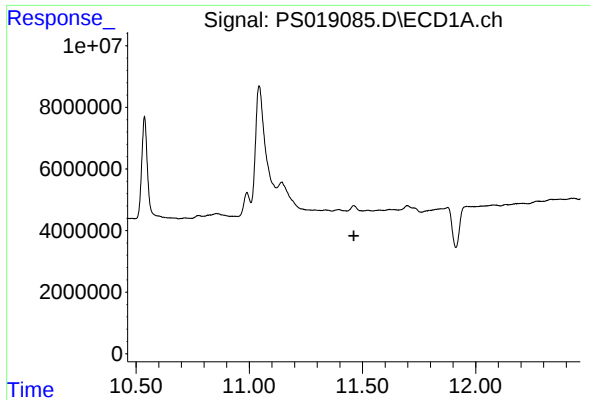

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

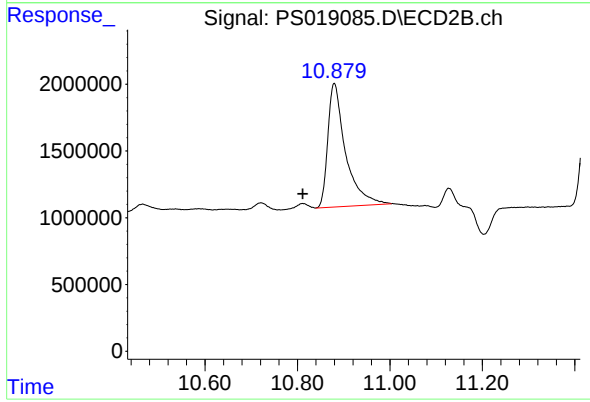

#16 DCPA

R.T.: 10.880 min
Delta R.T.: 0.068 min
Response: 24623191
Conc: 4.30 ng/ml