

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042022\
 Data File : PS019097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 20:34
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:05:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.798	1654.7E6	380.3E6	442.435	523.871
Target Compounds							
8) T	DICHLORPROP	0.000	7.611	0	2062934	N.D.	2.469
9) T	2,4-D	8.343	0.000	88434	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.257f	8.627f	25363668	8190056	1.274	1.739 #
12) T	2,4,5-T	9.481	9.107f	16456422	2844206	<MDL	<MDL #
13) T	2,4-DB	10.033	0.000	4913255	0	1.395	N.D. #
14) T	DINOSEB	11.139f	0.000	48141219	0	3.146	N.D. #
15) T	Picloram	11.028	10.872	60219568	9972032	2.247	1.684 #
16) T	DCPA	11.459	10.872f	2843208	9972032	<MDL	1.742 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042022\
Data File : PS019097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 20:34
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:05:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

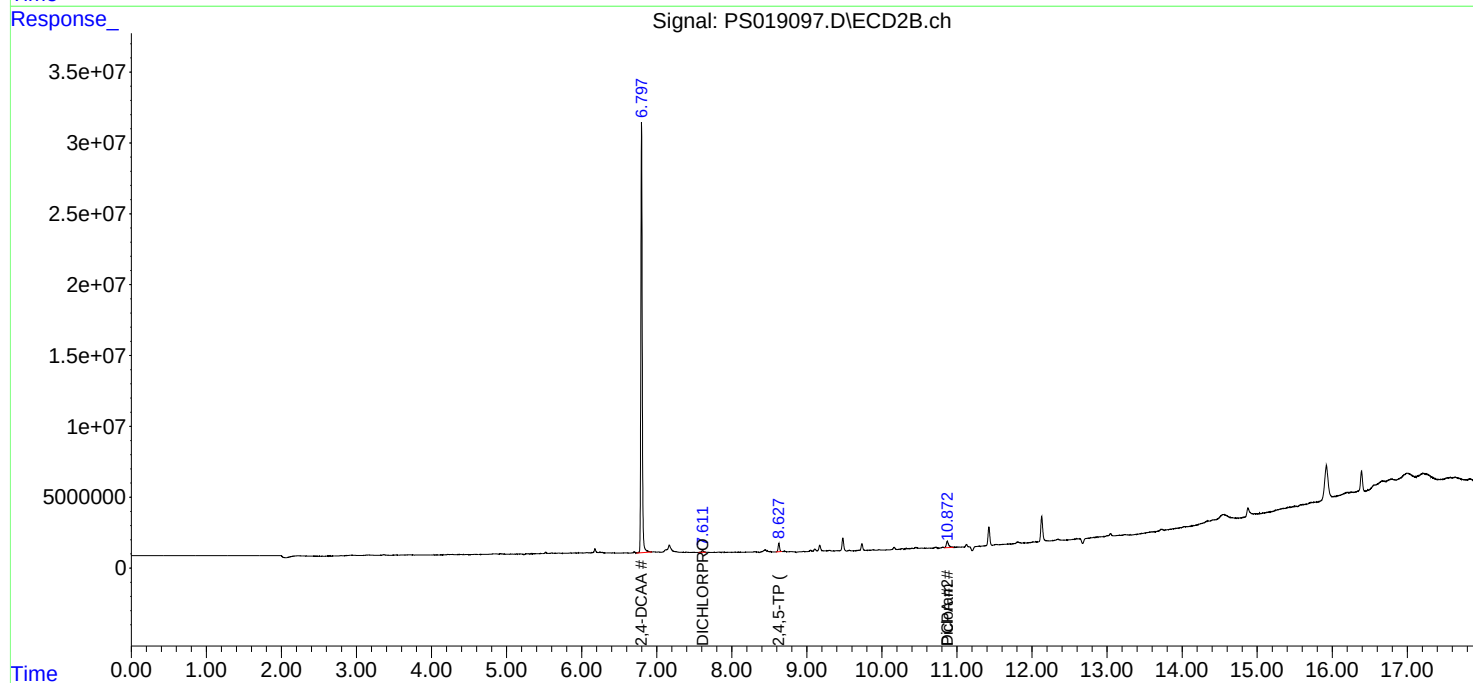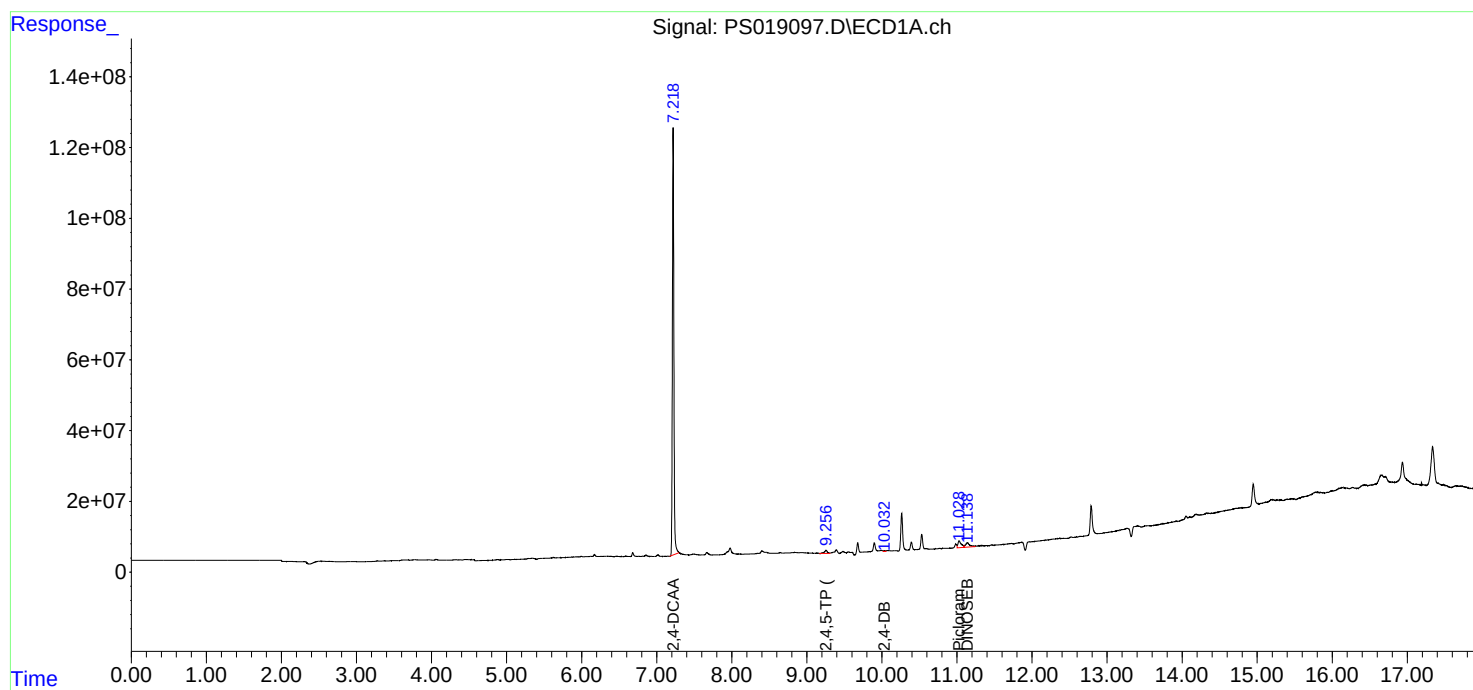


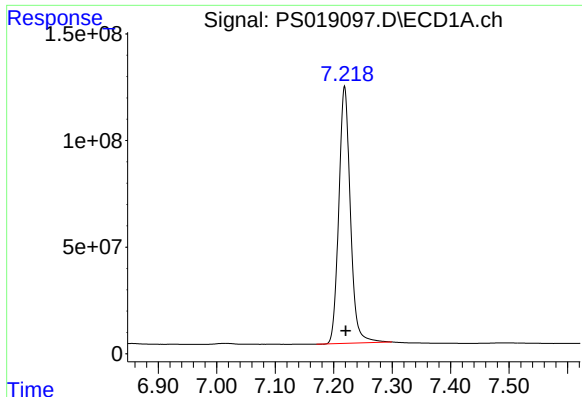

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.002 min
Response: 1654730260
Conc: 442.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

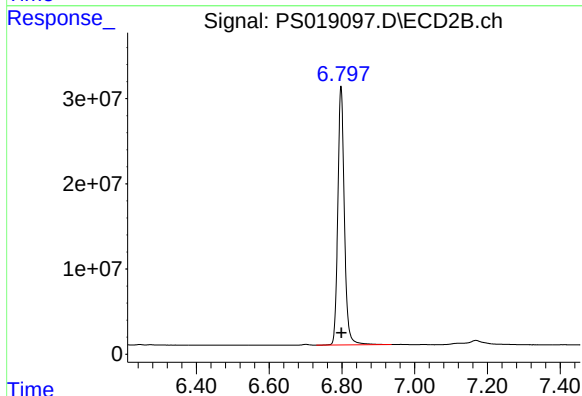


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: -0.001 min
Response: 380265829
Conc: 523.87 ng/ml

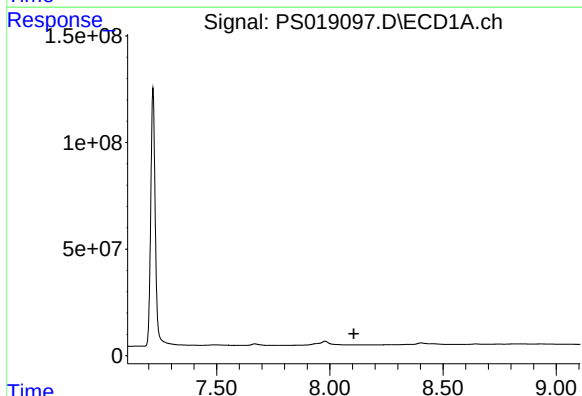


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.106 min
Response: 0
Conc: N.D.

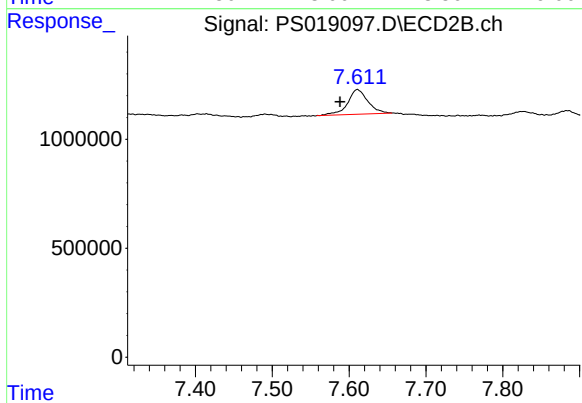

#8 DICHLORPROP


R.T.: 7.611 min
Delta R.T.: 0.023 min
Response: 2062934
Conc: 2.47 ng/ml

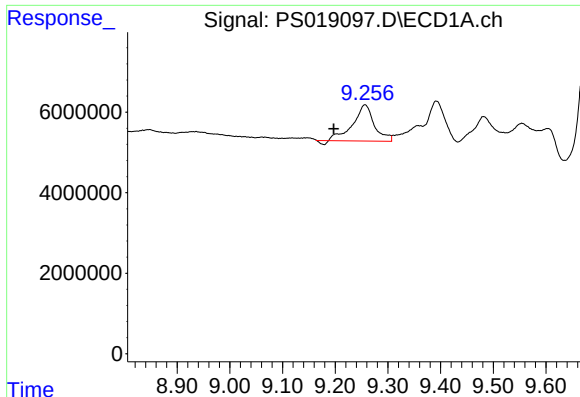

#11 2,4,5-TP (SILVEX)


R.T.: 9.257 min
Delta R.T.: 0.059 min
Response: 25363668
Conc: 1.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

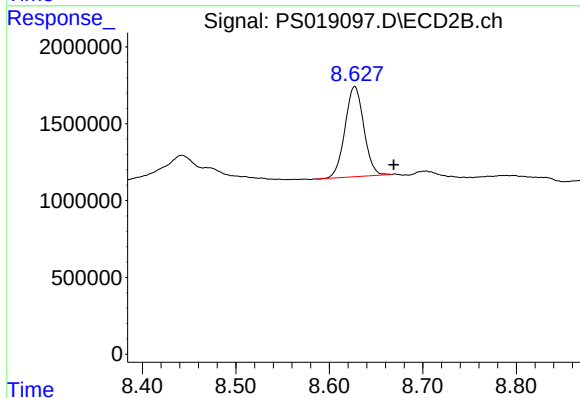


#11 2,4,5-TP (SILVEX)

R.T.: 8.627 min
Delta R.T.: -0.042 min
Response: 8190056
Conc: 1.74 ng/ml

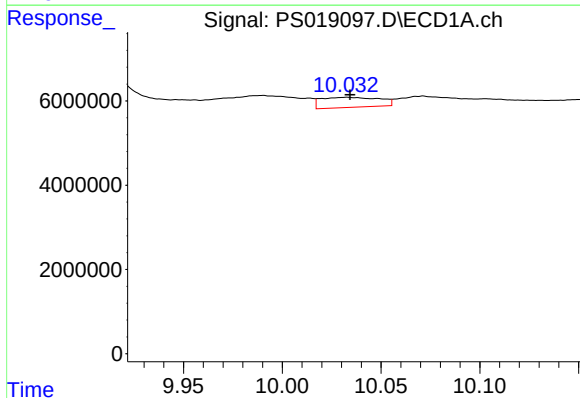


#13 2,4-DB

R.T.: 10.033 min
Delta R.T.: -0.002 min
Response: 4913255
Conc: 1.40 ng/ml

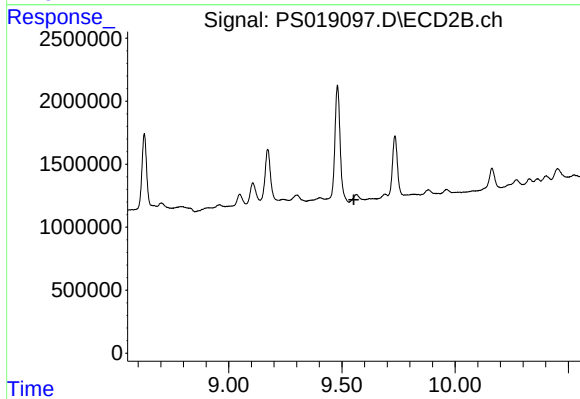

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.553 min
Response: 0
Conc: N.D.

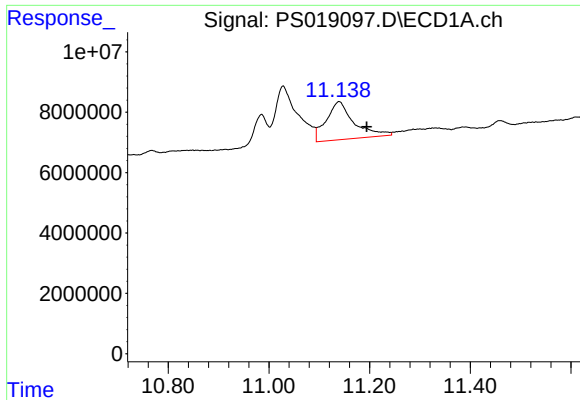

#14 DINOSEB


R.T.: 11.139 min
Delta R.T.: -0.055 min
Response: 48141219
Conc: 3.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

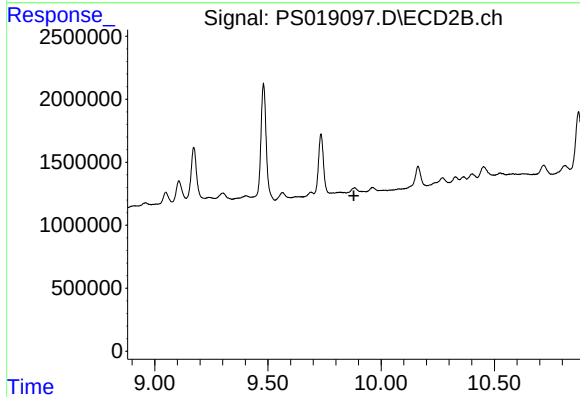


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

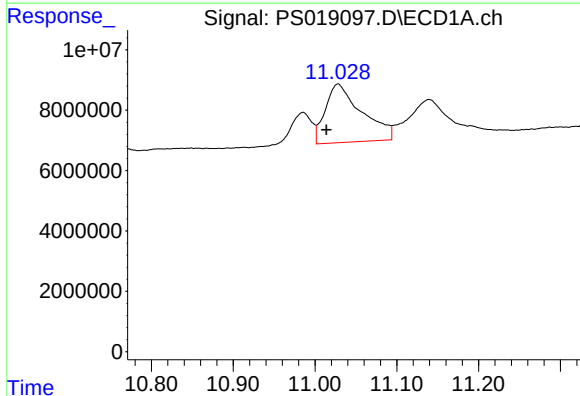


#15 Picloram

R.T.: 11.028 min
Delta R.T.: 0.014 min
Response: 60219568
Conc: 2.25 ng/ml

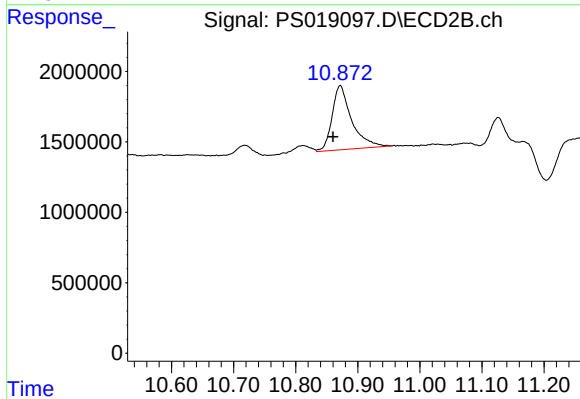

#15 Picloram


R.T.: 10.872 min
Delta R.T.: 0.012 min
Response: 9972032
Conc: 1.68 ng/ml

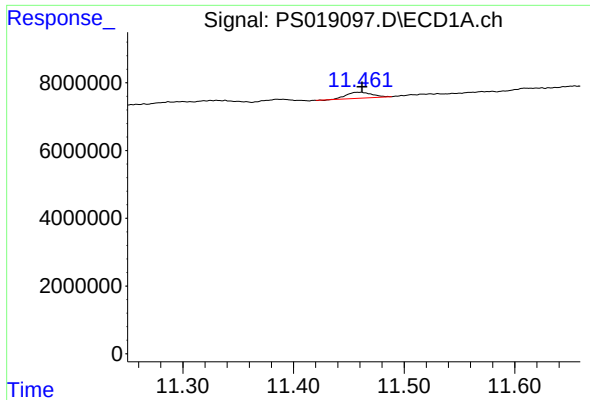

#16 DCPA

R.T.: 11.459 min
Delta R.T.: -0.003 min
Response: 2843208
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

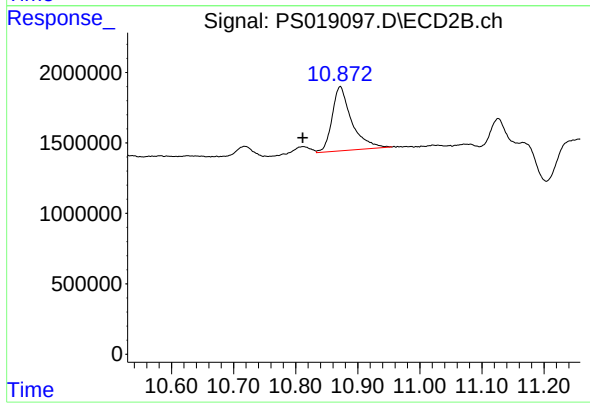

#16 DCPA

R.T.: 10.872 min
Delta R.T.: 0.061 min
Response: 9972032
Conc: 1.74 ng/ml