

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042023\
 Data File : PS022792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 19:46
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 21:45:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 12 14:05:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.483	6.859	1344.4E6	471.1E6	539.972	462.303
Target Compounds							
1) T	Dalapon	2.576	0.000	479567	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.835	0.000	877064	0	<MDL	N.D. #
3) T	4-Nitroph...	6.319	0.000	6178797	0	3.330	N.D. #
5) T	DICAMBA	6.632	0.000	461636	0	<MDL	N.D. #
6) T	MCP	6.818	0.000	20091410	0	2.388	N.D. #
7) T	MCPA	6.858f	7.312	8588002	236781	<MDL	<MDL #
8) T	DICHLORPROP	7.242	7.669	1771345	5896517	<MDL	5.295 #
9) T	2,4-D	7.444	7.884f	1546765	917396	<MDL	<MDL #
10) T	Pentachlo...	7.679	8.368	3377567	1064709	<MDL	<MDL #
11) T	2,4,5-TP ...	8.215	8.730	11769088	542408	<MDL	<MDL #
12) T	2,4,5-T	8.475	9.107	10005557	2117450	<MDL	<MDL #
13) T	2,4-DB	9.006	9.623	14388362	682600	3.367	<MDL #
14) T	DINOSEB	10.069	0.000	1666969	0	<MDL	N.D. #
15) T	Picloram	9.886	10.914	33187592	5922140	1.114	<MDL #
16) T	DCPA	10.336	10.874	6033449	1029491	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042023\
Data File : PS022792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 19:46
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 21:45:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
Quant Title : 8080.M
QLast Update : Wed Apr 12 14:05:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

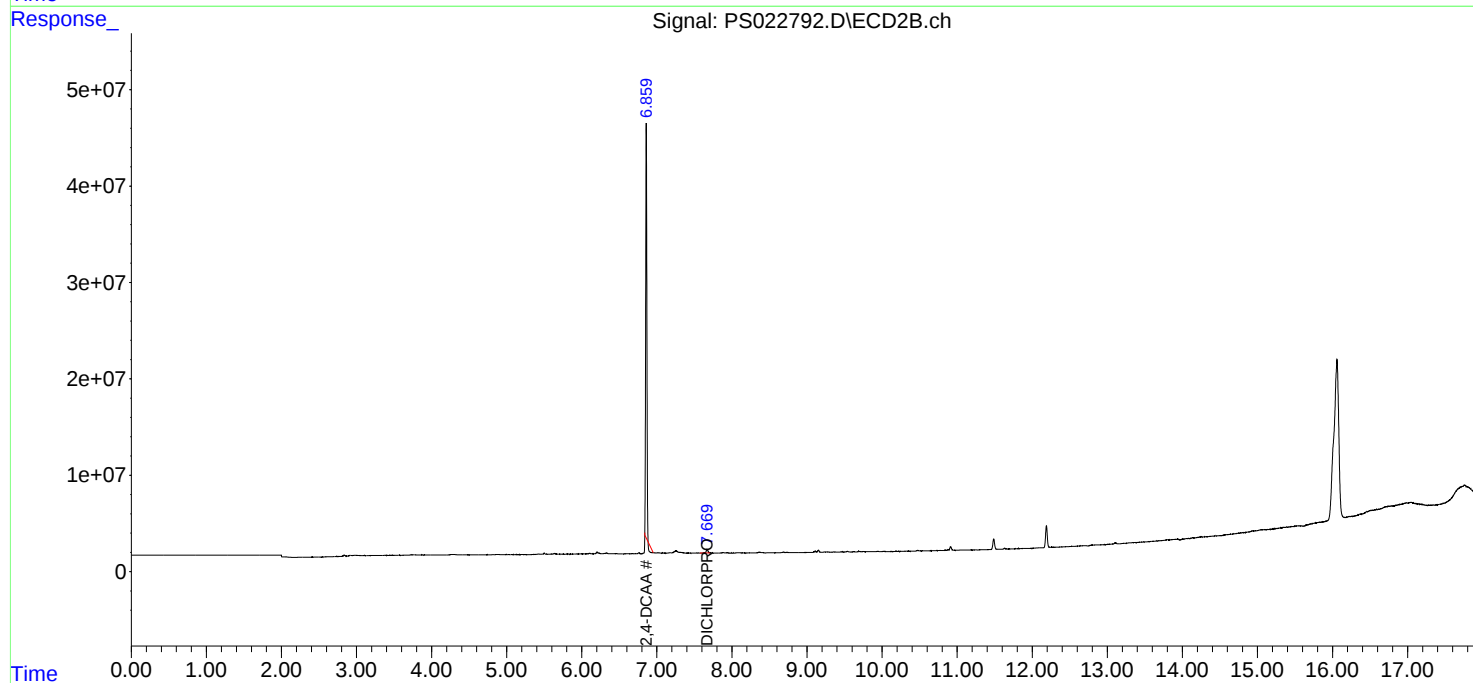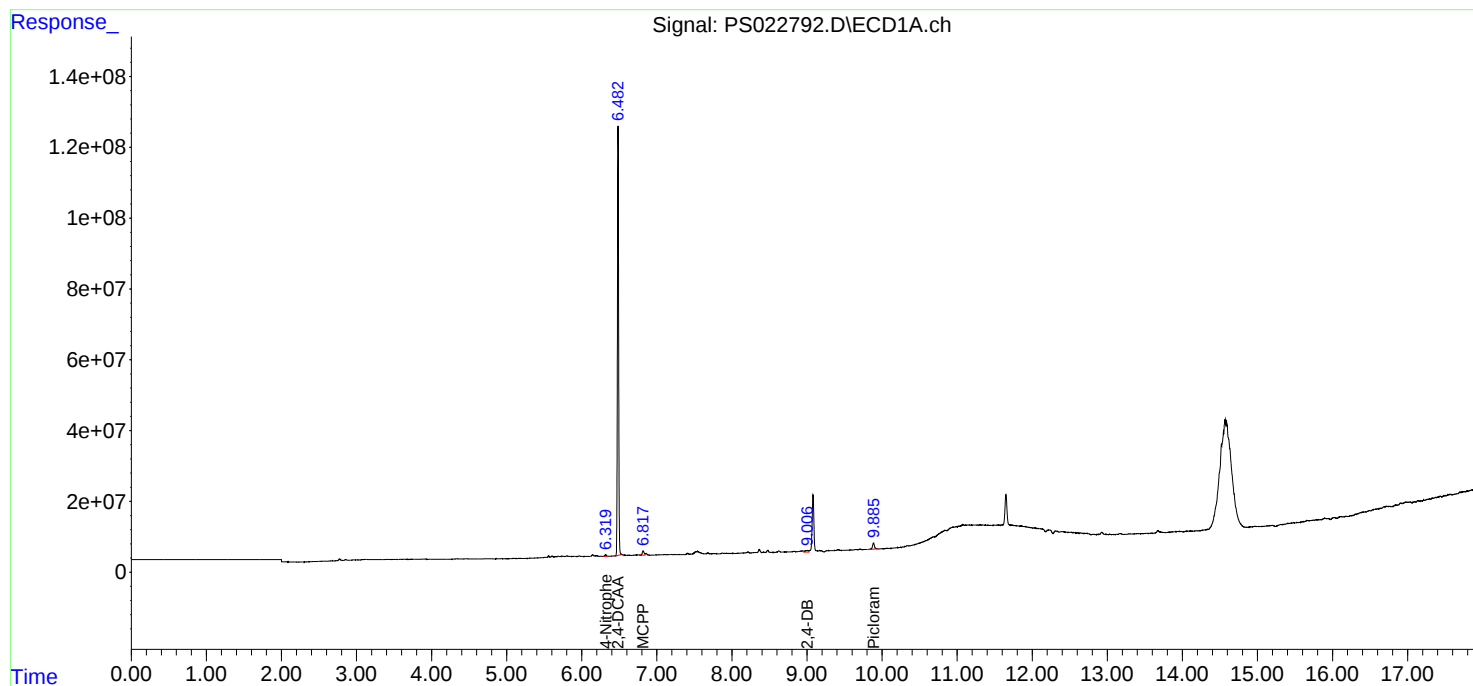


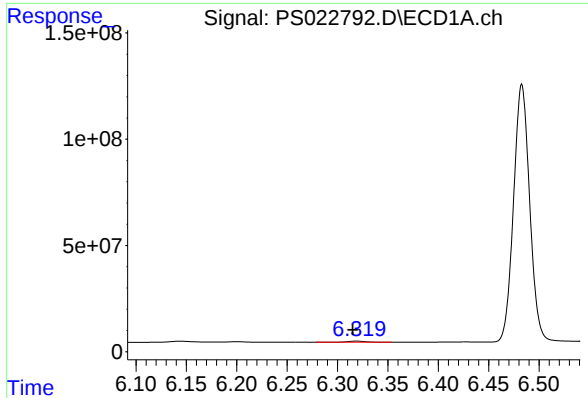

#3 4-Nitrophenol


R.T.: 6.319 min
Delta R.T.: 0.004 min
Response: 6178797
Conc: 3.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

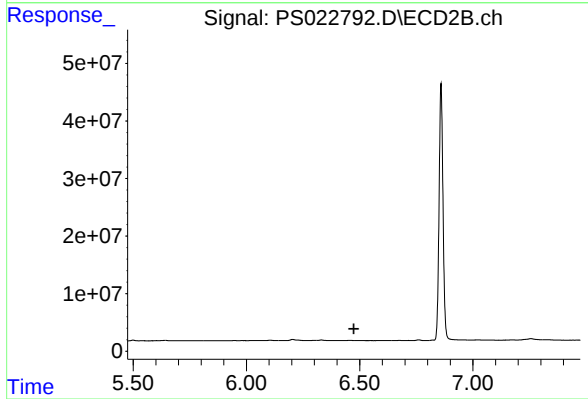


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

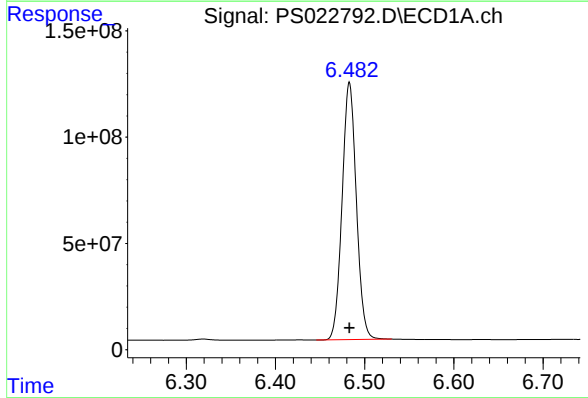


#4 2,4-DCAA

R.T.: 6.483 min
Delta R.T.: 0.000 min
Response: 1344370258
Conc: 539.97 ng/ml

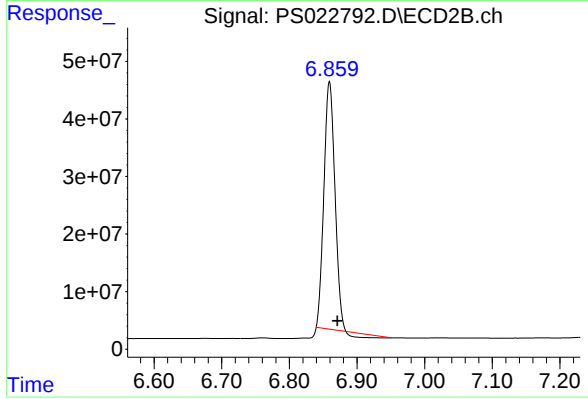

#4 2,4-DCAA


R.T.: 6.859 min
Delta R.T.: -0.012 min
Response: 471061857
Conc: 462.30 ng/ml

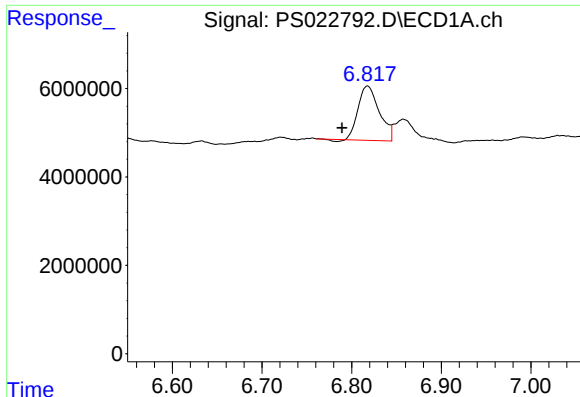

#6 MCP


R.T.: 6.818 min
Delta R.T.: 0.028 min
Response: 20091410
Conc: 2.39 ug/ml

Instrument :
ECD_S
ClientSampleId :

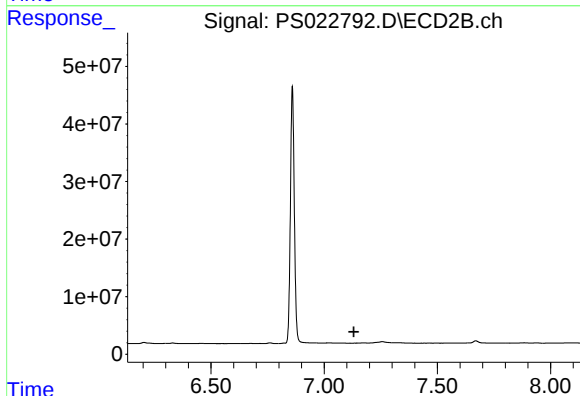


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.132 min
Response: 0
Conc: N.D.

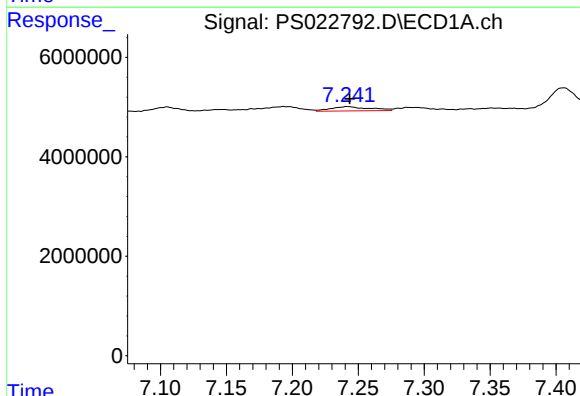


#8 DICHLORPROP

R.T.: 7.242 min
Delta R.T.: -0.002 min
Response: 1771345
Conc: N.D.

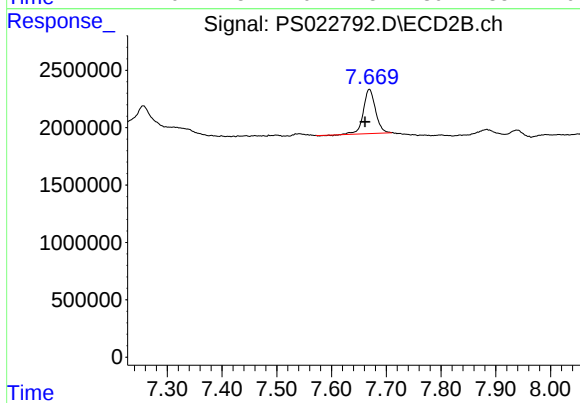

#8 DICHLORPROP


R.T.: 7.669 min
Delta R.T.: 0.008 min
Response: 5896517
Conc: 5.30 ng/ml

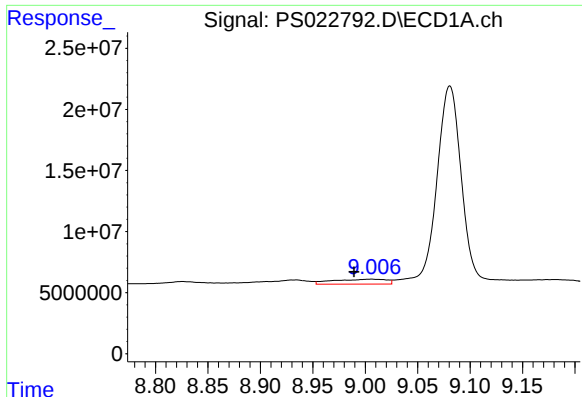

#13 2,4-DB


R.T.: 9.006 min
Delta R.T.: 0.016 min
Response: 14388362
Conc: 3.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

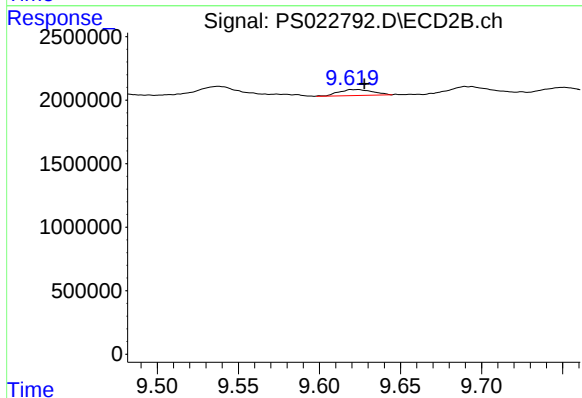


#13 2,4-DB

R.T.: 9.623 min
Delta R.T.: -0.005 min
Response: 682600
Conc: N.D.

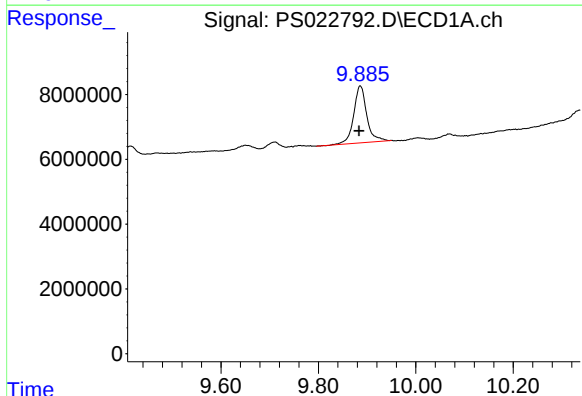

#15 Picloram

R.T.: 9.886 min
Delta R.T.: 0.003 min
Response: 33187592
Conc: 1.11 ng/ml

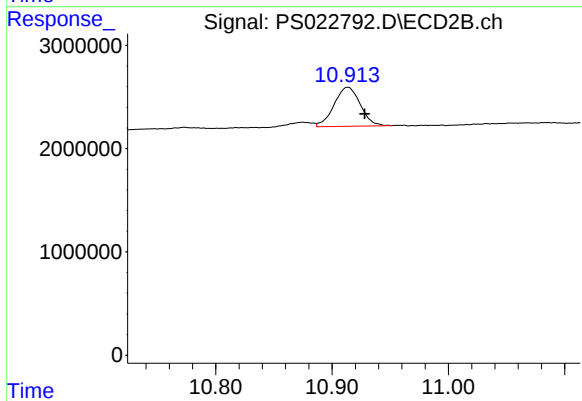

#15 Picloram

R.T.: 10.914 min
Delta R.T.: -0.014 min
Response: 5922140
Conc: N.D.