

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042023\
 Data File : PS022781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 15:13
 Operator : AR\AJ
 Sample : 02390-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SPC-1WC-23-04-17

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2023
 Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 21:35:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 12 14:05:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.483	6.859	458.0E6	216.1E6	183.948m	212.080m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042023\
Data File : PS022781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 15:13
Operator : AR\AJ
Sample : 02390-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SPC-1WC-23-04-17


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 21:35:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
Quant Title : 8080.M
QLast Update : Wed Apr 12 14:05:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

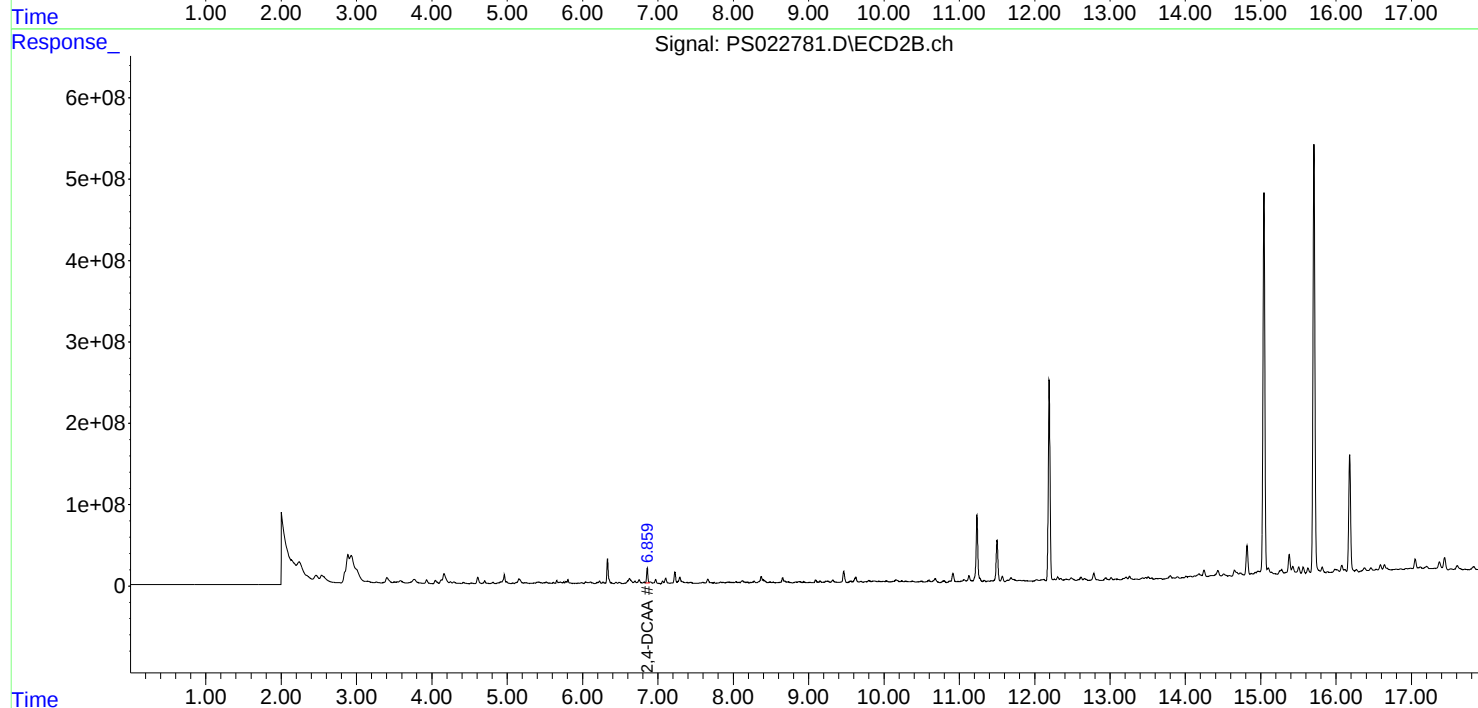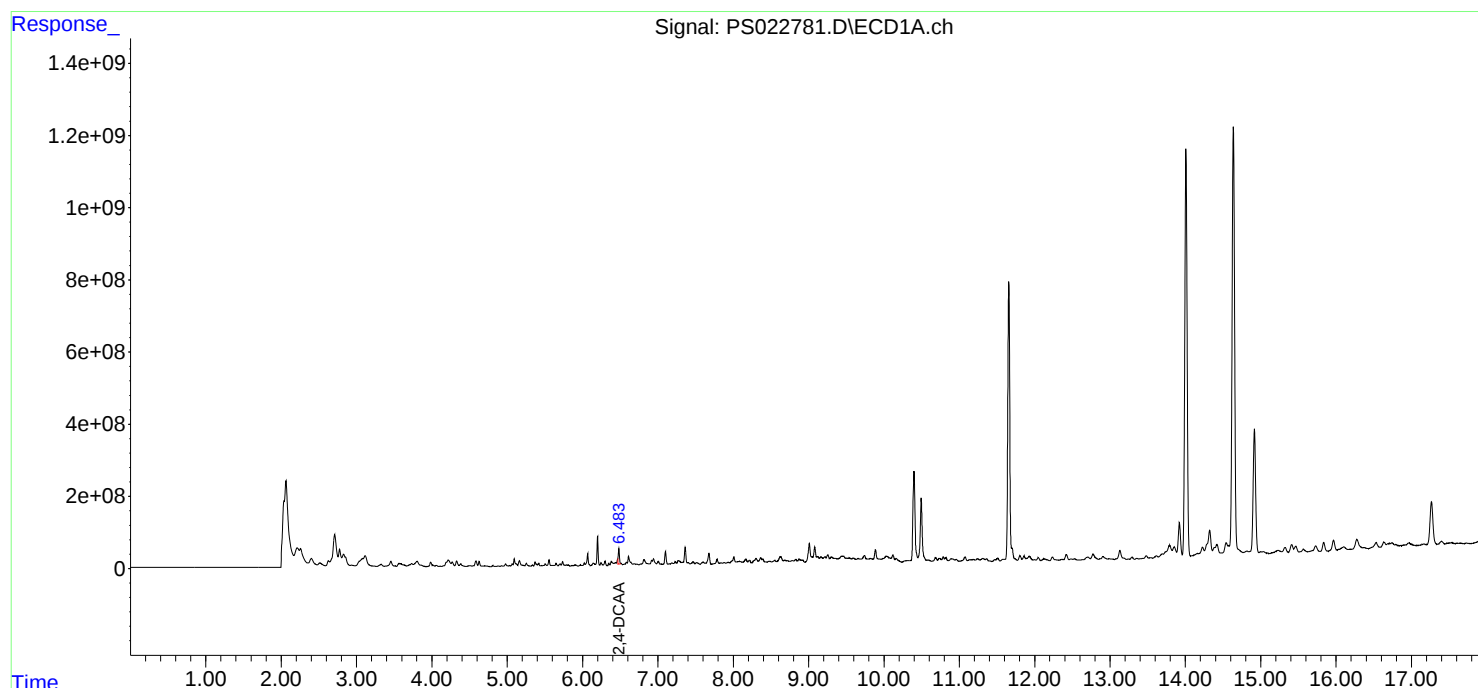

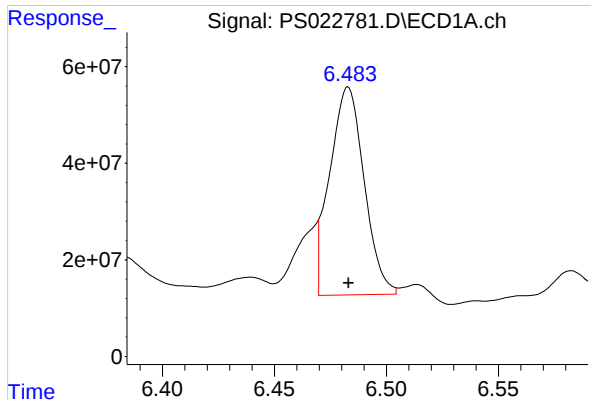


#4 2,4-DCAA

R.T.: 6.483 min
Delta R.T.: 0.000 min
Response: 457975637
Conc: 183.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
SPC-1WC-23-04-17

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

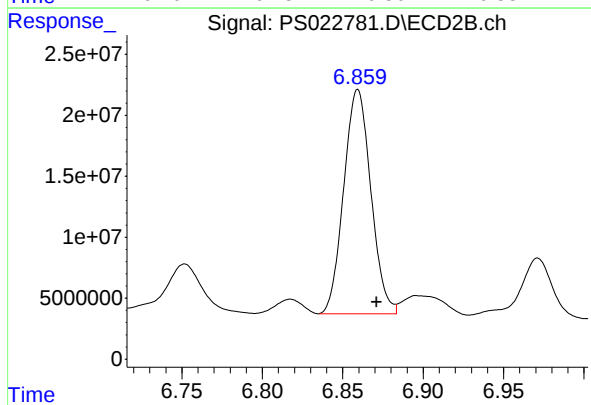

#4 2,4-DCAA

R.T.: 6.859 min
Delta R.T.: -0.012 min
Response: 216097841
Conc: 212.08 ng/ml m