

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042120\
 Data File : PS009904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 11:00
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 15:31:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.299	6.924	5257532	373894	8.707	<MDL #
Target Compounds							
2) T	3,5-DICHL...	6.489	0.000	863.9E6	0	1050.599	N.D. #
5) T	DICAMBA	0.000	7.093	0	904195	N.D.	<MDL
6) T	MCP	0.000	7.157	0	735.2E6	N.D.	446.673
8) T	DICHLORPROP	0.000	7.742	0	10489843	N.D.	20.841
9) T	2,4-D	8.421	0.000	858.6E6	0	1495.378	N.D. #
10) T	Pentachlo...	0.000	8.445	0	1980186	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.804	0	3642754	N.D.	1.393
12) T	2,4,5-T	0.000	9.186	0	2206700	N.D.	<MDL
13) T	2,4-DB	9.998	9.711	6376881	9274224	16.834	26.156 #
14) T	DINOSEB	0.000	10.024	0	1004487	N.D.	<MDL
15) T	Picloram	10.999	11.007	217.4E6	29556377	70.169	8.690 #
16) T	DCPA	0.000	10.956	0	4625799	N.D.	1.380



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042120\
Data File : PS009904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 11:00
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 15:31:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

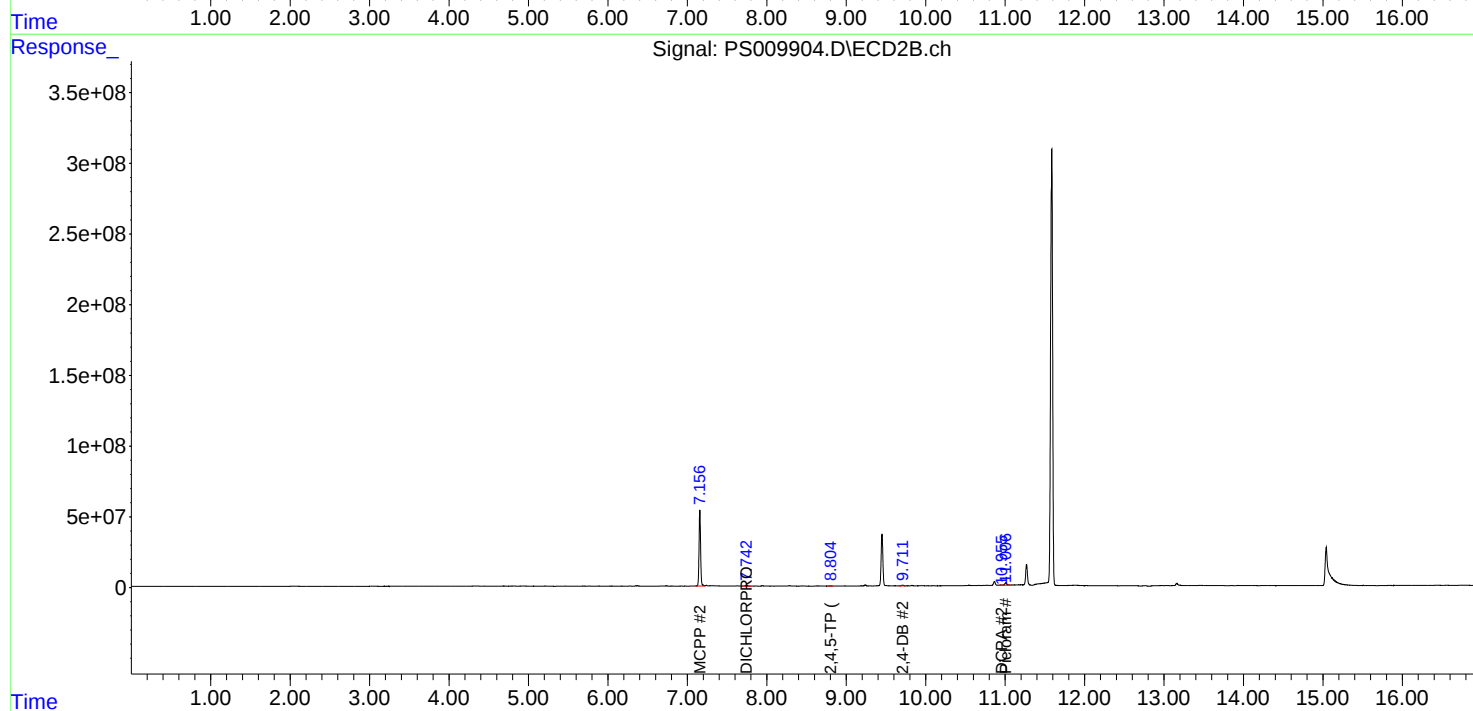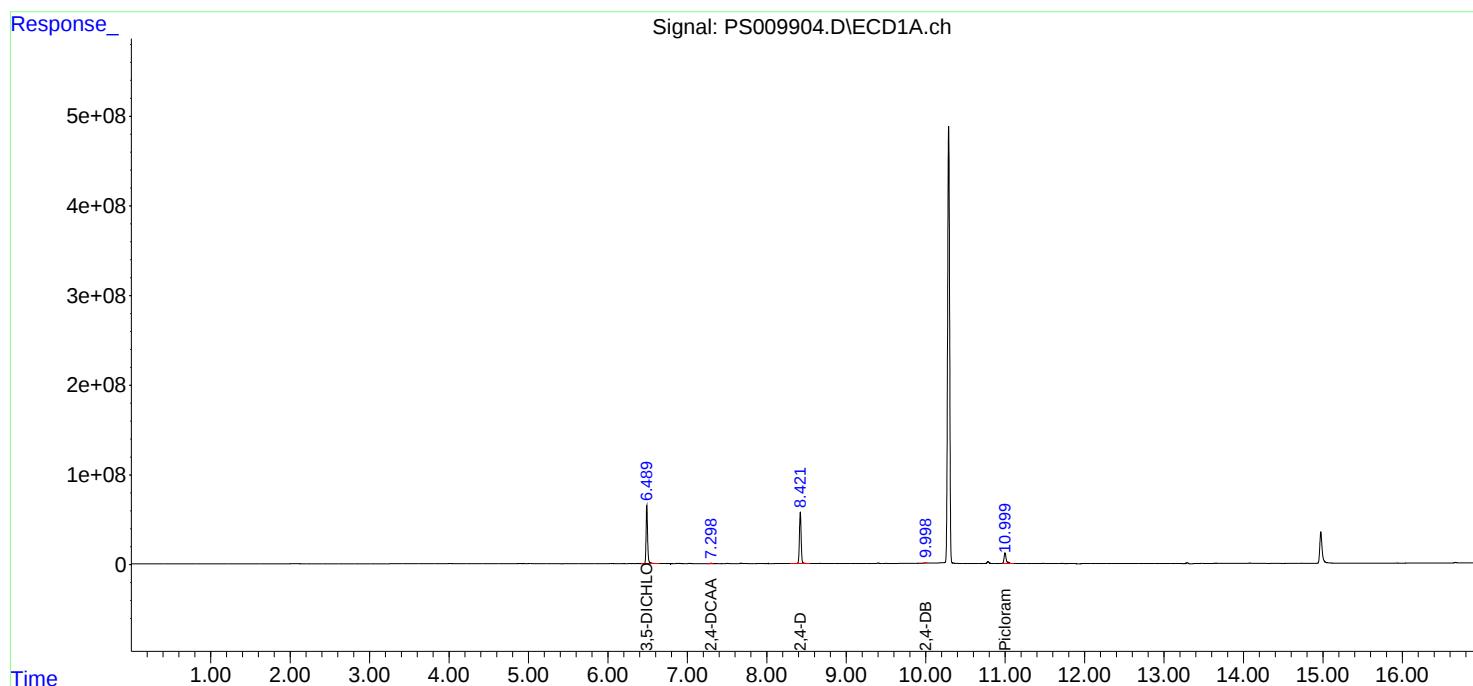


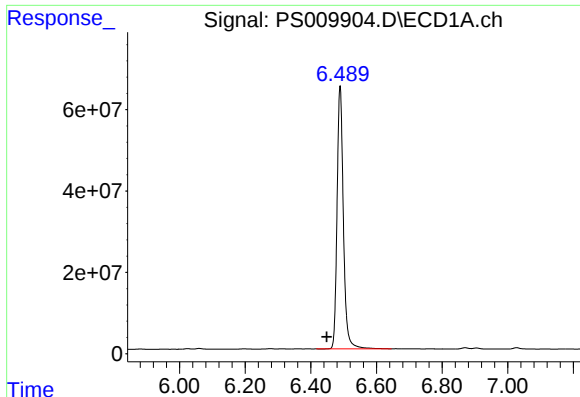

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.489 min
Delta R.T.: 0.041 min
Response: 863936099
Conc: 1050.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

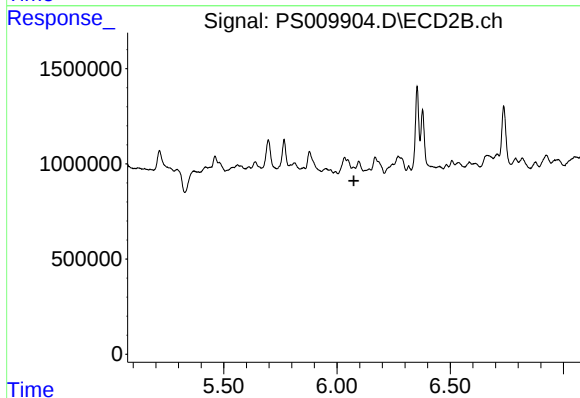


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.075 min
Response: 0
Conc: N.D.

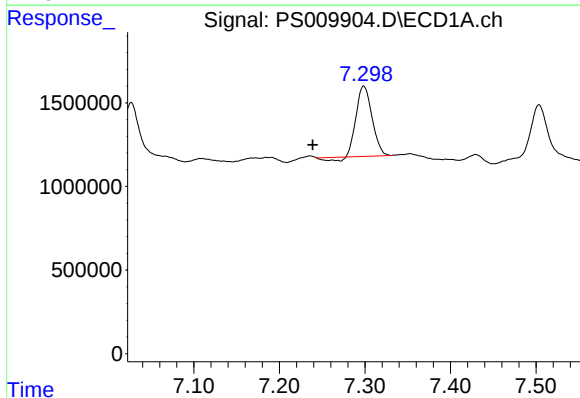


#4 2,4-DCAA

R.T.: 7.299 min
Delta R.T.: 0.060 min
Response: 5257532
Conc: 8.71 ng/ml

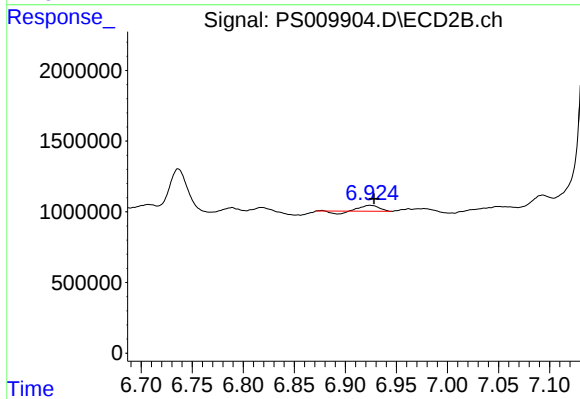

#4 2,4-DCAA


R.T.: 6.924 min
Delta R.T.: -0.004 min
Response: 373894
Conc: N.D.

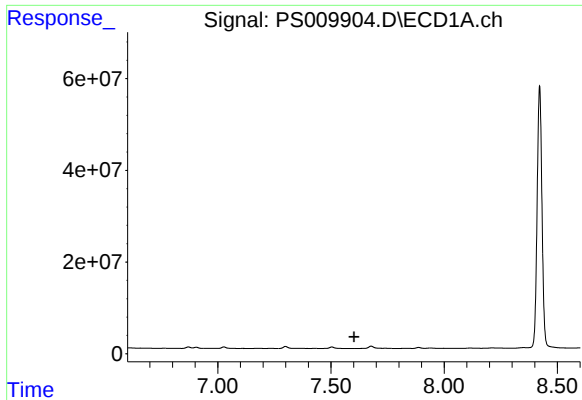

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

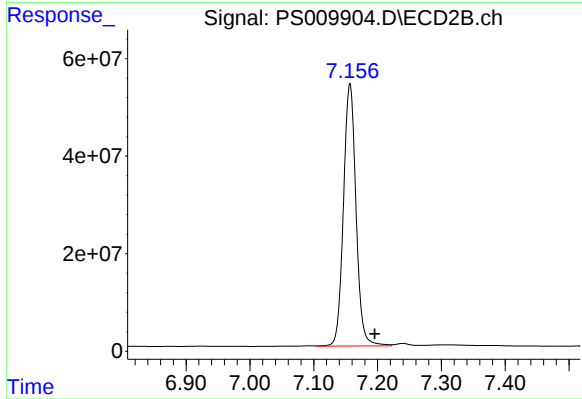


#6 MCP

R.T.: 7.157 min
Delta R.T.: -0.039 min
Response: 735214830
Conc: 446.67 ug/ml

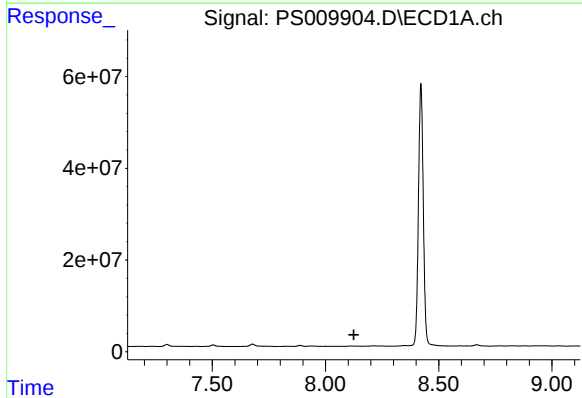


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

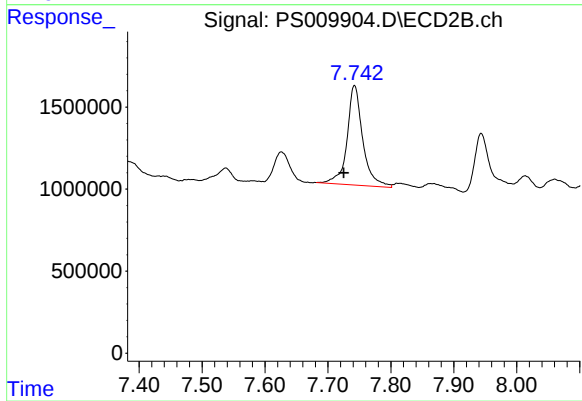

#8 DICHLORPROP


R.T.: 7.742 min
Delta R.T.: 0.017 min
Response: 10489843
Conc: 20.84 ng/ml

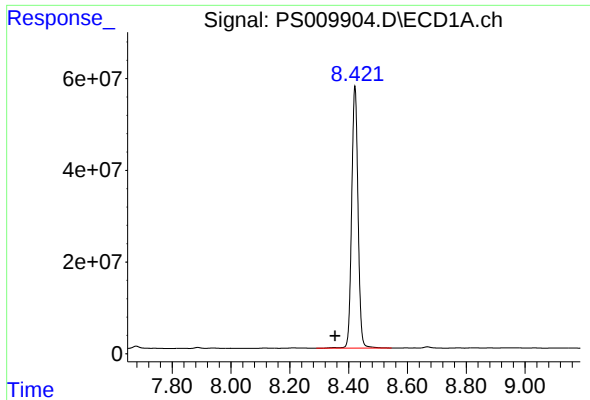

#9 2,4-D


R.T.: 8.421 min
Delta R.T.: 0.067 min
Response: 858623342
Conc: 1495.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

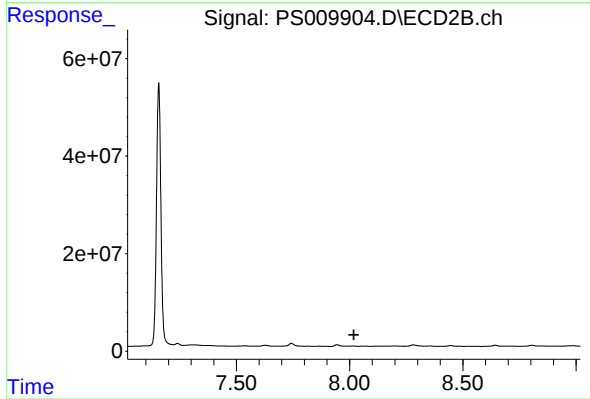


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.019 min
Response: 0
Conc: N.D.

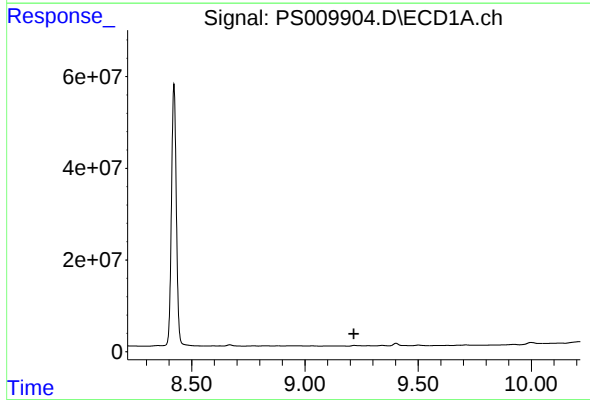


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

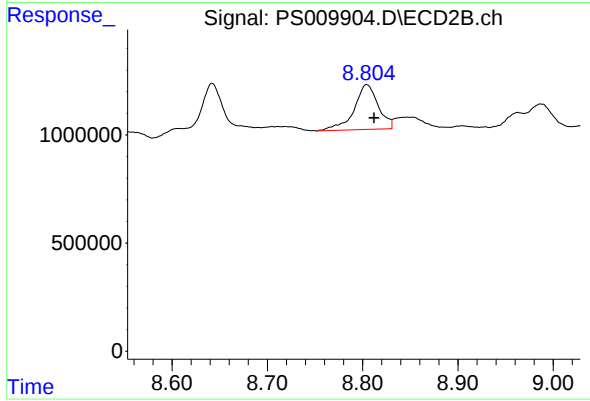

#11 2,4,5-TP (SILVEX)


R.T.: 8.804 min
Delta R.T.: -0.008 min
Response: 3642754
Conc: 1.39 ng/ml

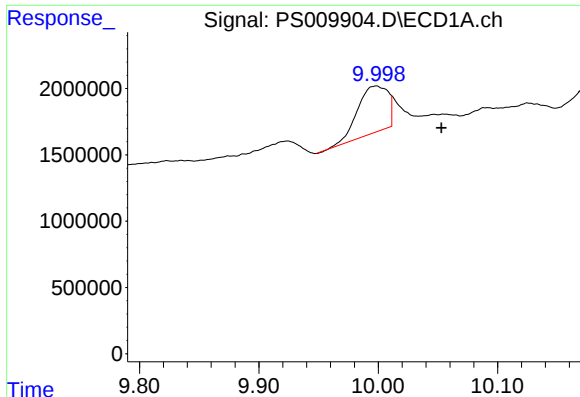

#13 2,4-DB


R.T.: 9.998 min
Delta R.T.: -0.055 min
Response: 6376881
Conc: 16.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

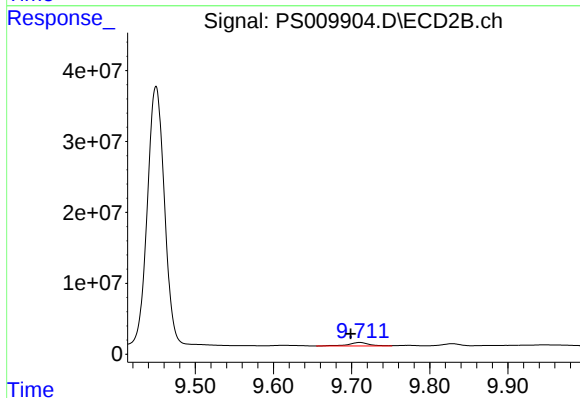


#13 2,4-DB

R.T.: 9.711 min
Delta R.T.: 0.012 min
Response: 9274224
Conc: 26.16 ng/ml

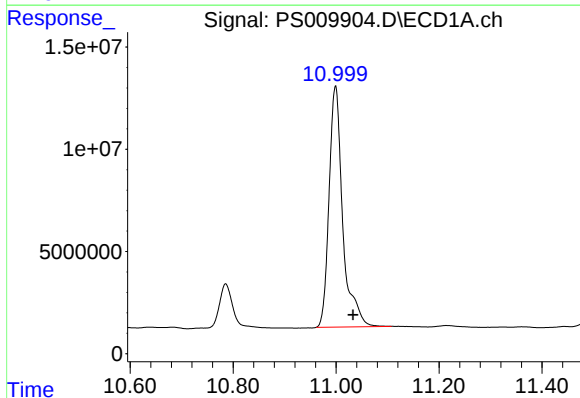


#15 Picloram

R.T.: 10.999 min
Delta R.T.: -0.034 min
Response: 217389796
Conc: 70.17 ng/ml

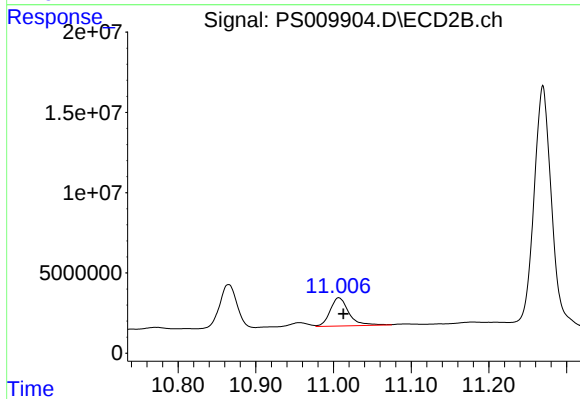

#15 Picloram


R.T.: 11.007 min
Delta R.T.: -0.006 min
Response: 29556377
Conc: 8.69 ng/ml

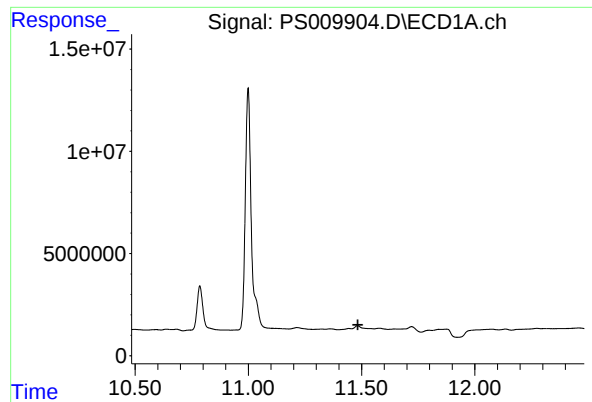

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

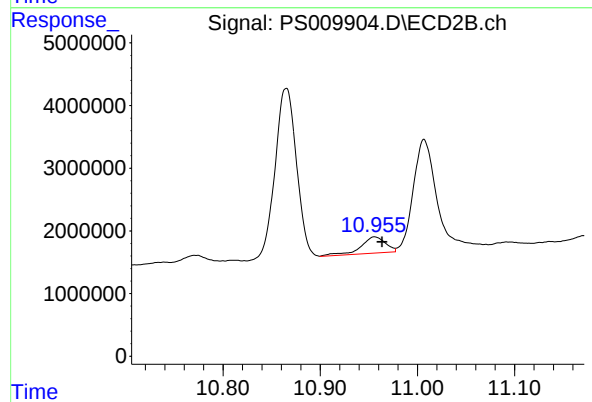

#16 DCPA

R.T.: 10.956 min
Delta R.T.: -0.008 min
Response: 4625799
Conc: 1.38 ng/ml