

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042120\
 Data File : PS009917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 17:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 18:14:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.237	6.923	348.4E6	344.1E6	576.970	694.749
Target Compounds							
5) T	DICAMBA	0.000	7.157	0	4922314	N.D.	2.475
6) T	MCPD	0.000	7.157	0	4922314	N.D.	2.991
7) T	MCPA	0.000	7.359	0	147089	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.745	0	3552689	N.D.	7.059
9) T	2,4-D	8.422	0.000	13744875	0	23.938	N.D. #
11) T	2,4,5-TP ...	0.000	8.805	0	955355	N.D.	<MDL
12) T	2,4,5-T	0.000	9.187	0	1035154	N.D.	<MDL
15) T	Picloram	10.999	11.008	14658871	1876793	4.732	<MDL #
16) T	DCPA	0.000	10.955	0	1774047	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042120\
Data File : PS009917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 17:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 18:14:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

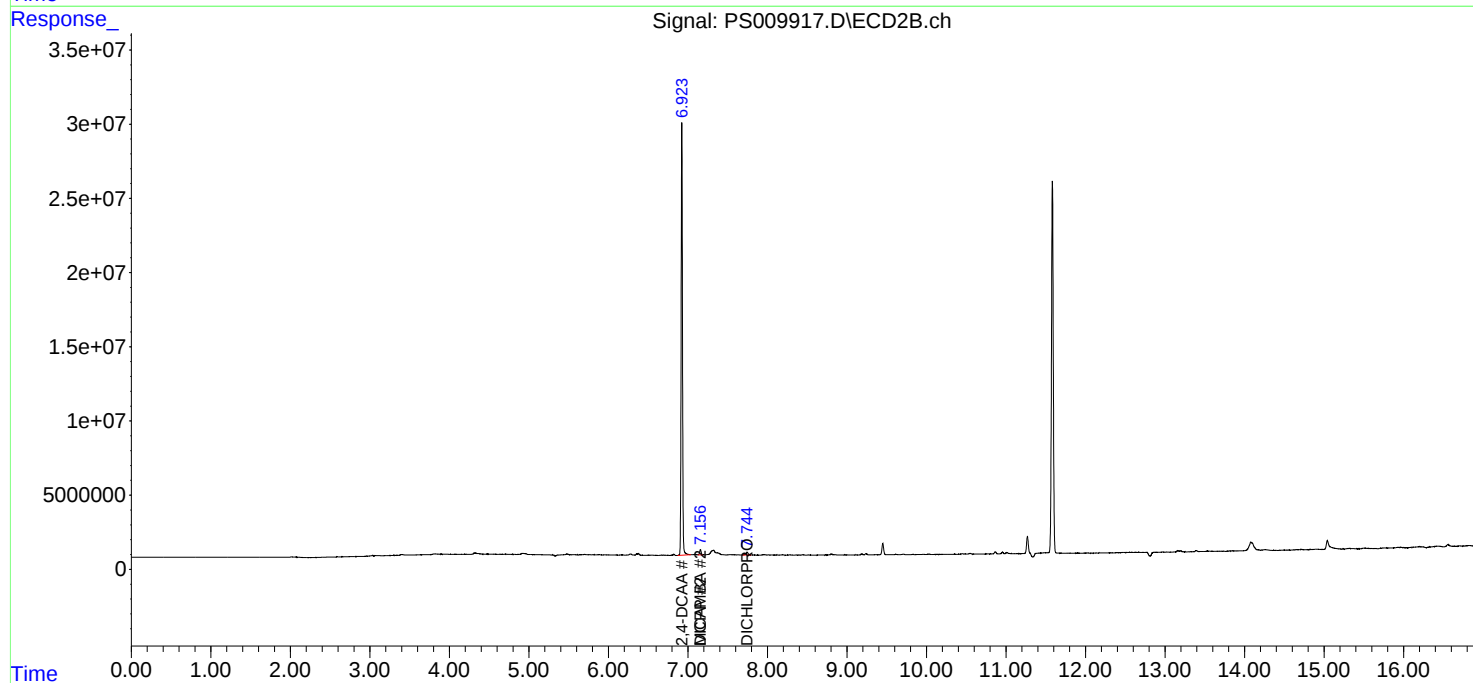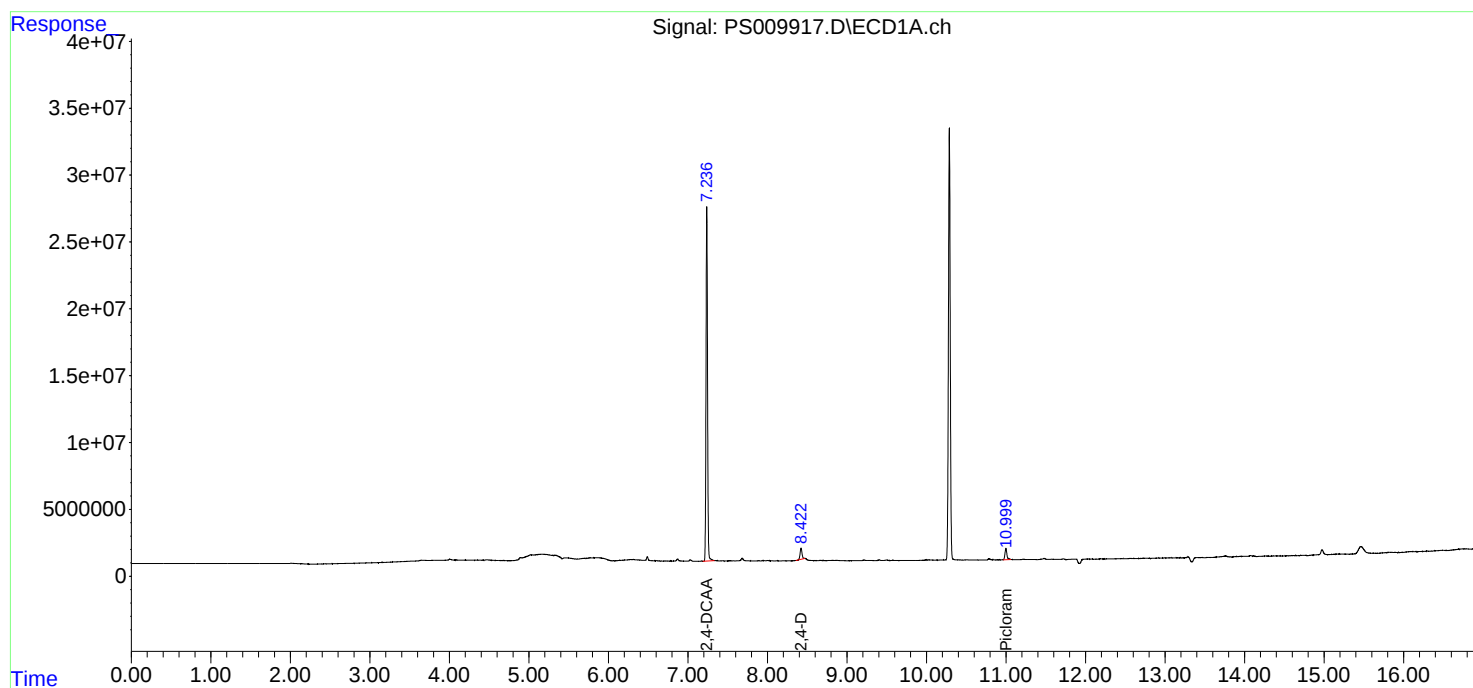


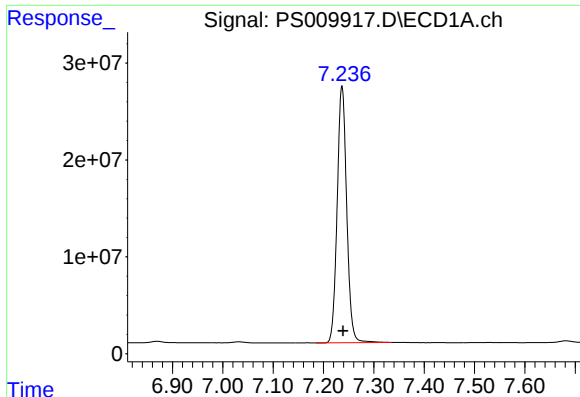

#4 2,4-DCAA


R.T.: 7.237 min
Delta R.T.: -0.002 min
Response: 348383197
Conc: 576.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

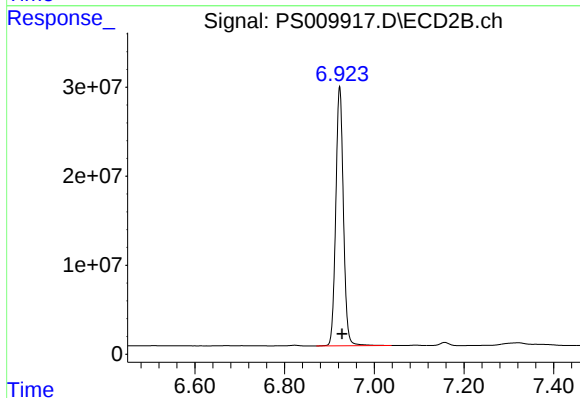


#4 2,4-DCAA

R.T.: 6.923 min
Delta R.T.: -0.005 min
Response: 344074203
Conc: 694.75 ng/ml

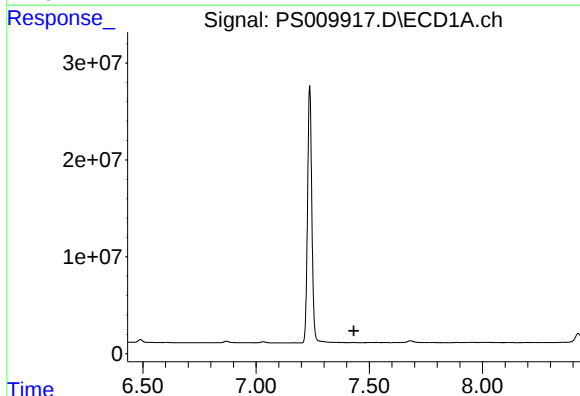


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

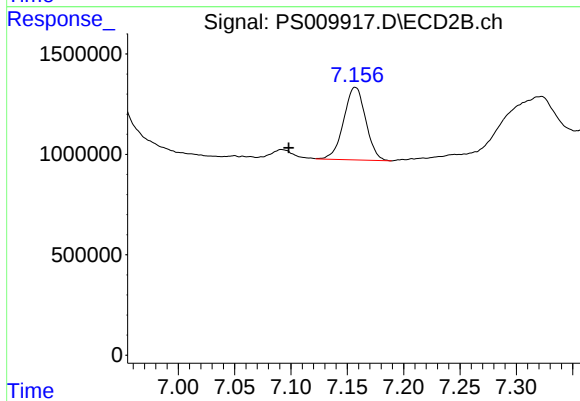

#5 DICAMBA


R.T.: 7.157 min
Delta R.T.: 0.059 min
Response: 4922314
Conc: 2.47 ng/ml

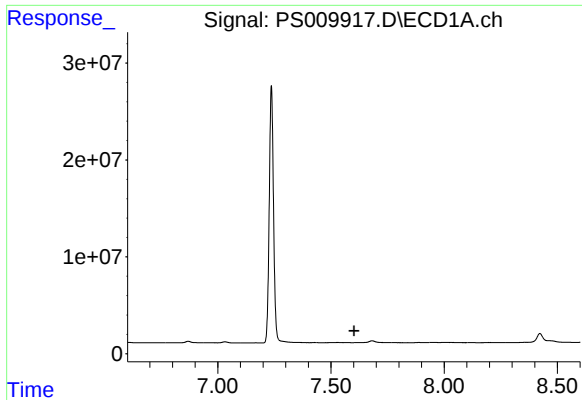

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

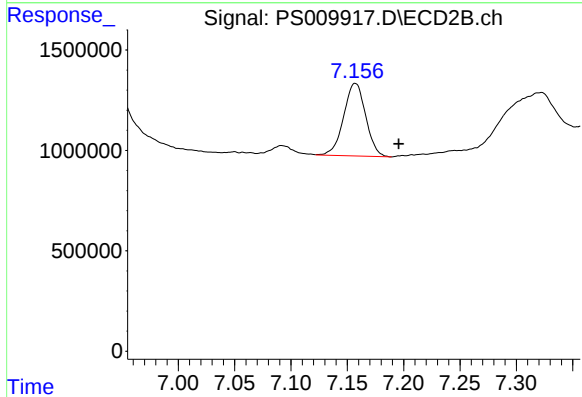


#6 MCP

R.T.: 7.157 min
Delta R.T.: -0.038 min
Response: 4922314
Conc: 2.99 ug/ml

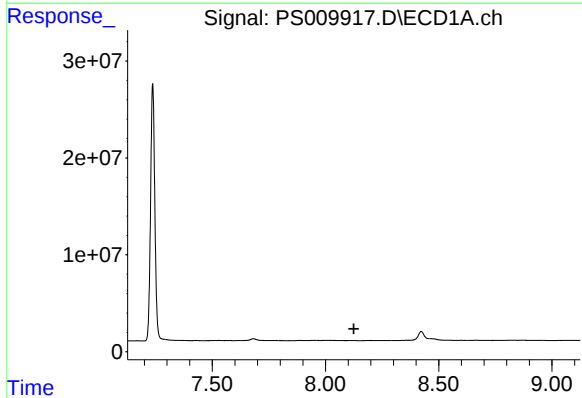


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

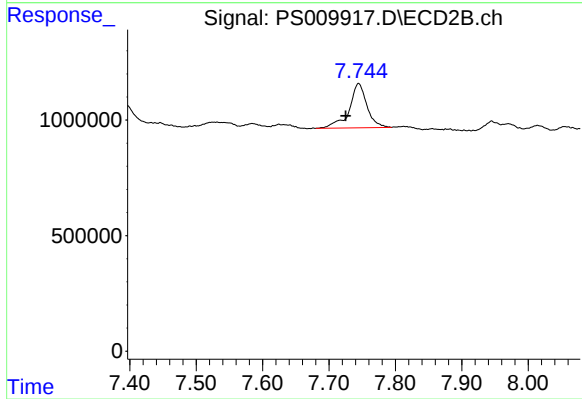

#8 DICHLORPROP


R.T.: 7.745 min
Delta R.T.: 0.019 min
Response: 3552689
Conc: 7.06 ng/ml

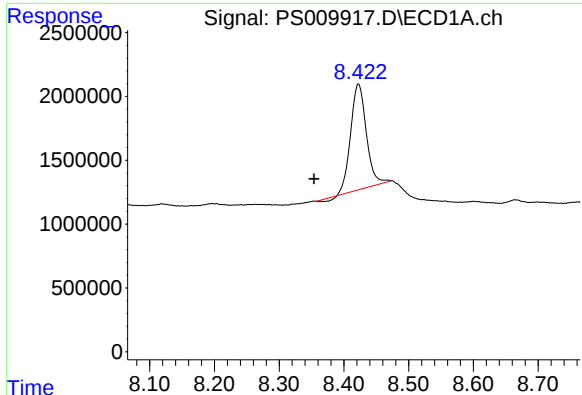

#9 2,4-D


R.T.: 8.422 min
Delta R.T.: 0.068 min
Response: 13744875
Conc: 23.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

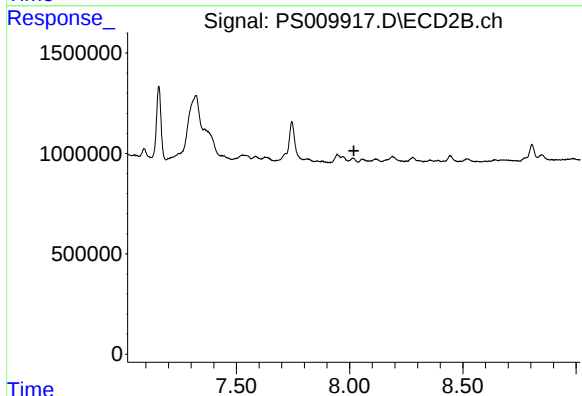


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.019 min
Response: 0
Conc: N.D.

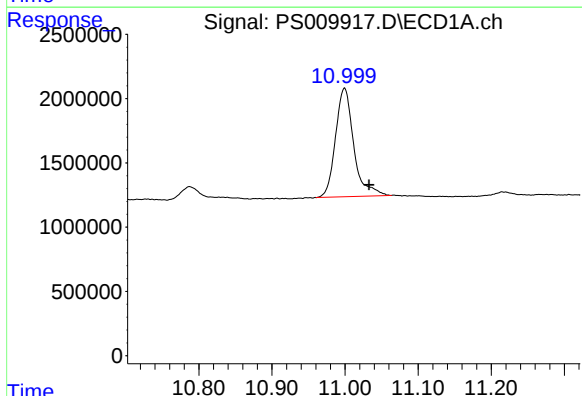

#15 Picloram

R.T.: 10.999 min
Delta R.T.: -0.033 min
Response: 14658871
Conc: 4.73 ng/ml

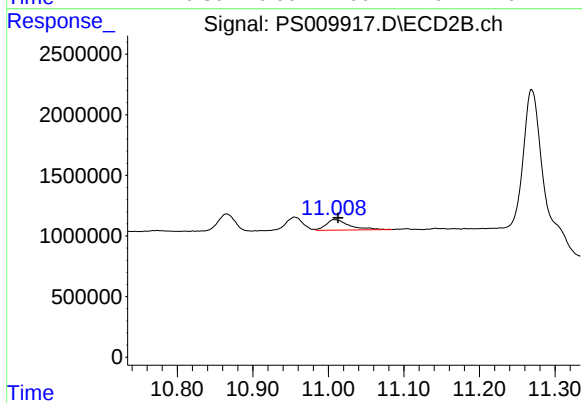

#15 Picloram

R.T.: 11.008 min
Delta R.T.: -0.005 min
Response: 1876793
Conc: N.D.