

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042120\
 Data File : PS009929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 21:59
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 03:01:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	6.922	351.1E6	349.5E6	581.484	705.636
Target Compounds							
5) T	DICAMBA	0.000	7.091	0	1426191	N.D.	<MDL
6) T	MCPD	0.000	7.156	0	6261865	N.D.	3.804
8) T	DICHLORPROP	0.000	7.744	0	3925457	N.D.	7.799
9) T	2,4-D	8.421	0.000	14016422	0	24.411	N.D. #
11) T	2,4,5-TP ...	0.000	8.803	0	1421855	N.D.	<MDL
12) T	2,4,5-T	0.000	9.185	0	1484049	N.D.	<MDL
14) T	DINOSEB	0.000	10.025	0	793168	N.D.	<MDL
15) T	Picloram	10.997	11.007	17584142	3745697	5.676	1.101 #
16) T	DCPA	0.000	10.953	0	2216979	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042120\
Data File : PS009929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 21:59
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 03:01:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

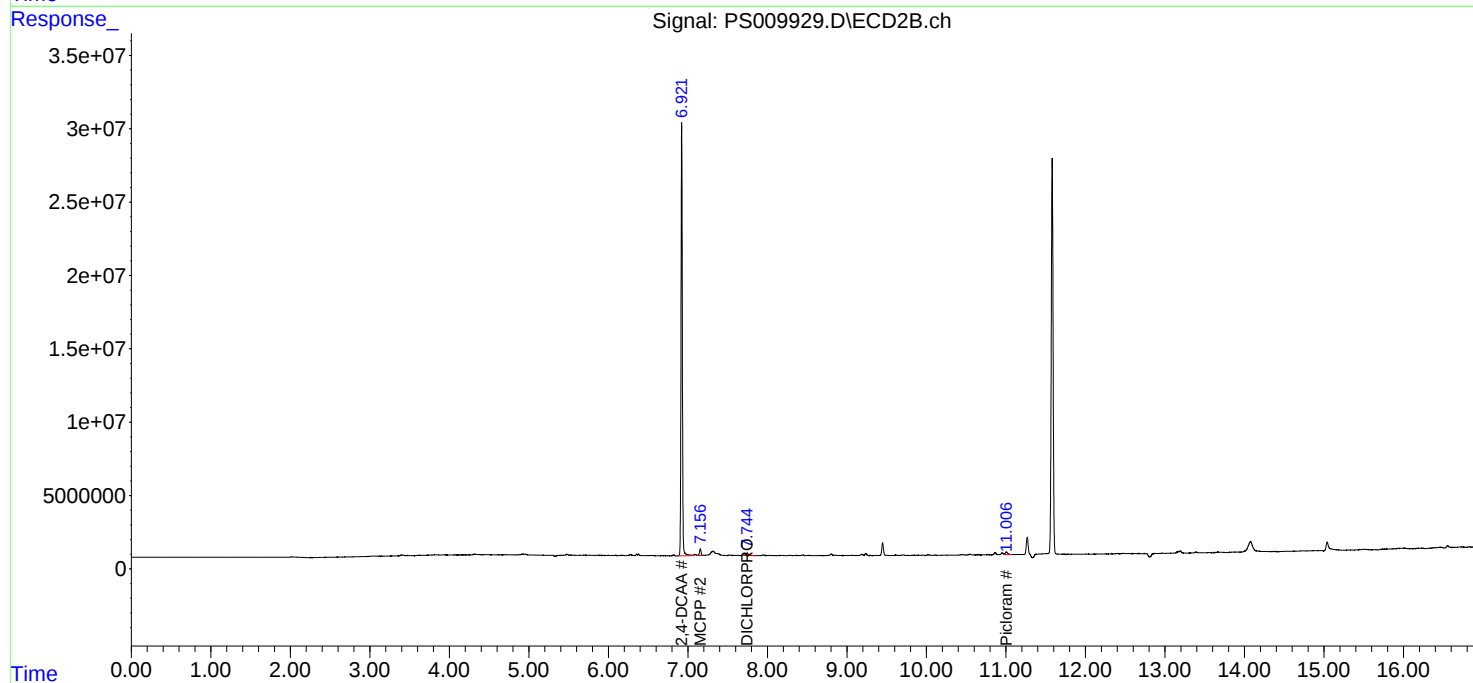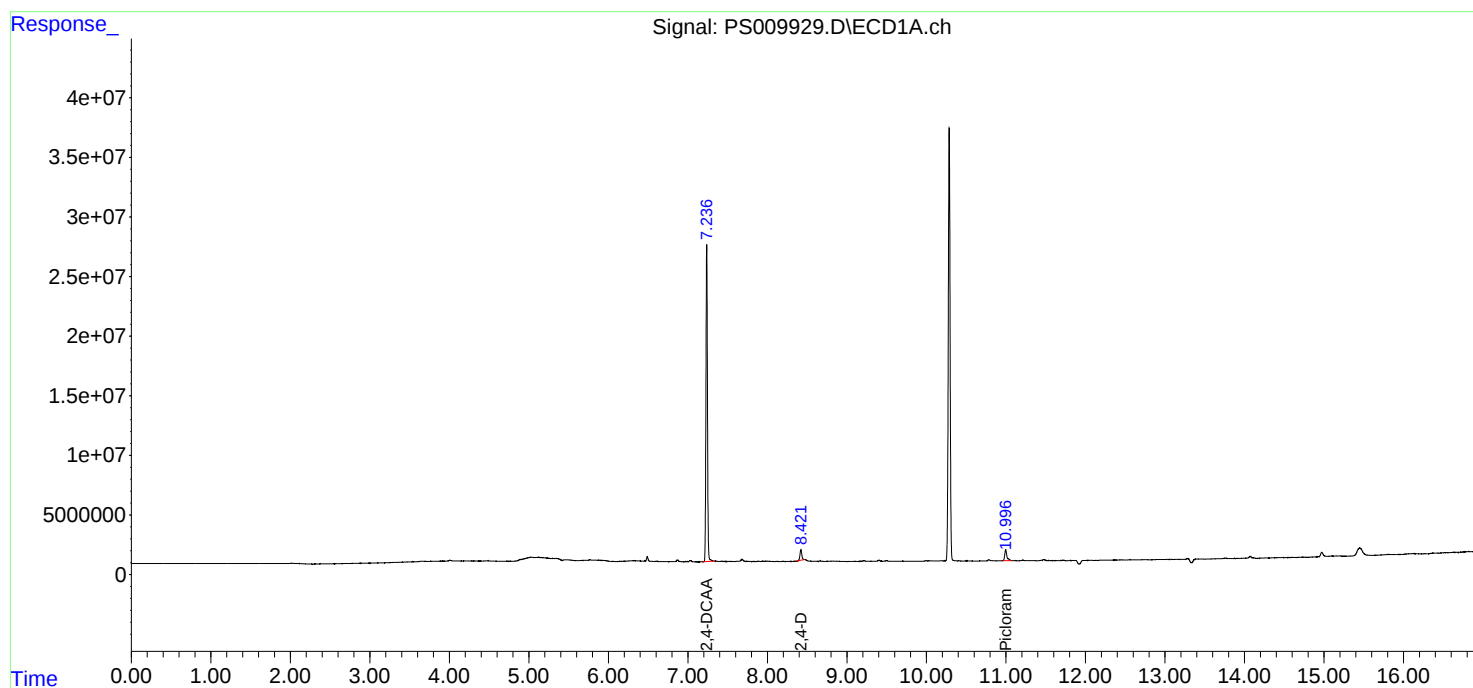


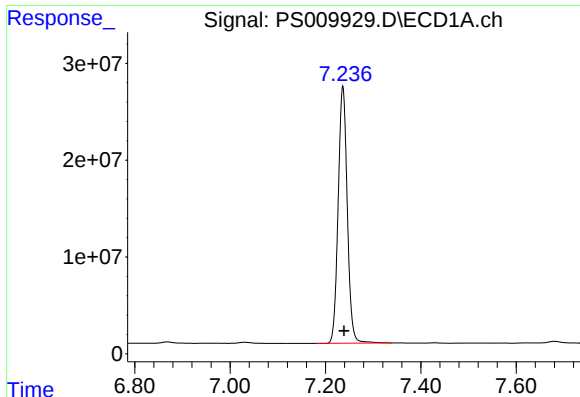

#4 2,4-DCAA


R.T.: 7.236 min
Delta R.T.: -0.003 min
Response: 351108959
Conc: 581.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

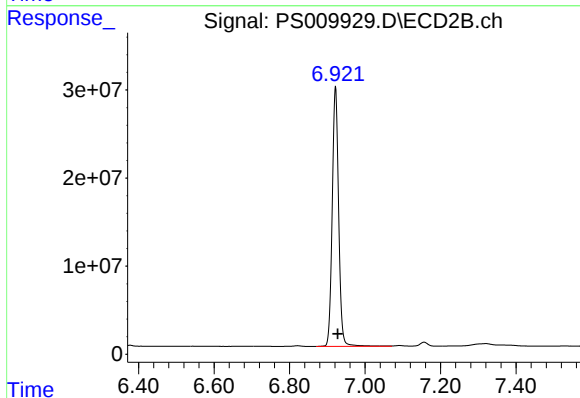


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.007 min
Response: 349466331
Conc: 705.64 ng/ml

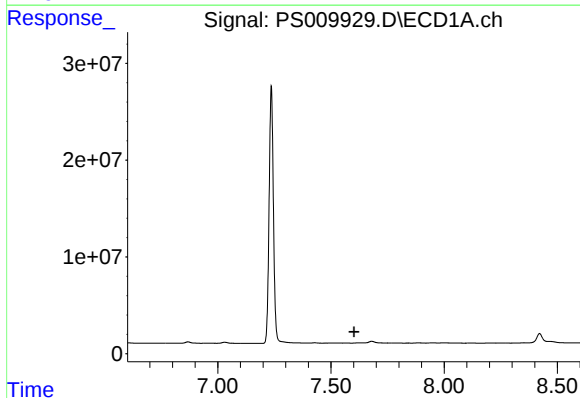


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.602 min
Response: 0
Conc: N.D.

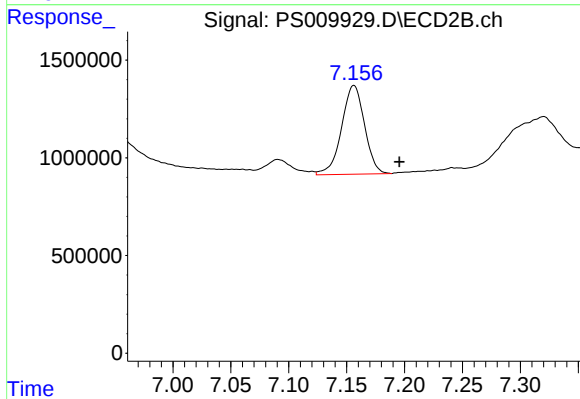

#6 MCP


R.T.: 7.156 min
Delta R.T.: -0.039 min
Response: 6261865
Conc: 3.80 ug/ml

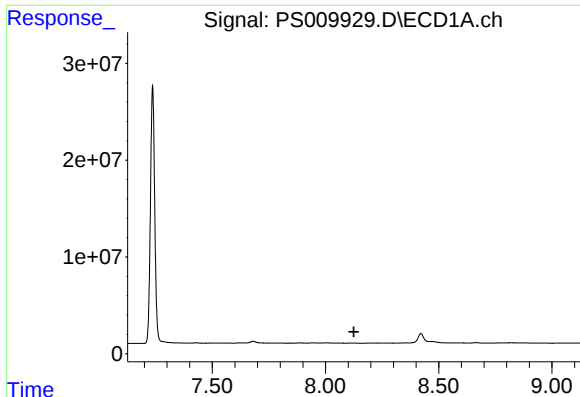

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

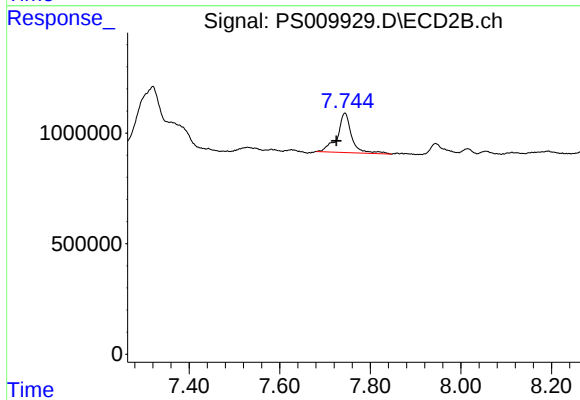


#8 DICHLORPROP

R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 3925457
Conc: 7.80 ng/ml

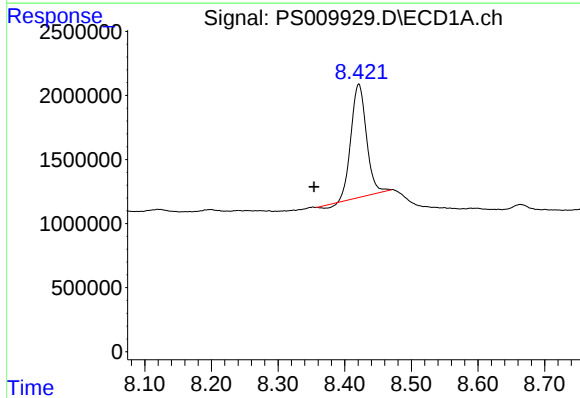


#9 2,4-D

R.T.: 8.421 min
Delta R.T.: 0.067 min
Response: 14016422
Conc: 24.41 ng/ml

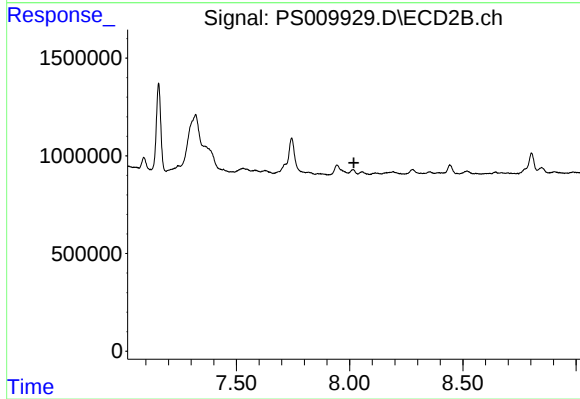

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.019 min
Response: 0
Conc: N.D.

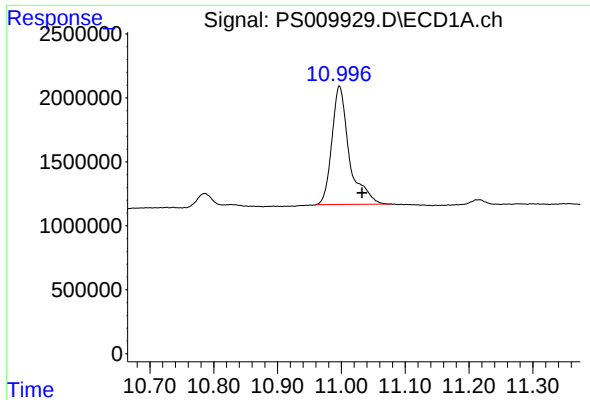

#15 Picloram

R.T.: 10.997 min
Delta R.T.: -0.036 min
Response: 17584142
Conc: 5.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

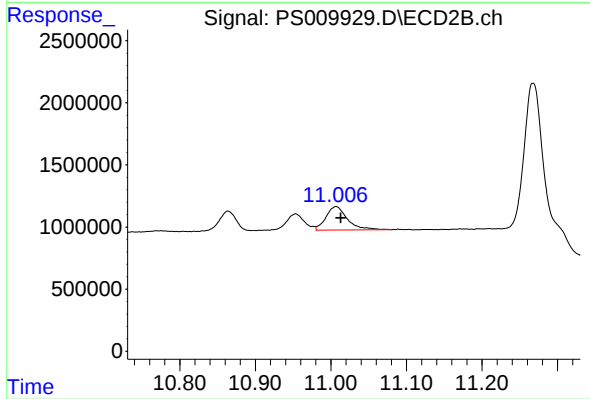

#15 Picloram

R.T.: 11.007 min
Delta R.T.: -0.006 min
Response: 3745697
Conc: 1.10 ng/ml