

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042120\
 Data File : PS009953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2020 07:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 08:48:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.922	353.8E6	342.0E6	585.937	690.583
Target Compounds							
2) T	3,5-DICHL...	6.487	0.000	5834095	0	7.095	N.D. #
5) T	DICAMBA	0.000	7.156	0	7326947	N.D.	3.684
6) T	MCP	0.000	7.156	0	7326947	N.D.	4.451
8) T	DICHLORPROP	0.000	7.744	0	2641345	N.D.	5.248
9) T	2,4-D	8.420	0.000	21390785	0	37.254	N.D. #
11) T	2,4,5-TP ...	0.000	8.804	0	1152784	N.D.	<MDL
12) T	2,4,5-T	0.000	9.185	0	1294927	N.D.	<MDL
15) T	Picloram	10.996	11.008	17619107	3127730	5.687	<MDL #
16) T	DCPA	0.000	10.953	0	1993317	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042120\
Data File : PS009953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2020 07:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 08:48:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

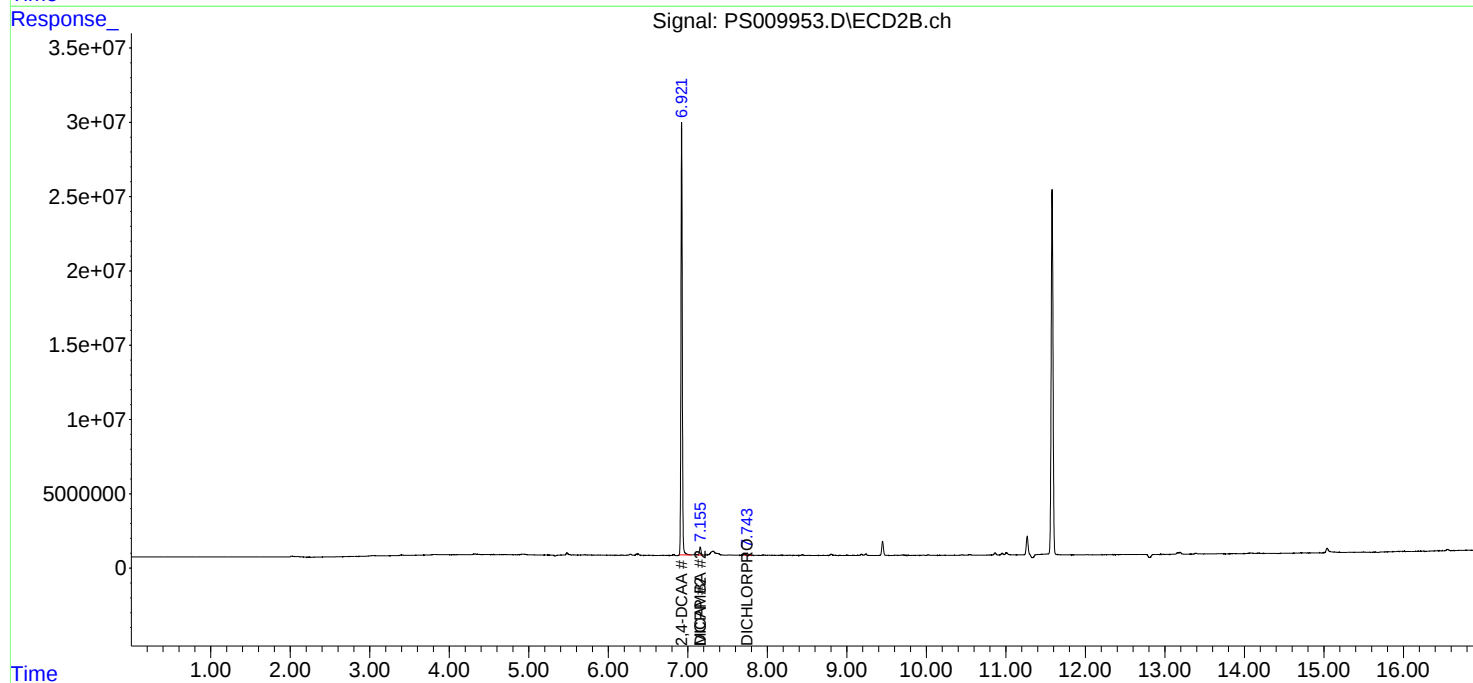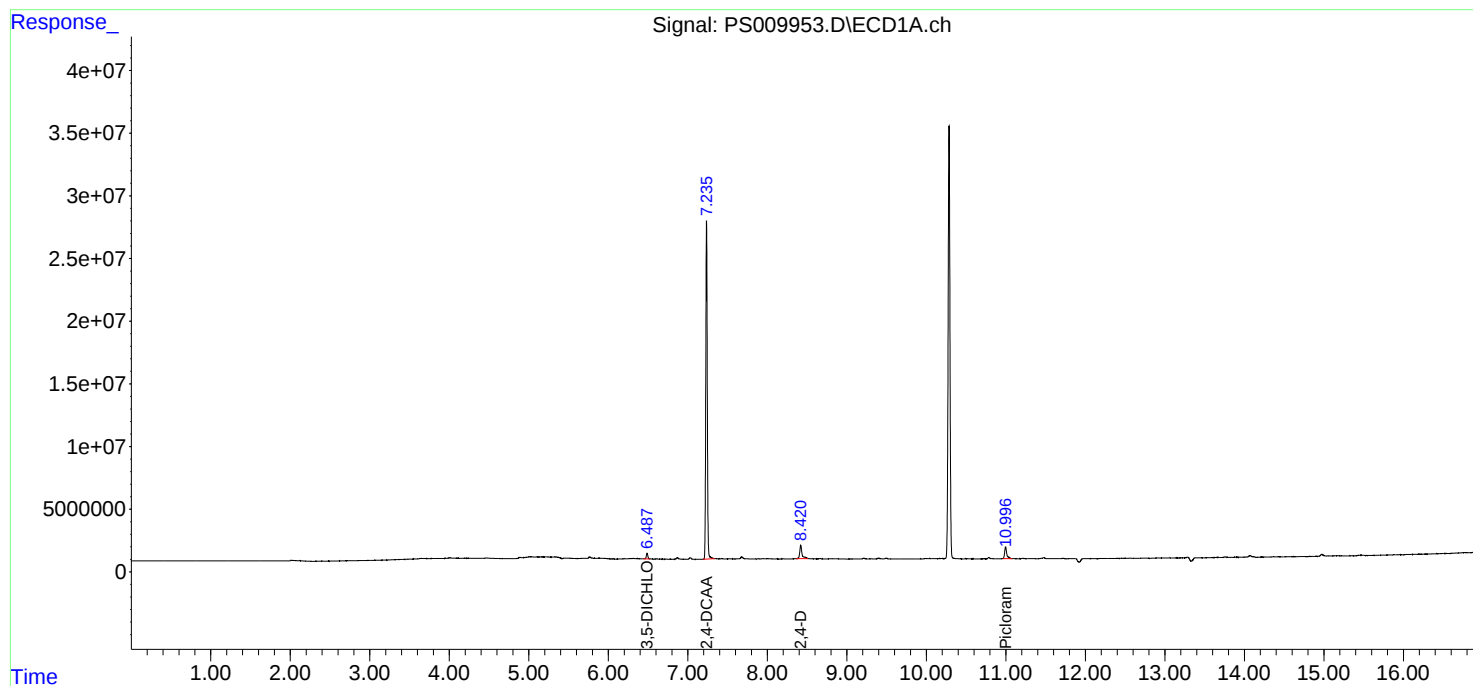


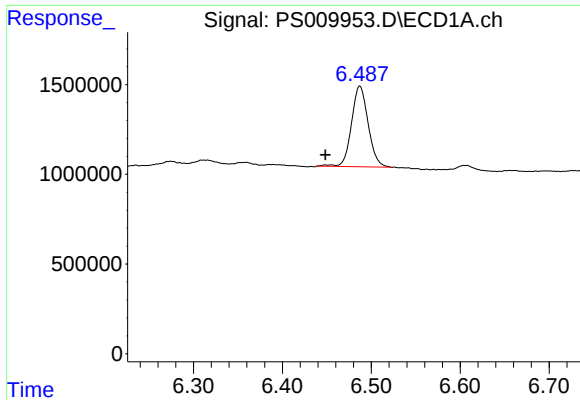

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.487 min
Delta R.T.: 0.039 min
Response: 5834095
Conc: 7.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

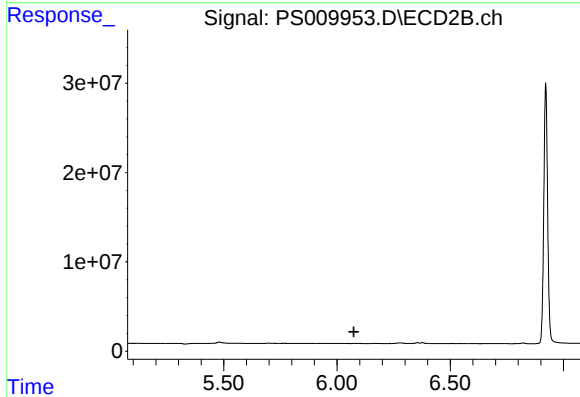


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.075 min
Response: 0
Conc: N.D.

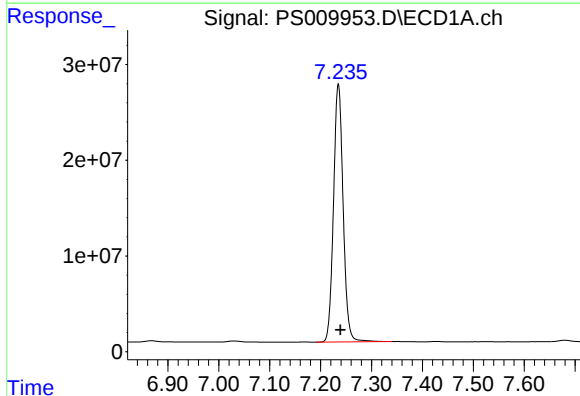


#4 2,4-DCAA

R.T.: 7.235 min
Delta R.T.: -0.004 min
Response: 353797844
Conc: 585.94 ng/ml

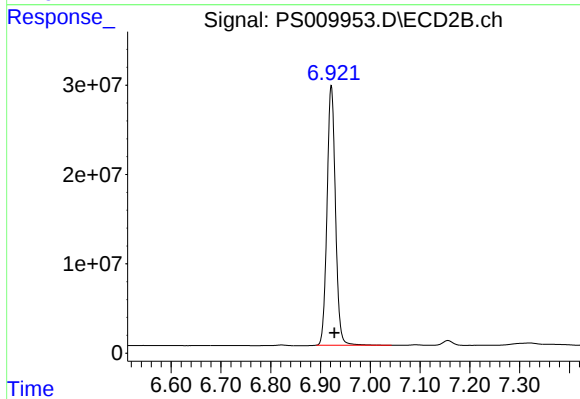

#4 2,4-DCAA


R.T.: 6.922 min
Delta R.T.: -0.007 min
Response: 342011028
Conc: 690.58 ng/ml

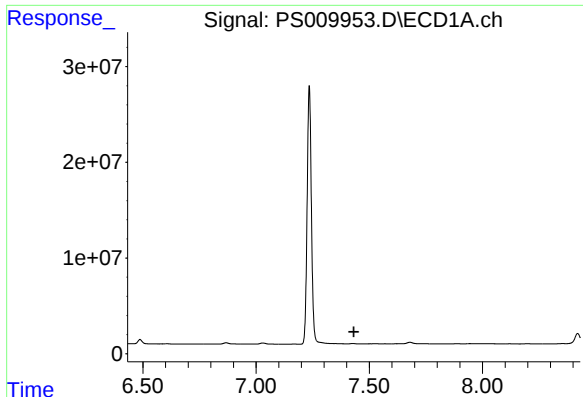

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

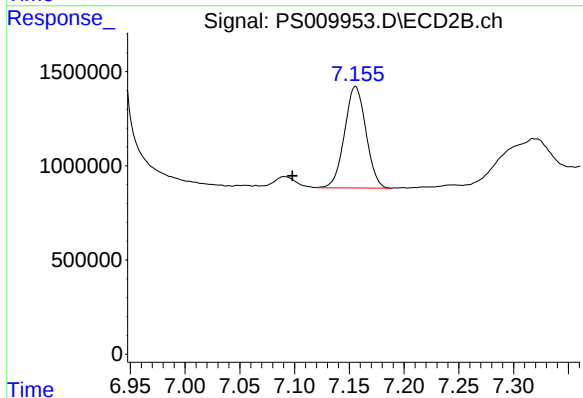


#5 DICAMBA

R.T.: 7.156 min
Delta R.T.: 0.058 min
Response: 7326947
Conc: 3.68 ng/ml

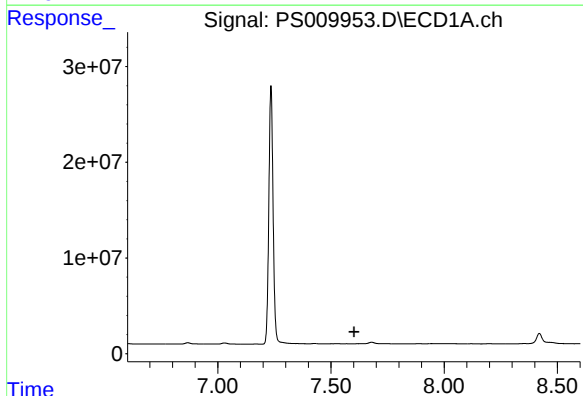


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.602 min
Response: 0
Conc: N.D.

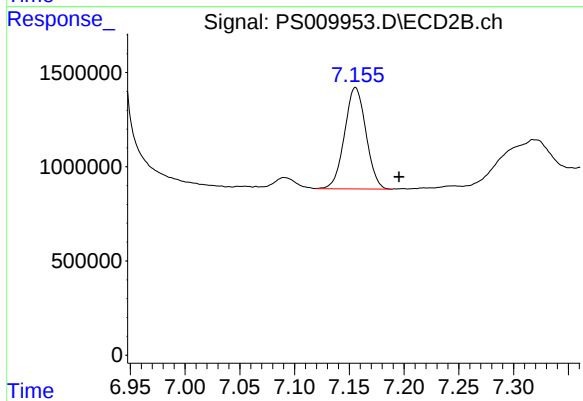

#6 MCP


R.T.: 7.156 min
Delta R.T.: -0.040 min
Response: 7326947
Conc: 4.45 ug/ml

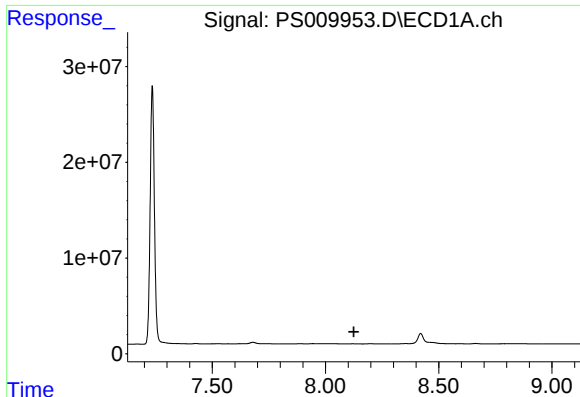

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

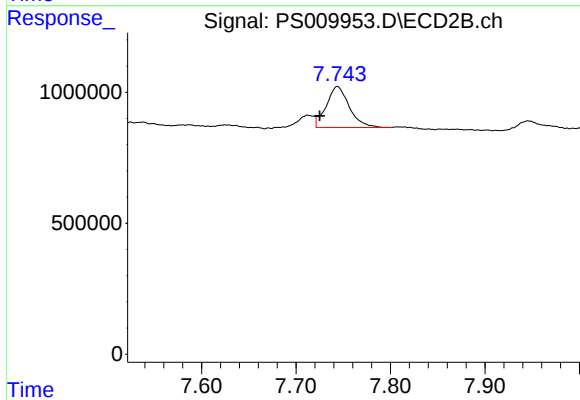


#8 DICHLORPROP

R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 2641345
Conc: 5.25 ng/ml

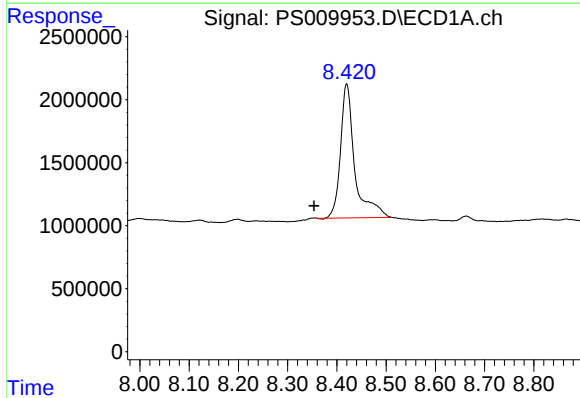


#9 2,4-D

R.T.: 8.420 min
Delta R.T.: 0.066 min
Response: 21390785
Conc: 37.25 ng/ml

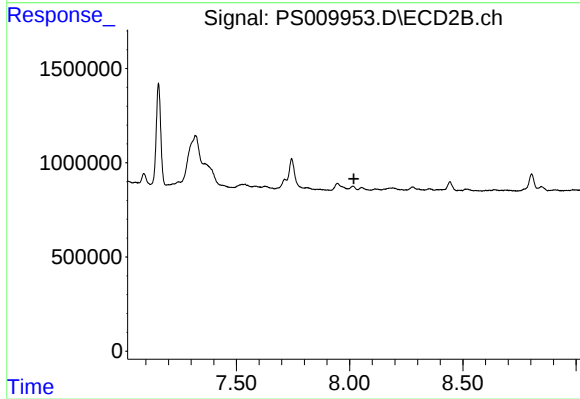

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.019 min
Response: 0
Conc: N.D.

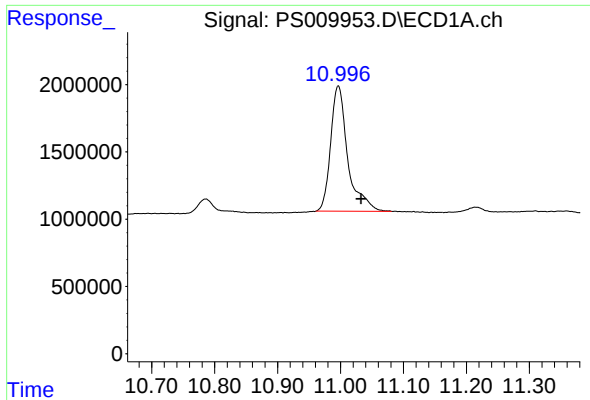

#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.036 min
Response: 17619107
Conc: 5.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

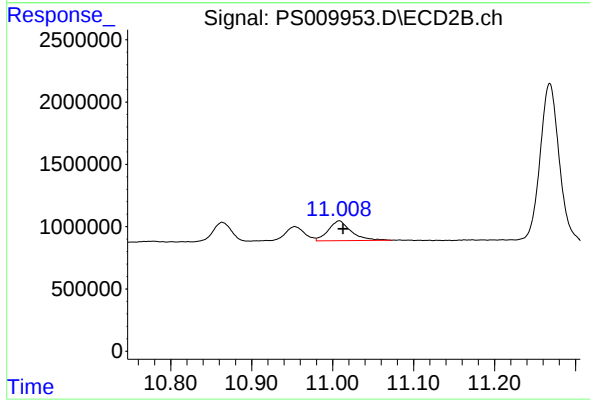

#15 Picloram

R.T.: 11.008 min
Delta R.T.: -0.005 min
Response: 3127730
Conc: N.D.