

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
 Data File : PS014713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 07:59
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 10:54:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) T	DICHLORPROP	0.000	7.700	0	14350995	N.D. 28.428
11) T	2,4,5-TP ...	0.000	8.728	0	7218135	N.D. 2.642
13) T	2,4-DB	0.000	9.583f	0	51356027	N.D. 148.055
15) T	Picloram	10.932	10.963	450.0E6	158.6E6	40.216 42.292
16) T	DCPA	0.000	10.897	0	5491727	N.D. 1.352



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
Data File : PS014713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 07:59
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 10:54:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

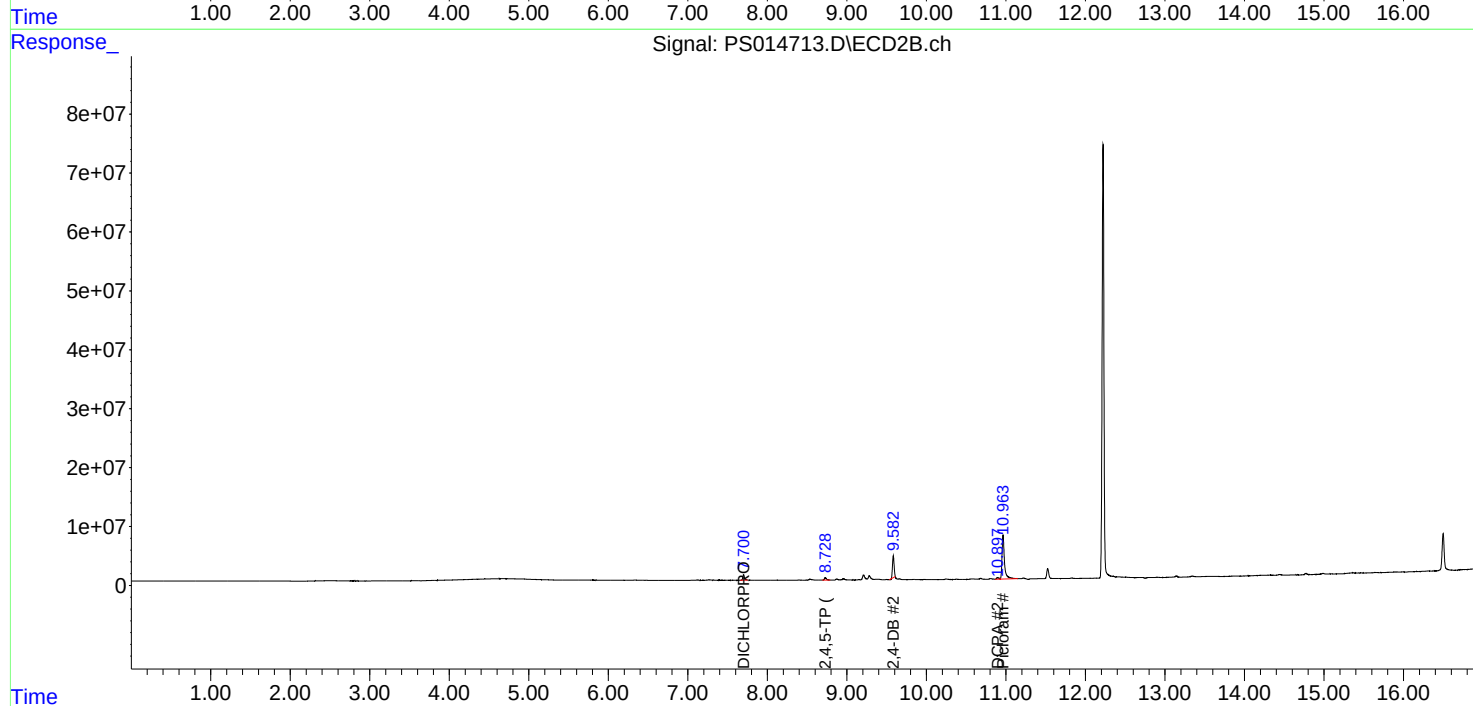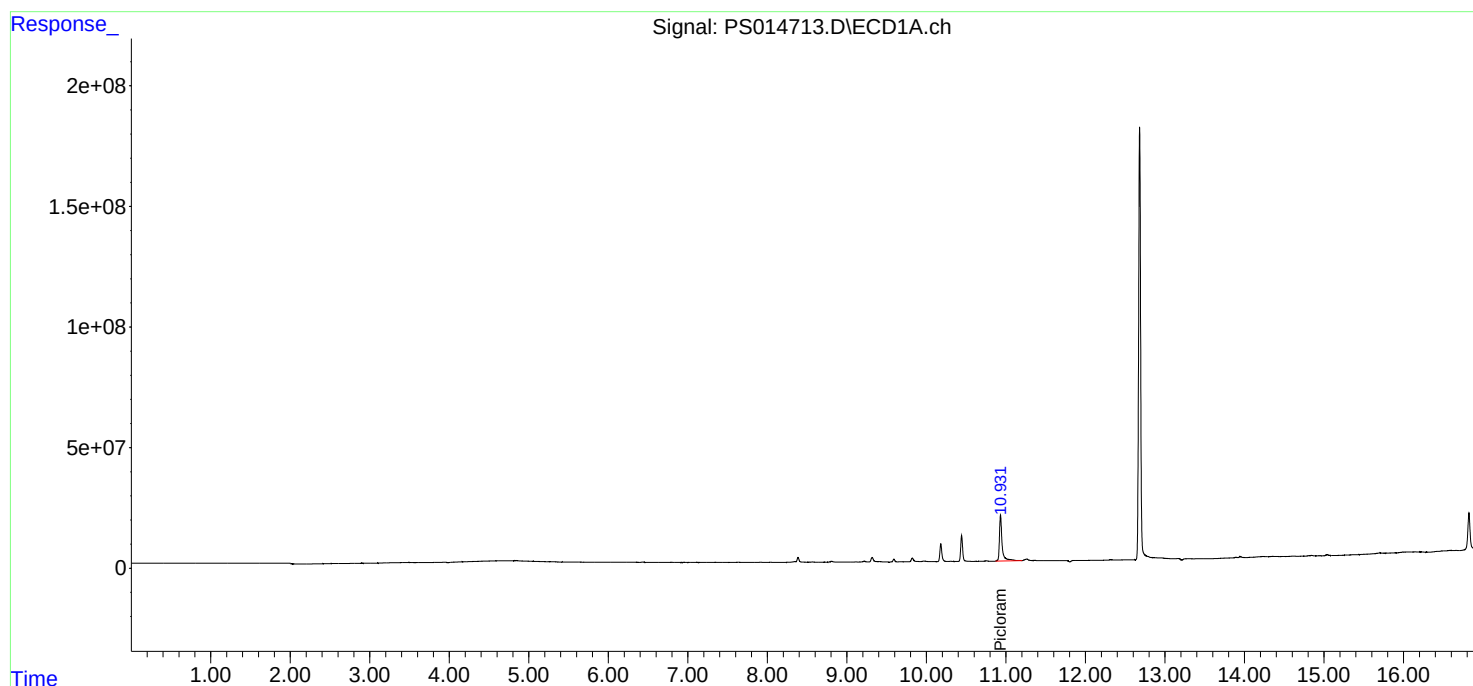


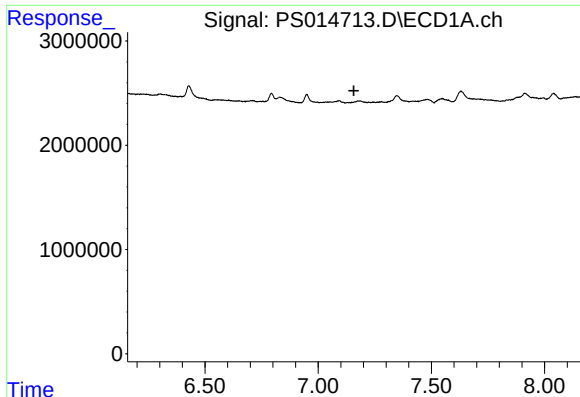

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

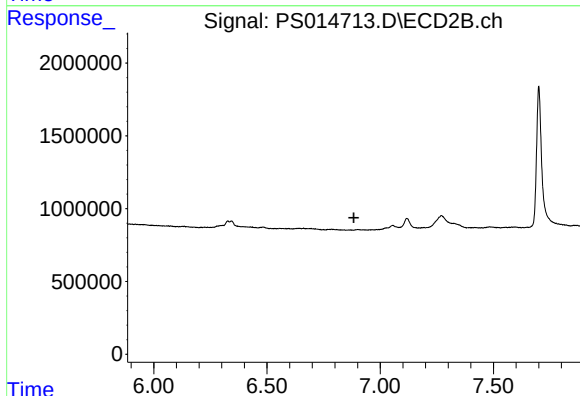


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

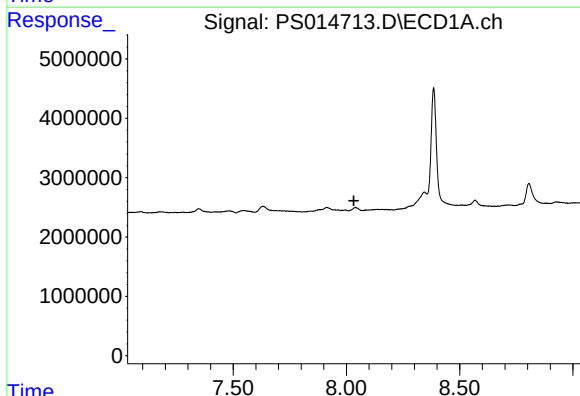


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

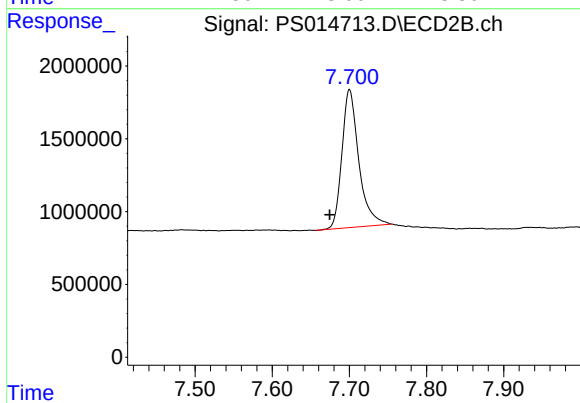

#8 DICHLORPROP


R.T.: 7.700 min
Delta R.T.: 0.025 min
Response: 14350995
Conc: 28.43 ng/ml

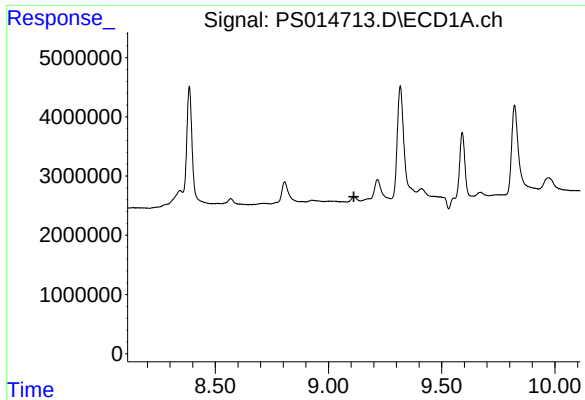

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

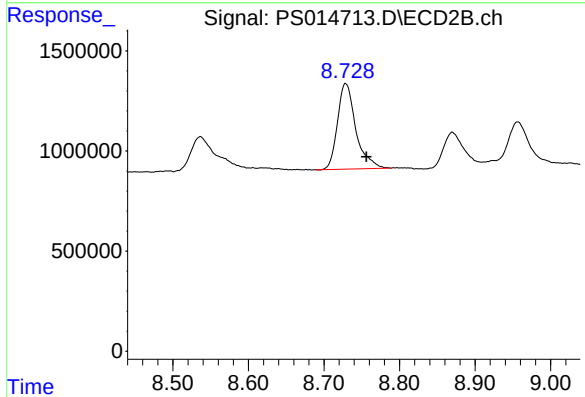


#11 2,4,5-TP (SILVEX)

R.T.: 8.728 min
Delta R.T.: -0.028 min
Response: 7218135
Conc: 2.64 ng/ml

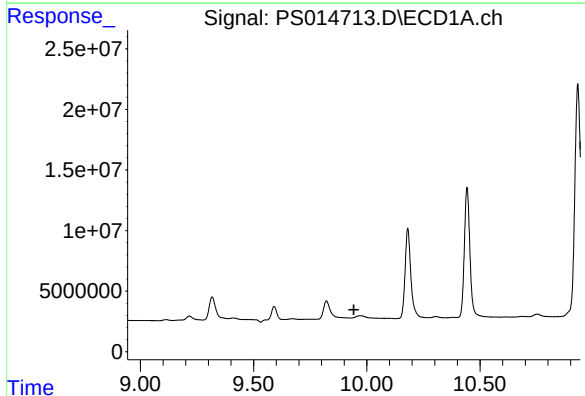


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.943 min
Response: 0
Conc: N.D.

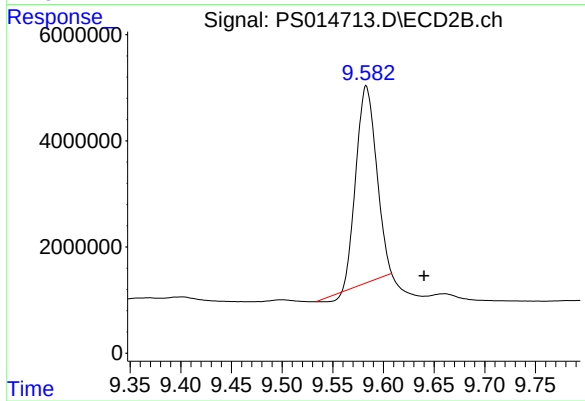

#13 2,4-DB


R.T.: 9.583 min
Delta R.T.: -0.057 min
Response: 51356027
Conc: 148.05 ng/ml

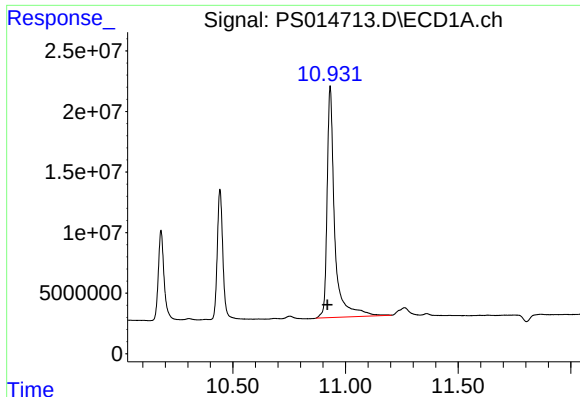

#15 Picloram


R.T.: 10.932 min
Delta R.T.: 0.013 min
Response: 449950019
Conc: 40.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

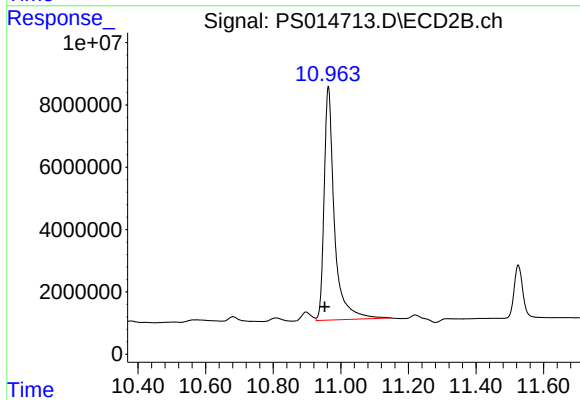


#15 Picloram

R.T.: 10.963 min
Delta R.T.: 0.011 min
Response: 158589663
Conc: 42.29 ng/ml

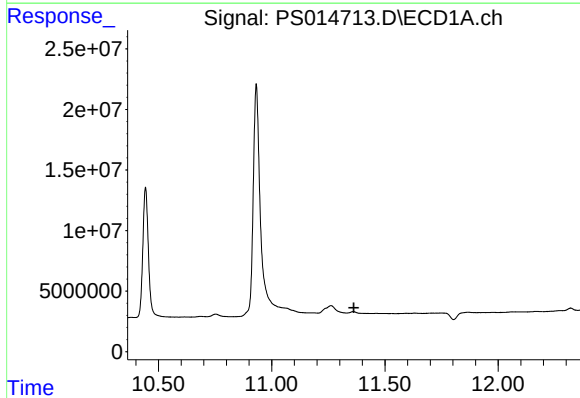

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.363 min
Response: 0
Conc: N.D.

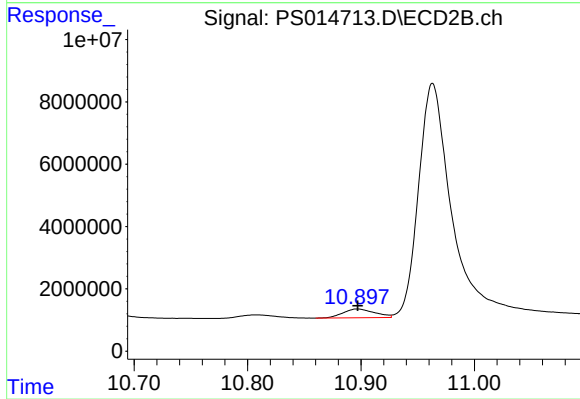

#16 DCPA

R.T.: 10.897 min
Delta R.T.: 0.000 min
Response: 5491727
Conc: 1.35 ng/ml