

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
 Data File : PS014714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 08:22
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 10:55:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	6.884	727.2E6	271.8E6	478.019	583.904
Target Compounds							
8) T	DICHLORPROP	0.000	7.702	0	10928717	N.D.	21.649
9) T	2,4-D	8.330f	0.000	8315576	0	5.230	N.D. #
11) T	2,4,5-TP ...	0.000	8.731	0	3775448	N.D.	1.382
13) T	2,4-DB	0.000	9.586f	0	23981098	N.D.	69.135
15) T	Picloram	10.939	10.970	160.0E6	59258613	14.300	15.803
16) T	DCPA	0.000	10.903	0	2559902	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
Data File : PS014714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 08:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 10:55:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

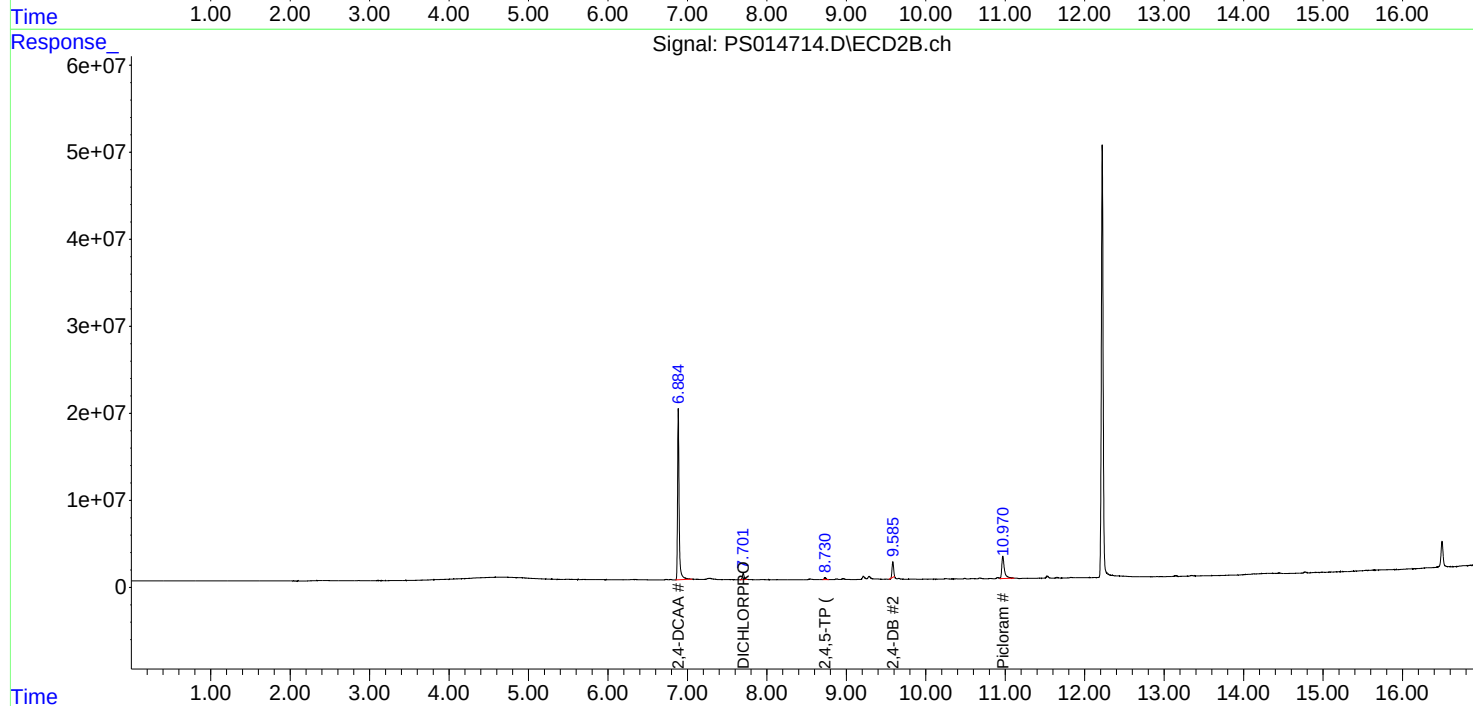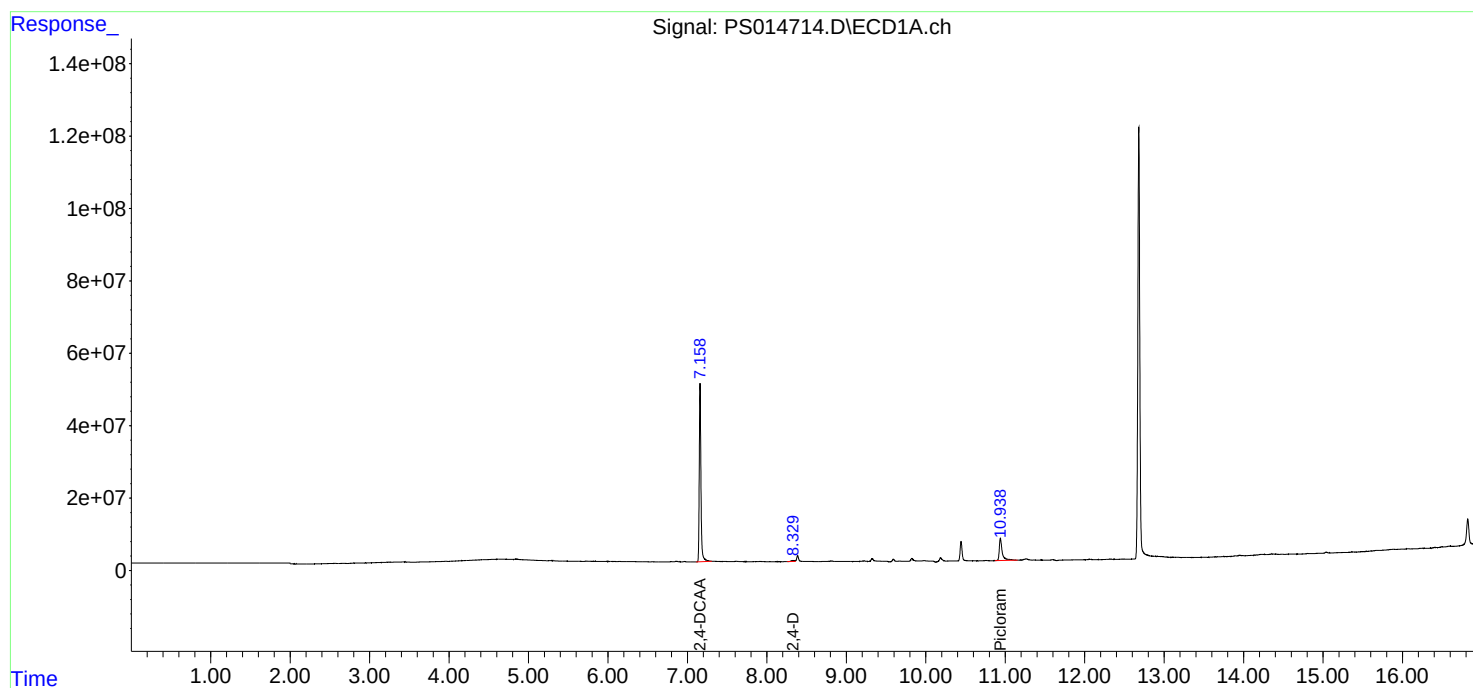


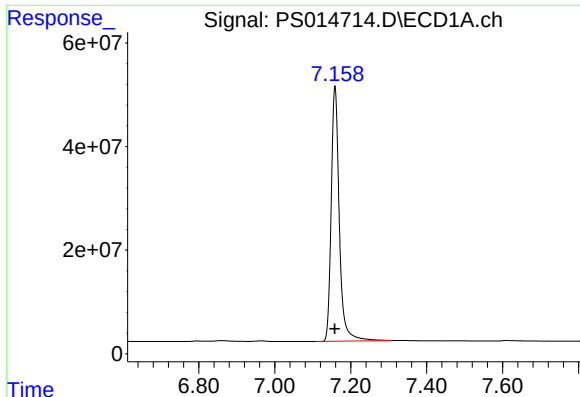

#4 2,4-DCAA


R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 727160112
Conc: 478.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

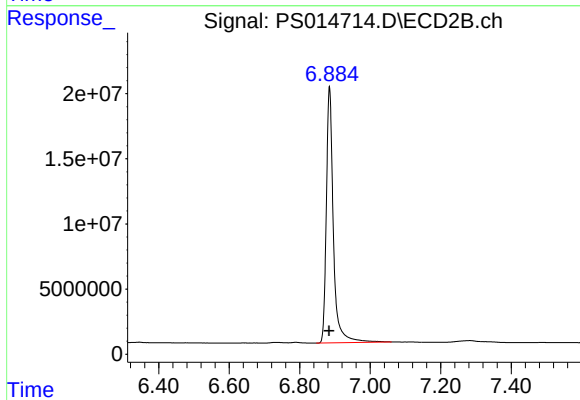


#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 271780845
Conc: 583.90 ng/ml

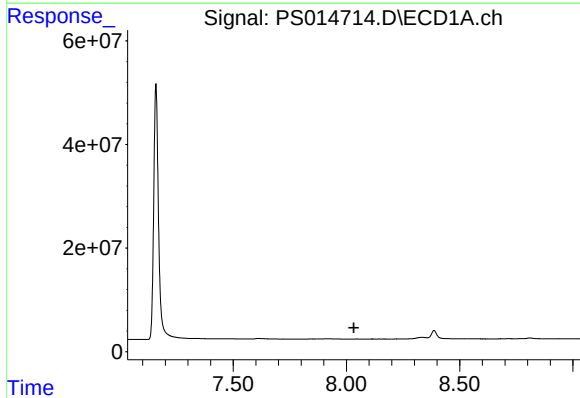


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

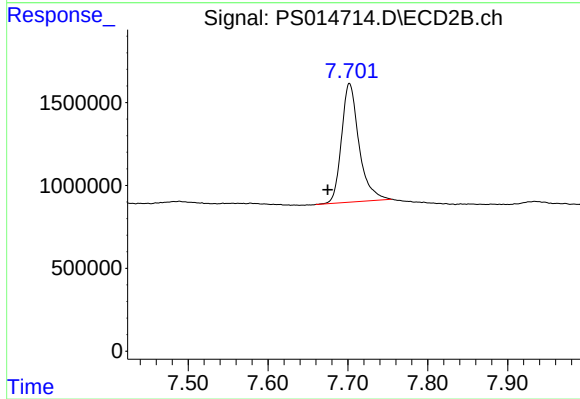

#8 DICHLORPROP


R.T.: 7.702 min
Delta R.T.: 0.027 min
Response: 10928717
Conc: 21.65 ng/ml

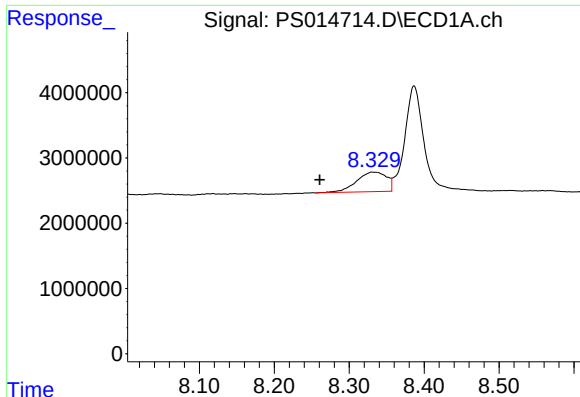

#9 2,4-D


R.T.: 8.330 min
Delta R.T.: 0.069 min
Response: 8315576
Conc: 5.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

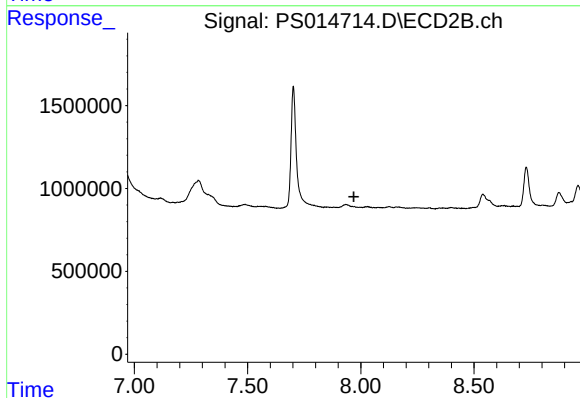


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.970 min
Response: 0
Conc: N.D.

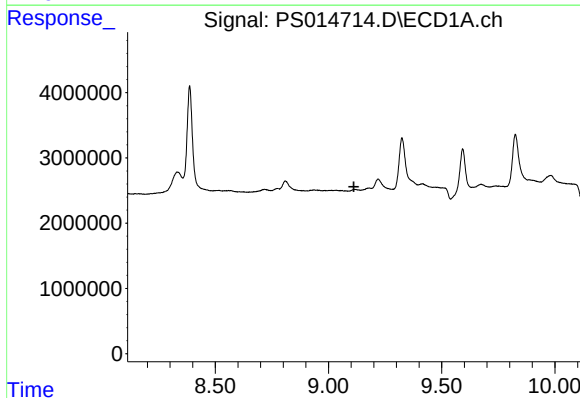


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.112 min
Response: 0
Conc: N.D.

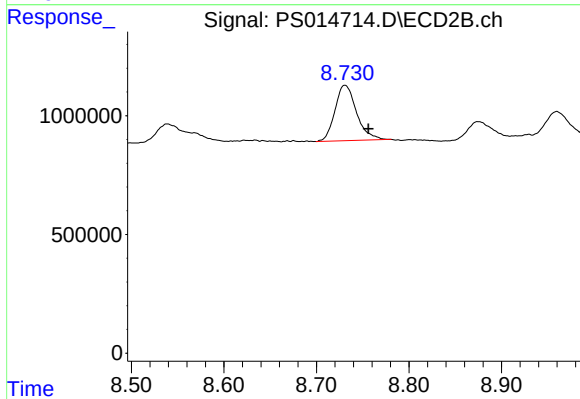

#11 2,4,5-TP (SILVEX)


R.T.: 8.731 min
Delta R.T.: -0.025 min
Response: 3775448
Conc: 1.38 ng/ml

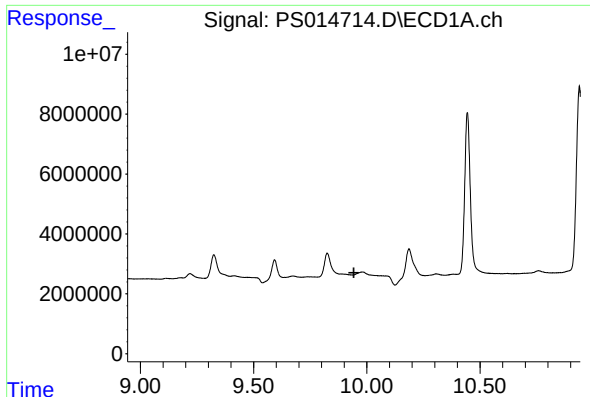

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.943 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

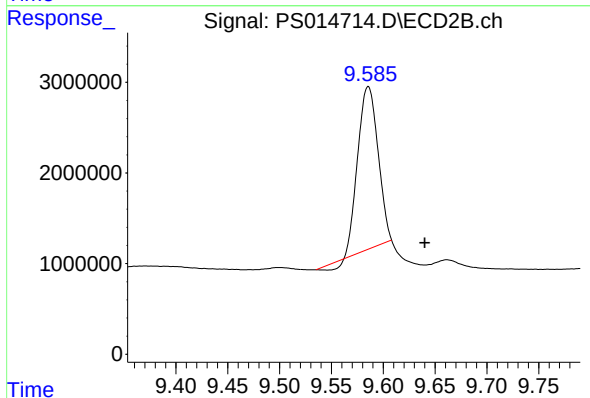


#13 2,4-DB

R.T.: 9.586 min
Delta R.T.: -0.054 min
Response: 23981098
Conc: 69.14 ng/ml

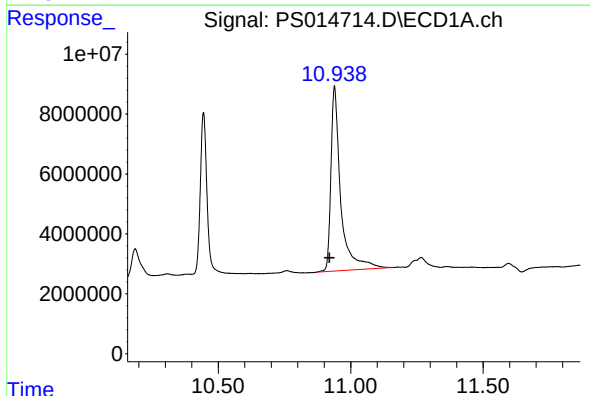

#15 Picloram

R.T.: 10.939 min
Delta R.T.: 0.020 min
Response: 159989644
Conc: 14.30 ng/ml

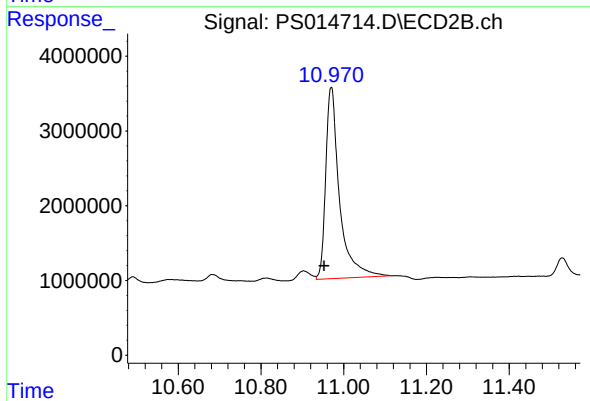

#15 Picloram

R.T.: 10.970 min
Delta R.T.: 0.017 min
Response: 59258613
Conc: 15.80 ng/ml