

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
 Data File : PS014726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 13:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 14:45:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.884	690.7E6	255.6E6	454.068	549.153
Target Compounds							
8) T	DICHLORPROP	0.000	7.703	0	8441943	N.D.	16.723
11) T	2,4,5-TP ...	0.000	8.731	0	5806731	N.D.	2.126
12) T	2,4,5-T	9.326f	0.000	7585750	0	<MDL	N.D. #
13) T	2,4-DB	9.916	9.587f	44816703	14433447	29.451	41.610 #
15) T	Picloram	10.944	10.972	106.0E6	41497456	9.478	11.066
16) T	DCPA	11.415f	0.000	4002439	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
Data File : PS014726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 13:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 14:45:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

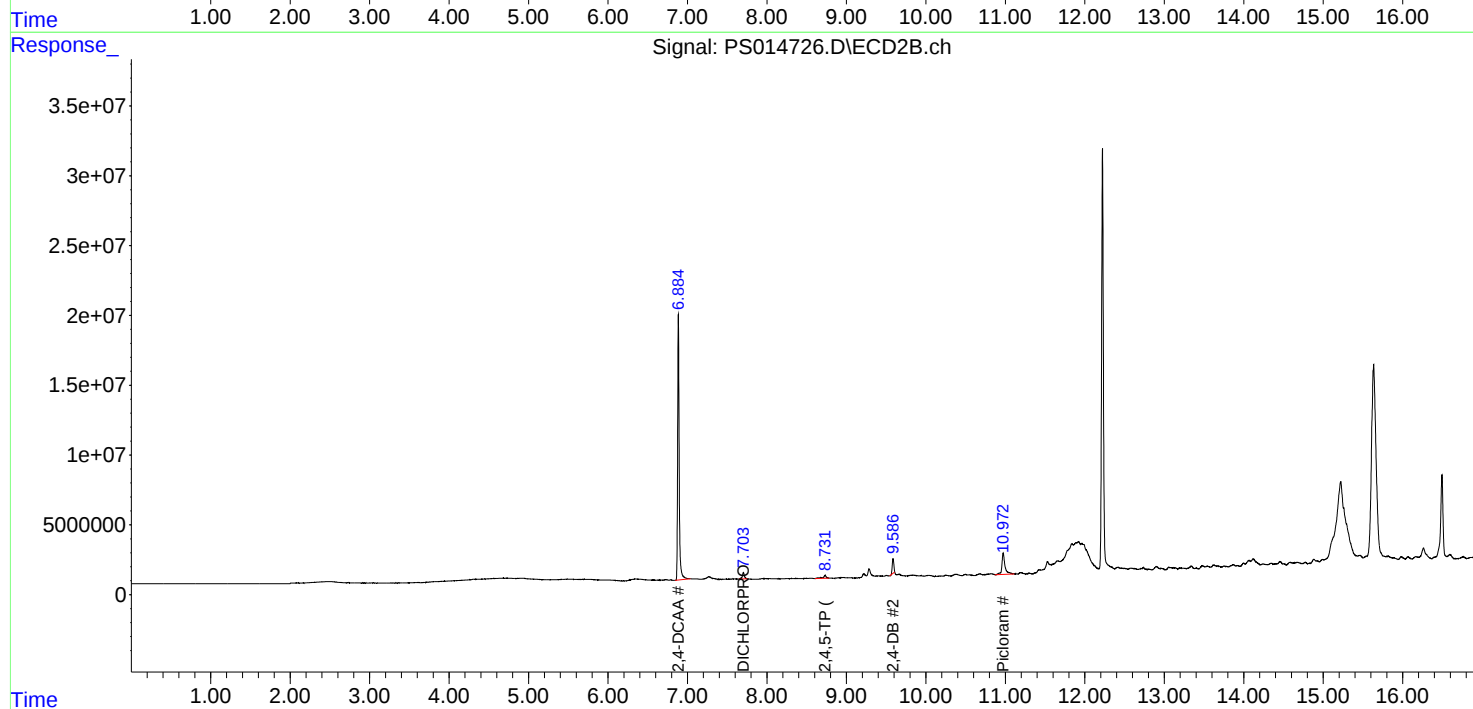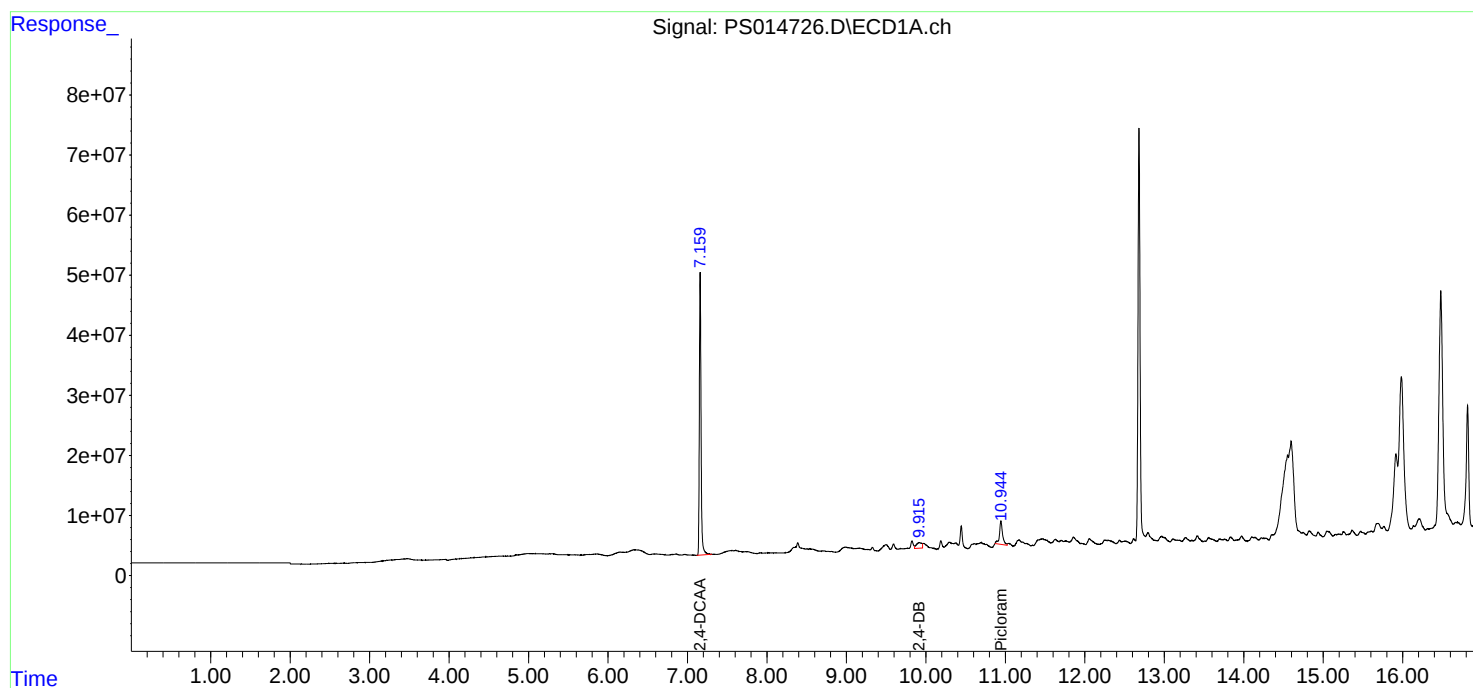


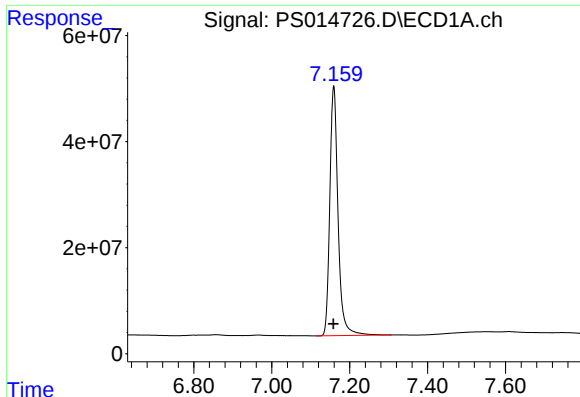

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.001 min
Response: 690726274
Conc: 454.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

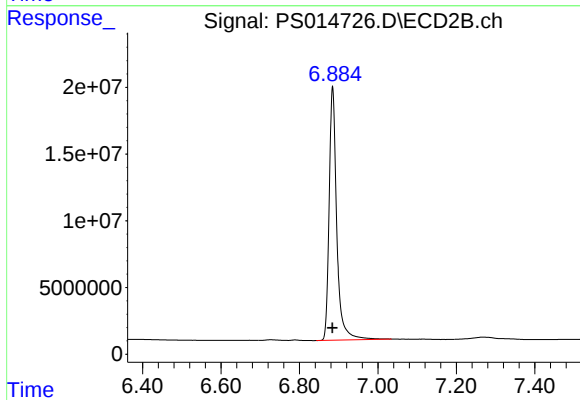


#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 255605886
Conc: 549.15 ng/ml

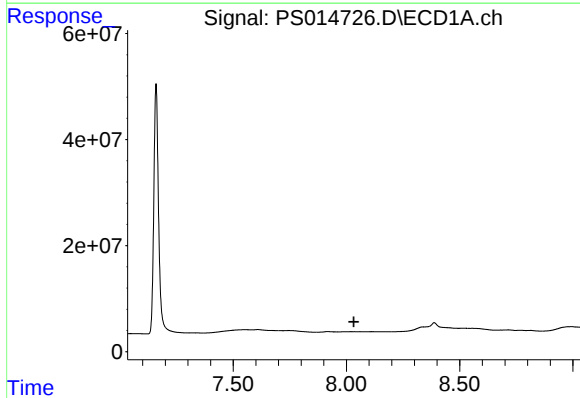


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

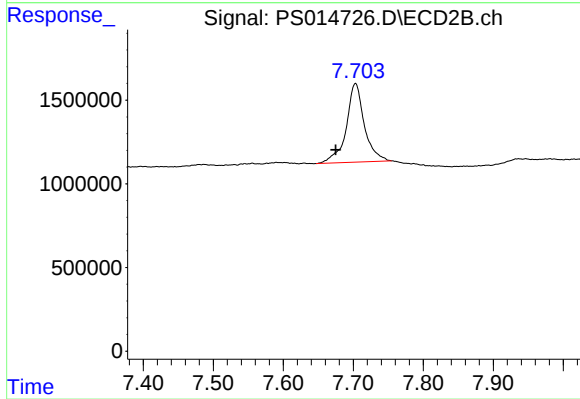

#8 DICHLORPROP


R.T.: 7.703 min
Delta R.T.: 0.028 min
Response: 8441943
Conc: 16.72 ng/ml

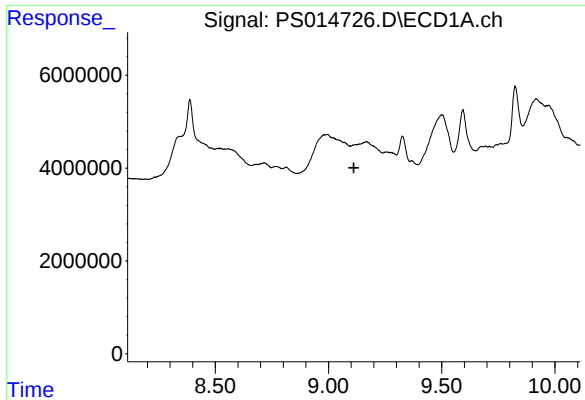

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

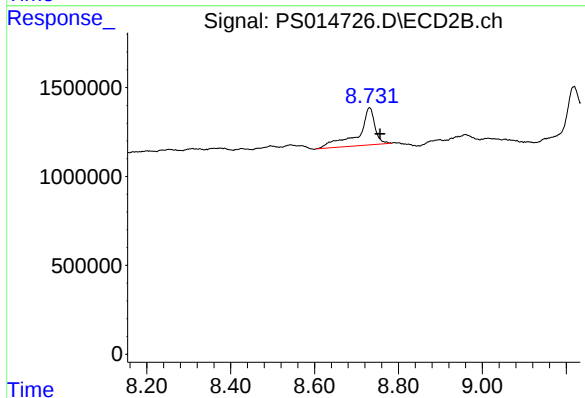


#11 2,4,5-TP (SILVEX)

R.T.: 8.731 min
Delta R.T.: -0.025 min
Response: 5806731
Conc: 2.13 ng/ml

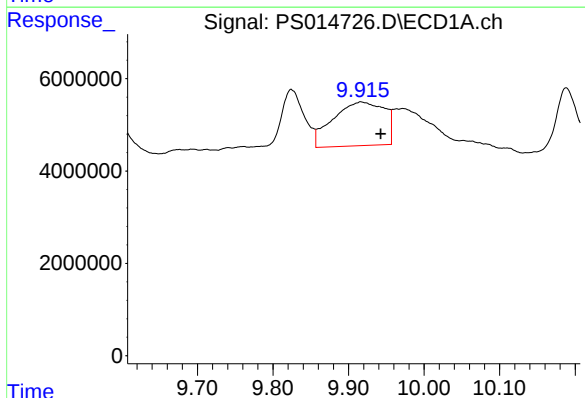


#13 2,4-DB

R.T.: 9.916 min
Delta R.T.: -0.026 min
Response: 44816703
Conc: 29.45 ng/ml

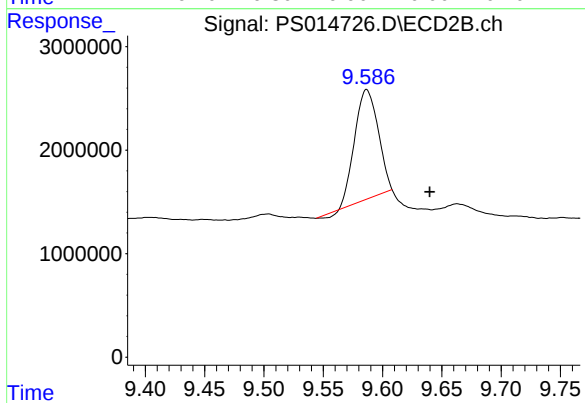

#13 2,4-DB


R.T.: 9.587 min
Delta R.T.: -0.053 min
Response: 14433447
Conc: 41.61 ng/ml

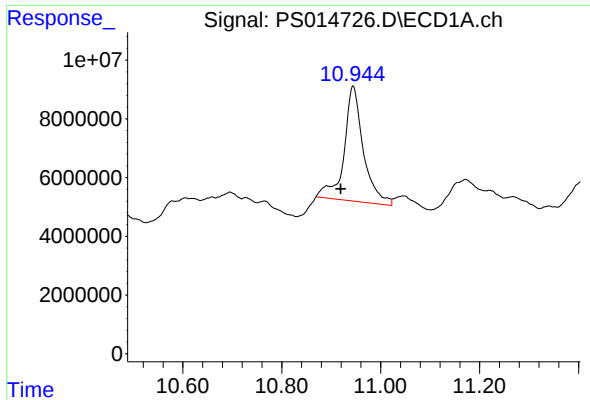

#15 Picloram

R.T.: 10.944 min
Delta R.T.: 0.025 min
Response: 106038952
Conc: 9.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

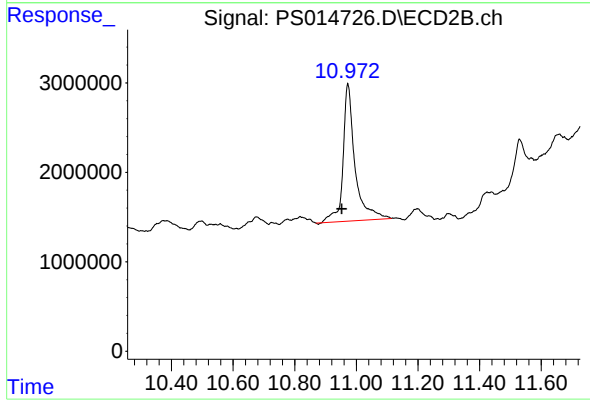

#15 Picloram

R.T.: 10.972 min
Delta R.T.: 0.020 min
Response: 41497456
Conc: 11.07 ng/ml