

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
 Data File : PS014734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 16:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 17:31:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.885	691.7E6	258.6E6	454.741	555.623
Target Compounds							
8) T	DICHLORPROP	0.000	7.706	0	5513678	N.D.	10.922
11) T	2,4,5-TP ...	0.000	8.737	0	1914963	N.D.	<MDL
12) T	2,4,5-T	9.334f	0.000	14242920	0	1.731	N.D. #
13) T	2,4-DB	0.000	9.590f	0	5977267	N.D.	17.232
15) T	Picloram	10.948	10.975	139.6E6	53751835	12.480	14.334



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
Data File : PS014734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 16:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 17:31:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

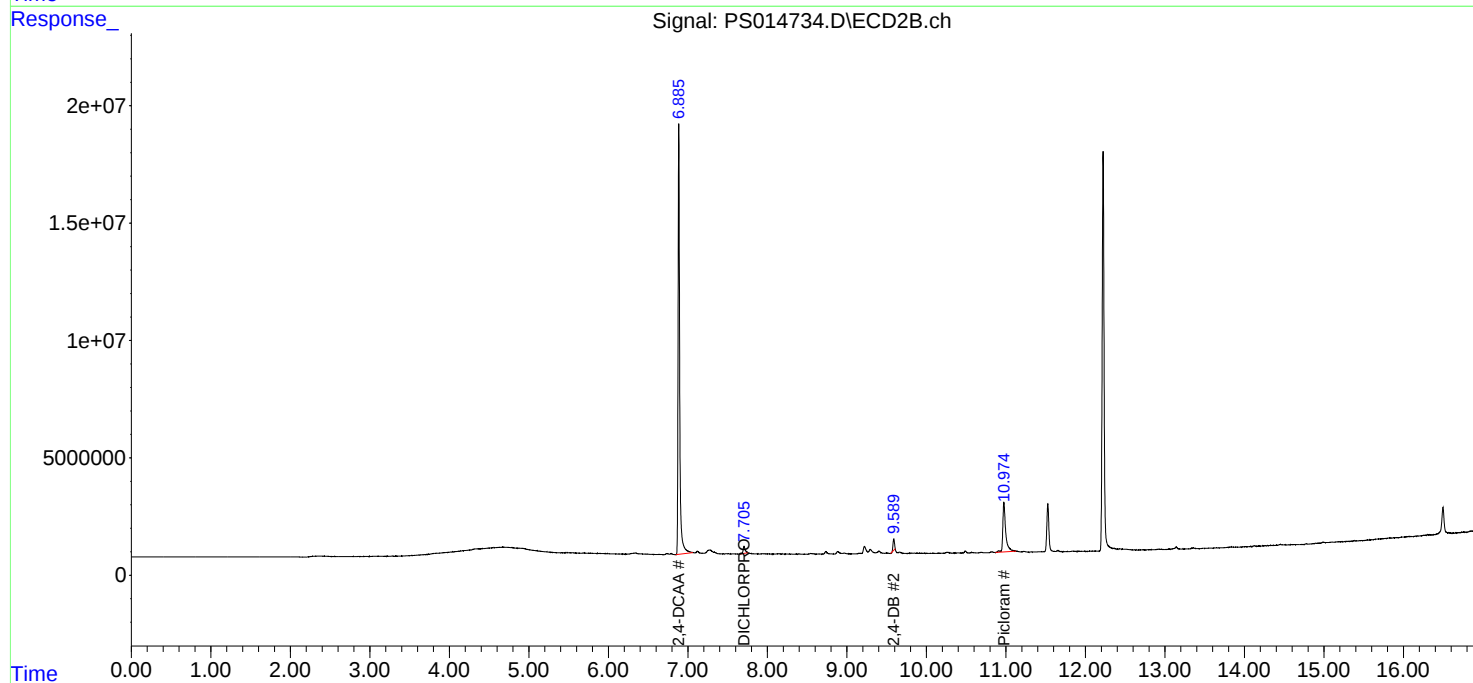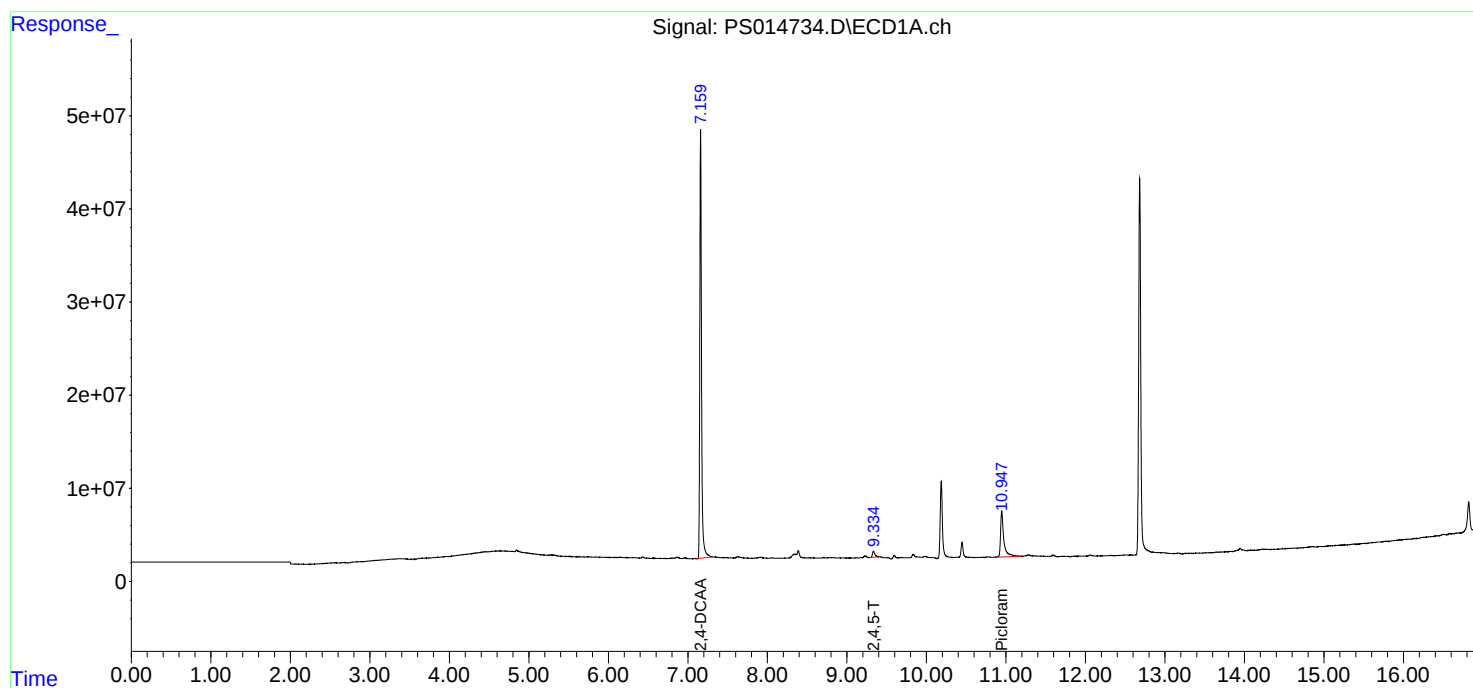


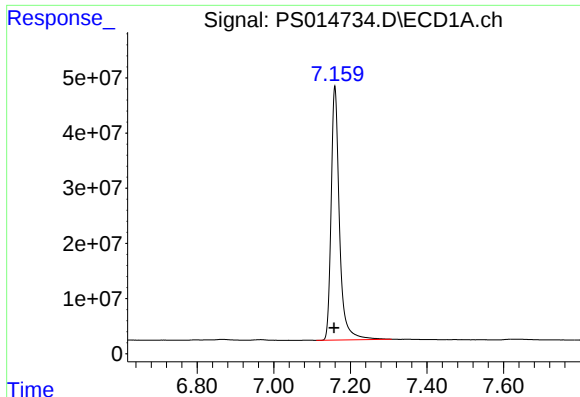

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.002 min
Response: 691749276
Conc: 454.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

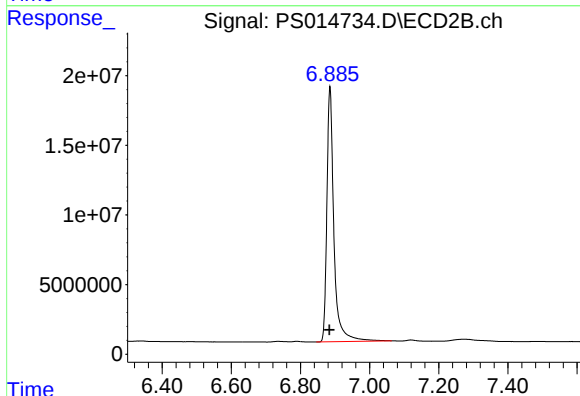


#4 2,4-DCAA

R.T.: 6.885 min
Delta R.T.: 0.002 min
Response: 258617142
Conc: 555.62 ng/ml

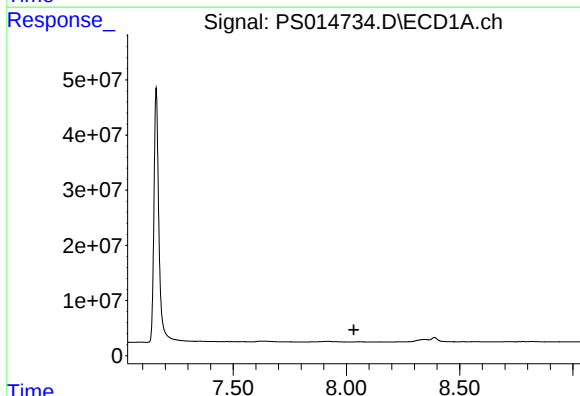


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

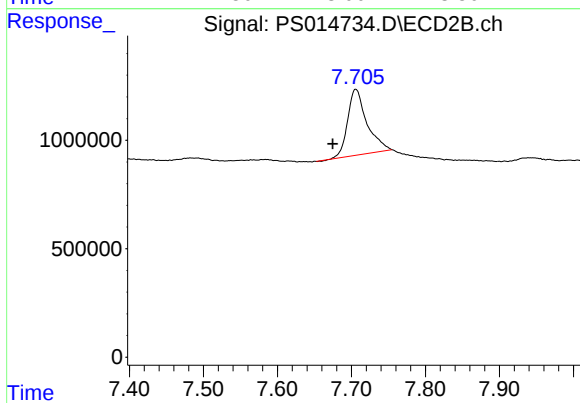

#8 DICHLORPROP


R.T.: 7.706 min
Delta R.T.: 0.031 min
Response: 5513678
Conc: 10.92 ng/ml

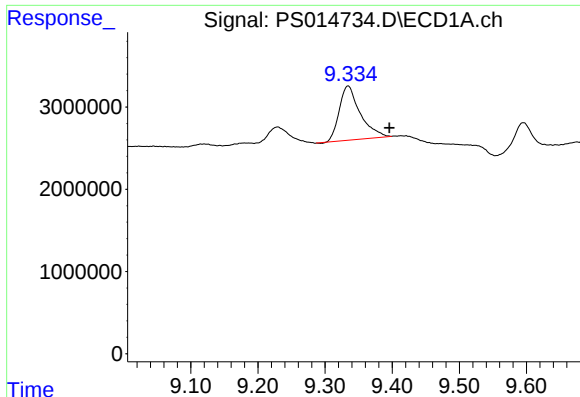

#12 2,4,5-T


R.T.: 9.334 min
Delta R.T.: -0.062 min
Response: 14242920
Conc: 1.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

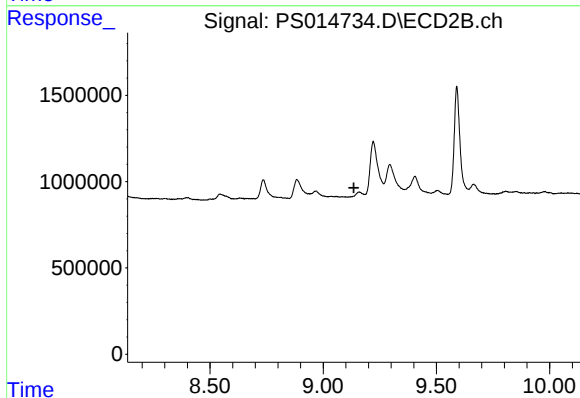


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.135 min
Response: 0
Conc: N.D.

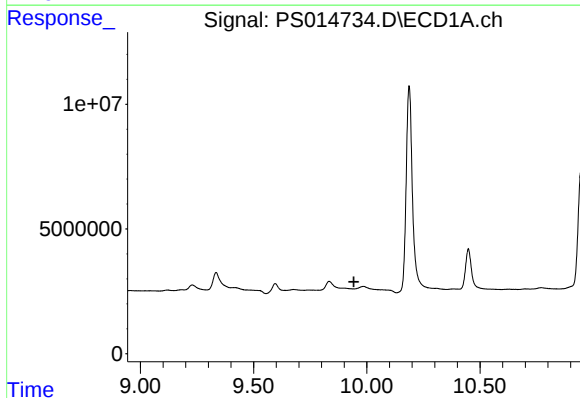


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.943 min
Response: 0
Conc: N.D.

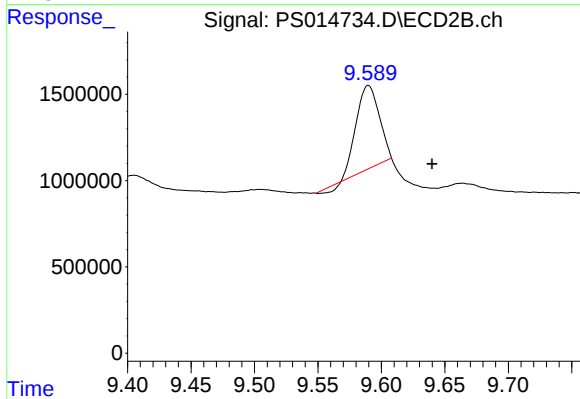

#13 2,4-DB


R.T.: 9.590 min
Delta R.T.: -0.050 min
Response: 5977267
Conc: 17.23 ng/ml

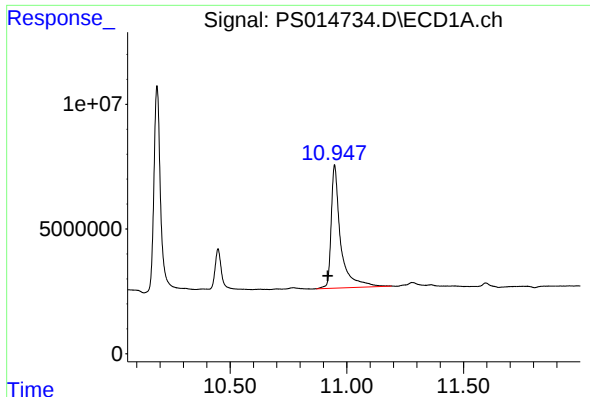

#15 Picloram

R.T.: 10.948 min
Delta R.T.: 0.029 min
Response: 139627702
Conc: 12.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

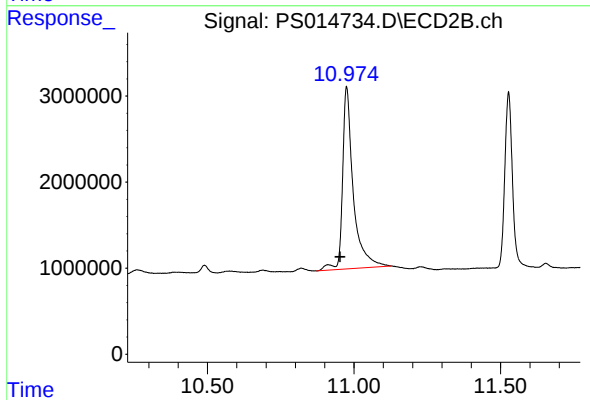

#15 Picloram

R.T.: 10.975 min
Delta R.T.: 0.022 min
Response: 53751835
Conc: 14.33 ng/ml