

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042122\
 Data File : PS019106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2022 09:40
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 01:23:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.474f	0.000	9468420	0	1.904	N.D.	#
5) T	DICAMBA	7.415	7.023f	13059569	1976768	<MDL	<MDL	#
6) T	MCP	0.000	7.023f	0	1976768	N.D.	<MDL	#
7) T	MCPA	7.677f	0.000	9618374	0	<MDL	N.D.	#
8) T	DICHLORPROP	0.000	7.612	0	2489501	N.D.	2.979	#
9) T	2,4-D	8.351	0.000	22847502	0	5.567	N.D.	#
10) T	Pentachlo...	8.651	0.000	9371243	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.205	8.629	18491246	1928389	<MDL	<MDL	#
12) T	2,4,5-T	9.491	9.052	13811397	1515579	<MDL	<MDL	#
13) T	2,4-DB	10.047	0.000	4944420	0	1.404	N.D.	#
15) T	Picloram	10.992	10.873	86126165	68326469	3.214	11.540	#
16) T	DCPA	11.467	10.873f	4046943	68326469	<MDL	11.937	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042122\
Data File : PS019106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2022 09:40
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 01:23:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

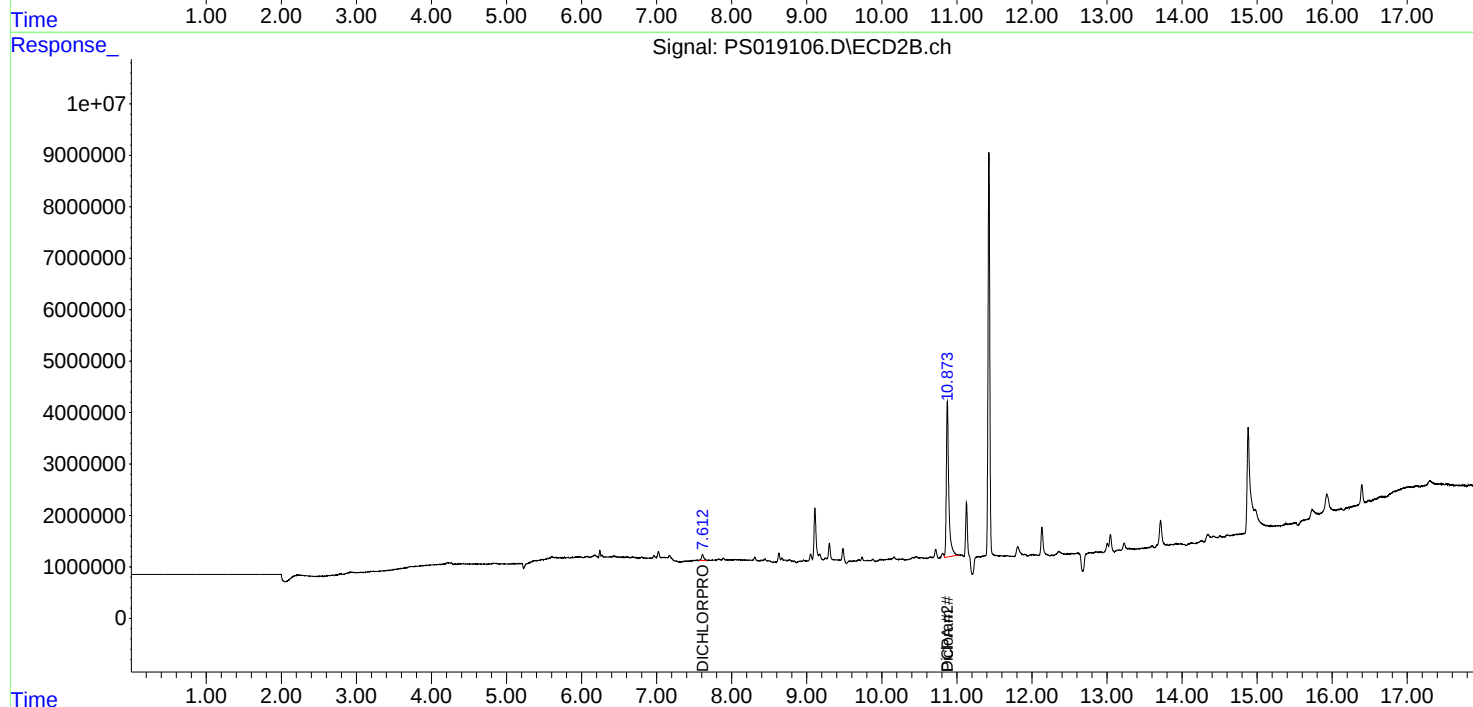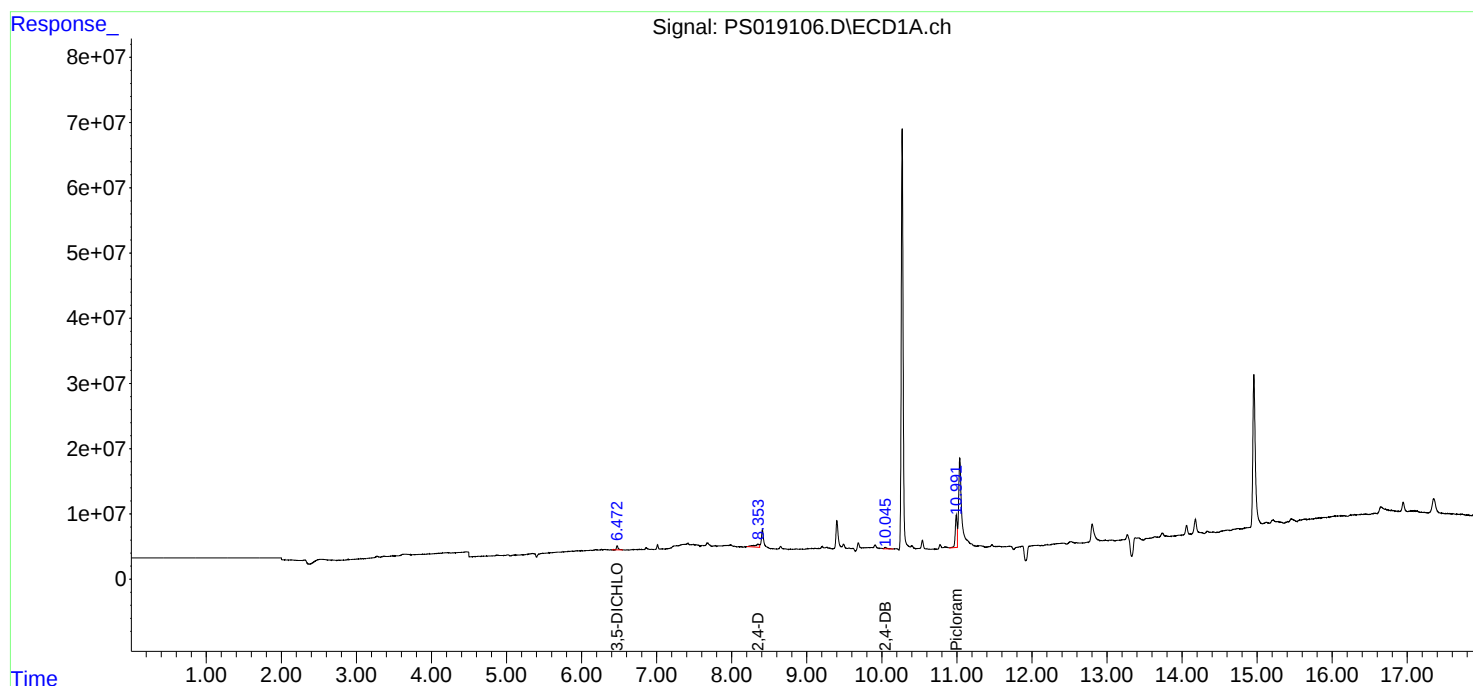


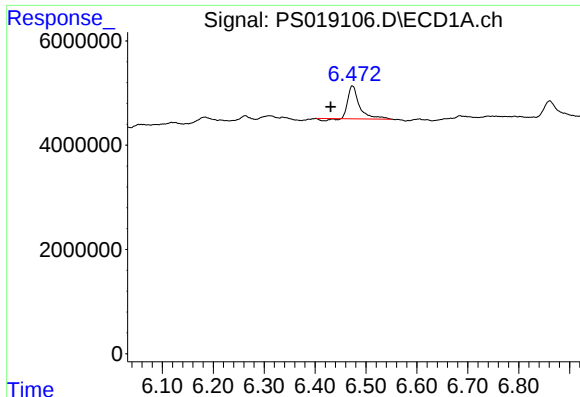

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.474 min
Delta R.T.: 0.043 min
Response: 9468420
Conc: 1.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

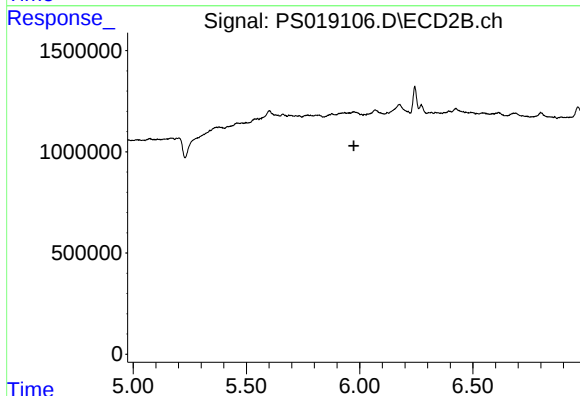


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.975 min
Response: 0
Conc: N.D.

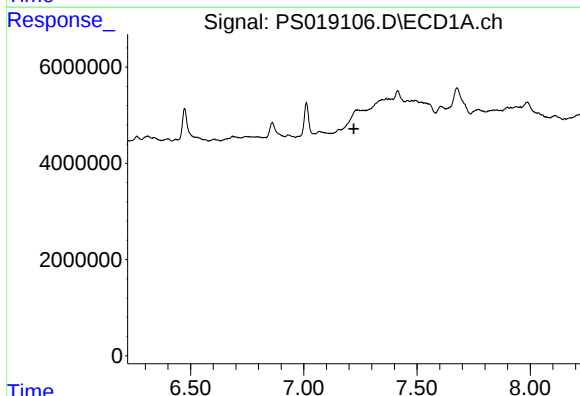


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.221 min
Response: 0
Conc: N.D.

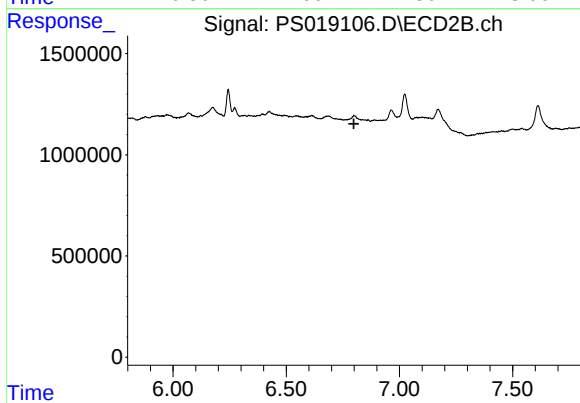

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

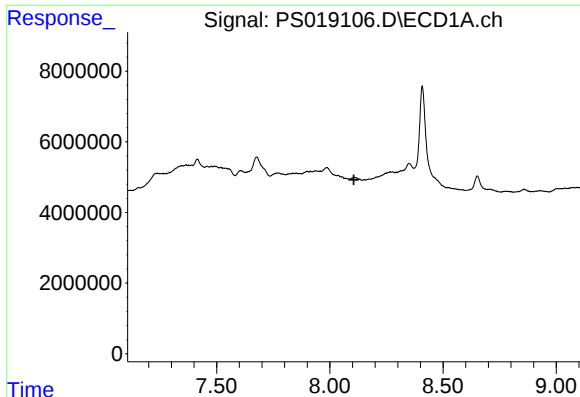

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

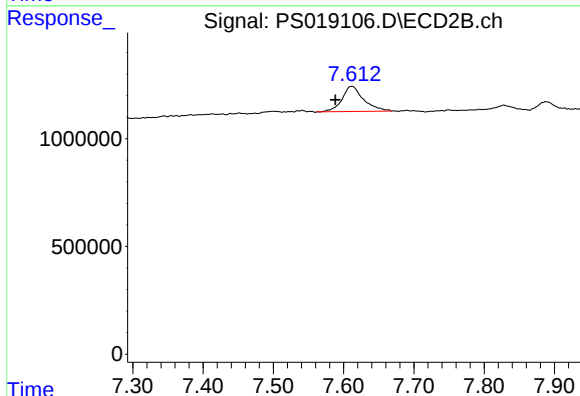


#8 DICHLORPROP

R.T.: 7.612 min
Delta R.T.: 0.024 min
Response: 2489501
Conc: 2.98 ng/ml

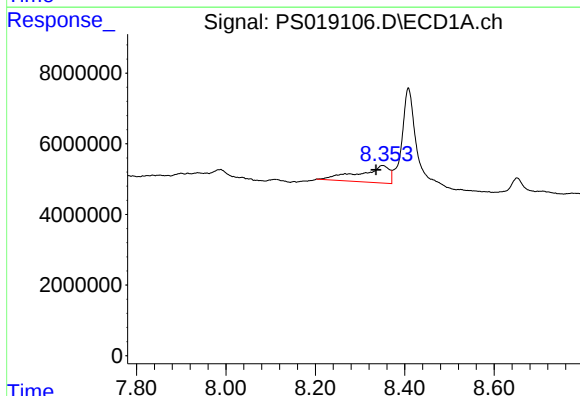


#9 2,4-D

R.T.: 8.351 min
Delta R.T.: 0.015 min
Response: 22847502
Conc: 5.57 ng/ml

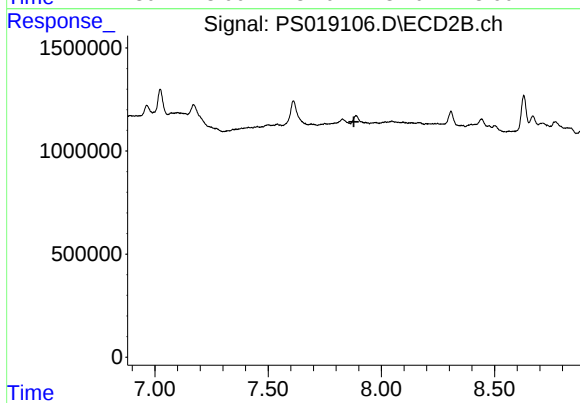

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.879 min
Response: 0
Conc: N.D.

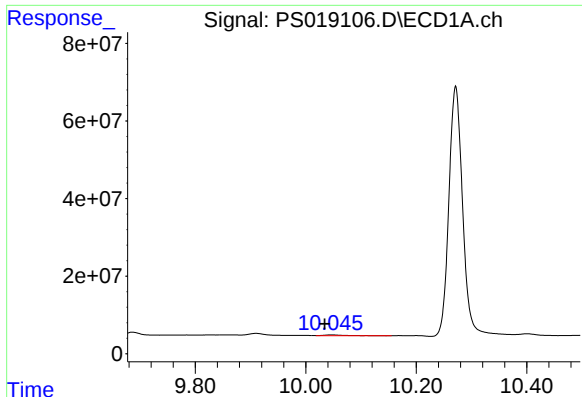

#13 2,4-DB


R.T.: 10.047 min
Delta R.T.: 0.012 min
Response: 4944420
Conc: 1.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

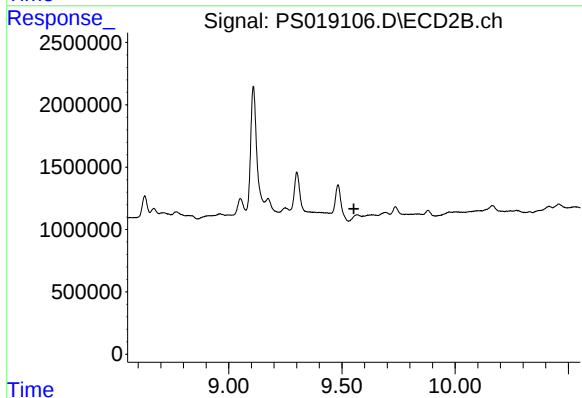


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.553 min
Response: 0
Conc: N.D.

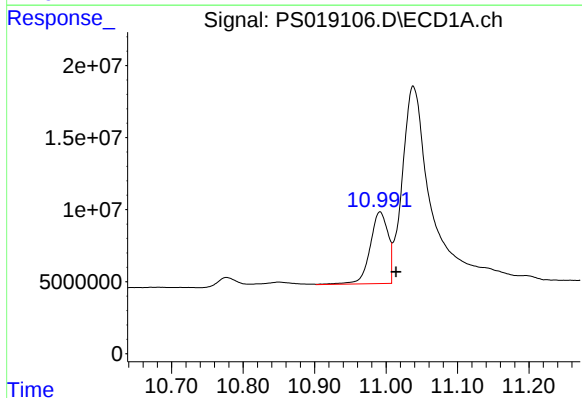


#15 Picloram

R.T.: 10.992 min
Delta R.T.: -0.022 min
Response: 86126165
Conc: 3.21 ng/ml

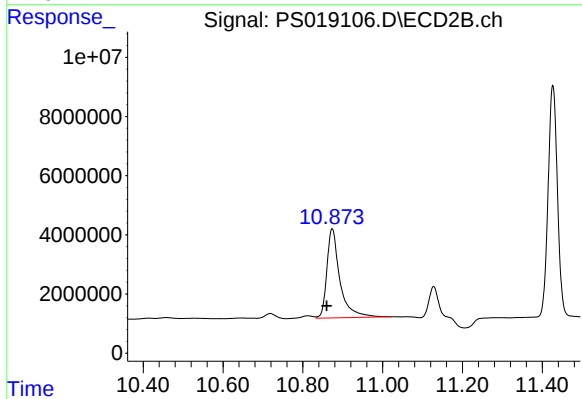

#15 Picloram


R.T.: 10.873 min
Delta R.T.: 0.014 min
Response: 68326469
Conc: 11.54 ng/ml

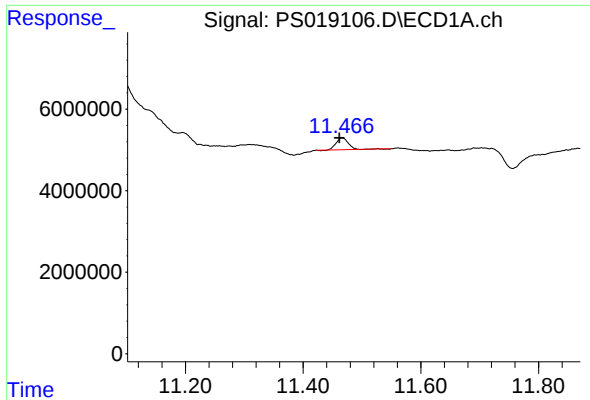

#16 DCPA

R.T.: 11.467 min
Delta R.T.: 0.005 min
Response: 4046943
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

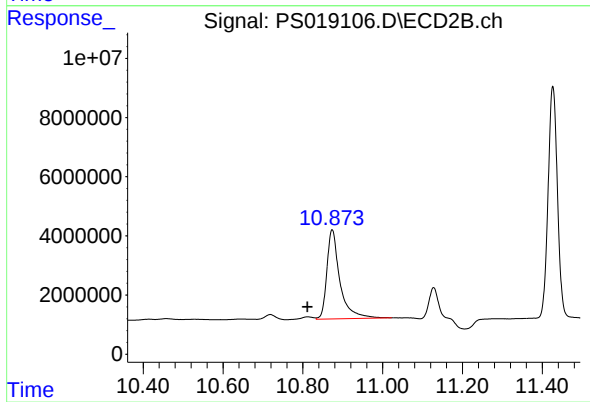

#16 DCPA

R.T.: 10.873 min
Delta R.T.: 0.062 min
Response: 68326469
Conc: 11.94 ng/ml