

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042122\
 Data File : PS019115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2022 14:34
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 01:25:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.222	6.797	1561.0E6	355.8E6	417.364	490.114
Target Compounds							
7) T	MCPA	7.677f	0.000	11577571	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.614	0	2231561	N.D.	2.670
9) T	2,4-D	8.329	0.000	7066667	0	1.722	N.D. #
11) T	2,4,5-TP ...	9.210	8.629	301664	7985208	<MDL	1.696 #
12) T	2,4,5-T	9.492	9.114f	5645819	6597885	<MDL	1.528 #
13) T	2,4-DB	10.003	0.000	2396327	0	<MDL	N.D. #
14) T	DINOSEB	11.146f	0.000	43953608	0	2.873	N.D. #
15) T	Picloram	10.994	10.883	18604513	11939543	<MDL	2.016 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042122\
Data File : PS019115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2022 14:34
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 01:25:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

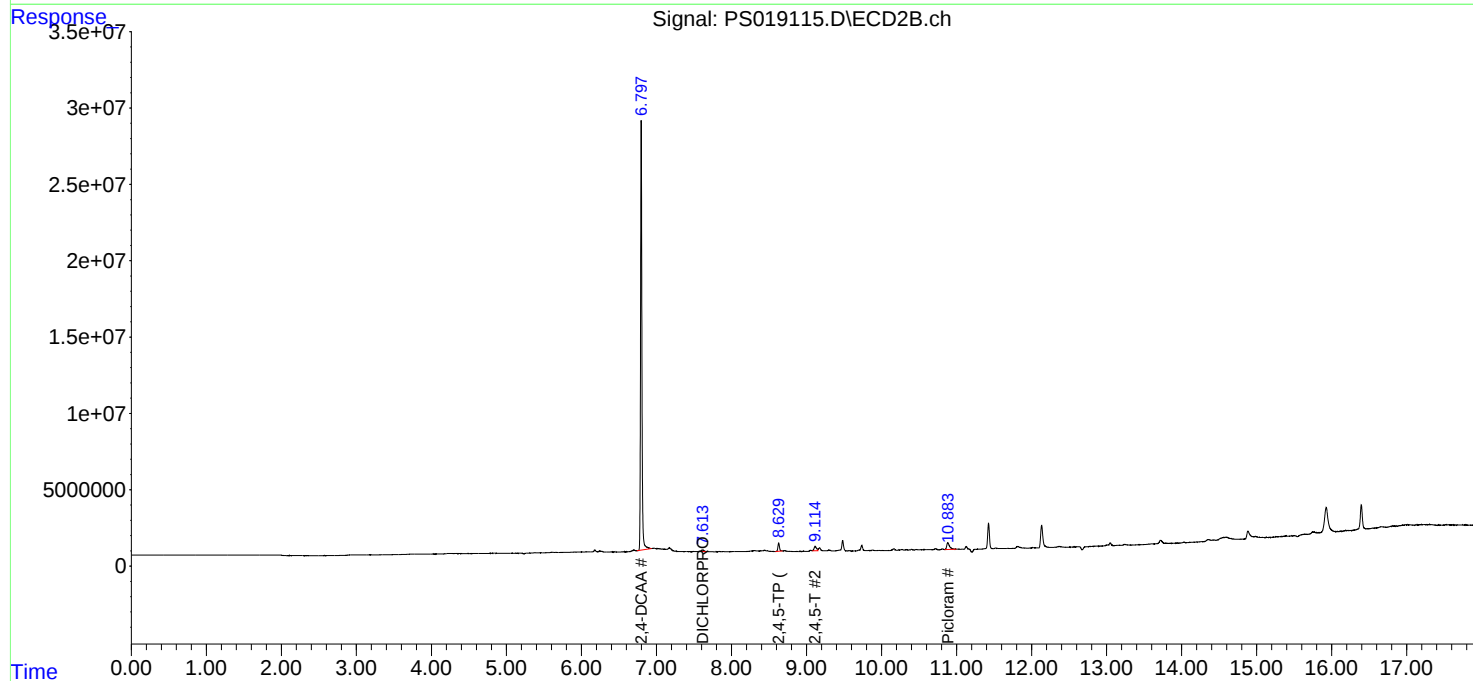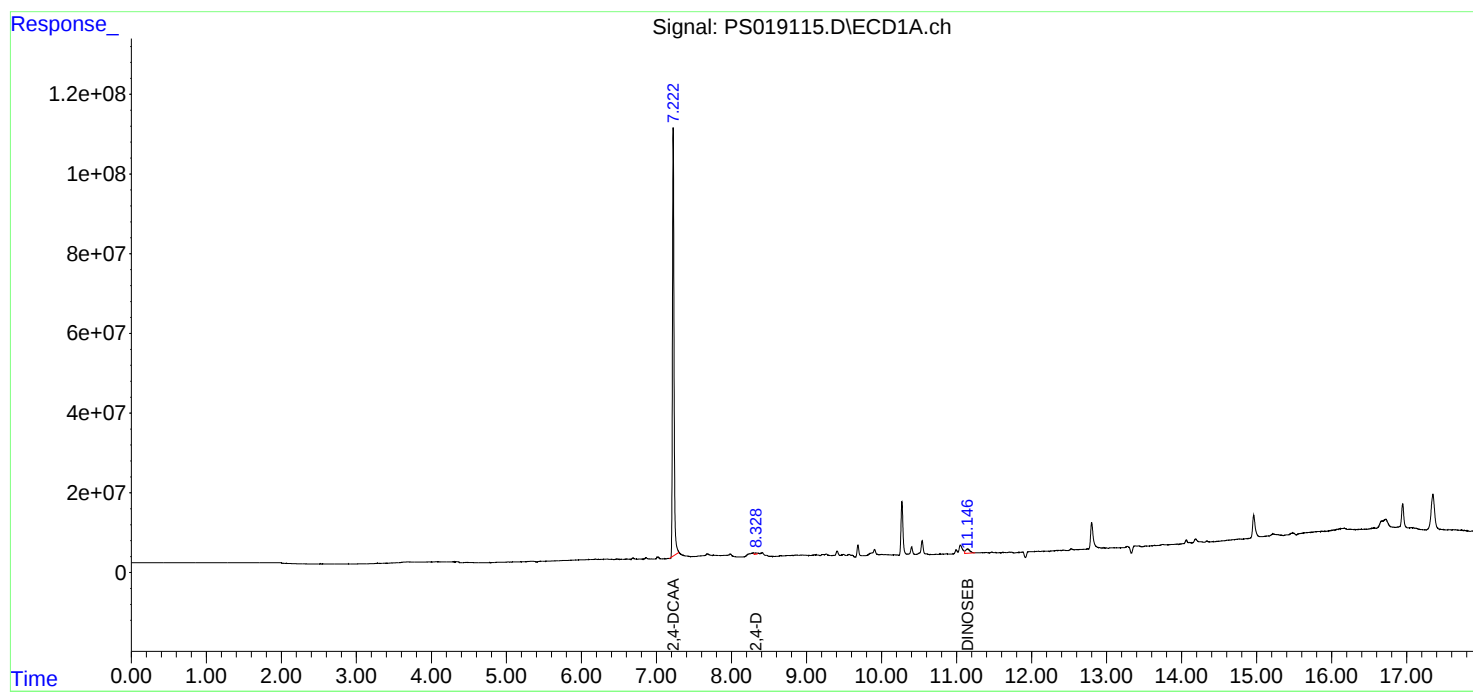


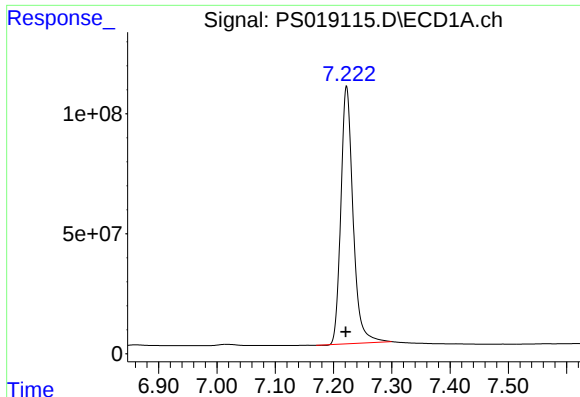

#4 2,4-DCAA


R.T.: 7.222 min
Delta R.T.: 0.001 min
Response: 1560963517
Conc: 417.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

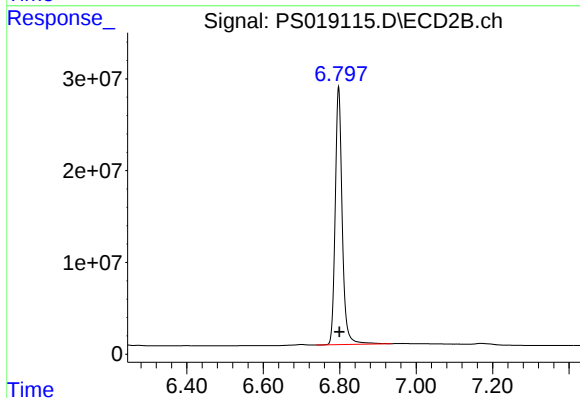


#4 2,4-DCAA

R.T.: 6.797 min
Delta R.T.: -0.002 min
Response: 355762371
Conc: 490.11 ng/ml

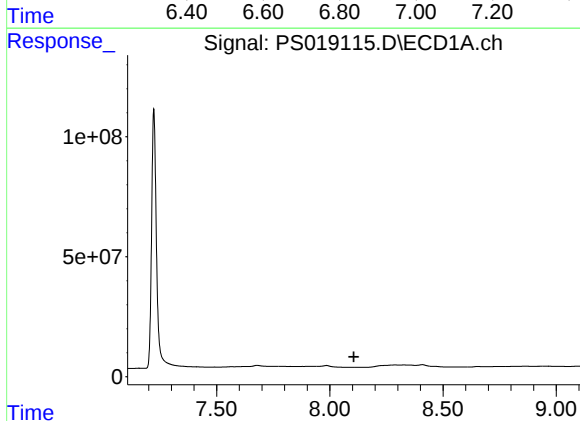


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.106 min
Response: 0
Conc: N.D.

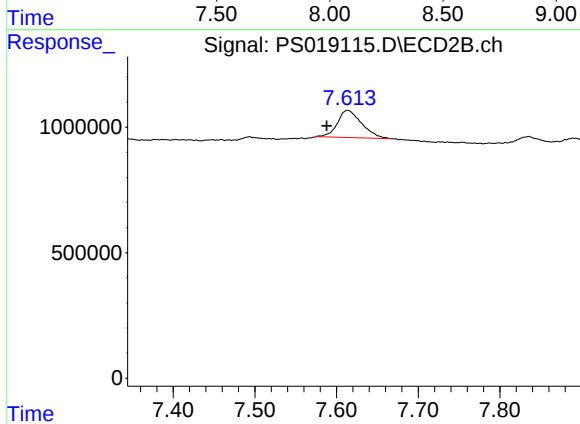

#8 DICHLORPROP


R.T.: 7.614 min
Delta R.T.: 0.025 min
Response: 2231561
Conc: 2.67 ng/ml

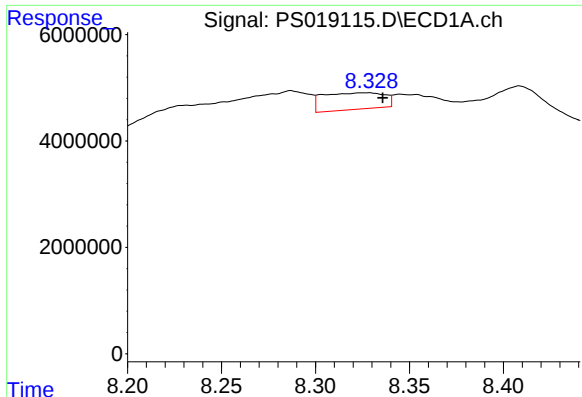

#9 2,4-D


R.T.: 8.329 min
Delta R.T.: -0.007 min
Response: 7066667
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

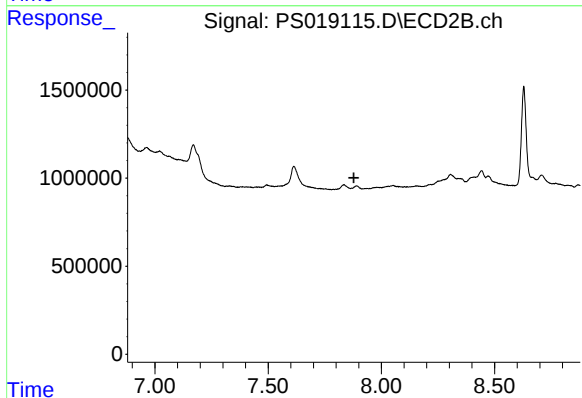


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.879 min
Response: 0
Conc: N.D.

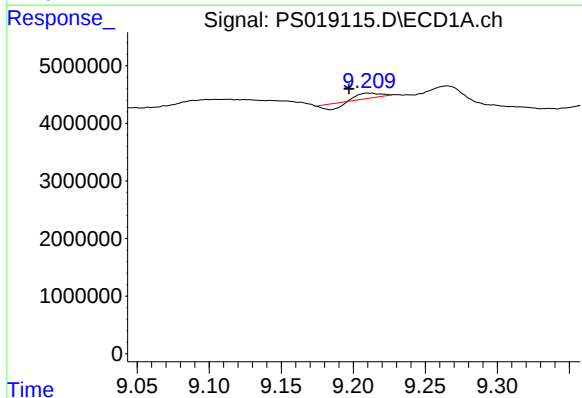


#11 2,4,5-TP (SILVEX)

R.T.: 9.210 min
Delta R.T.: 0.013 min
Response: 301664
Conc: N.D.

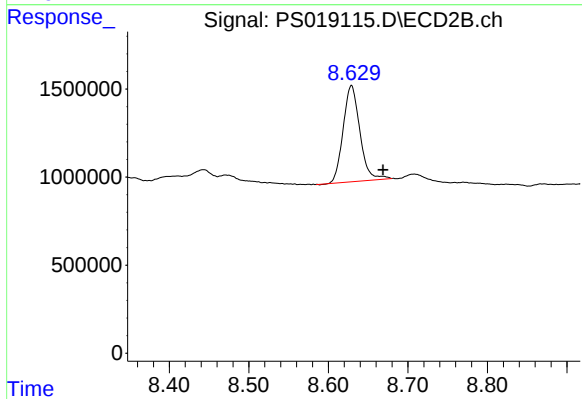

#11 2,4,5-TP (SILVEX)


R.T.: 8.629 min
Delta R.T.: -0.040 min
Response: 7985208
Conc: 1.70 ng/ml

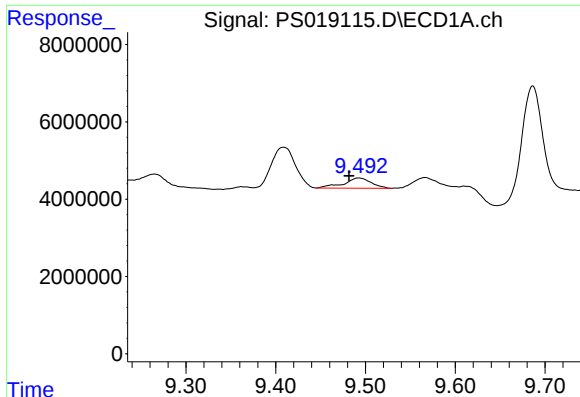

#12 2,4,5-T


R.T.: 9.492 min
Delta R.T.: 0.011 min
Response: 5645819
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

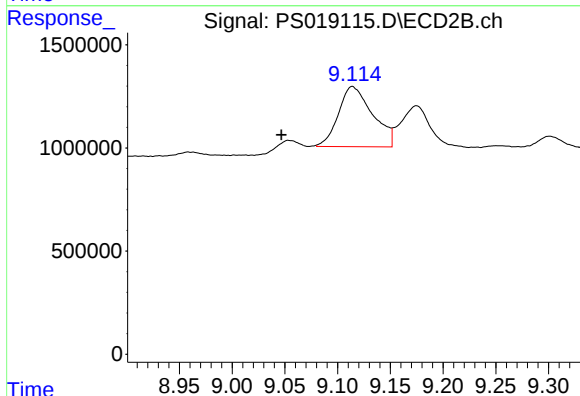


#12 2,4,5-T

R.T.: 9.114 min
Delta R.T.: 0.067 min
Response: 6597885
Conc: 1.53 ng/ml

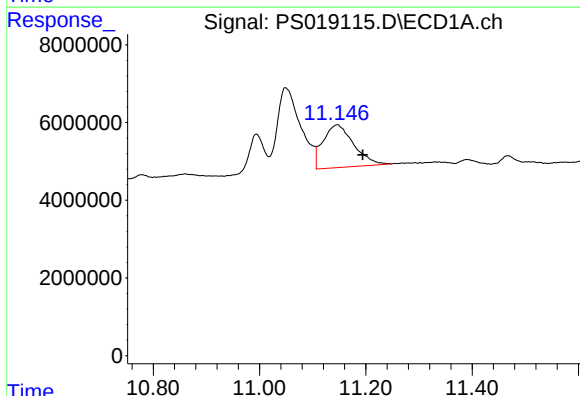


#14 DINOSEB

R.T.: 11.146 min
Delta R.T.: -0.048 min
Response: 43953608
Conc: 2.87 ng/ml

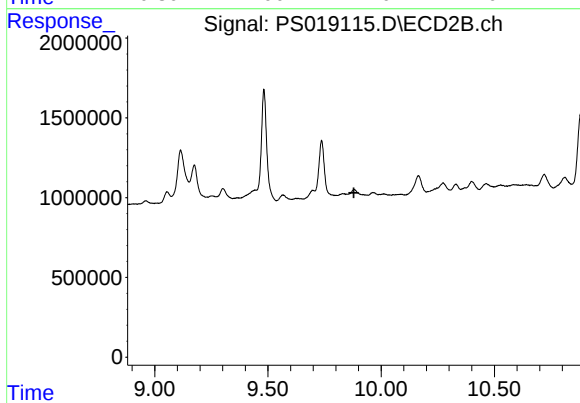

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.880 min
Response: 0
Conc: N.D.

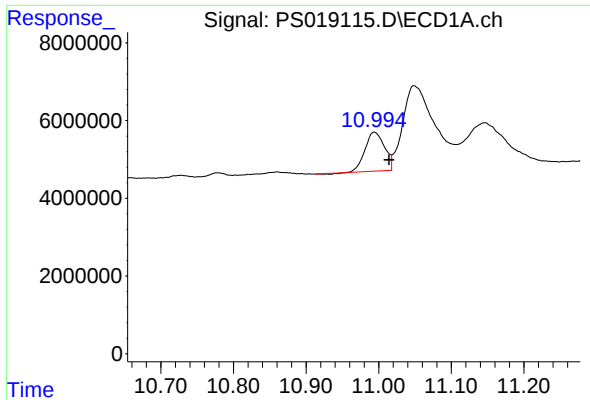

#15 Picloram

R.T.: 10.994 min
Delta R.T.: -0.020 min
Response: 18604513
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

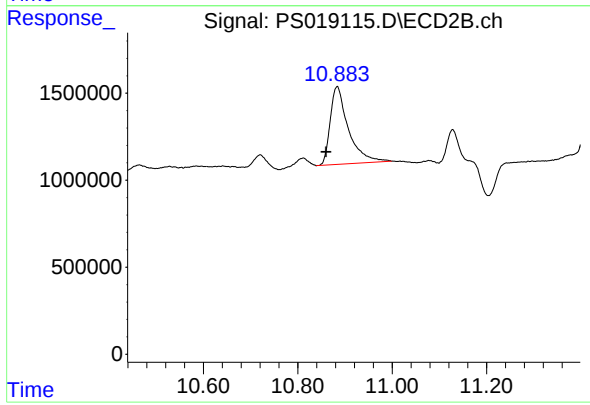

#15 Picloram

R.T.: 10.883 min
Delta R.T.: 0.024 min
Response: 11939543
Conc: 2.02 ng/ml